


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG083119\
 Data File : BG042641.D
 Acq On : 31 Aug 2019 20:58
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG082219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 22 14:29:15 2019

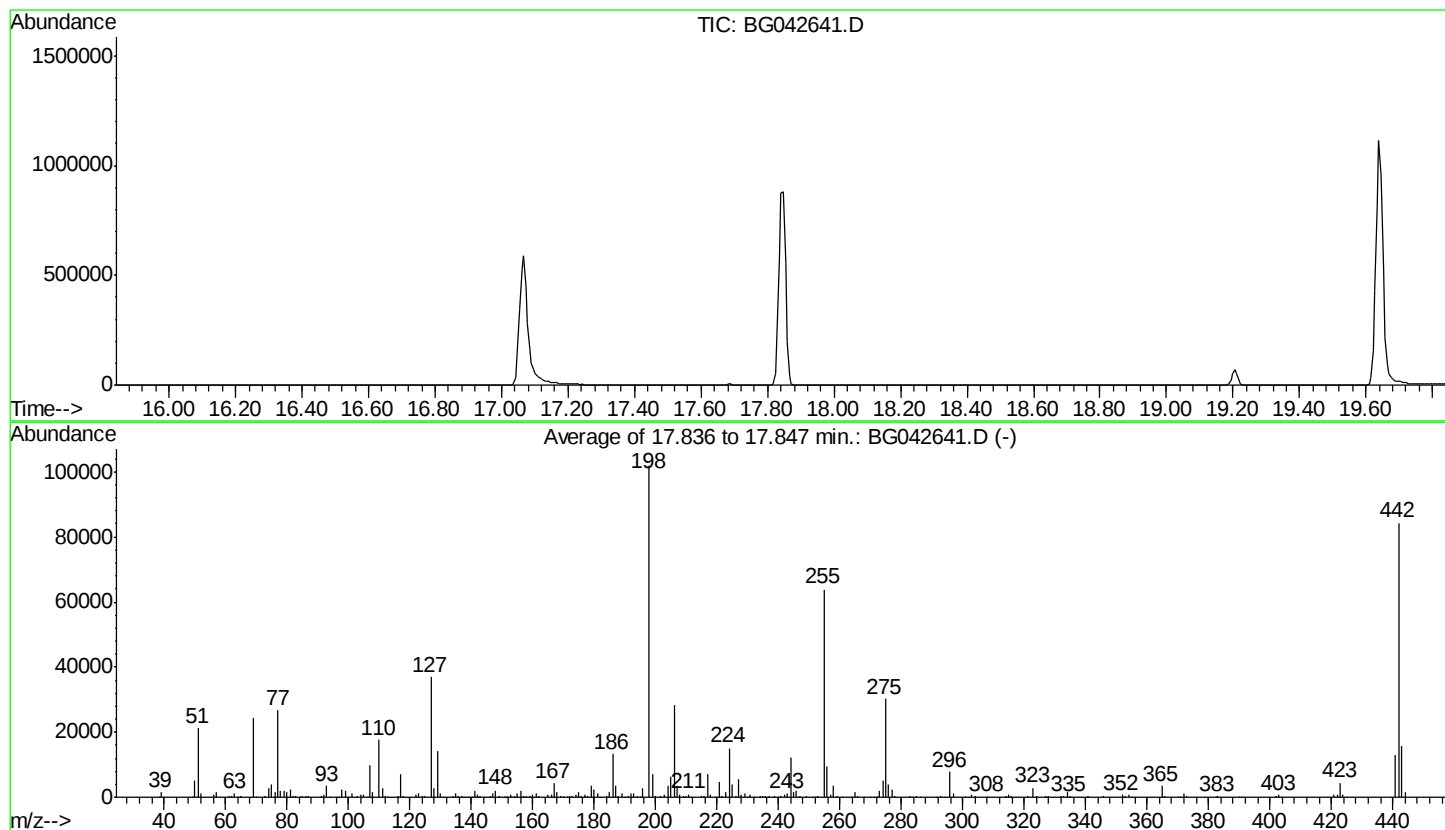

AutoFind: Scans 2510, 2511, 2512; Background Corrected with Scan 2504

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	20.7	21141	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	23.8	24296	PASS
70	69	0.00	2	0.3	66	PASS
127	198	10	80	36.3	36941	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101904	PASS
199	198	5	9	7.0	7159	PASS
275	198	10	60	29.6	30176	PASS
365	198	1	100	3.4	3424	PASS
441	198	0.01	100	12.6	12817	PASS
442	198	50	100	82.7	84261	PASS
443	442	15	24	18.8	15807	PASS