

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090320\
 Data File : BG046516.D
 Acq On : 3 Sep 2020 14:46
 Operator : CG/JU
 Sample : PB131395BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB131395BL

Quant Time: Sep 03 15:51:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 15:06:53 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.93	152	77281	20.00	ng	0.00
21) Naphthalene-d8	10.73	136	319713	20.00	ng	0.00
39) Acenaphthene-d10	14.56	164	207367	20.00	ng	0.00
64) Phenanthrene-d10	17.30	188	490739	20.00	ng	0.00
76) Chrysene-d12	21.55	240	522723	20.00	ng	0.00
86) Perylene-d12	24.65	264	523387	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.51	112	506436	116.07	ng	0.00
7) Phenol-d6	7.10	99	636030	102.83	ng	0.00
23) Nitrobenzene-d5	9.08	82	420681	75.21	ng	0.00
42) 2,4,6-Tribromophenol	16.05	330	267457	95.19	ng	0.00
45) 2-Fluorobiphenyl	13.18	172	1061122	78.12	ng	0.00
79) Terphenyl-d14	19.92	244	1670815	68.02	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.08	70	53425	14.440	ng	# 75
51) 2,6-Dinitrotoluene	14.56	165	27445	7.761	ng	# 33
57) 2,4-Dinitrotoluene	14.56	165	27445	5.443	ng	# 33
67) 4-Bromophenyl-phenylether	16.05	248	20644	3.606	ng	# 1
77) Benzidine	19.92	184	24767	2.039	ng	# 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090320\
Data File : BG046516.D
Acq On : 3 Sep 2020 14:46
Operator : CG/JU
Sample : PB131395BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB131395BL

Quant Time: Sep 03 15:51:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 15:06:53 2020
Response via : Initial Calibration

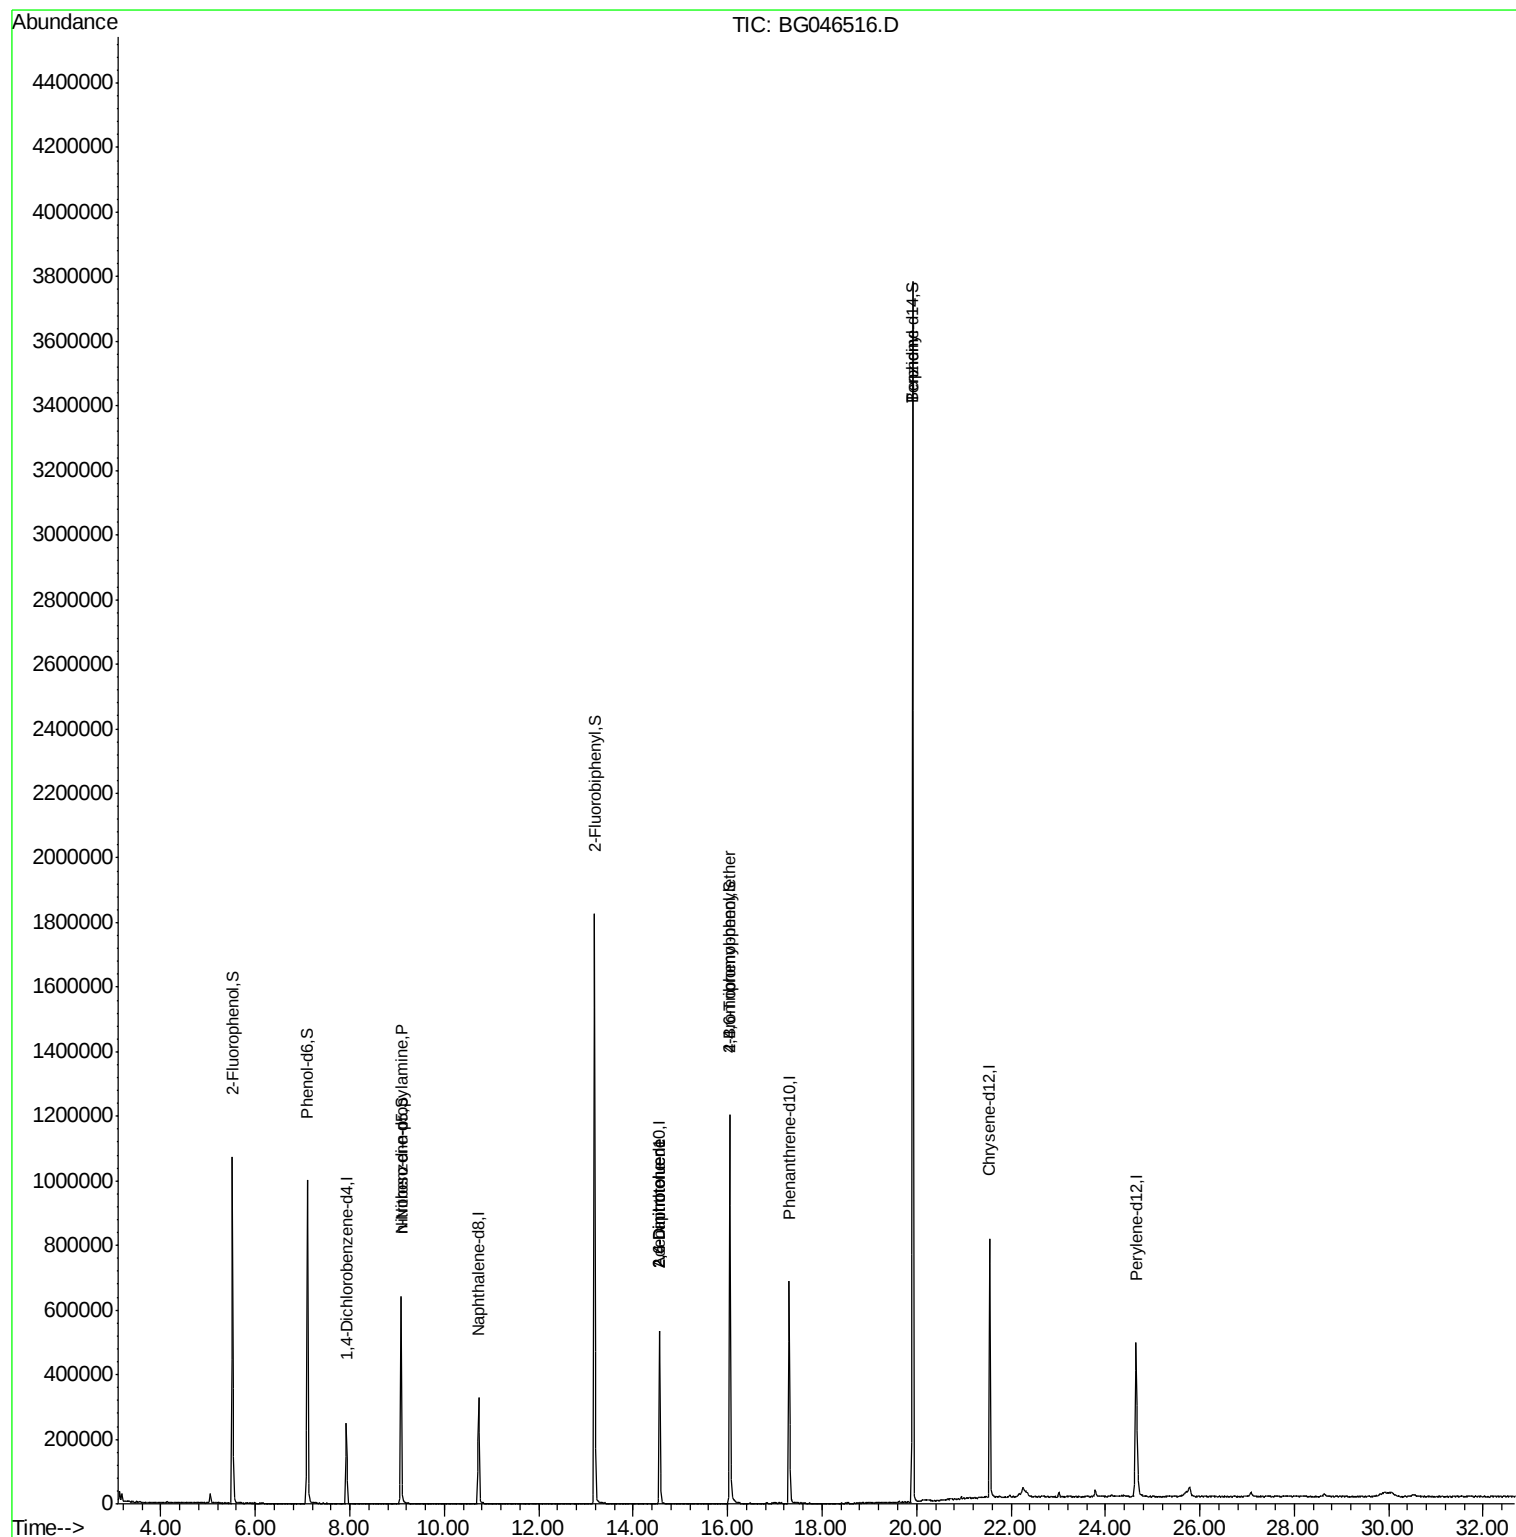



#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 7.93 min Scan# 824

Delta R.T. -0.01 min

Lab File: BG046516.D

Acq: 3 Sep 2020 14:46

Instrument :

BNA_G

ClientSampleId :

PB131395BL


Tot Ion:152 Resp: 77281

Ion Ratio Lower Upper

152 100

150 144.8 119.5 179.3




115 49.8 44.3 66.5

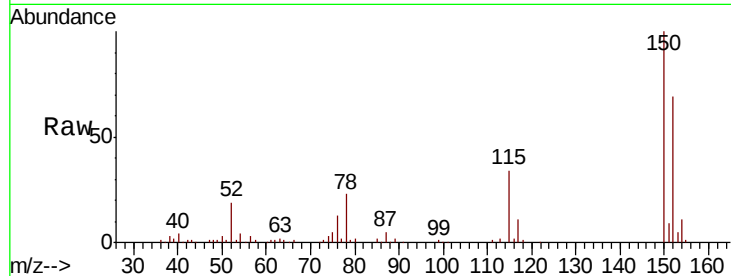

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

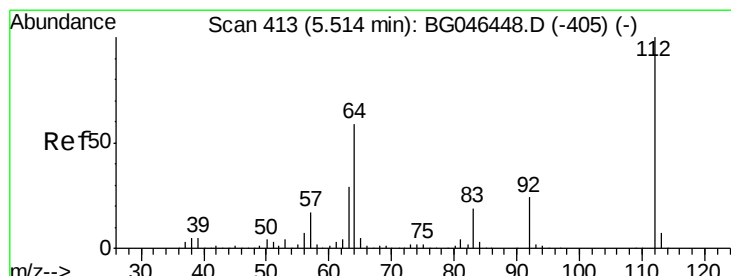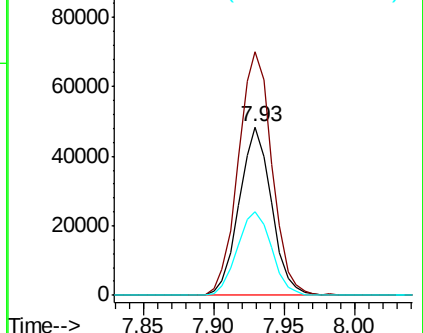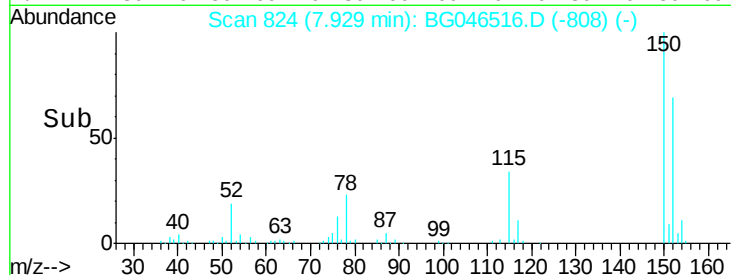

#5

2-Fluorophenol

Concen: 116.069 ng

RT: 5.51 min Scan# 413

Delta R.T. 0.00 min

Lab File: BG046516.D

Acq: 3 Sep 2020 14:46


Tgt Ion:112 Resp: 506436

Ion Ratio Lower Upper

112 100

64 62.7 47.0 70.6



63 30.6 23.5 35.3

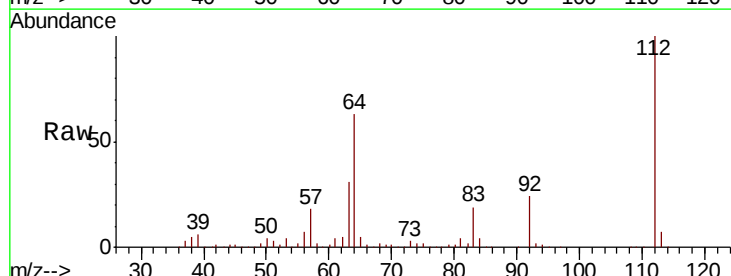


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

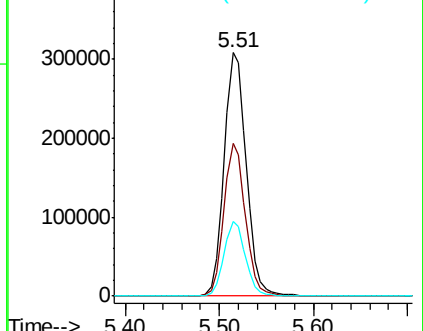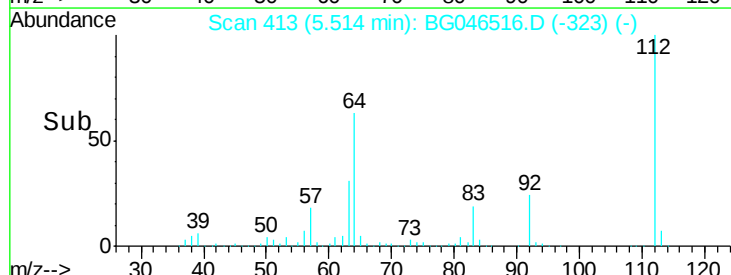

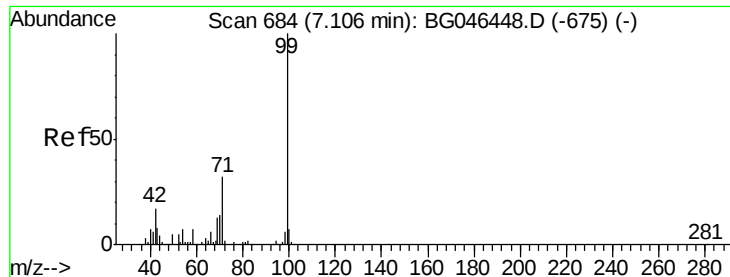

#7

Phenol-d6

Concen: 102.829 ng

RT: 7.10 min Scan# 683

Delta R.T. -0.01 min

Lab File: BG046516.D

Acq: 3 Sep 2020 14:46

Instrument :

BNA_G

ClientSampleId :

PB131395BL





Tot Ion: 99 Resp: 636030

Ion Ratio Lower Upper

99 100

42 16.7 13.3 19.9

71 32.8 25.3 37.9

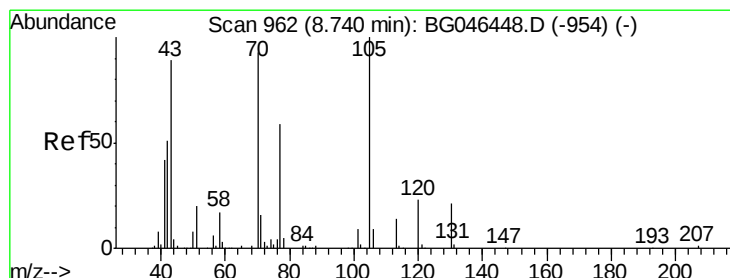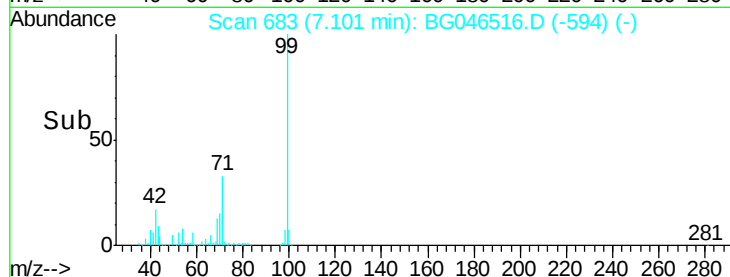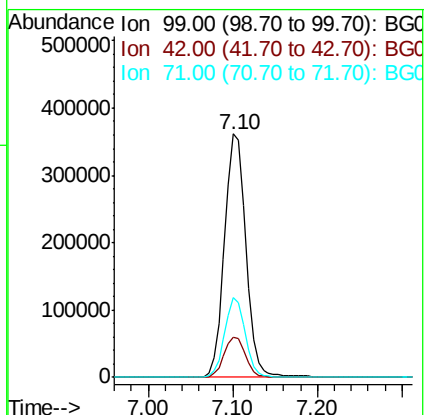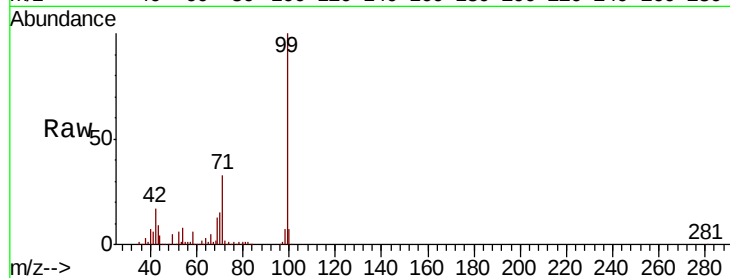

#19

n-Nitroso-di-n-propylamine

Concen: 14.440 ng

RT: 9.08 min Scan# 1020

Delta R.T. 0.35 min

Lab File: BG046516.D

Acq: 3 Sep 2020 14:46

Tgt Ion: 70 Resp: 53425




Ion Ratio Lower Upper


70 100

42 41.8 44.2 66.2#

101 0.0 7.8 11.8#

130 2.7 18.2 27.4#

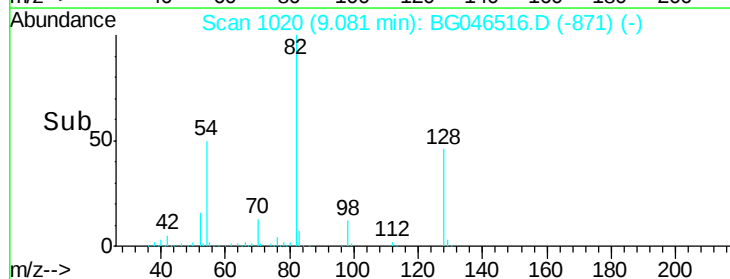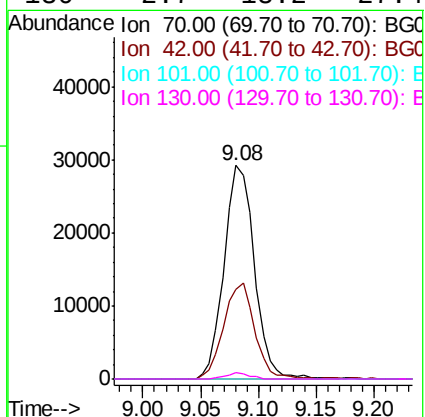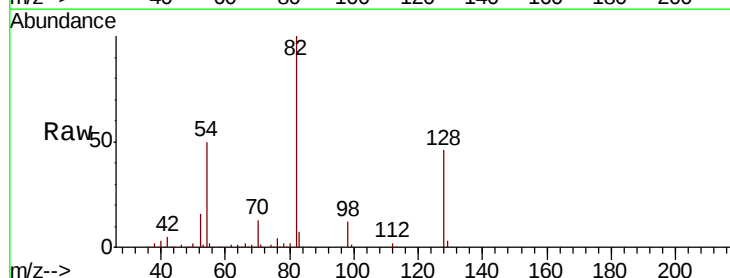







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.73 min Scan# 1300
Delta R.T. 0.00 min
Lab File: BG046516.D
Acq: 3 Sep 2020 14:46

Instrument :
BNA_G
ClientSampleId :
PB131395BL

Tot Ion:136	Resp:	319713
Ion Ratio	Lower	Upper
136 100		
137 11.3	8.8	13.2
54 8.3	6.1	9.1
68 5.9	4.8	7.2

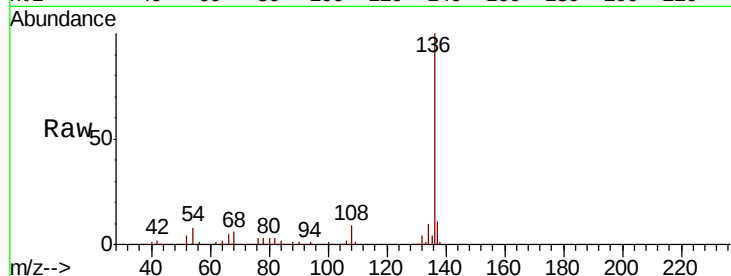


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

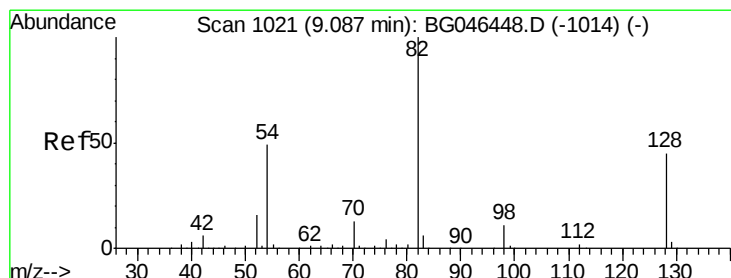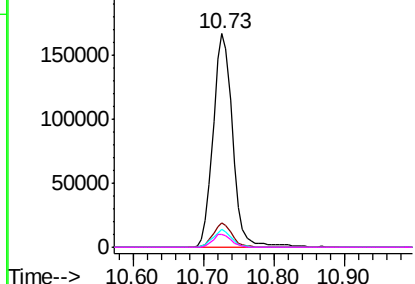




#23
Nitrobenzene-d5
Concen: 75.205 ng
RT: 9.08 min Scan# 1020
Delta R.T. -0.01 min
Lab File: BG046516.D
Acq: 3 Sep 2020 14:46

Tgt	Ion: 82	Resp:	420681
Ion	Ratio	Lower	Upper
82	100		
128	45.8	35.7	53.5
54	50.4	39.4	59.0



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

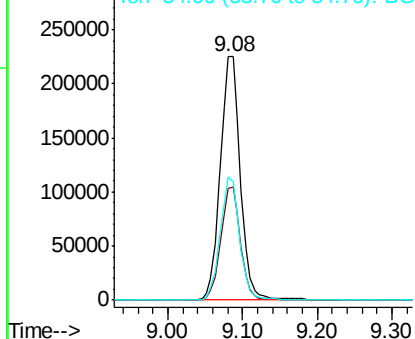



#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.56 min Scan# 1952

Delta R.T. -0.01 min

Lab File: BG046516.D

Acq: 3 Sep 2020 14:46

Instrument :

BNA_G

ClientSampleId :

PB131395BL


Tot Ion:164 Resp: 207367

Ion Ratio Lower Upper

164 100

162 104.2 83.3 124.9




160 44.4 35.0 52.6

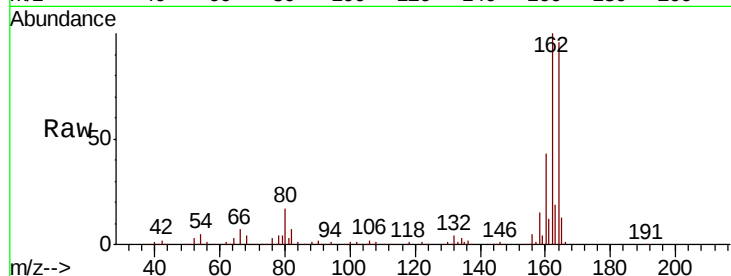

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

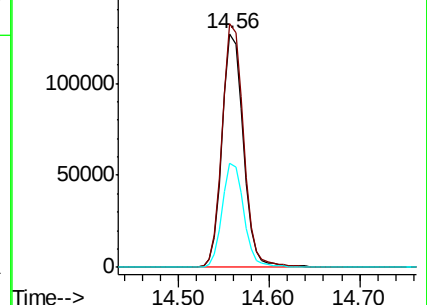

#42

2,4,6-Tribromophenol

Concen: 95.191 ng

RT: 16.05 min Scan# 2206

Delta R.T. 0.00 min

Lab File: BG046516.D

Acq: 3 Sep 2020 14:46


Tgt Ion:330 Resp: 267457

Ion Ratio Lower Upper

330 100

332 96.8 76.1 114.1



141 33.3 26.1 39.1




Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

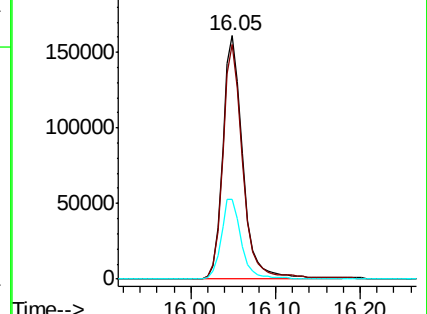







#45
 2-Fluorobiphenyl
 Concen: 78.116 ng
 RT: 13.18 min Scan# 1718
 Delta R.T. -0.01 min
 Lab File: BG046516.D
 Acq: 3 Sep 2020 14:46

Instrument :
 BNA_G
 ClientSampleId :
 PB131395BL

Tot Ion:172 Resp: 1061122
 Ion Ratio Lower Upper
 172 100
 171 38.0 31.8 47.6
 170 24.9 20.3 30.5




Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


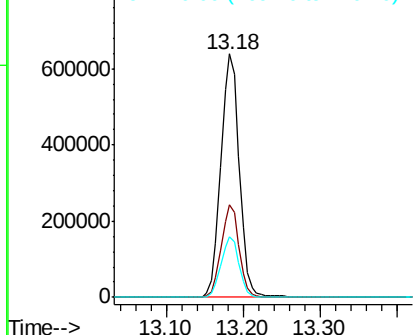



#51
 2,6-Dinitrotoluene
 Concen: 7.761 ng
 RT: 14.56 min Scan# 1952
 Delta R.T. 0.42 min
 Lab File: BG046516.D
 Acq: 3 Sep 2020 14:46

Tgt Ion:165 Resp: 27445
 Ion Ratio Lower Upper
 165 100
 63 1.6 34.2 51.4#
 89 0.0 37.0 55.4#



Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BG0
 Ion 89.00 (88.70 to 89.70): BG0

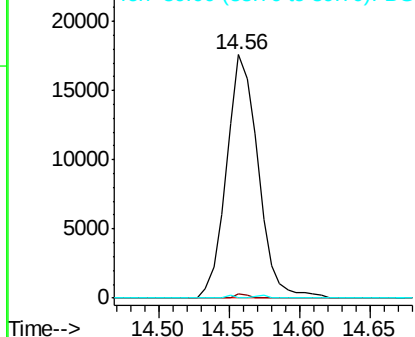


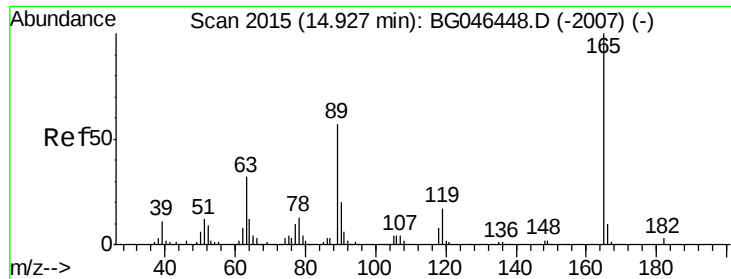




#57
 2,4-Dinitrotoluene
 Concen: 5.443 ng
 RT: 14.56 min Scan# 1952
 Delta R.T. -0.37 min
 Lab File: BG046516.D
 Acq: 3 Sep 2020 14:46

Instrument :
 BNA_G
 ClientSampleId :
 PB131395BL

Tot Ion:165 Resp: 27445
 Ion Ratio Lower Upper
 165 100
 63 1.6 25.4 38.0#
 89 0.0 45.9 68.9#
 182 0.0 2.3 3.5#




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC
 Ion 182.00 (181.70 to 182.70): E

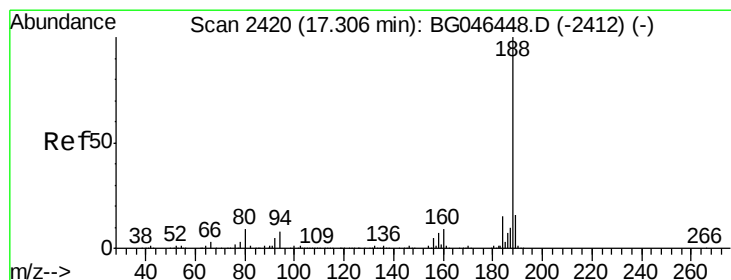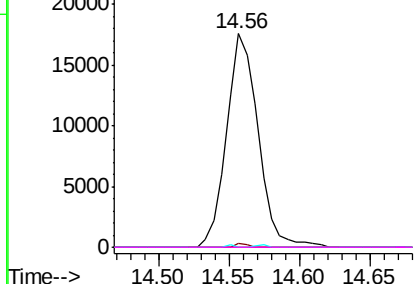




#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.30 min Scan# 2419
 Delta R.T. -0.01 min
 Lab File: BG046516.D
 Acq: 3 Sep 2020 14:46

Tgt Ion:188 Resp: 490739
 Ion Ratio Lower Upper
 188 100
 94 7.7 6.3 9.5
 80 8.5 6.9 10.3

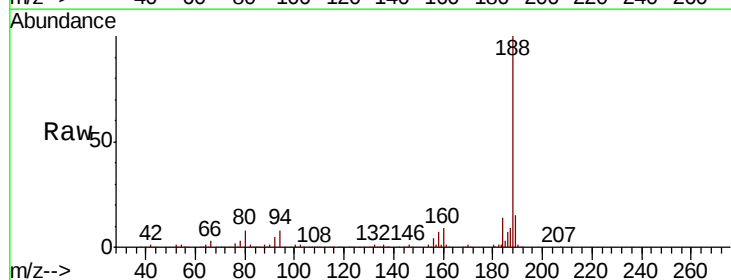

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

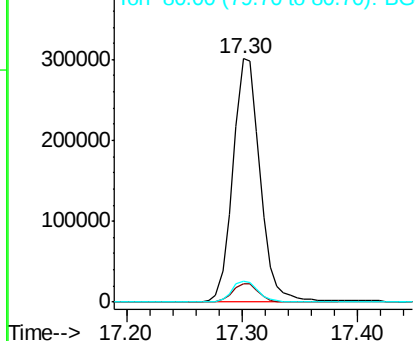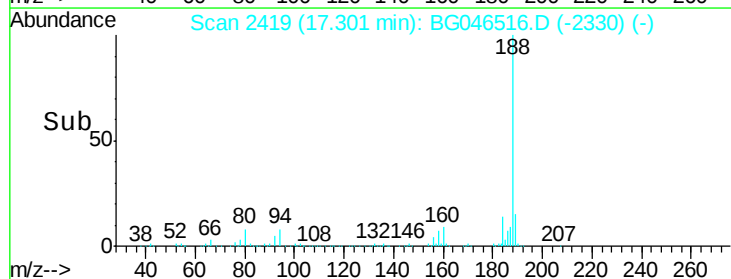


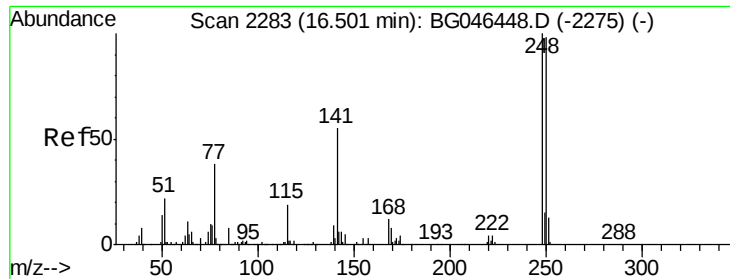




#67
4-Bromophenyl-phenylether
Concen: 3.606 ng
RT: 16.05 min Scan# 2206
Delta R.T. -0.45 min
Lab File: BG046516.D
Acq: 3 Sep 2020 14:46

Instrument :
BNA_G
ClientSampleId :
PB131395BL

Tot Ion:248 Resp: 20644
Ion Ratio Lower Upper
248 100
250 191.8 78.6 118.0#
141 405.1 43.9 65.9#

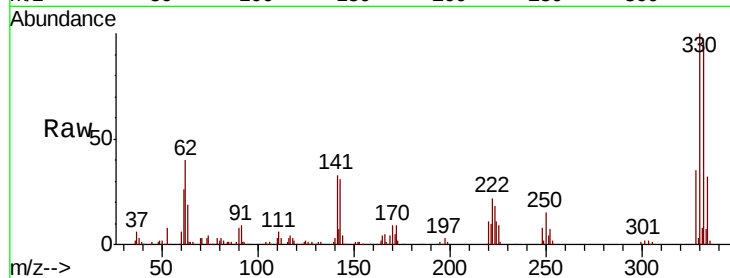


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

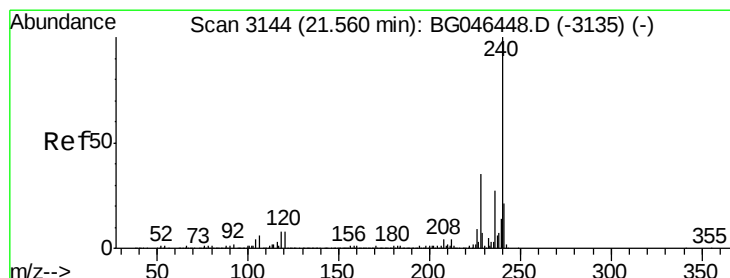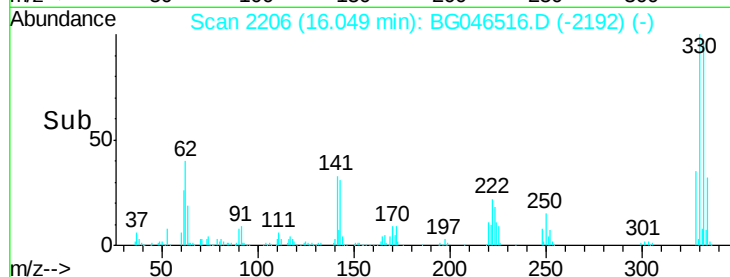
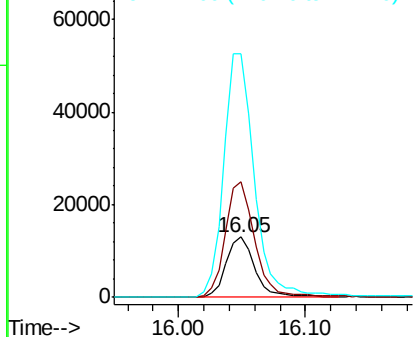



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.55 min Scan# 3142
Delta R.T. -0.01 min
Lab File: BG046516.D
Acq: 3 Sep 2020 14:46

Tgt Ion:240 Resp: 522723
Ion Ratio Lower Upper
240 100
120 8.3 6.6 10.0
236 26.0 21.4 32.2

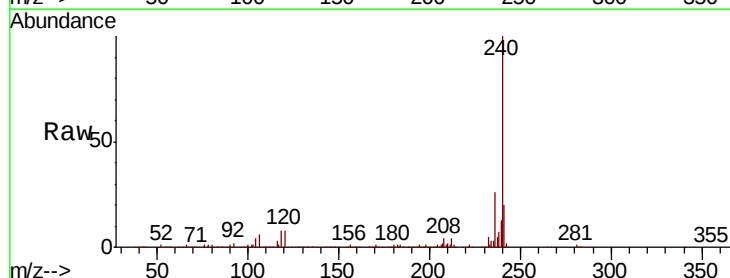

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

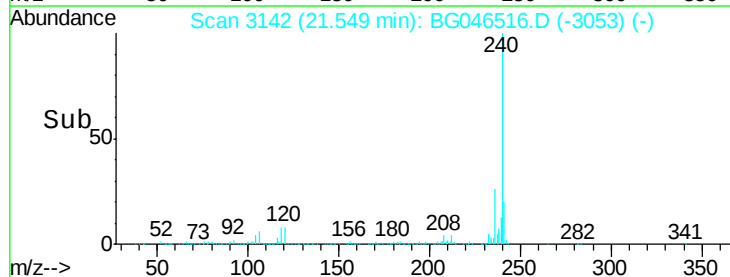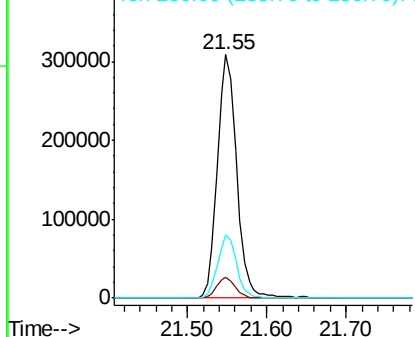



#77

Benzidine

Concen: 2.039 ng

RT: 19.92 min Scan# 2865

Delta R.T. 0.39 min

Lab File: BG046516.D

Acq: 3 Sep 2020 14:46

Instrument :

BNA_G

ClientSampleId :

PB131395BL


Tot Ion:184 Resp: 24767

Ion Ratio Lower Upper

184 100

185 18.1 11.8 17.8#




183 15.8 10.7 16.1

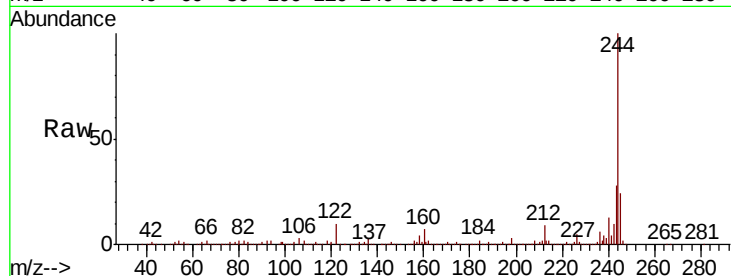

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

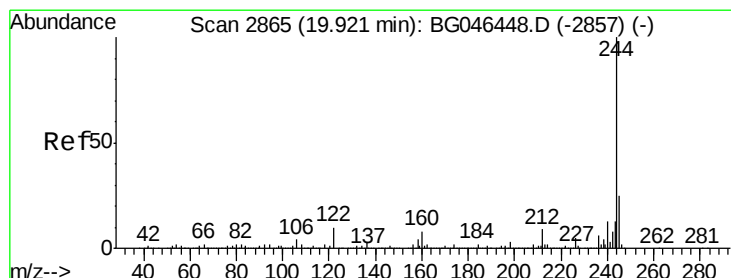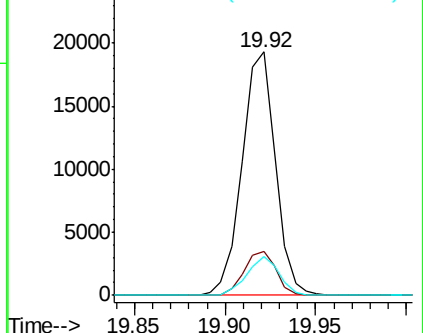

#79

Terphenyl-d14

Concen: 68.024 ng

RT: 19.92 min Scan# 2865

Delta R.T. 0.00 min

Lab File: BG046516.D

Acq: 3 Sep 2020 14:46


Tgt Ion:244 Resp: 1670815

Ion Ratio Lower Upper

244 100

212 8.7 6.9 10.3



122 9.6 8.2 12.4




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

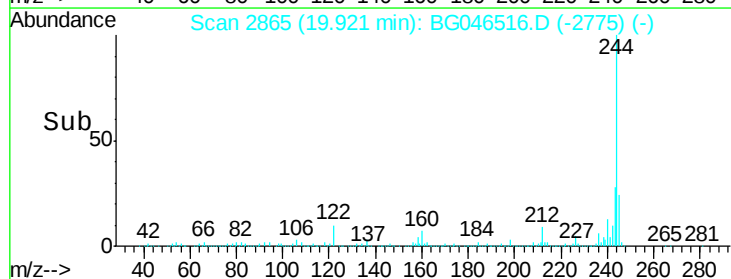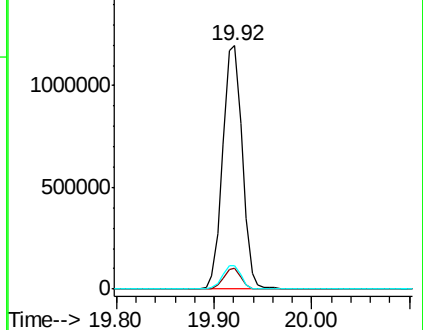

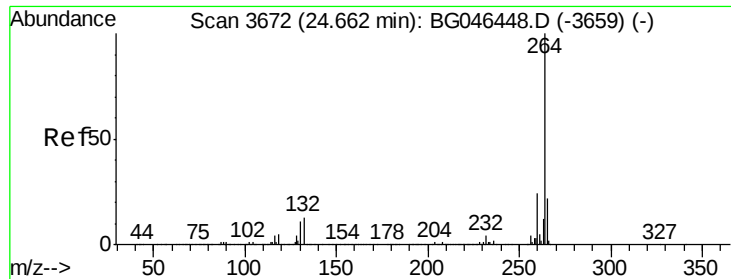

#86
Pervlene-d12
Concen: 20.000 ng
RT: 24.65 min Scan# 3670
Delta R.T. -0.01 min
Lab File: BG046516.D
Acq: 3 Sep 2020 14:46

Instrument :
BNA_G
ClientSampleId :
PB131395BL

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.2	28.8
265	21.3	17.9	26.9

