
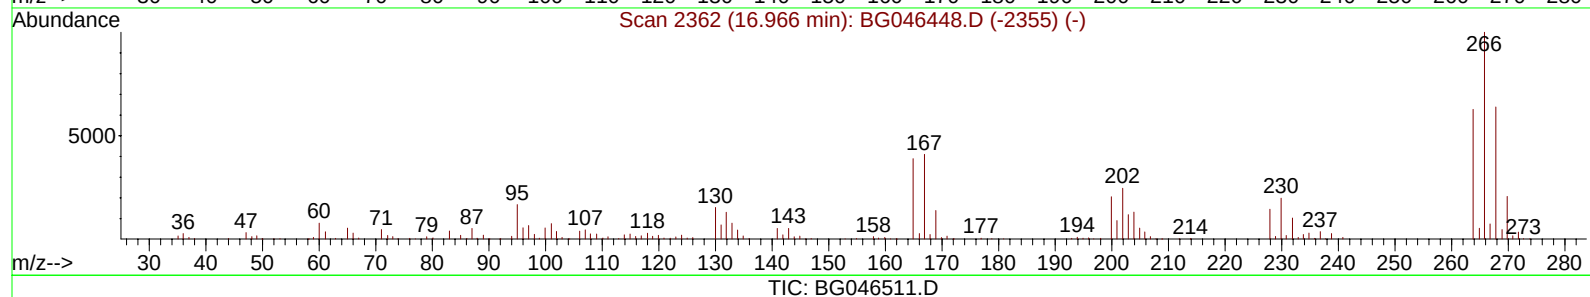
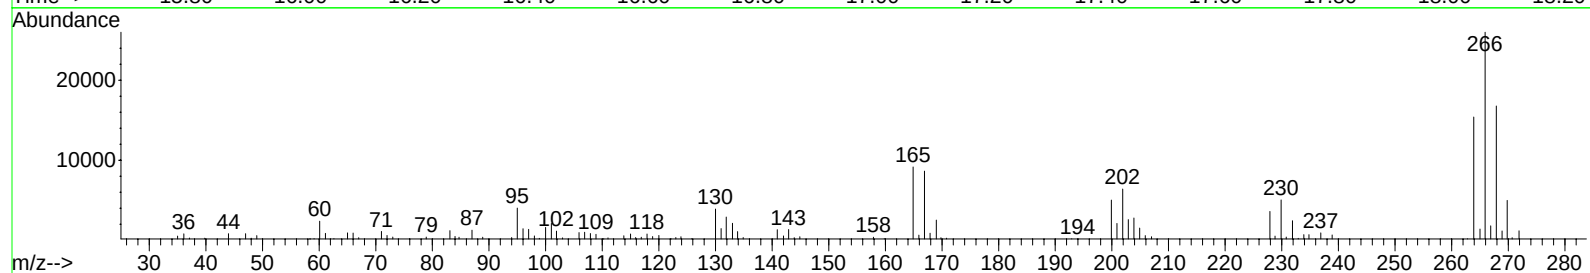


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090320\
Data File : BG046511.D
Acq On : 3 Sep 2020 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 18:54:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 15:06:53 2020
Response via : Initial Calibration

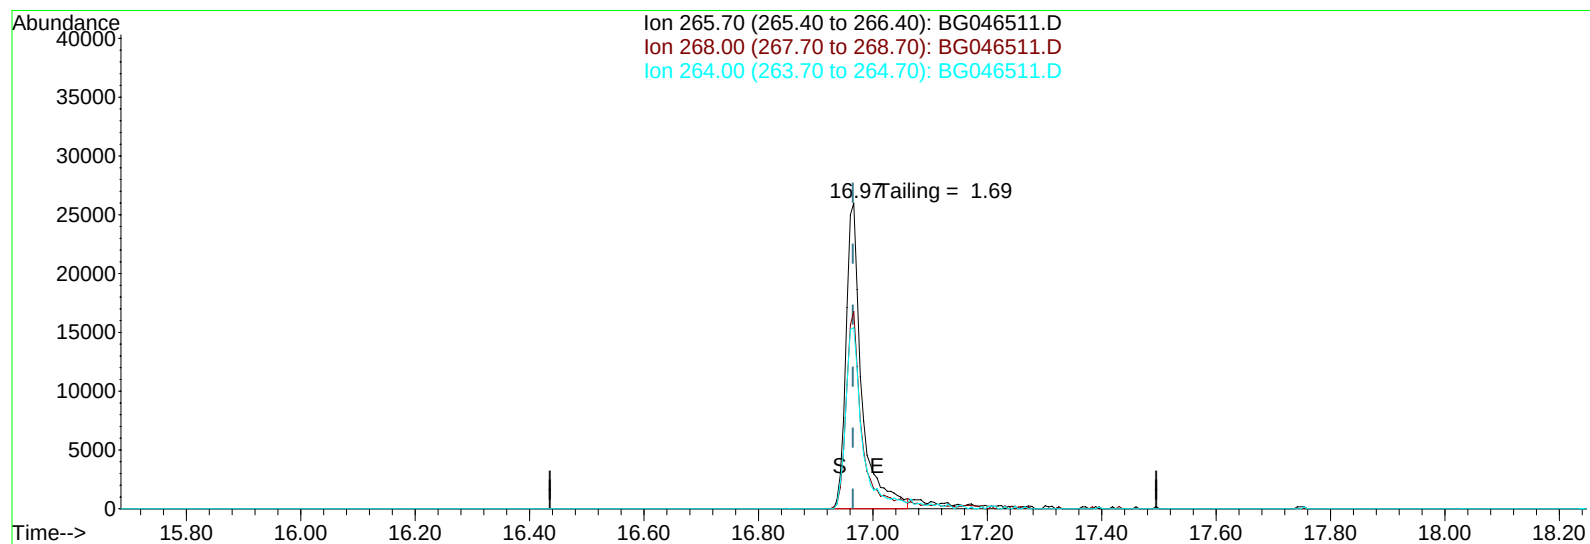

(70) Pentachlorophenol (C)




16.966min (+0.001) 23954.41ng

response 51586

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.52
264.00	62.70	59.25
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090320\
Data File : BG046511.D
Acq On : 3 Sep 2020 9:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 18:54:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 15:06:53 2020
Response via : Initial Calibration

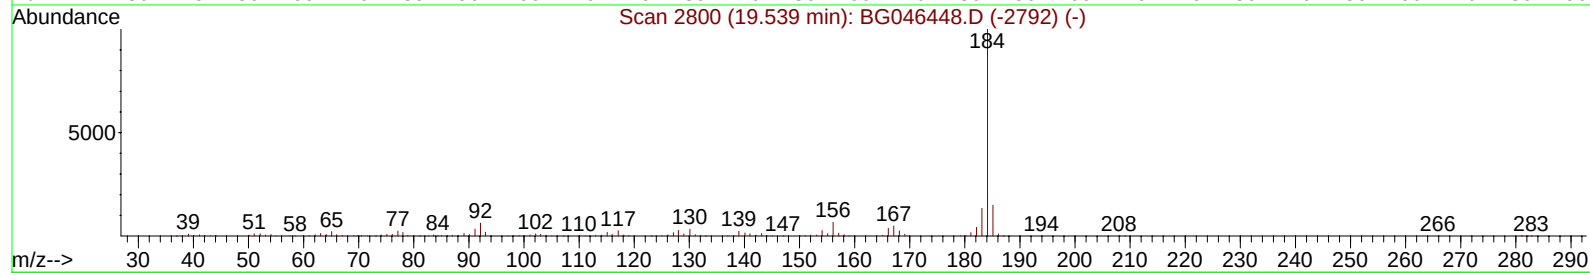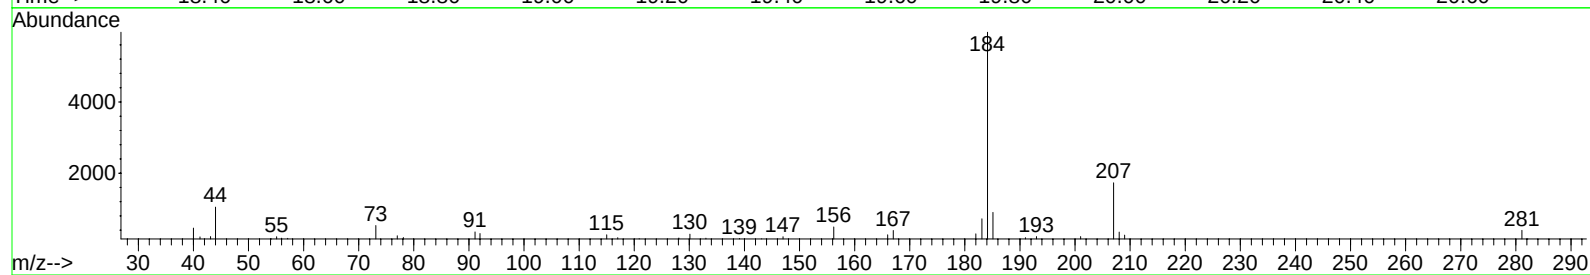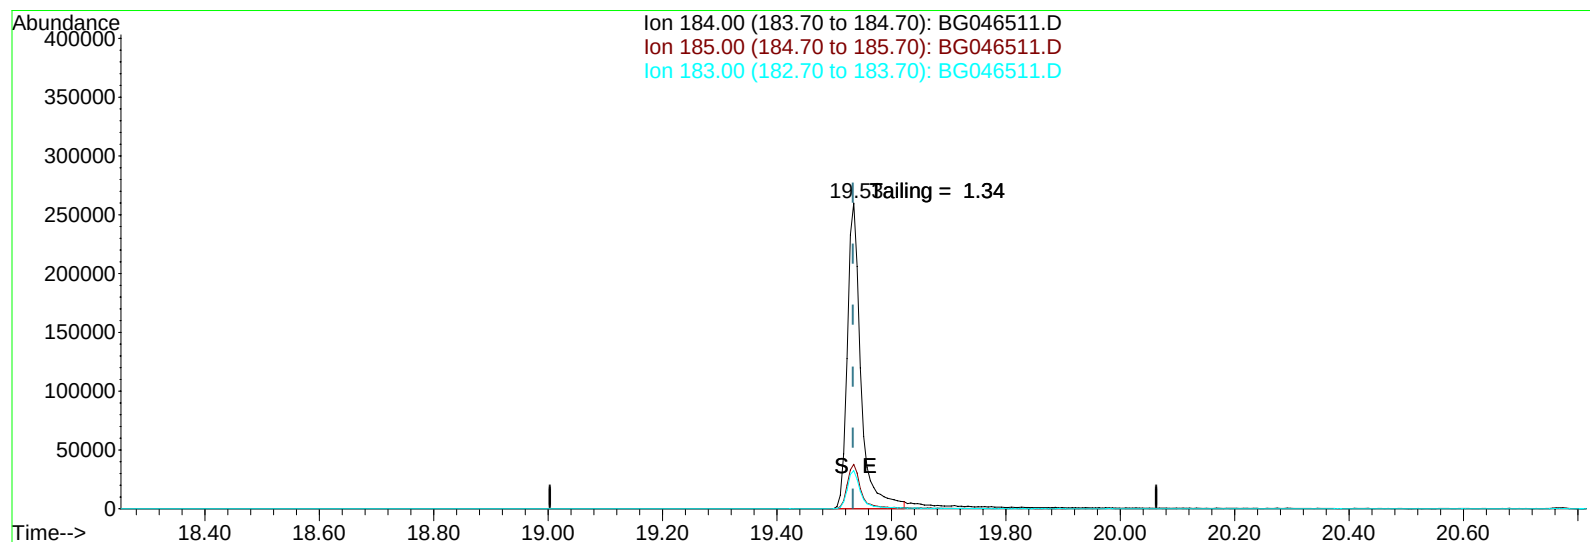

TIC: BG046511.D

(77) Benzidine

19.622min (+0.089) 0.00ng m

response 3299

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	15.07
183.00	13.40	12.07
0.00	0.00	0.00