
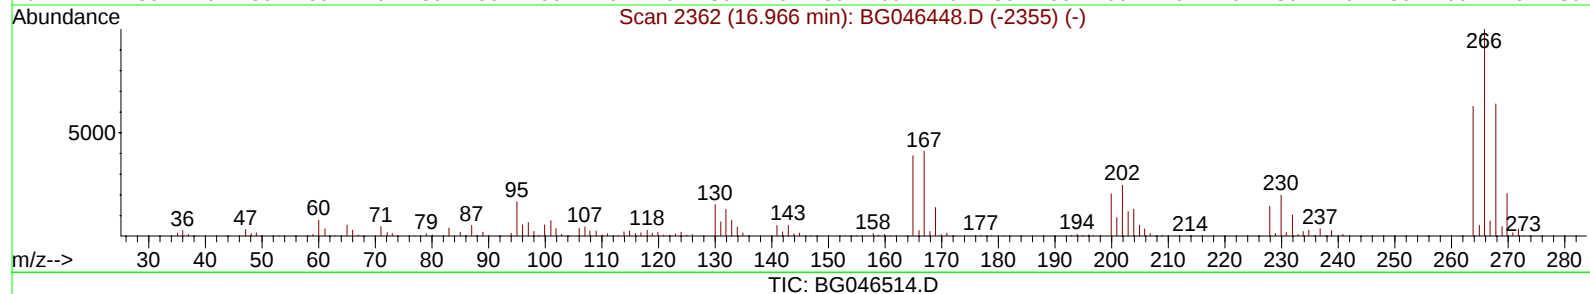
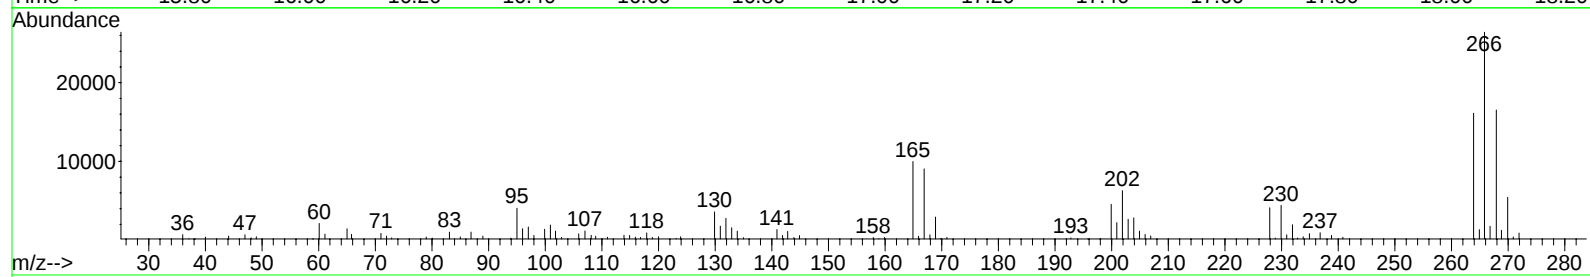


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090320\
Data File : BG046514.D
Acq On : 3 Sep 2020 13:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 18:57:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 15:06:53 2020
Response via : Initial Calibration

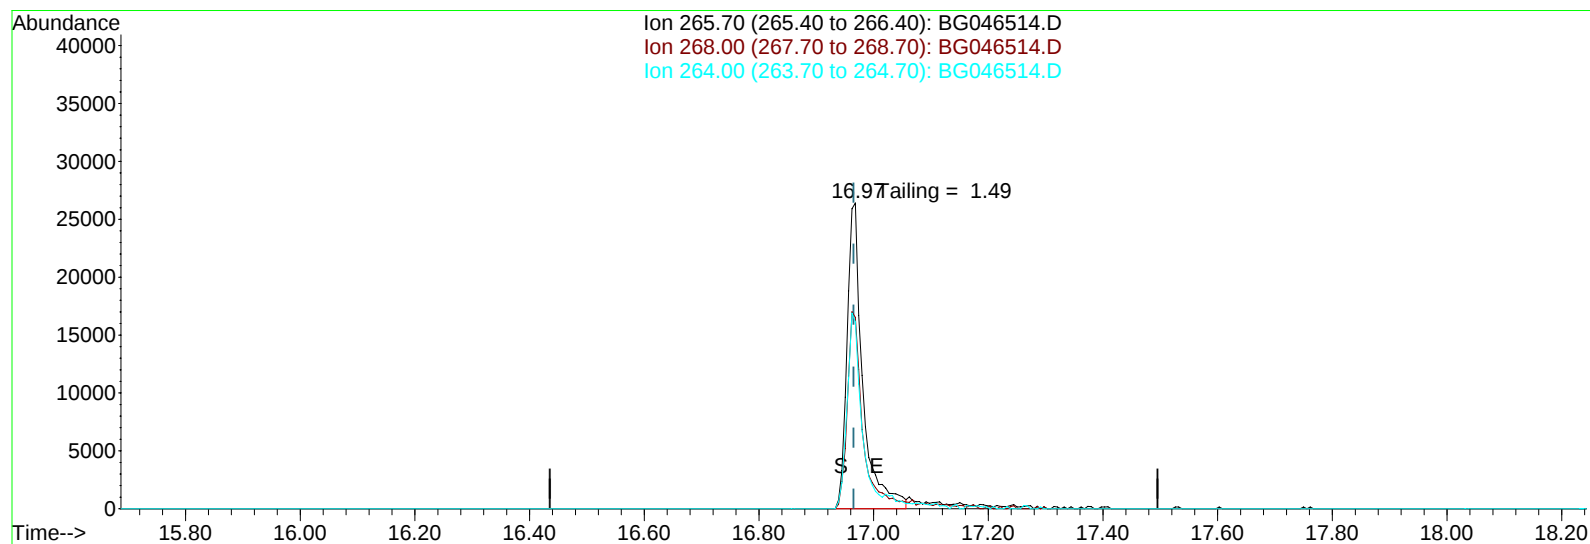

(70) Pentachlorophenol (C)




16.968min (+0.003) 31934.10ng

response 51955

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.59
264.00	62.70	61.10
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG090320\
 Data File : BG046514.D
 Acq On : 3 Sep 2020 13:26
 Operator : CG/JU
 Sample : DF TPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 03 18:57:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG082520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 15:06:53 2020
 Response via : Initial Calibration

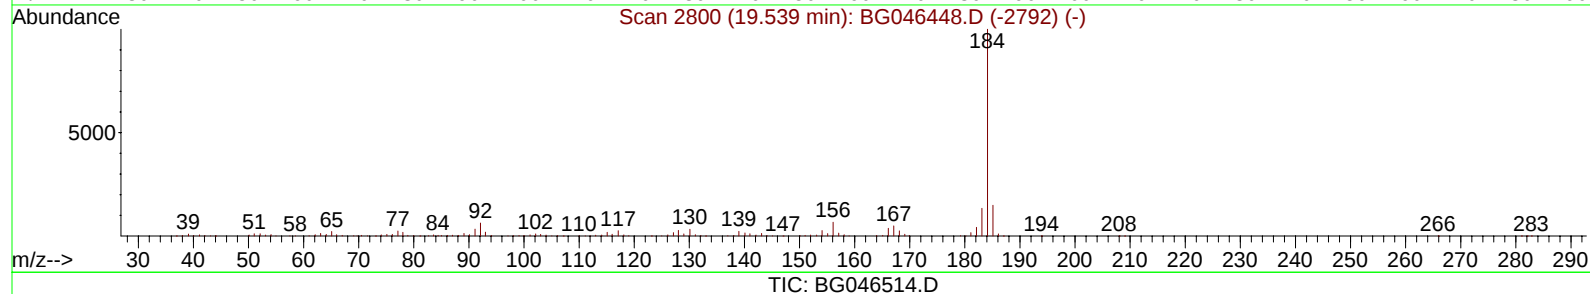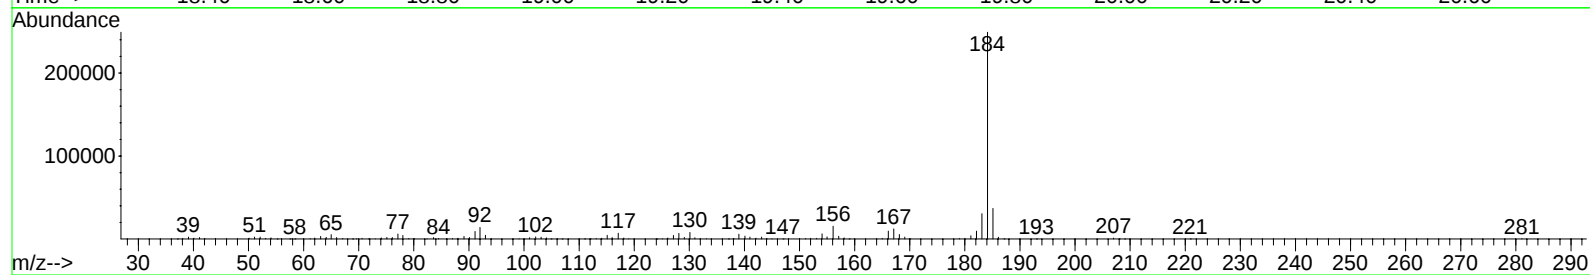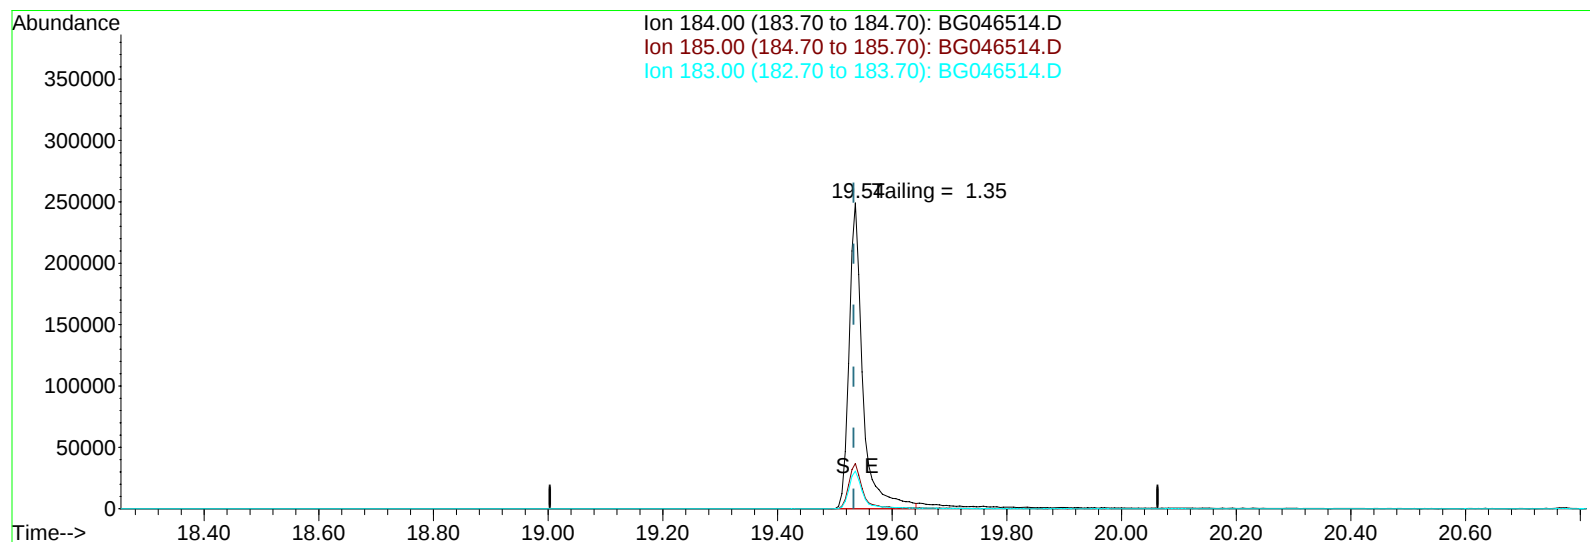

(77) Benzidine

19.536min (+0.003) 0.00ng

response 429671

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.82
183.00	13.40	12.29
0.00	0.00	0.00