

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047492.D
 Acq On : 1 Dec 2020 10:12
 Operator : CG/JU
 Sample : L4793-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.044	118	120	124	rVB3	4926	3435	0.53%	0.062%
2	4.150	135	138	143	rVB	12471	16136	2.51%	0.290%
3	4.314	165	166	169	rVB2	2948	1986	0.31%	0.036%
4	4.414	181	183	186	rVB3	2055	2231	0.35%	0.040%
5	4.808	249	250	252	rBV	3204	1920	0.30%	0.035%
6	5.078	293	296	297	rBV	2268	2060	0.32%	0.037%
7	5.108	299	301	303	rBV2	1833	1912	0.30%	0.034%
8	5.125	303	304	309	rBV2	2252	2885	0.45%	0.052%
9	5.325	333	338	344	rBV4	4049	7295	1.13%	0.131%
10	5.948	441	444	446	rBV4	2117	1719	0.27%	0.031%
11	6.001	451	453	456	rBV	1838	1851	0.29%	0.033%
12	6.089	466	468	469	rVB	3533	2349	0.37%	0.042%
13	6.101	469	470	472	rBV	2641	1924	0.30%	0.035%
14	6.195	484	486	490	rVB	1403	1683	0.26%	0.030%
15	6.700	571	572	576	rBV	1727	1817	0.28%	0.033%
16	6.788	585	587	590	rBV	1665	1826	0.28%	0.033%
17	6.888	602	604	606	rBV	1977	1667	0.26%	0.030%
18	6.941	608	613	614	rBV	1463	1760	0.27%	0.032%
19	7.399	684	691	701	rBV3	85930	190612	29.62%	3.432%
20	7.581	716	722	727	rVB2	52564	87664	13.62%	1.578%
21	7.793	748	758	764	rBV2	83958	150755	23.43%	2.714%
22	8.098	808	810	812	rVB2	1918	1685	0.26%	0.030%
23	8.134	812	816	818	rBV2	2215	2667	0.41%	0.048%
24	8.269	833	839	845	rVB	126146	214529	33.33%	3.862%
25	8.586	891	893	896	rBV	1473	1737	0.27%	0.031%
26	8.680	907	909	913	rVB	1882	1826	0.28%	0.033%
27	8.721	913	916	920	rBV	1544	2461	0.38%	0.044%
28	8.844	933	937	939	rVB	2611	2706	0.42%	0.049%
29	8.956	950	956	966	rBV3	80906	144820	22.50%	2.607%
30	9.097	977	980	987	rVB2	4592	7131	1.11%	0.128%
31	9.432	1029	1037	1045	rBV	81946	151614	23.56%	2.730%
32	9.843	1105	1107	1113	rVB	7356	8425	1.31%	0.152%
33	10.161	1155	1161	1169	rVB3	77459	145124	22.55%	2.613%
34	10.266	1177	1179	1182	rBV3	1097	1675	0.26%	0.030%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047492.D
 Acq On : 1 Dec 2020 10:12
 Operator : CG/JU
 Sample : L4793-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

35	10.701	1246	1253	1264	rBV2	108893	206196	32.04%	3.712%
36	10.795	1267	1269	1270	rBV2	2476	1580	0.25%	0.028%
37	11.001	1300	1304	1306	rBV2	1997	1927	0.30%	0.035%
38	11.095	1312	1320	1329	rBV	158560	289387	44.97%	5.210%
39	11.218	1334	1341	1348	rVV3	44039	84083	13.07%	1.514%
40	12.170	1499	1503	1504	rBV3	1460	1837	0.29%	0.033%
41	12.570	1568	1571	1574	rBV3	1862	2013	0.31%	0.036%
42	12.658	1583	1586	1590	rBV2	2187	2828	0.44%	0.051%
43	13.192	1671	1677	1679	rBV	1266	2218	0.34%	0.040%
44	13.280	1690	1692	1697	rBV	1834	2432	0.38%	0.044%
45	13.322	1697	1699	1702	rVB	2362	1742	0.27%	0.031%
46	13.392	1710	1711	1716	rBV	1072	1592	0.25%	0.029%
47	13.474	1722	1725	1727	rBV	1493	1627	0.25%	0.029%
48	13.651	1750	1755	1757	rBV	1866	2517	0.39%	0.045%
49	13.762	1771	1774	1777	rVB2	4408	4601	0.71%	0.083%
50	14.103	1830	1832	1834	rBV2	1944	1799	0.28%	0.032%
51	14.268	1854	1860	1865	rBV	201203	307622	47.80%	5.538%
52	14.315	1865	1868	1877	rVB	50231	74767	11.62%	1.346%
53	14.397	1877	1882	1885	rBV	1787	3156	0.49%	0.057%
54	14.573	1906	1912	1923	rVB	202286	333874	51.88%	6.011%
55	14.761	1941	1944	1948	rBV	2775	3409	0.53%	0.061%
56	14.879	1957	1964	1971	rBV	260074	410450	63.78%	7.389%
57	14.931	1971	1973	1977	rBV	1239	1916	0.30%	0.034%
58	15.037	1982	1991	1998	rBV2	73423	126927	19.72%	2.285%
59	15.190	2014	2017	2022	rVB3	7774	12748	1.98%	0.230%
60	15.231	2022	2024	2026	rBV3	1931	1691	0.26%	0.030%
61	15.266	2028	2030	2034	rVB2	6374	7237	1.12%	0.130%
62	15.513	2070	2072	2074	rVB	3559	1873	0.29%	0.034%
63	15.701	2102	2104	2106	rVB	2990	1614	0.25%	0.029%
64	15.742	2108	2111	2114	rBV	2366	4093	0.64%	0.074%
65	15.866	2125	2132	2138	rBV	276868	425355	66.09%	7.658%
66	15.966	2144	2149	2157	rBV2	72570	122893	19.10%	2.212%
67	16.483	2234	2237	2238	rBV2	2814	2004	0.31%	0.036%
68	16.582	2253	2254	2255	rBV	4234	2196	0.34%	0.040%
69	16.635	2262	2263	2266	rBV2	3354	3240	0.50%	0.058%
70	16.735	2277	2280	2281	rBV	3045	3111	0.48%	0.056%
71	16.911	2308	2310	2315	rVB	2812	2876	0.45%	0.052%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047492.D
 Acq On : 1 Dec 2020 10:12
 Operator : CG/JU
 Sample : L4793-15
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B42

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

72	16.959	2315	2318	2321	rBV	3125	4724	0.73%	0.085%
73	17.141	2346	2349	2351	rBV	4716	5479	0.85%	0.099%
74	17.170	2353	2354	2356	rBV	3873	2227	0.35%	0.040%
75	17.270	2366	2371	2372	rBV	2911	3363	0.52%	0.061%
76	17.352	2381	2385	2387	rVB3	6652	6825	1.06%	0.123%
77	17.617	2424	2430	2435	rBV	329423	517331	80.39%	9.314%
78	17.711	2441	2446	2455	rVB	288212	462924	71.93%	8.334%
79	17.875	2473	2474	2477	rVB3	4807	3811	0.59%	0.069%
80	17.940	2483	2485	2486	rVB2	3781	1796	0.28%	0.032%
81	18.163	2521	2523	2525	rBV3	3784	2005	0.31%	0.036%
82	18.192	2526	2528	2531	rVB	4549	3806	0.59%	0.069%
83	18.257	2537	2539	2543	rVB4	4434	4808	0.75%	0.087%
84	18.533	2582	2586	2593	rVB5	14610	21819	3.39%	0.393%
85	18.610	2596	2599	2604	rBV5	8532	14468	2.25%	0.260%
86	18.674	2605	2610	2614	rBV5	18132	33629	5.23%	0.605%
87	19.644	2771	2775	2780	rVB	131452	188711	29.32%	3.397%
88	19.978	2827	2832	2836	rBV	393184	643561	100.00%	11.586%


Sum of corrected areas: 5554605

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
Data File : BG047492.D
Acq On : 1 Dec 2020 10:12
Operator : CG/JU
Sample : L4793-15
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B42

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

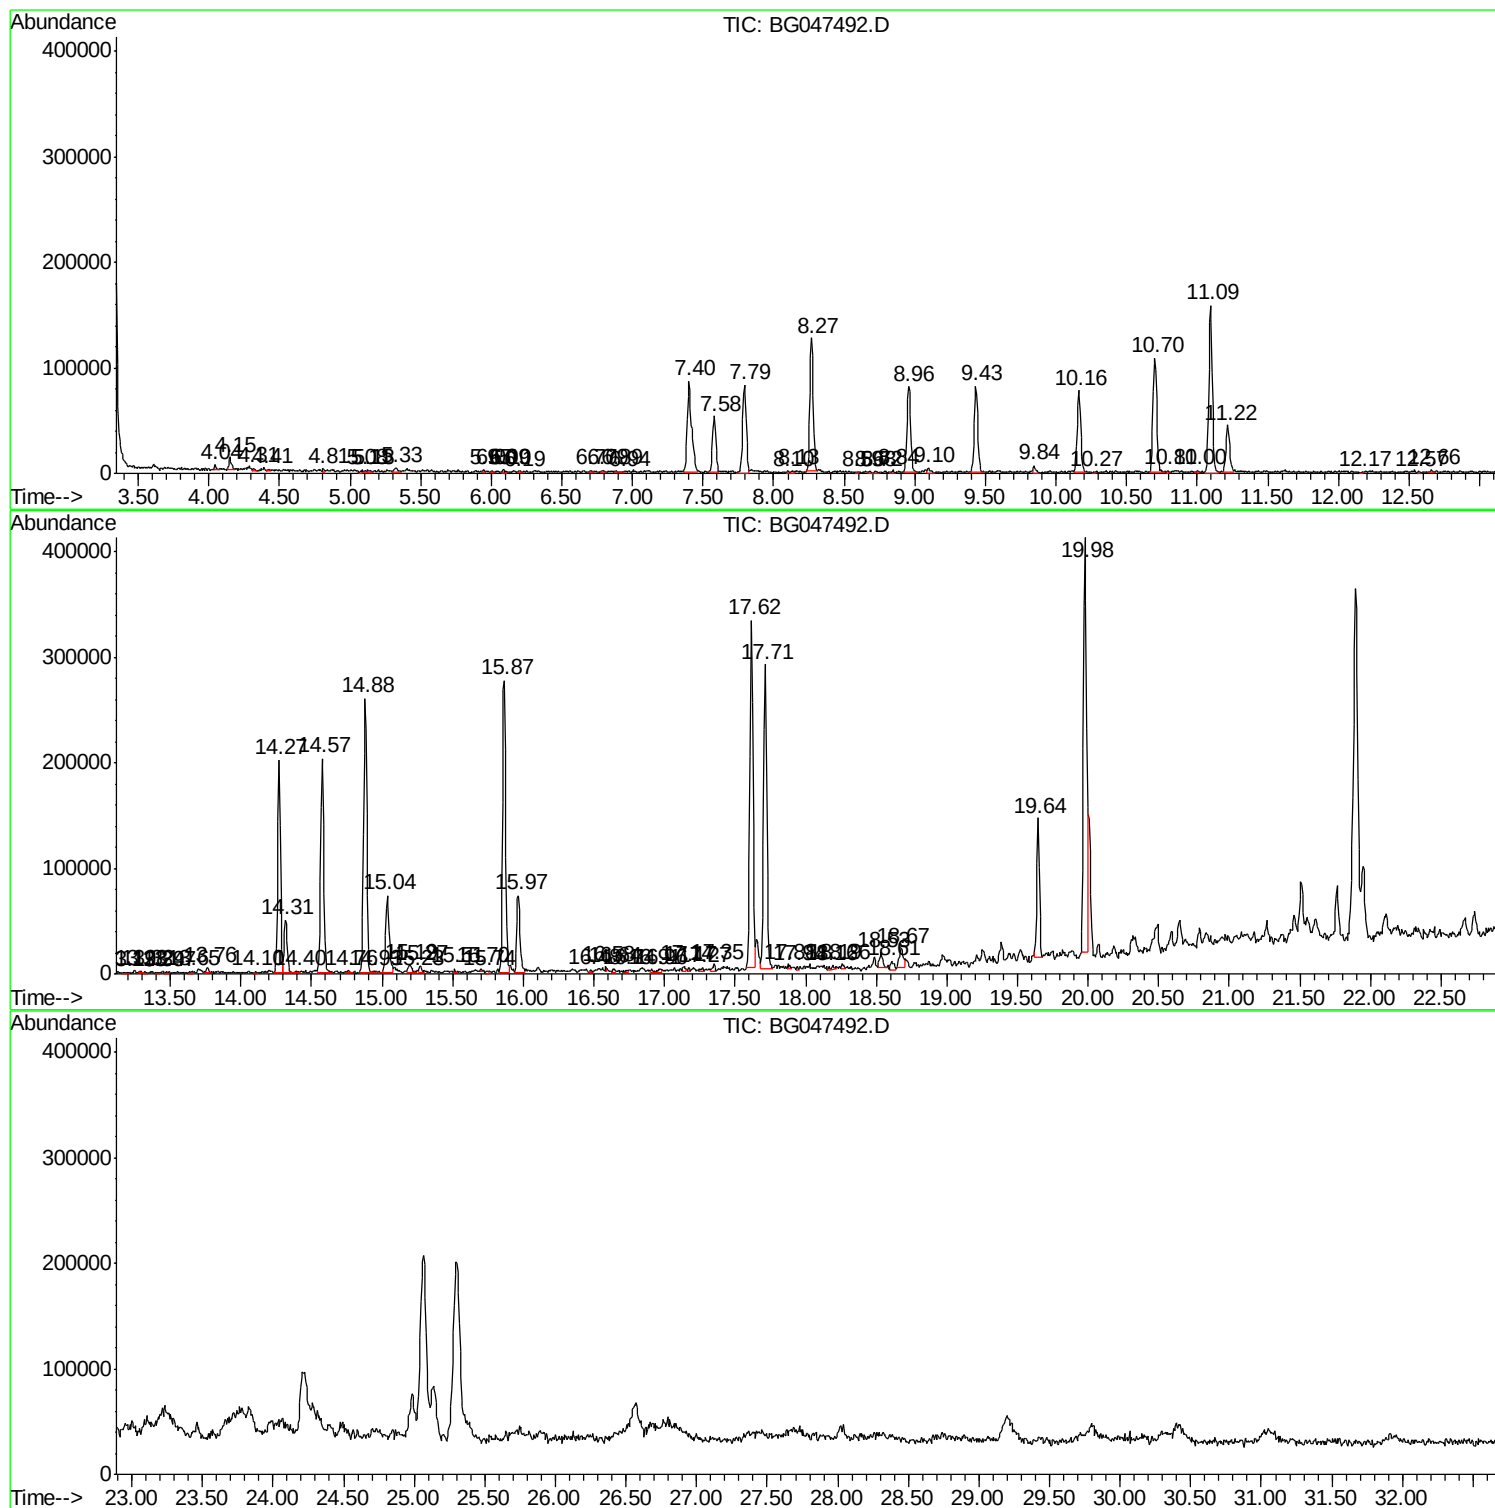

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120120\
Data File : BG047492.D
Acq On : 1 Dec 2020 10:12
Operator : CG/JU
Sample : L4793-15
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B42

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120120\
Data File : BG047492.D
Acq On : 1 Dec 2020 10:12
Operator : CG/JU
Sample : L4793-15
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B42

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc