

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047495.D
 Acq On : 1 Dec 2020 12:12
 Operator : CG/JU
 Sample : L4793-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0BG7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.724	234	236	239	rVB	2960	2442	0.43%	0.045%
2	4.965	275	277	280	rBV	2058	2085	0.36%	0.038%
3	5.188	313	315	317	rBV	2372	1689	0.29%	0.031%
4	5.211	317	319	323	rBV2	1412	1467	0.26%	0.027%
5	5.311	334	336	337	rBV	2836	2831	0.49%	0.052%
6	5.429	354	356	359	rVB	1995	1869	0.33%	0.034%
7	5.540	373	375	378	rVB	2306	2228	0.39%	0.041%
8	5.588	381	383	385	rVB	2778	1948	0.34%	0.036%
9	5.617	387	388	391	rBV	1572	1537	0.27%	0.028%
10	5.864	425	430	435	rBV2	2176	4926	0.86%	0.090%
11	5.940	441	443	445	rBV	2030	1999	0.35%	0.037%
12	6.058	462	463	466	rBV	1907	2321	0.40%	0.042%
13	6.181	481	484	487	rVB	3039	2563	0.45%	0.047%
14	6.304	502	505	508	rBV2	1615	2311	0.40%	0.042%
15	6.504	537	539	542	rBV	1809	1466	0.26%	0.027%
16	7.021	625	627	632	rVB	1803	1770	0.31%	0.032%
17	7.074	632	636	638	rBV	1807	1481	0.26%	0.027%
18	7.397	686	691	701	rVB3	73648	146342	25.47%	2.677%
19	7.573	716	721	728	rVB	46418	78269	13.62%	1.432%
20	7.720	744	746	749	rVB	3021	1944	0.34%	0.036%
21	7.750	749	751	752	rBV	2965	2149	0.37%	0.039%
22	7.791	752	758	765	rVV2	71563	125532	21.85%	2.296%
23	7.961	786	787	789	rBV2	1714	1510	0.26%	0.028%
24	8.202	824	828	831	rBV2	1299	1647	0.29%	0.030%
25	8.267	831	839	846	rBV	120079	207510	36.12%	3.796%
26	8.349	851	853	855	rBV	2455	2255	0.39%	0.041%
27	8.766	919	924	927	rVB	1086	1946	0.34%	0.036%
28	8.954	948	956	964	rBV2	77230	137448	23.93%	2.514%
29	9.230	999	1003	1004	rBV2	1526	1881	0.33%	0.034%
30	9.430	1031	1037	1046	rVB	77320	139514	24.29%	2.552%
31	9.583	1061	1063	1067	rBV	1728	2055	0.36%	0.038%
32	9.841	1102	1107	1113	rBV3	3864	8233	1.43%	0.151%
33	9.882	1113	1114	1117	rBV3	1817	1706	0.30%	0.031%
34	9.976	1128	1130	1134	rBV3	1500	2207	0.38%	0.040%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047495.D
 Acq On : 1 Dec 2020 12:12
 Operator : CG/JU
 Sample : L4793-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0BG7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

35	10.047	1139	1142	1143	rBV3	1428	1431	0.25%	0.026%
36	10.100	1147	1151	1153	rBV3	1577	2086	0.36%	0.038%
37	10.159	1155	1161	1170	rVB2	66931	122942	21.40%	2.249%
38	10.699	1247	1253	1260	rBV	95963	174878	30.44%	3.199%
39	11.093	1313	1320	1329	rBV	146831	268126	46.67%	4.904%
40	11.216	1333	1341	1349	rBV	73505	139844	24.34%	2.558%
41	12.009	1473	1476	1479	rVB	1385	1614	0.28%	0.030%
42	12.051	1479	1483	1485	rBV	1248	2000	0.35%	0.037%
43	12.074	1485	1487	1489	rBV	1550	1541	0.27%	0.028%
44	12.333	1528	1531	1534	rBV	1916	2054	0.36%	0.038%
45	12.773	1605	1606	1609	rVB	2674	1657	0.29%	0.030%
46	12.832	1614	1616	1619	rBV	1768	1927	0.34%	0.035%
47	13.073	1656	1657	1661	rBV	1412	1629	0.28%	0.030%
48	13.243	1683	1686	1689	rVB	2907	2818	0.49%	0.052%
49	13.760	1769	1774	1776	rBV2	5040	5548	0.97%	0.101%
50	13.854	1786	1790	1794	rBV2	1010	1674	0.29%	0.031%
51	13.937	1800	1804	1805	rVB2	1930	2075	0.36%	0.038%
52	13.954	1805	1807	1808	rBV2	1655	1432	0.25%	0.026%
53	14.271	1853	1861	1865	rBV	193052	277575	48.32%	5.077%
54	14.313	1865	1868	1874	rVB2	74674	112343	19.56%	2.055%
55	14.407	1881	1884	1885	rBV	1747	1441	0.25%	0.026%
56	14.518	1900	1903	1904	rBV	1651	1451	0.25%	0.027%
57	14.577	1907	1913	1920	rVB	188076	300005	52.22%	5.487%
58	14.689	1930	1932	1934	rBV	1827	1454	0.25%	0.027%
59	14.877	1957	1964	1971	rBV2	240152	399006	69.45%	7.298%
60	14.994	1981	1984	1986	rVB2	1860	1717	0.30%	0.031%
61	15.035	1986	1991	1999	rBV2	67613	121875	21.21%	2.229%
62	15.588	2083	2085	2086	rBV2	2010	1751	0.30%	0.032%
63	15.864	2125	2132	2139	rBV2	245314	387765	67.50%	7.093%
64	15.964	2144	2149	2154	rBV2	58243	95874	16.69%	1.754%
65	16.099	2169	2172	2174	rBV	2904	2959	0.52%	0.054%
66	16.322	2208	2210	2211	rBV	2135	1461	0.25%	0.027%
67	16.434	2226	2229	2231	rBV	2238	2115	0.37%	0.039%
68	16.486	2235	2238	2240	rVB	2501	2269	0.39%	0.042%
69	16.563	2249	2251	2253	rBV	2307	1860	0.32%	0.034%
70	16.604	2256	2258	2260	rVB	1802	1449	0.25%	0.027%
71	16.622	2260	2261	2262	rBV	2895	1483	0.26%	0.027%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047495.D
 Acq On : 1 Dec 2020 12:12
 Operator : CG/JU
 Sample : L4793-22
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0BG7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

72	16.692	2270	2273	2275	rBV	1773	1992	0.35%	0.036%
73	16.739	2278	2281	2282	rVB	2271	2078	0.36%	0.038%
74	16.810	2292	2293	2295	rBV	1781	1476	0.26%	0.027%
75	16.839	2296	2298	2302	rVV3	3601	4769	0.83%	0.087%
76	17.062	2332	2336	2337	rBV	1632	2065	0.36%	0.038%
77	17.115	2342	2345	2346	rBV	1922	2146	0.37%	0.039%
78	17.139	2346	2349	2353	rBV2	6038	8124	1.41%	0.149%
79	17.615	2423	2430	2436	rBV	356673	523304	91.09%	9.572%
80	17.714	2441	2447	2456	rVB2	268979	424786	73.94%	7.770%
81	18.067	2505	2507	2508	rBV2	1970	1586	0.28%	0.029%
82	18.267	2539	2541	2543	rBV	2824	1846	0.32%	0.034%
83	18.367	2556	2558	2561	rVB	3184	2219	0.39%	0.041%
84	19.648	2773	2776	2782	rVB	32488	43960	7.65%	0.804%
85	19.977	2827	2832	2846	rVB	361847	574483	100.00%	10.508%
86	21.898	3153	3159	3165	rBV2	303694	522121	90.89%	9.550%


Sum of corrected areas: 5467165

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
Data File : BG047495.D
Acq On : 1 Dec 2020 12:12
Operator : CG/JU
Sample : L4793-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0BG7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

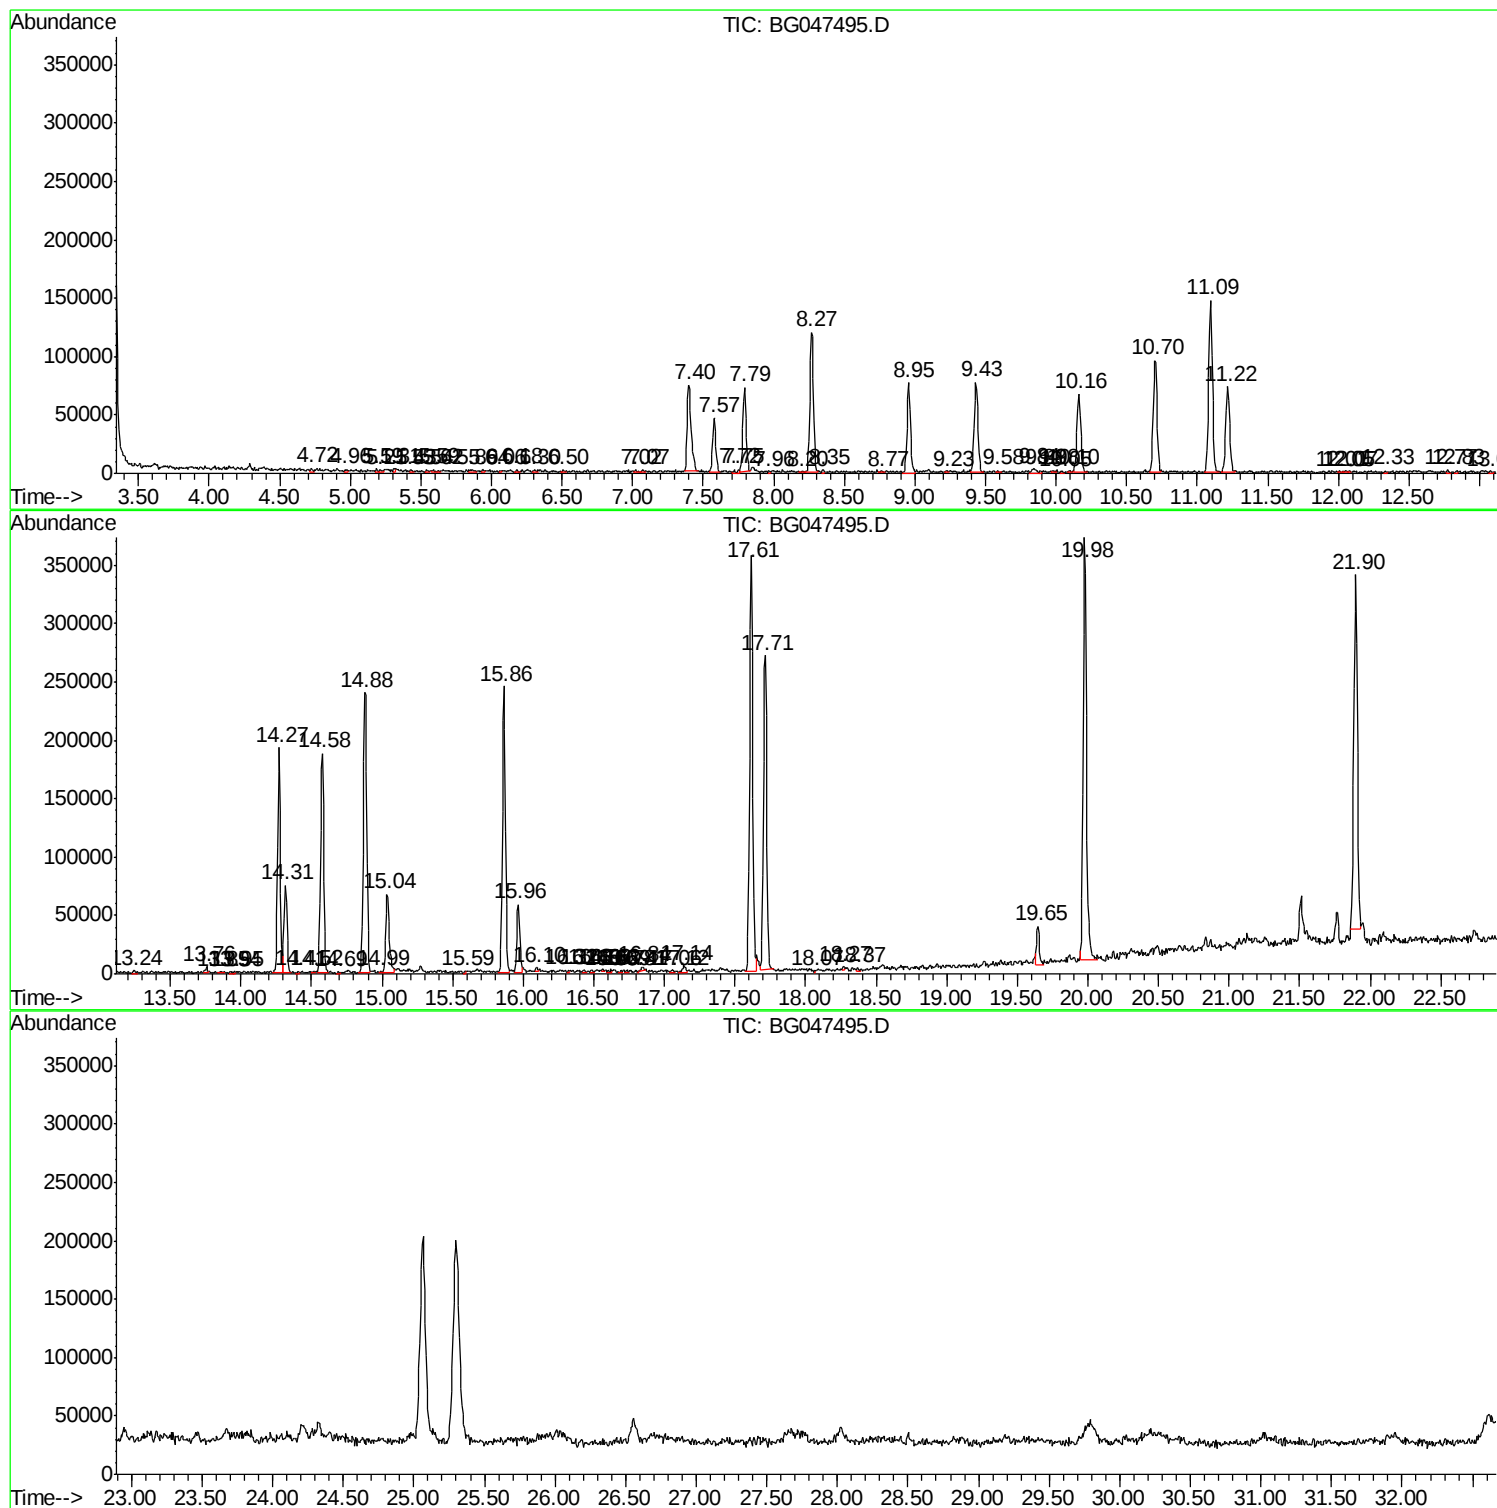

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120120\
Data File : BG047495.D
Acq On : 1 Dec 2020 12:12
Operator : CG/JU
Sample : L4793-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0BG7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120120\
Data File : BG047495.D
Acq On : 1 Dec 2020 12:12
Operator : CG/JU
Sample : L4793-22
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0BG7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc