

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047521.D
 Acq On : 2 Dec 2020 7:57
 Operator : CG/JU
 Sample : L4865-21
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B19

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.814	80	81	83	rBV2	2570	2121	0.36%	0.038%
2	4.237	150	153	154	rBV2	2213	1904	0.32%	0.034%
3	4.278	156	160	164	rVV4	6014	9359	1.57%	0.168%
4	4.602	213	215	218	rBV2	2351	1622	0.27%	0.029%
5	4.866	258	260	264	rBV2	1917	2721	0.46%	0.049%
6	4.960	274	276	279	rBV2	1977	2054	0.34%	0.037%
7	5.177	310	313	316	rBV	1968	1889	0.32%	0.034%
8	5.318	330	337	342	rBV5	10650	19576	3.29%	0.352%
9	5.618	386	388	392	rBV	2450	3306	0.56%	0.059%
10	5.888	432	434	438	rBV	1275	1621	0.27%	0.029%
11	6.012	452	455	458	rBV	1731	2134	0.36%	0.038%
12	6.112	469	472	476	rBV	1685	3077	0.52%	0.055%
13	6.623	556	559	560	rBV	3075	2336	0.39%	0.042%
14	6.817	591	592	595	rVB	3252	2238	0.38%	0.040%
15	6.846	595	597	599	rBV	1733	2059	0.35%	0.037%
16	7.287	668	672	675	rVB3	1935	2855	0.48%	0.051%
17	7.392	684	690	701	rVB3	66399	137051	23.02%	2.463%
18	7.575	716	721	728	rVB	43366	72852	12.24%	1.309%
19	7.786	751	757	766	rVB4	71277	126588	21.26%	2.275%
20	7.945	781	784	786	rVB4	1955	1709	0.29%	0.031%
21	8.268	832	839	846	rBV2	125880	220228	36.99%	3.957%
22	8.685	906	910	913	rBV2	2523	2593	0.44%	0.047%
23	8.955	949	956	965	rVB3	62524	110465	18.55%	1.985%
24	9.055	971	973	976	rBV3	1971	1659	0.28%	0.030%
25	9.085	976	978	983	rVV	3904	4661	0.78%	0.084%
26	9.190	993	996	999	rBV	1802	1797	0.30%	0.032%
27	9.220	999	1001	1004	rBV	1909	2105	0.35%	0.038%
28	9.343	1021	1022	1025	rBV	1360	1515	0.25%	0.027%
29	9.431	1029	1037	1045	rVB2	72540	140984	23.68%	2.533%
30	9.531	1052	1054	1056	rBV2	2240	1873	0.31%	0.034%
31	9.696	1079	1082	1086	rBV2	1508	1787	0.30%	0.032%
32	9.748	1088	1091	1094	rBV2	1135	1530	0.26%	0.027%
33	9.831	1099	1105	1106	rBV2	3534	4781	0.80%	0.086%
34	9.913	1116	1119	1120	rBV2	1465	1576	0.26%	0.028%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047521.D
 Acq On : 2 Dec 2020 7:57
 Operator : CG/JU
 Sample : L4865-21
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B19

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

35	9.954	1122	1126	1130	rVV2	1621	2639	0.44%	0.047%
36	9.989	1130	1132	1135	rVB2	1814	1662	0.28%	0.030%
37	10.072	1143	1146	1148	rBV2	1444	1684	0.28%	0.030%
38	10.160	1154	1161	1169	rVB3	68424	129400	21.73%	2.325%
39	10.630	1237	1241	1244	rBV3	913	1528	0.26%	0.027%
40	10.694	1246	1252	1260	rVB2	98776	178896	30.05%	3.214%
41	10.865	1279	1281	1283	rVB2	2013	1897	0.32%	0.034%
42	10.912	1286	1289	1292	rBV2	1371	1556	0.26%	0.028%
43	10.947	1292	1295	1297	rBV2	1562	1708	0.29%	0.031%
44	11.094	1313	1320	1327	rBV	163875	300706	50.50%	5.403%
45	11.211	1335	1340	1348	rVV3	62470	116252	19.52%	2.089%
46	11.288	1352	1353	1358	rVB3	1960	1558	0.26%	0.028%
47	11.811	1440	1442	1445	rVB3	1610	1519	0.26%	0.027%
48	11.964	1466	1468	1472	rVB3	2201	2067	0.35%	0.037%
49	12.005	1472	1475	1478	rBV3	2201	2315	0.39%	0.042%
50	12.052	1481	1483	1489	rBV	1348	2004	0.34%	0.036%
51	12.351	1531	1534	1536	rBV	1718	1683	0.28%	0.030%
52	12.498	1557	1559	1562	rVB	2045	1901	0.32%	0.034%
53	12.545	1565	1567	1570	rVV	2545	2329	0.39%	0.042%
54	12.651	1582	1585	1587	rBV	2748	3585	0.60%	0.064%
55	12.716	1594	1596	1600	rVB	1431	1714	0.29%	0.031%
56	13.274	1690	1691	1695	rBV	2274	1633	0.27%	0.029%
57	13.391	1708	1711	1715	rBV	1476	1881	0.32%	0.034%
58	13.450	1719	1721	1723	rBV	1830	1683	0.28%	0.030%
59	13.485	1723	1727	1730	rBV	1076	1841	0.31%	0.033%
60	13.685	1757	1761	1764	rVB	2276	2749	0.46%	0.049%
61	13.714	1764	1766	1768	rBV	1982	1605	0.27%	0.029%
62	13.756	1770	1773	1774	rBV	3145	2303	0.39%	0.041%
63	13.838	1784	1787	1789	rBV	1919	2006	0.34%	0.036%
64	14.267	1853	1860	1865	rBV	193503	289519	48.63%	5.202%
65	14.314	1865	1868	1874	rVB2	32750	48508	8.15%	0.872%
66	14.402	1881	1883	1885	rBV2	2512	1965	0.33%	0.035%
67	14.572	1906	1912	1919	rBV	190051	297986	50.05%	5.354%
68	14.878	1956	1964	1973	rVB	292447	462369	77.66%	8.308%
69	15.036	1985	1991	1999	rBV3	63554	111966	18.81%	2.012%
70	15.107	2001	2003	2005	rVB	2726	1983	0.33%	0.036%
71	15.266	2027	2030	2035	rVV2	6916	9665	1.62%	0.174%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047521.D
 Acq On : 2 Dec 2020 7:57
 Operator : CG/JU
 Sample : L4865-21
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B19

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

72	15.307	2035	2037	2040	rVB	2145	2225	0.37%	0.040%
73	15.577	2080	2083	2087	rVB	2192	2834	0.48%	0.051%
74	15.624	2087	2091	2094	rBV	2045	3810	0.64%	0.068%
75	15.859	2125	2131	2138	rBV	239958	386055	64.84%	6.937%
76	15.965	2143	2149	2158	rBV2	59050	97588	16.39%	1.753%
77	16.206	2189	2190	2194	rBV2	1973	1957	0.33%	0.035%
78	16.253	2196	2198	2200	rBV2	2620	1984	0.33%	0.036%
79	16.729	2277	2279	2280	rBV2	3083	2078	0.35%	0.037%
80	16.917	2309	2311	2314	rVB2	3190	2816	0.47%	0.051%
81	17.046	2332	2333	2338	rVB2	3800	4367	0.73%	0.078%
82	17.610	2423	2429	2435	rBV	379139	595404	100.00%	10.698%
83	17.710	2440	2446	2453	rVV2	277777	424687	71.33%	7.631%
84	19.978	2827	2832	2842	rVB2	350579	572413	96.14%	10.285%
85	21.893	3153	3158	3164	rVB2	345541	572343	96.13%	10.284%


Sum of corrected areas: 5565452

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
Data File : BG047521.D
Acq On : 2 Dec 2020 7:57
Operator : CG/JU
Sample : L4865-21
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B19

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

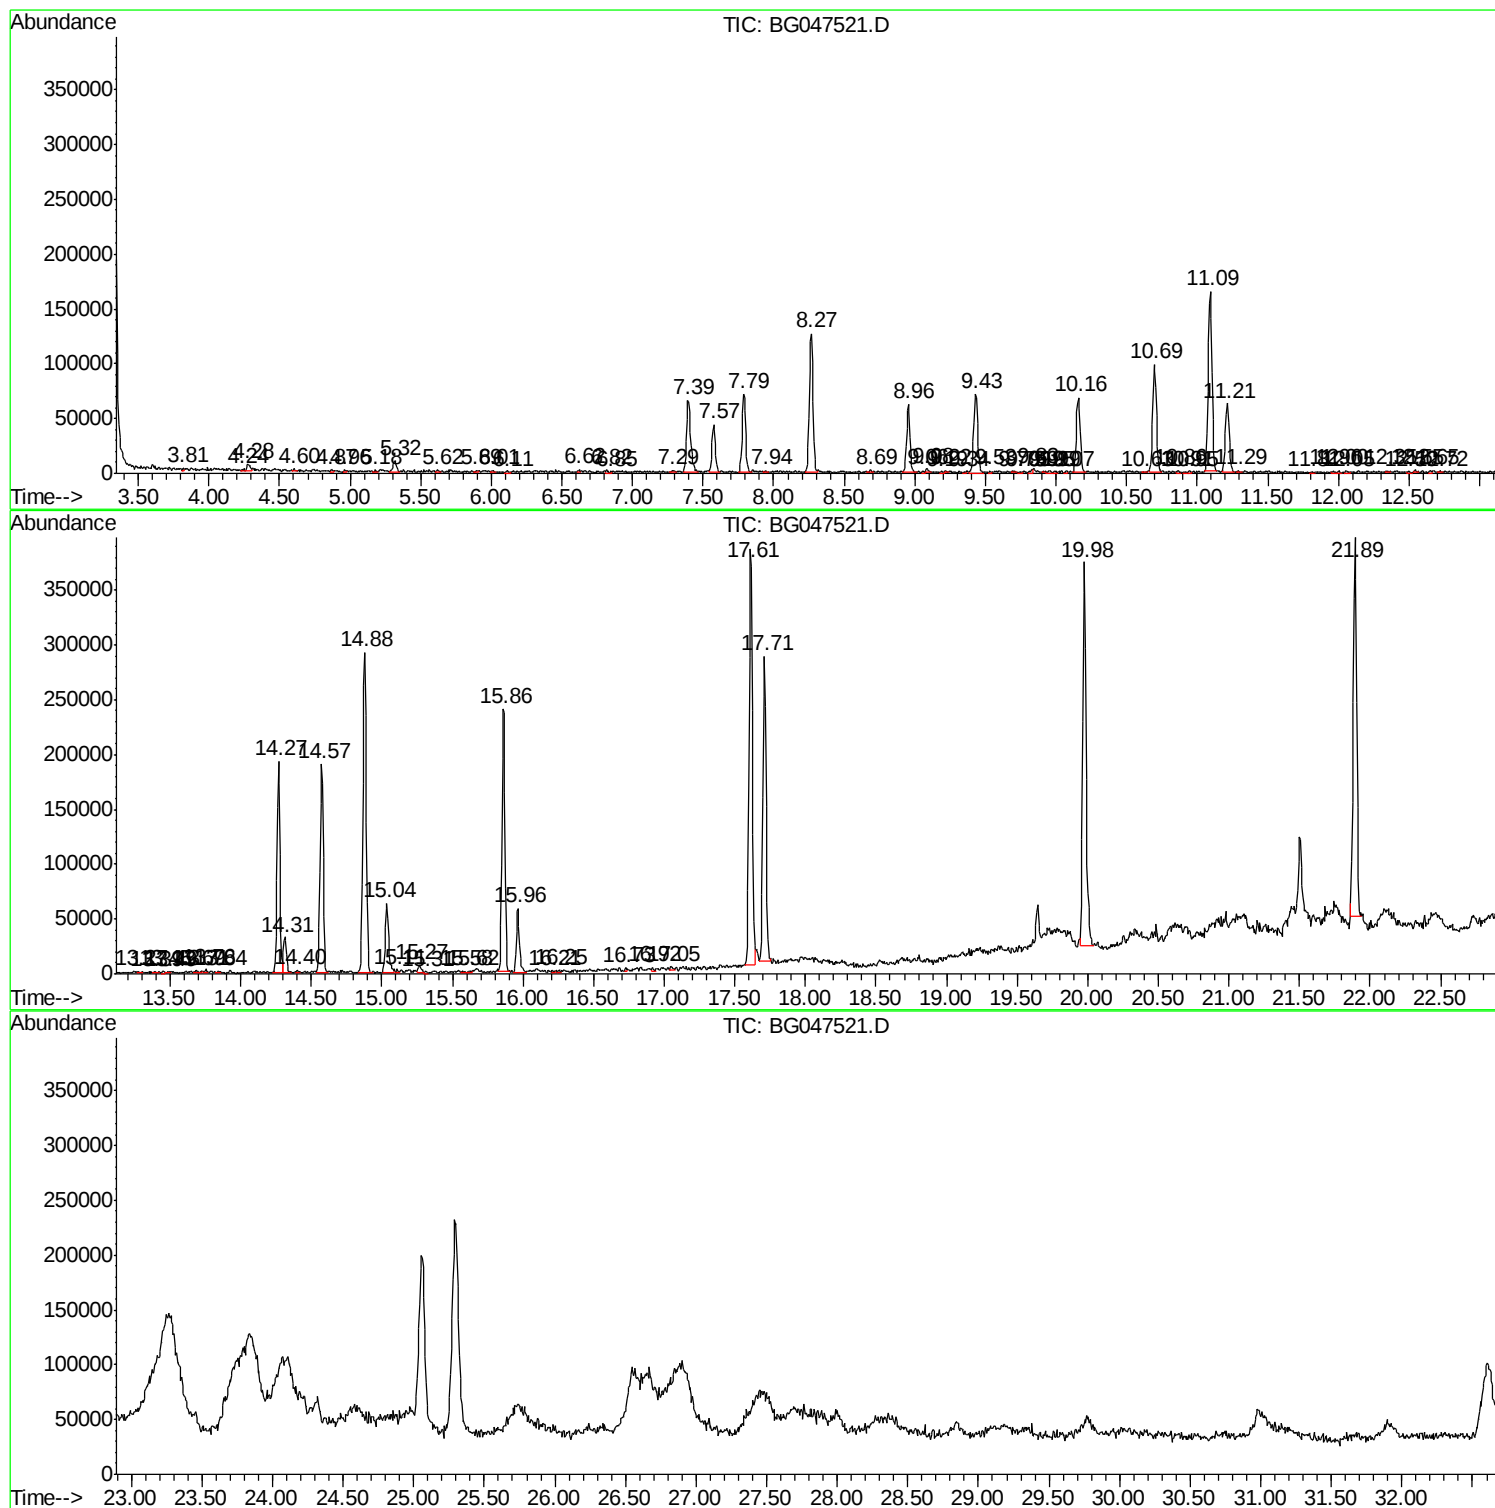

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120120\
Data File : BG047521.D
Acq On : 2 Dec 2020 7:57
Operator : CG/JU
Sample : L4865-21
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B19

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120120\
Data File : BG047521.D
Acq On : 2 Dec 2020 7:57
Operator : CG/JU
Sample : L4865-21
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B19

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc