

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047522.D
 Acq On : 2 Dec 2020 8:37
 Operator : CG/JU
 Sample : L4865-22
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.279	158	160	165	rVB3	3636	4339	0.66%	0.077%
2	4.555	205	207	210	rVB	1970	1776	0.27%	0.031%
3	4.761	239	242	243	rVB2	2625	2032	0.31%	0.036%
4	4.802	245	249	251	rBV2	2381	3025	0.46%	0.054%
5	4.896	262	265	269	rBV2	2715	3733	0.57%	0.066%
6	5.007	282	284	286	rBV	2004	1943	0.30%	0.034%
7	5.201	315	317	319	rBV	2432	1884	0.29%	0.033%
8	5.319	332	337	340	rBV3	7041	10938	1.66%	0.194%
9	5.583	379	382	386	rVV3	1801	2512	0.38%	0.045%
10	5.630	388	390	394	rVB	1820	2055	0.31%	0.036%
11	5.818	418	422	425	rVB	2192	2916	0.44%	0.052%
12	5.865	425	430	431	rBV	1441	2389	0.36%	0.042%
13	6.394	517	520	523	rVB2	2127	2735	0.42%	0.048%
14	6.459	528	531	533	rBV2	1776	1860	0.28%	0.033%
15	6.600	553	555	557	rBV2	1312	1769	0.27%	0.031%
16	6.623	557	559	562	rVB3	3850	3445	0.52%	0.061%
17	6.846	595	597	601	rVB3	1633	1935	0.29%	0.034%
18	6.946	612	614	617	rVB3	2960	1940	0.29%	0.034%
19	6.976	617	619	623	rBV3	1626	2023	0.31%	0.036%
20	7.075	630	636	637	rBV3	1640	2147	0.33%	0.038%
21	7.181	652	654	656	rBV	1807	1863	0.28%	0.033%
22	7.346	680	682	685	rBV	1209	1679	0.26%	0.030%
23	7.393	685	690	701	rVV4	50723	111577	16.95%	1.977%
24	7.498	705	708	711	rVB4	2551	2550	0.39%	0.045%
25	7.575	714	721	728	rBV	40770	72818	11.06%	1.290%
26	7.786	749	757	764	rBV2	64303	112235	17.05%	1.989%
27	7.986	790	791	794	rBV2	3409	2426	0.37%	0.043%
28	8.262	831	838	845	rBV	135646	242495	36.83%	4.297%
29	8.392	858	860	864	rVB	1681	2126	0.32%	0.038%
30	8.433	864	867	870	rBV	1925	2227	0.34%	0.039%
31	8.956	949	956	962	rVB2	57232	102300	15.54%	1.813%
32	9.091	975	979	980	rBV2	1755	1855	0.28%	0.033%
33	9.431	1030	1037	1044	rBV	74915	138125	20.98%	2.447%
34	9.502	1047	1049	1053	rVB	1465	1903	0.29%	0.034%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047522.D
 Acq On : 2 Dec 2020 8:37
 Operator : CG/JU
 Sample : L4865-22
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

35	9.596	1062	1065	1068	rVB	1826	2233	0.34%	0.040%
36	9.843	1102	1107	1113	rBV3	4772	8559	1.30%	0.152%
37	9.984	1129	1131	1135	rVB3	1868	2533	0.38%	0.045%
38	10.160	1154	1161	1168	rVB2	63357	118589	18.01%	2.101%
39	10.695	1246	1252	1262	rVB2	86618	160782	24.42%	2.849%
40	11.094	1313	1320	1326	rBV	188150	327943	49.81%	5.811%
41	11.212	1330	1340	1349	rBV3	65838	125426	19.05%	2.222%
42	11.306	1352	1356	1359	rVB3	1720	2090	0.32%	0.037%
43	12.287	1521	1523	1526	rBV3	1500	1863	0.28%	0.033%
44	12.322	1526	1529	1532	rVB3	2294	2319	0.35%	0.041%
45	12.434	1545	1548	1551	rVB	2497	2690	0.41%	0.048%
46	12.469	1551	1554	1555	rBV	1844	1890	0.29%	0.033%
47	12.845	1614	1618	1621	rBV	1566	2102	0.32%	0.037%
48	13.145	1667	1669	1671	rVB	2418	1987	0.30%	0.035%
49	13.174	1671	1674	1678	rBV	2230	2831	0.43%	0.050%
50	13.321	1697	1699	1702	rVB	1614	1713	0.26%	0.030%
51	13.762	1770	1774	1778	rVB4	3294	5322	0.81%	0.094%
52	13.820	1780	1784	1788	rBV4	1666	2837	0.43%	0.050%
53	14.202	1846	1849	1854	rVB4	9137	12453	1.89%	0.221%
54	14.267	1854	1860	1865	rBV	186915	269559	40.94%	4.776%
55	14.314	1865	1868	1875	rVB	45633	60462	9.18%	1.071%
56	14.461	1891	1893	1896	rBV	1970	2007	0.30%	0.036%
57	14.573	1904	1912	1919	rBV	182975	297432	45.18%	5.270%
58	14.714	1934	1936	1938	rVB	2293	1684	0.26%	0.030%
59	14.731	1938	1939	1941	rBV	1934	1747	0.27%	0.031%
60	14.831	1953	1956	1958	rBV2	9190	10373	1.58%	0.184%
61	14.878	1958	1964	1971	rVB2	304096	492037	74.73%	8.718%
62	15.037	1985	1991	1998	rBV3	35000	60825	9.24%	1.078%
63	15.272	2025	2031	2038	rVB4	5037	9366	1.42%	0.166%
64	15.589	2083	2085	2088	rBV4	1741	1777	0.27%	0.031%
65	15.642	2092	2094	2098	rVV2	2639	3126	0.47%	0.055%
66	15.701	2102	2104	2106	rVB	3439	2649	0.40%	0.047%
67	15.718	2106	2107	2110	rBV	1760	1875	0.28%	0.033%
68	15.859	2125	2131	2139	rVB	243564	381456	57.94%	6.759%
69	15.924	2139	2142	2144	rBV	2576	3121	0.47%	0.055%
70	15.965	2144	2149	2156	rVB2	54551	84049	12.77%	1.489%
71	16.100	2168	2172	2174	rVB	3636	4114	0.62%	0.073%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
 Data File : BG047522.D
 Acq On : 2 Dec 2020 8:37
 Operator : CG/JU
 Sample : L4865-22
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0B67

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
 Title : SVOA CALIBRATION

72	16.511	2241	2242	2246	rBV2	2019	1712	0.26%	0.030%
73	16.641	2262	2264	2267	rVB2	3124	2272	0.35%	0.040%
74	16.835	2296	2297	2303	rBV2	2916	3914	0.59%	0.069%
75	17.140	2344	2349	2353	rVB3	7417	9819	1.49%	0.174%
76	17.234	2363	2365	2369	rVB3	2600	2826	0.43%	0.050%
77	17.334	2381	2382	2385	rBV	4160	3288	0.50%	0.058%
78	17.393	2391	2392	2395	rBV	3187	3164	0.48%	0.056%
79	17.610	2423	2429	2438	rBV	433515	651060	98.89%	11.536%
80	17.710	2440	2446	2452	rVB2	278600	431157	65.49%	7.640%
81	18.474	2574	2576	2577	rBV	3793	2693	0.41%	0.048%
82	19.978	2826	2832	2839	rBV	358540	545995	82.93%	9.674%
83	21.893	3153	3158	3164	rVB2	381470	658380	100.00%	11.666%


Sum of corrected areas: 5643676

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG120120\
Data File : BG047522.D
Acq On : 2 Dec 2020 8:37
Operator : CG/JU
Sample : L4865-22
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B67

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

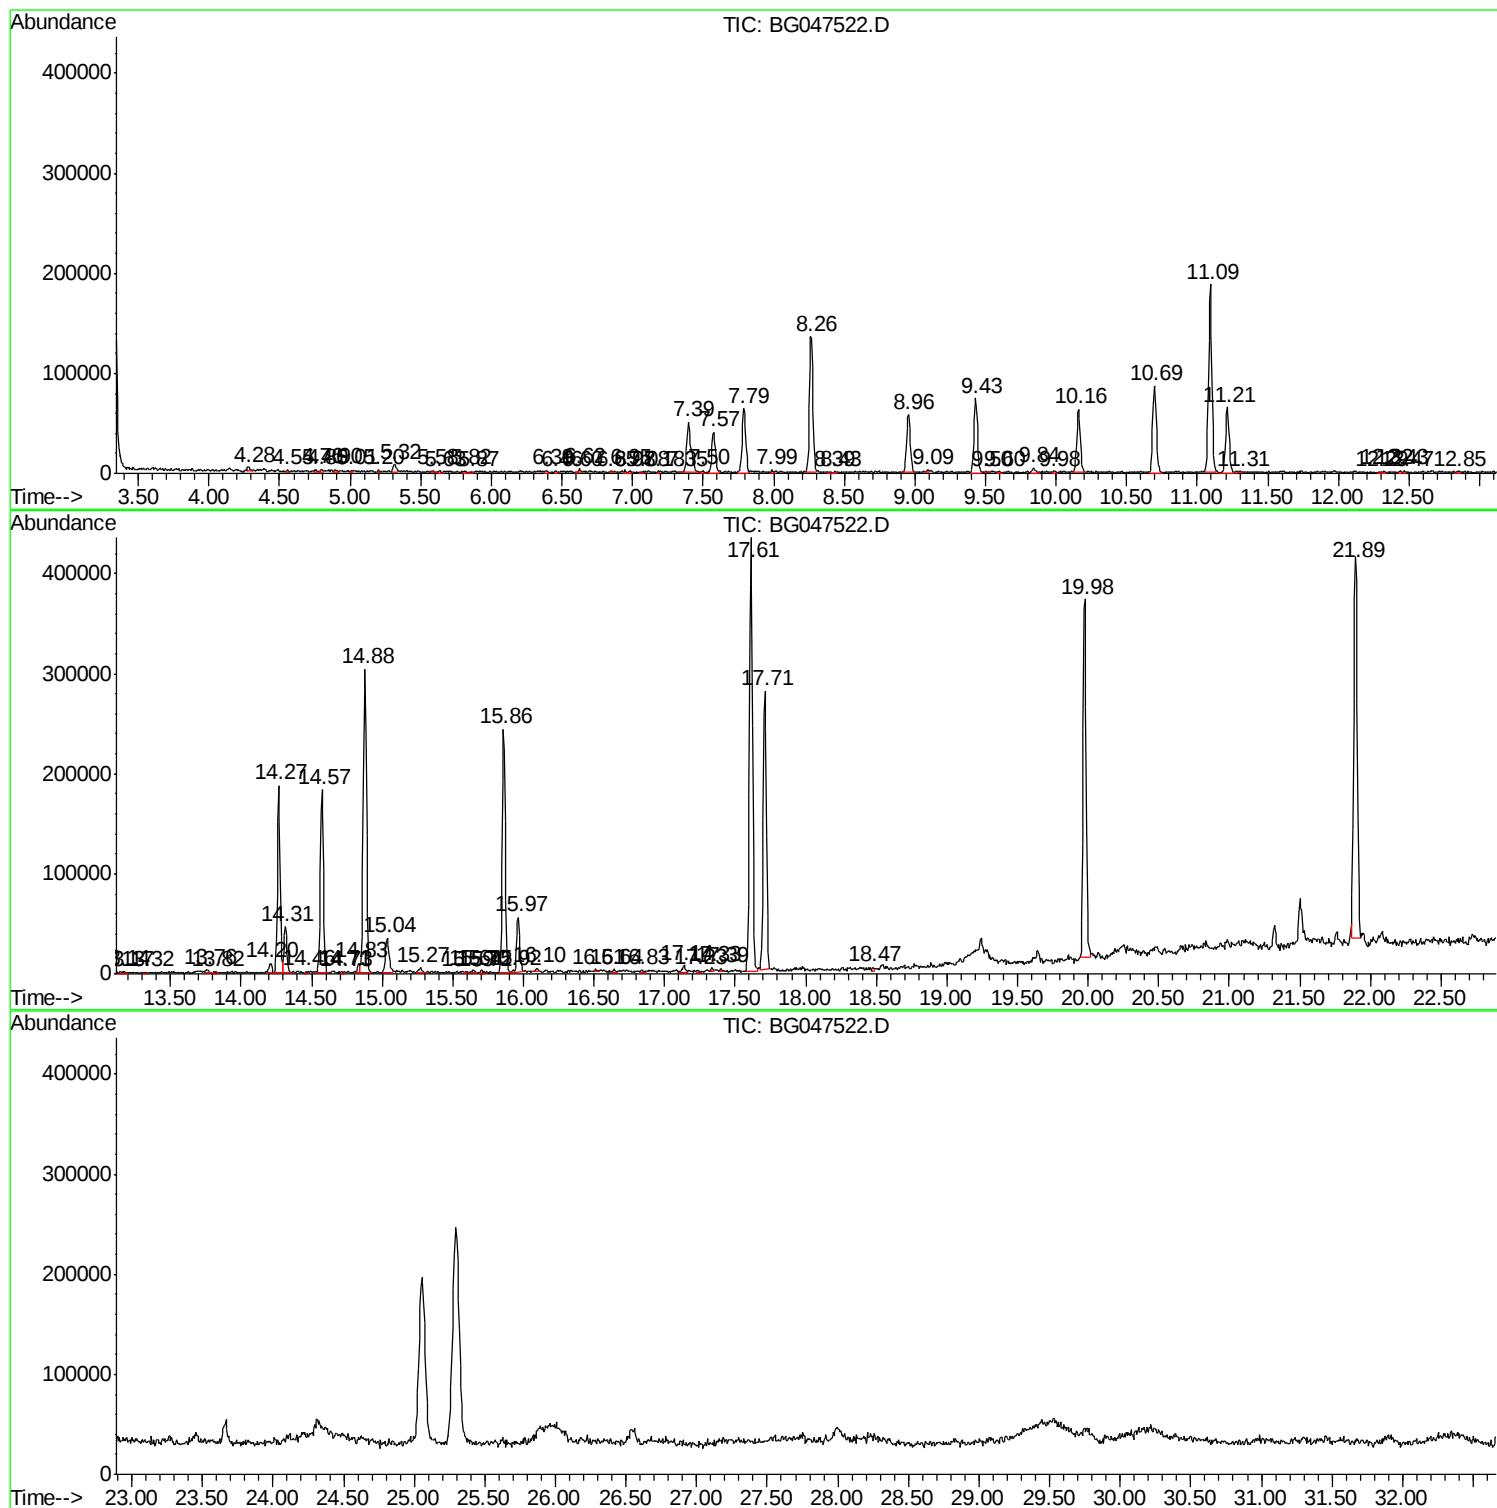

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120120\
Data File : BG047522.D
Acq On : 2 Dec 2020 8:37
Operator : CG/JU
Sample : L4865-22
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B67

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG120120\
Data File : BG047522.D
Acq On : 2 Dec 2020 8:37
Operator : CG/JU
Sample : L4865-22
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0B67

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG111920MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc