

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051612.D
 Acq On : 18 Dec 2021 1:49
 Operator : CG/JU
 Sample : M5121-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL64

Quant Time: Dec 18 02:25:28 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 14 14:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.275	152	38856	20.000	ng/ul	-0.01
20) Naphthalene-d8	11.112	136	159979	20.000	ng/ul	#-0.01
38) Acenaphthene-d10	14.913	164	115252	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.656	188	254847	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.980	240	216250	20.000	ng/ul	# 0.00
88) Perylene-d12	25.475	264	230562	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.599	96	3429	3.665	ng/uL	0.00
4) Pyridine-d5	4.033	84	15542	5.498	ng/ul	-0.01
7) Phenol-d5	7.405	99	82033	23.645	ng/ul	-0.01
9) Bis-(2-Chloroethyl)eth...	7.582	67	48367	23.451	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.799	132	57596	23.870	ng/ul	-0.01
15) 4-Methylphenol-d8	8.968	113	64686	24.121	ng/ul	-0.01
21) Nitrobenzene-d5	9.444	128	30427	25.942	ng/ul	-0.01
24) 2-Nitrophenol-d4	10.178	143	32930	25.683	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.719	165	65276	23.476	ng/ul	-0.01
31) 4-Chloroaniline-d4	11.230	131	50965	13.922	ng/ul	-0.01
46) Dimethylphthalate-d6	14.296	166	208221	22.572	ng/ul	-0.02
49) Acenaphthylene-d8	14.607	160	272287	23.767	ng/ul	0.00
54) 4-Nitrophenol-d4	15.071	143	25663	17.107	ng/ul	0.00
60) Fluorene-d10	15.900	176	185908	22.494	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.000	200	18699	14.083	ng/ul	-0.01
73) Anthracene-d10	17.756	188	291495	23.978	ng/ul	0.00
81) Pyrene-d10	20.029	212	305525	23.475	ng/ul	-0.01
92) Benzo(a)pyrene-d12	25.234	264	283325	23.355	ng/ul	-0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.845	149	27463	3.954	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051612.D
Acq On : 18 Dec 2021 1:49
Operator : CG/JU
Sample : M5121-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL64

Quant Time: Dec 18 02:25:28 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 14 14:19:57 2021
Response via : Initial Calibration

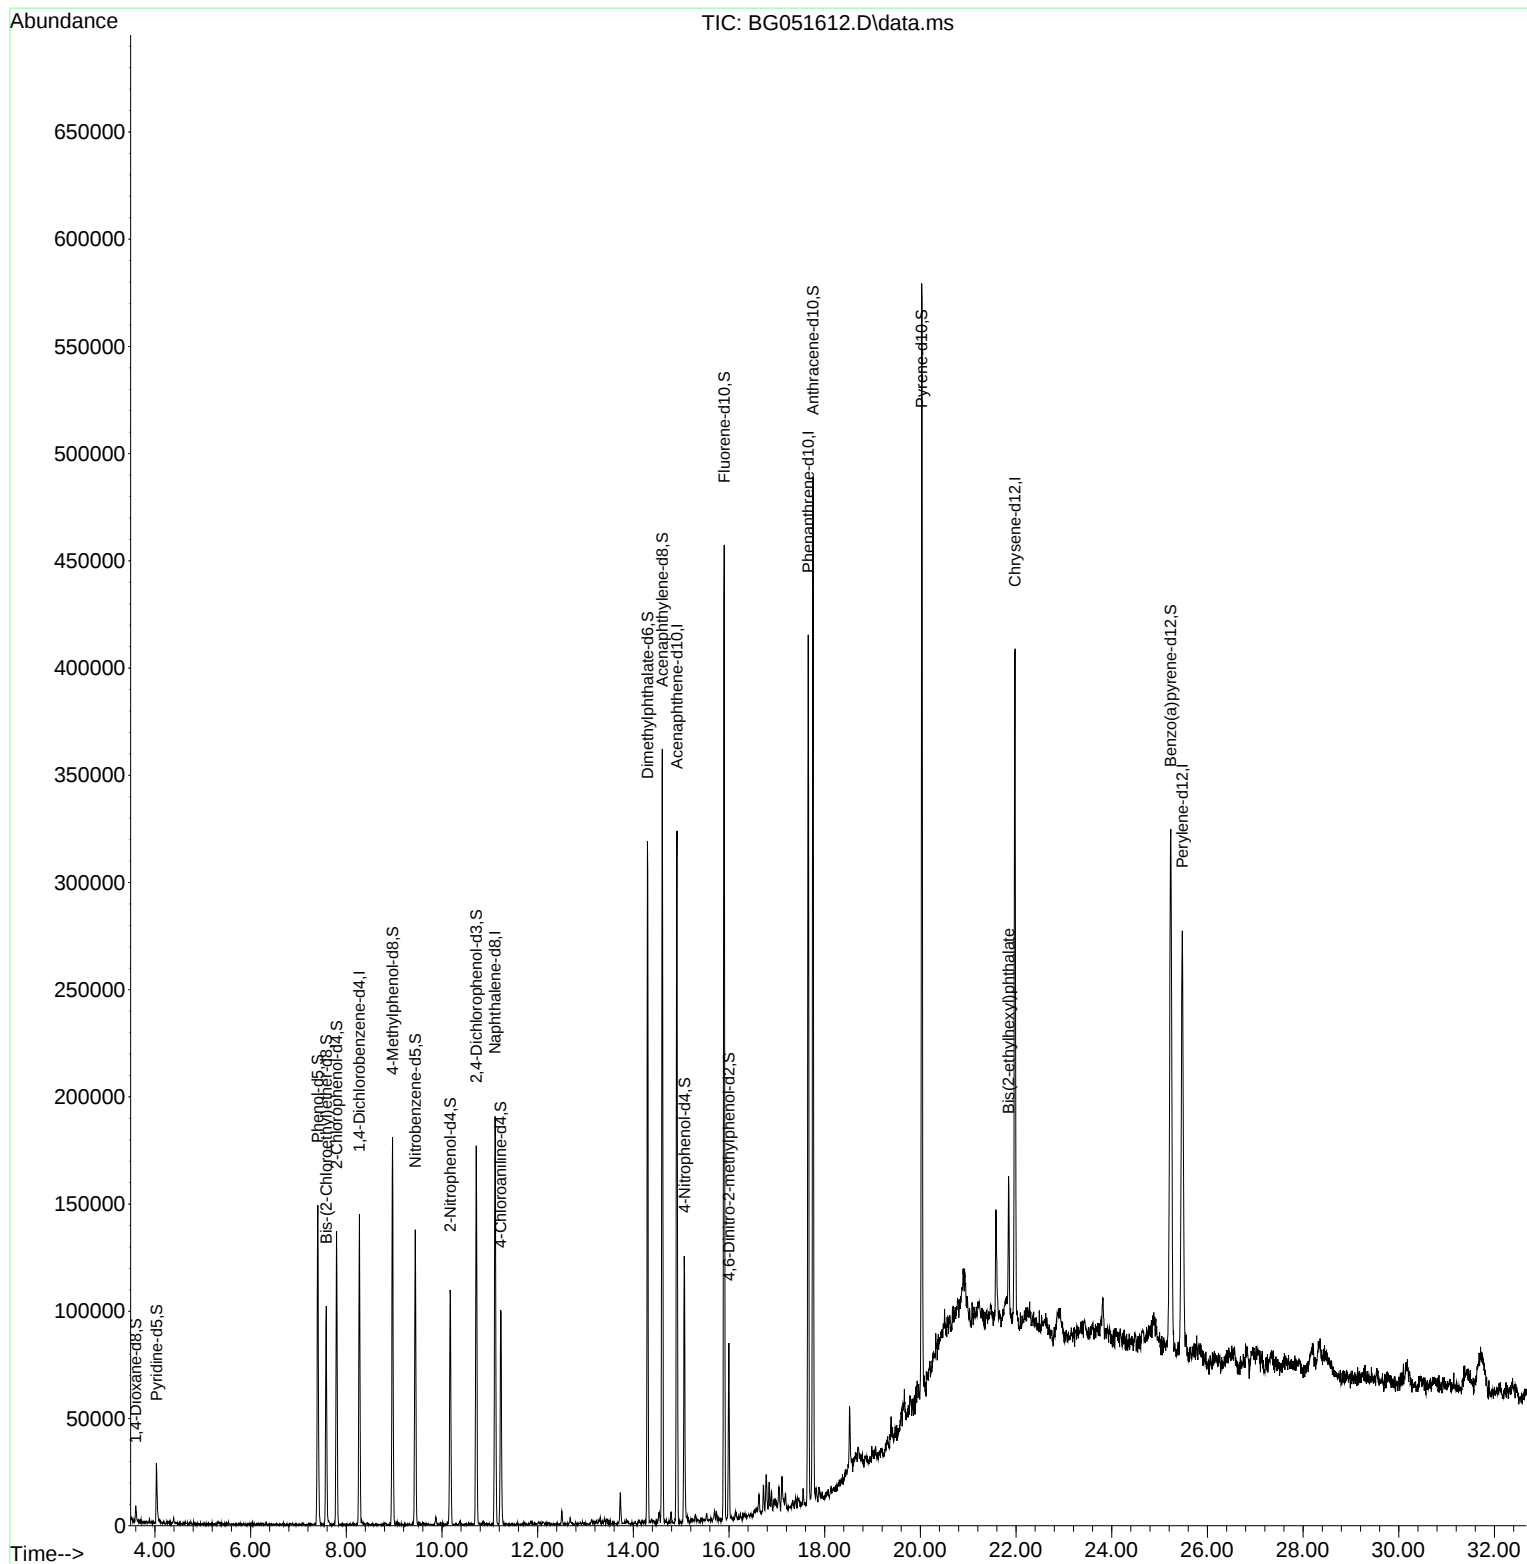

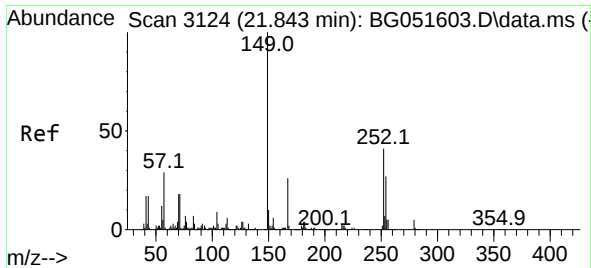

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 3.954 ng/ul
 RT: 21.845 min Scan# 31
 Delta R.T. -0.024 min
 Lab File: BG051612.D
 Acq: 18 Dec 2021 1:49

Instrument :
 BNA_G
 ClientSampleId :
 BGL64

Tgt Ion	Ratio	Lower	Upper
149	100		
167	26.5	21.1	31.7
279	4.2	2.7	4.1#

