

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051615.D
 Acq On : 18 Dec 2021 3:50
 Operator : CG/JU
 Sample : M5121-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL50

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 12/20/2021
 Supervised By :mohammad ahmed 12/24/2021

Quant Time: Dec 18 04:34:41 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 14 14:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.275	152	36285	20.000	ng/u1	-0.01
20) Naphthalene-d8	11.113	136	158772	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.908	164	111622	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.657	188	251642	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.974	240	226274	20.000	ng/u1	#-0.01
88) Perylene-d12	25.476	264	234411	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.599	96	4265	4.882	ng/uL	0.00
4) Pyridine-d5	4.028	84	45716	17.318	ng/u1	-0.02
7) Phenol-d5	7.406	99	87183	26.910	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.576	67	52410	27.212	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.800	132	61976	27.505	ng/u1	-0.01
15) 4-Methylphenol-d8	8.963	113	68412	27.318	ng/u1	-0.02
21) Nitrobenzene-d5	9.444	128	31827	27.342	ng/u1	-0.01
24) 2-Nitrophenol-d4	10.179	143	36084	28.357	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.719	165	69146	25.057	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.230	131	41813	11.508	ng/u1	-0.01
46) Dimethylphthalate-d6	14.297	166	220719	24.705	ng/u1	-0.02
49) Acenaphthylene-d8	14.602	160	282250	25.438	ng/u1	-0.01
54) 4-Nitrophenol-d4	15.066	143	31887m	21.948	ng/u1	-0.01
60) Fluorene-d10	15.900	176	197429	24.665	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.994	200	25573	19.505	ng/u1	-0.02
73) Anthracene-d10	17.757	188	309847	25.812	ng/u1	0.00
81) Pyrene-d10	20.030	212	348049	25.557	ng/u1	-0.01
92) Benzo(a)pyrene-d12	25.229	264	307910	24.965	ng/u1	-0.02
Target Compounds						
					Qvalue	
8) Phenol	7.429	94	5268	1.635	ng/u1#	70

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051615.D
Acq On : 18 Dec 2021 3:50
Operator : CG/JU
Sample : M5121-01
Misc :
ALS Vial : 29 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BGL50

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 12/20/2021
Supervised By :mohammad ahmed 12/24/2021

Quant Time: Dec 18 04:34:41 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 14 14:19:57 2021
Response via : Initial Calibration

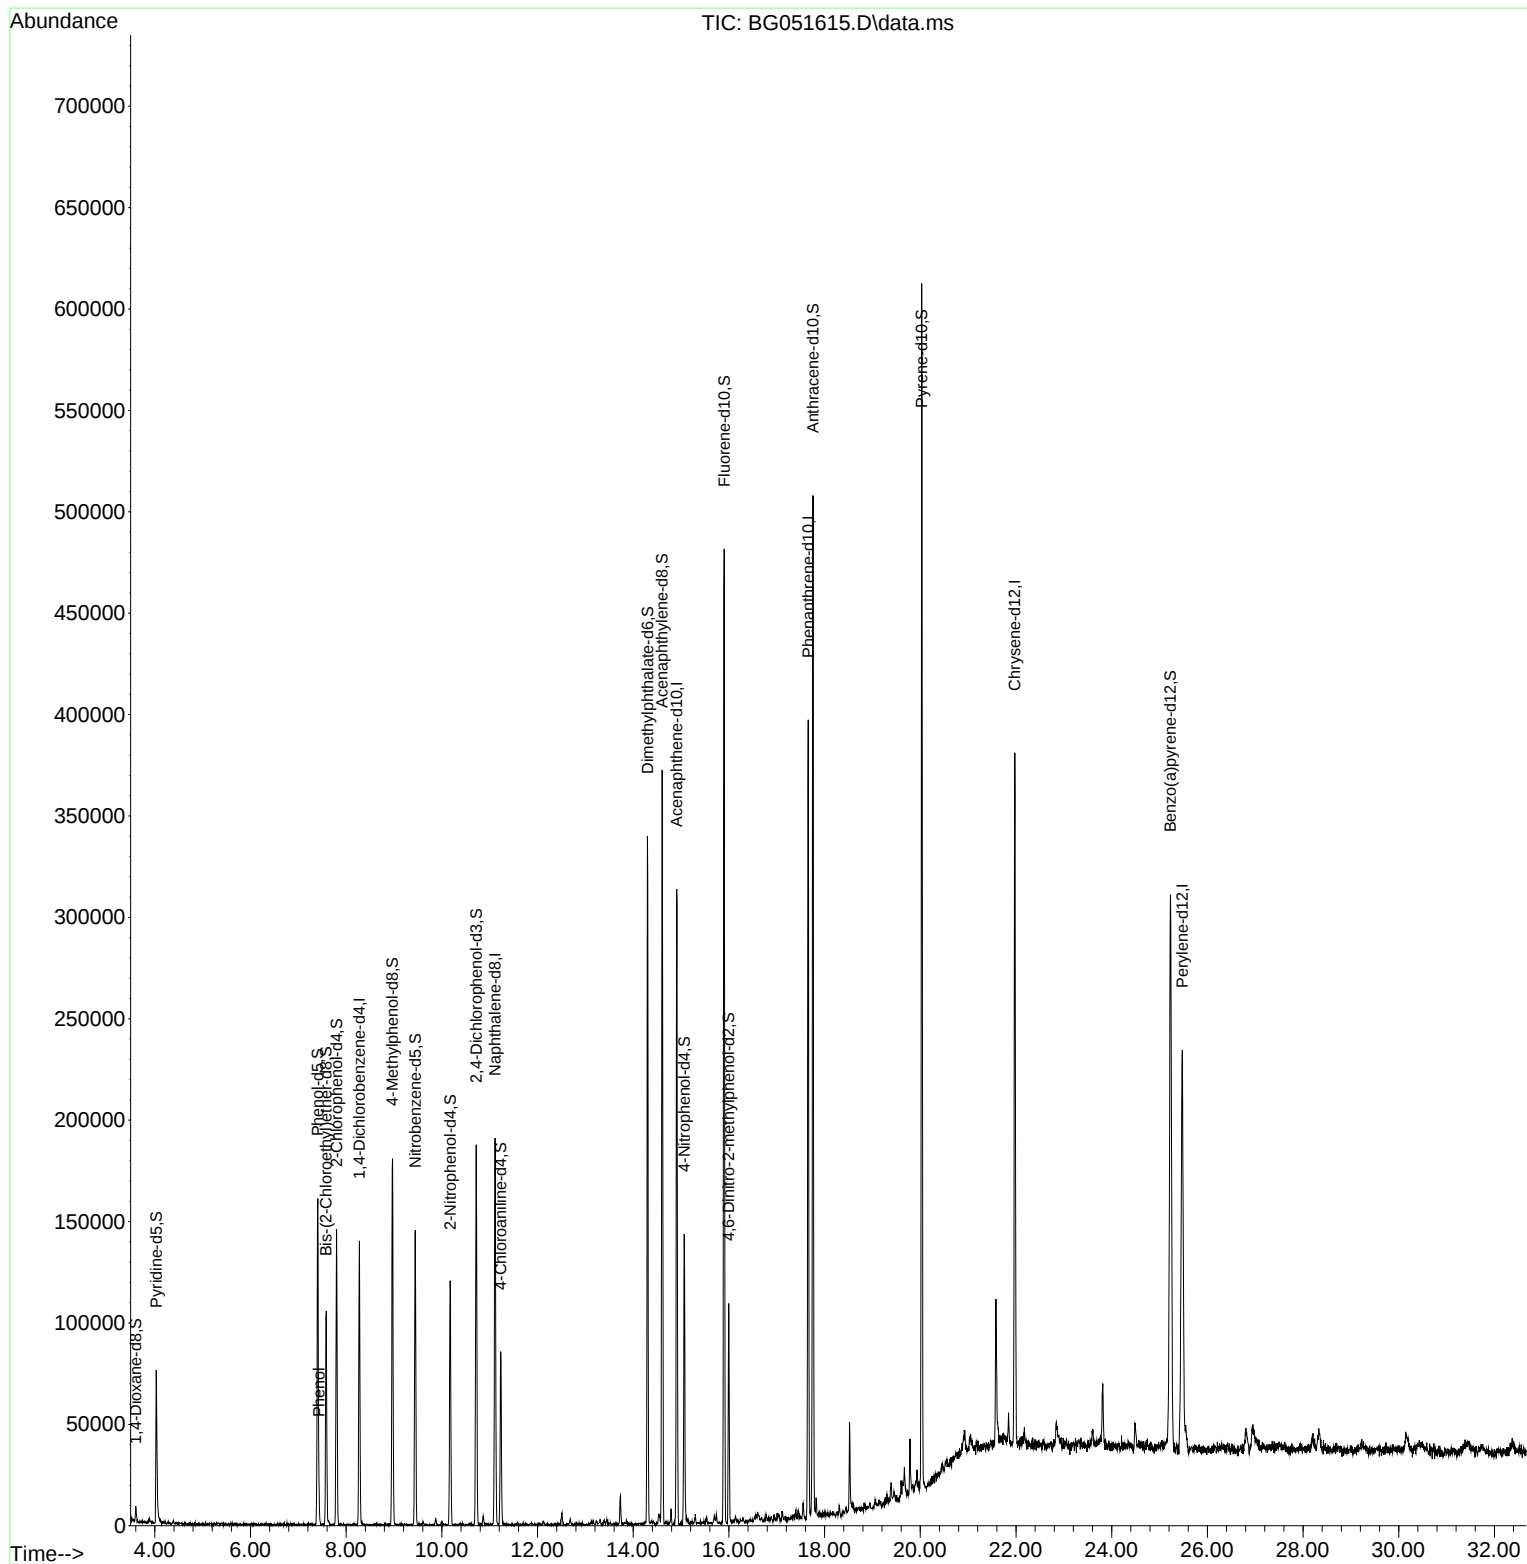

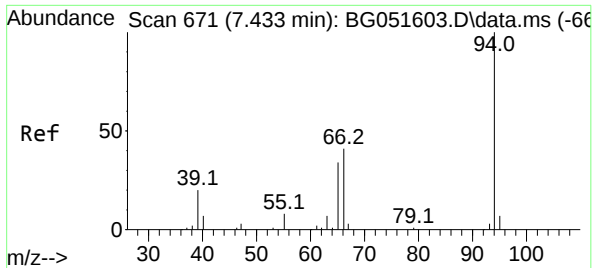

Phenol

Concen: 1.635 ng/ul

RT: 7.429 min Scan# 61

Delta R.T. -0.011 min

Lab File: BG051615.D

Acq: 18 Dec 2021 3:50

Instrument :

BNA_G

ClientSampleId :

BGL50

Tgt Ion: 94 Resp: 526

Ion Ratio Lower Upper

94 100

65 41.9 25.1 37.7

66 63.2 31.6 47.4

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 12/20/2021

Supervised By :mohammad ahmed 12/24/2021

