

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051630.D
 Acq On : 18 Dec 2021 14:38
 Operator : CG/JU
 Sample : M5034-02
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C00V0

Quant Time: Dec 18 20:36:21 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 14 14:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.276	152	46800	20.000	ng/u1	-0.01
20) Naphthalene-d8	11.113	136	195054	20.000	ng/u1	#-0.01
38) Acenaphthene-d10	14.908	164	138081	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.657	188	316955	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.975	240	301665	20.000	ng/u1	#-0.01
88) Perylene-d12	25.470	264	310499	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.600	96	7575	6.722	ng/uL	0.00
4) Pyridine-d5	4.028	84	102856	30.209	ng/u1	-0.02
7) Phenol-d5	7.406	99	174320	41.717	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.582	67	101652	40.921	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.800	132	121942	41.959	ng/u1	-0.01
15) 4-Methylphenol-d8	8.969	113	136563	42.280	ng/u1	-0.01
21) Nitrobenzene-d5	9.445	128	63603	44.476	ng/u1	-0.01
24) 2-Nitrophenol-d4	10.179	143	73690	47.138	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.719	165	140537	41.455	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.230	131	124013	27.784	ng/u1	-0.01
46) Dimethylphthalate-d6	14.303	166	445903	40.346	ng/u1	-0.01
49) Acenaphthylene-d8	14.602	160	553011	40.289	ng/u1	-0.01
54) 4-Nitrophenol-d4	15.066	143	65772	36.596	ng/u1	-0.01
60) Fluorene-d10	15.901	176	385094	38.891	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	16.000	200	58990	35.722	ng/u1	-0.01
73) Anthracene-d10	17.757	188	602830	39.871	ng/u1	0.00
81) Pyrene-d10	20.030	212	685806	37.774	ng/u1	-0.01
92) Benzo(a)pyrene-d12	25.235	264	663280	40.599	ng/u1	-0.02
Target Compounds						
					Qvalue	
8) Phenol	7.430	94	10086	2.427	ng/u1#	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051630.D
Acq On : 18 Dec 2021 14:38
Operator : CG/JU
Sample : M5034-02
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C00V0

Quant Time: Dec 18 20:36:21 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 14 14:19:57 2021
Response via : Initial Calibration

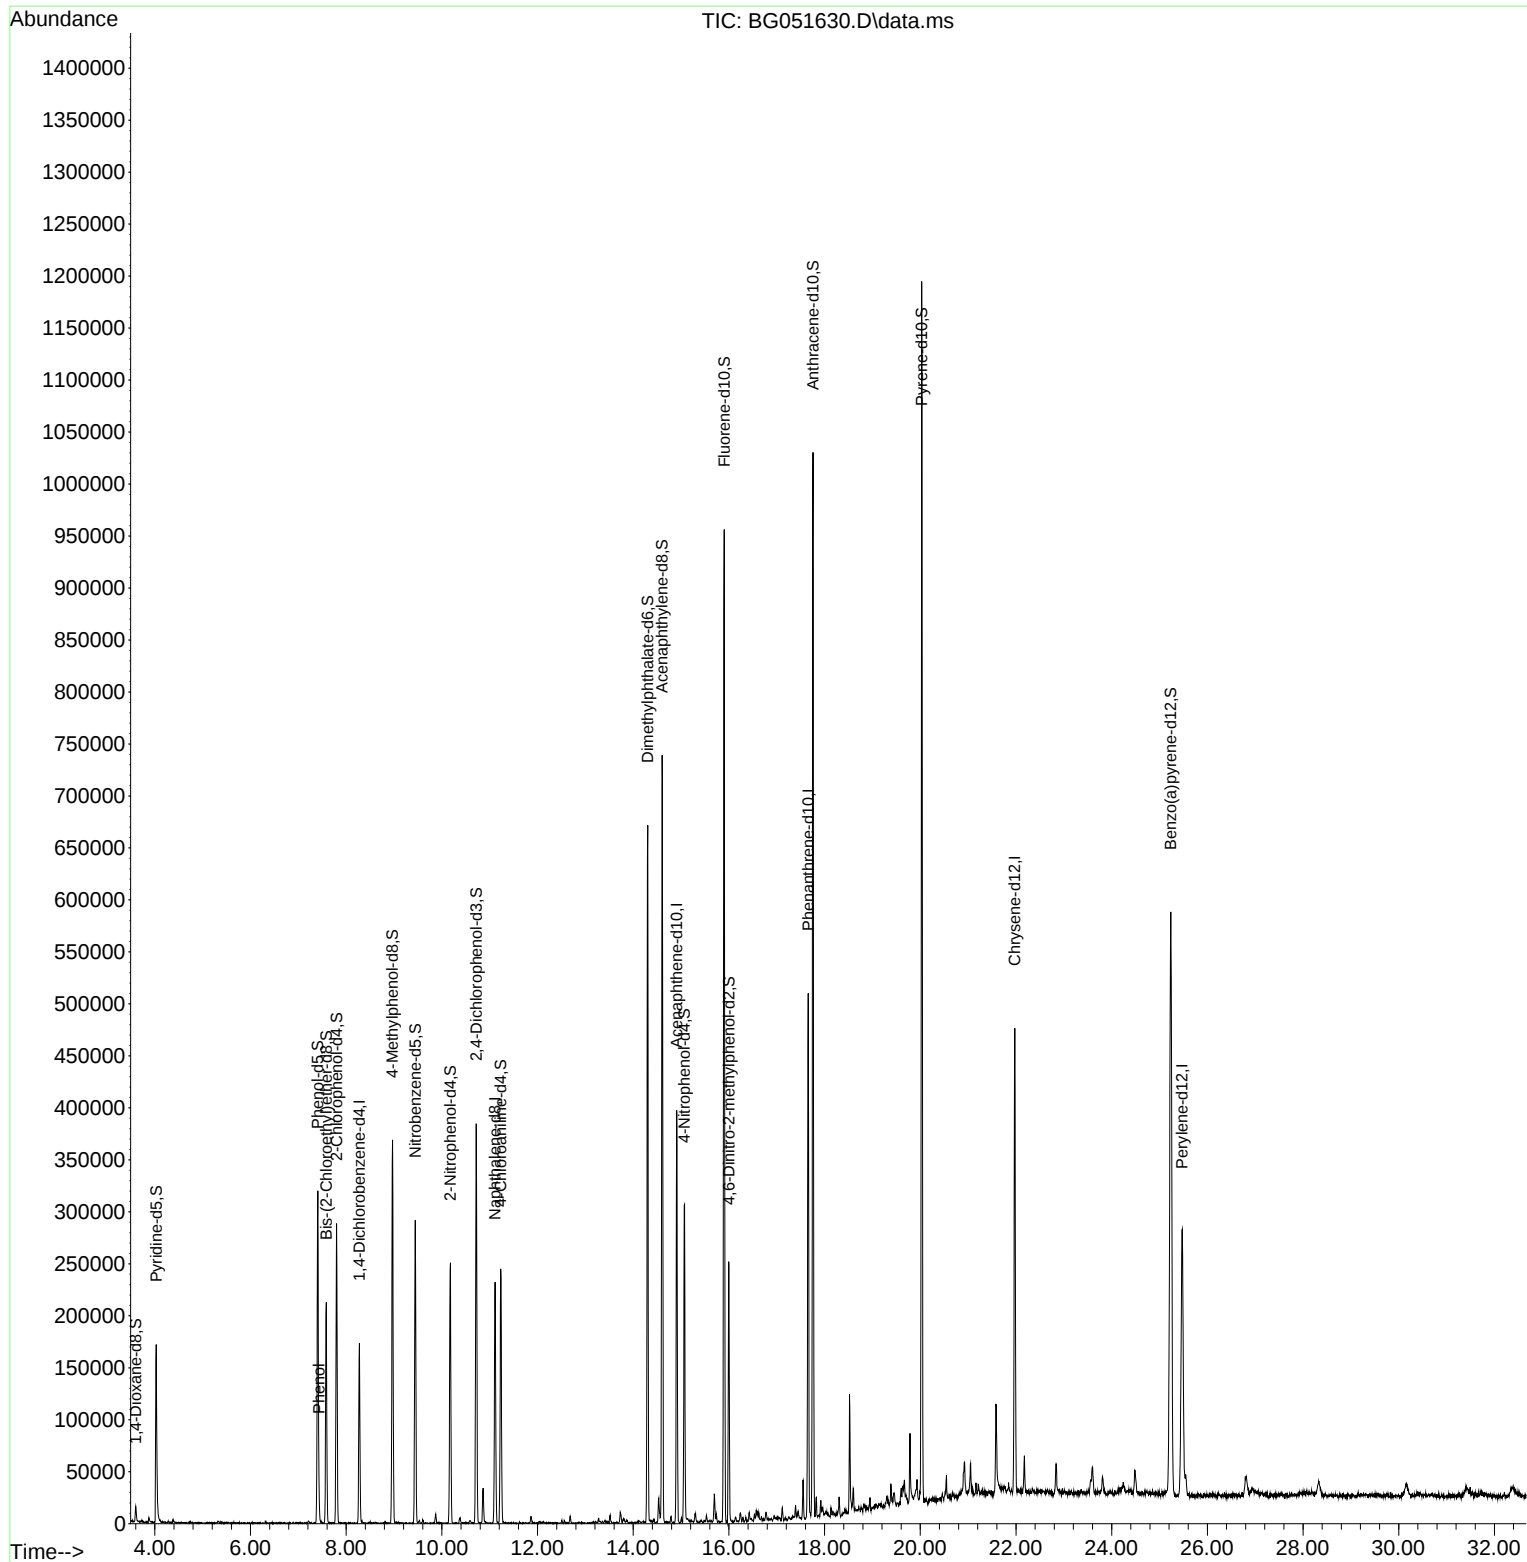

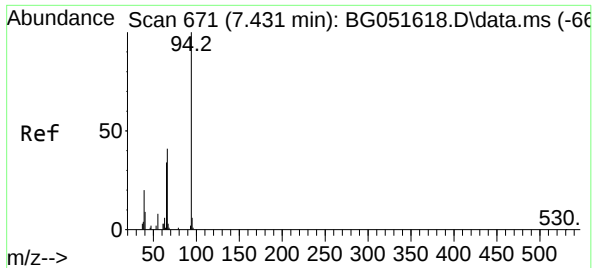

Phenol

Concen: 2.427 ng/ul

RT: 7.430 min Scan# 61

Delta R.T. -0.011 min

Lab File: BG051630.D


Acq: 18 Dec 2021 14:38

Instrument :

BNA_G

ClientSampleId :

C00V0

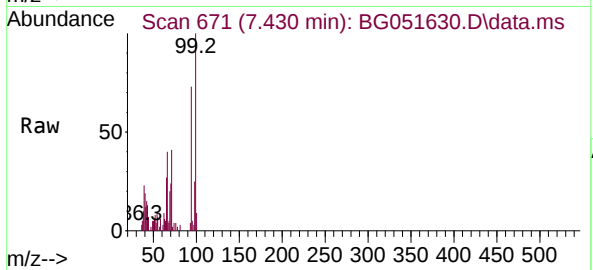

Tgt Ion: 94 Resp: 10086

Ion Ratio Lower Upper

94 100

65 36.6 25.1 37.7

66 55.0 31.6 47.4#

