

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051637.D
 Acq On : 18 Dec 2021 20:05
 Operator : CG/JU
 Sample : M5153-11
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL77

Quant Time: Dec 18 20:58:17 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 14 14:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.275	152	34634	20.000	ng/u1	-0.01
20) Naphthalene-d8	11.112	136	137413	20.000	ng/u1	#-0.01
38) Acenaphthene-d10	14.907	164	102720	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.656	188	246318	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.974	240	239567	20.000	ng/u1	#-0.01
88) Perylene-d12	25.469	264	246245	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.593	96	3886	4.660	ng/uL	-0.01
4) Pyridine-d5	4.028	84	27493	10.911	ng/u1	-0.02
7) Phenol-d5	7.406	99	84447	27.308	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.576	67	47497	25.837	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.799	132	58825	27.351	ng/u1	-0.01
15) 4-Methylphenol-d8	8.962	113	62784	26.266	ng/u1	-0.02
21) Nitrobenzene-d5	9.444	128	28751	28.538	ng/u1	-0.01
24) 2-Nitrophenol-d4	10.172	143	32566	29.570	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.719	165	65475	27.415	ng/u1	-0.01
31) 4-Chloroaniline-d4	11.230	131	50165	15.953	ng/u1	-0.01
46) Dimethylphthalate-d6	14.296	166	216337	26.313	ng/u1	-0.02
49) Acenaphthylene-d8	14.602	160	270874	26.528	ng/u1	-0.01
54) 4-Nitrophenol-d4	15.066	143	33965	25.404	ng/u1	-0.01
60) Fluorene-d10	15.894	176	194877	26.456	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.994	200	32413	25.257	ng/u1	-0.02
73) Anthracene-d10	17.756	188	321691	27.378	ng/u1	0.00
81) Pyrene-d10	20.030	212	381596	26.466	ng/u1	-0.01
92) Benzo(a)pyrene-d12	25.234	264	356913	27.547	ng/u1	-0.02
Target Compounds						
					Qvalue	
8) Phenol	7.435	94	4503	1.464	ng/u1	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051637.D
Acq On : 18 Dec 2021 20:05
Operator : CG/JU
Sample : M5153-11
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL77


Quant Time: Dec 18 20:58:17 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 14 14:19:57 2021
Response via : Initial Calibration

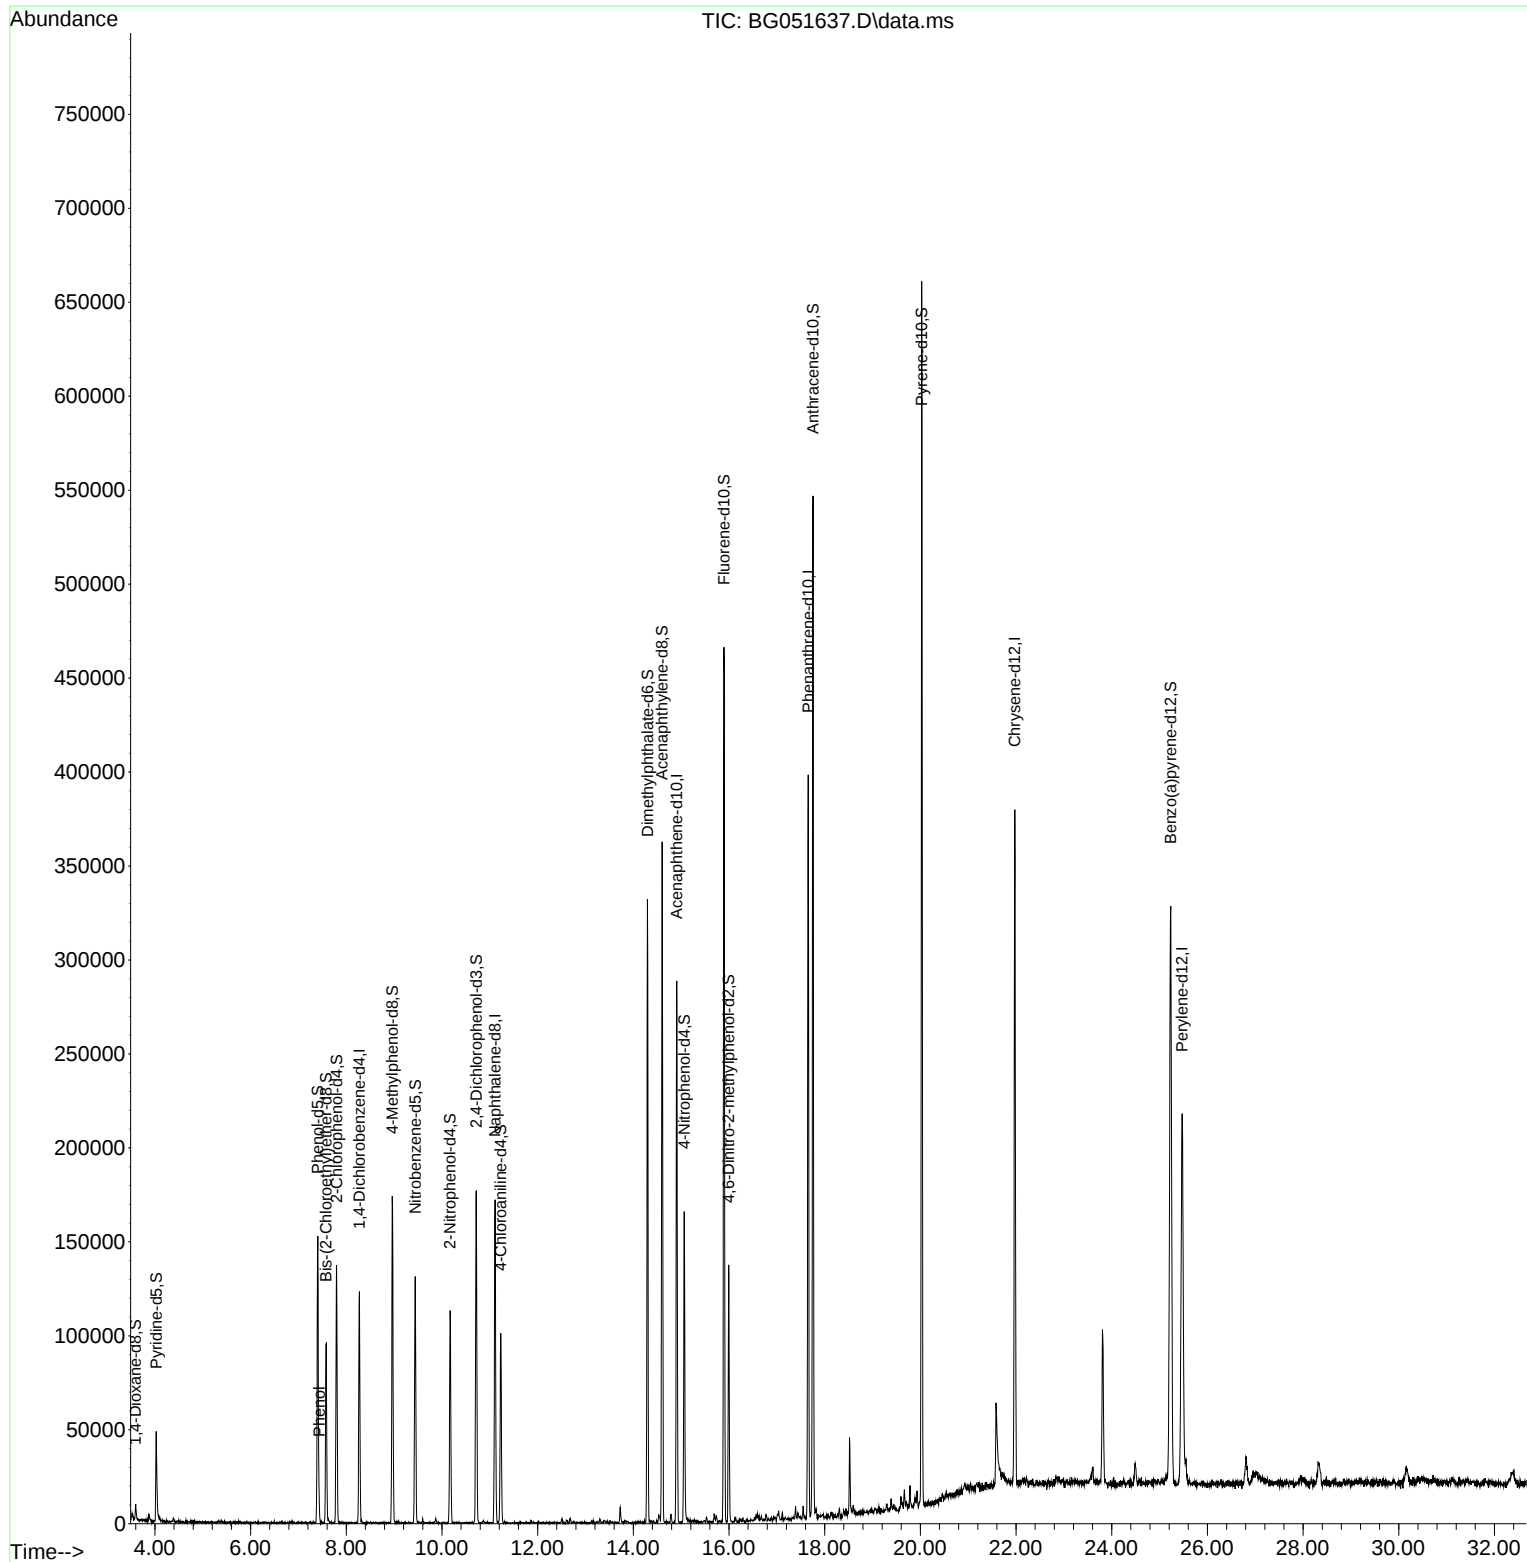

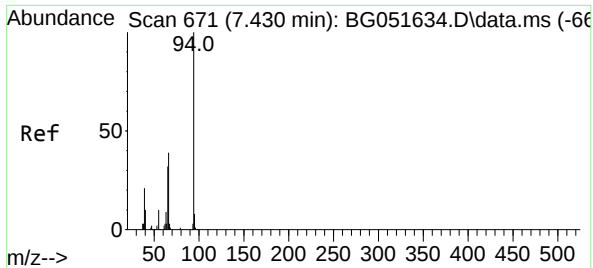

Phenol
 Concen: 1.464 ng/ul
 RT: 7.435 min Scan# 61
 Delta R.T. -0.006 min
 Lab File: BG051637.D
 Acq: 18 Dec 2021 20:05

Instrument :
 BNA_G
 ClientSampleId :
 BGL77

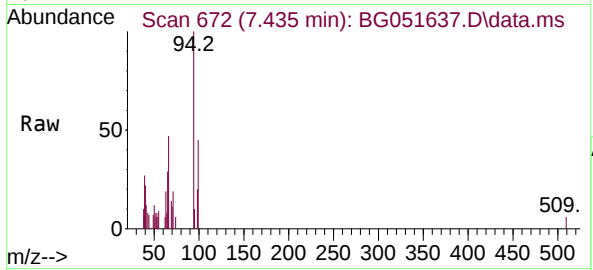

Tgt Ion: 94	Resp:	4503
Ion	Ratio	Lower Upper
94	100	
65	28.9	25.1 37.7
66	46.9	31.6 47.4

