

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051638.D
 Acq On : 18 Dec 2021 20:45
 Operator : CG/JU
 Sample : M5153-10
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL75

Quant Time: Dec 19 00:04:57 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 14 14:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.276	152	33085	20.000	ng/ul	-0.01
20) Naphthalene-d8	11.113	136	135352	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.908	164	93089	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.657	188	210904	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.975	240	214639	20.000	ng/ul	#-0.01
88) Perylene-d12	25.476	264	231331	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.606	96	4256	5.342	ng/uL	0.00
4) Pyridine-d5	4.029	84	32337	13.434	ng/ul	-0.02
7) Phenol-d5	7.401	99	79953	27.065	ng/ul	-0.02
9) Bis-(2-Chloroethyl)eth...	7.577	67	48547	27.645	ng/ul	-0.02
11) 2-Chlorophenol-d4	7.800	132	53480	26.030	ng/ul	-0.01
15) 4-Methylphenol-d8	8.963	113	62001	27.153	ng/ul	-0.02
21) Nitrobenzene-d5	9.445	128	29190	29.415	ng/ul	-0.01
24) 2-Nitrophenol-d4	10.173	143	30831	28.421	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.714	165	62590	26.606	ng/ul	-0.02
31) 4-Chloroaniline-d4	11.231	131	49757	16.065	ng/ul	-0.01
46) Dimethylphthalate-d6	14.297	166	196034	26.310	ng/ul	-0.02
49) Acenaphthylene-d8	14.603	160	251211	27.148	ng/ul	-0.01
54) 4-Nitrophenol-d4	15.067	143	32618	26.920	ng/ul	-0.01
60) Fluorene-d10	15.895	176	175615	26.308	ng/ul	-0.01
65) 4,6-Dinitro-2-methylph...	15.995	200	28914	26.313	ng/ul	-0.02
73) Anthracene-d10	17.751	188	281927	28.022	ng/ul	-0.01
81) Pyrene-d10	20.031	212	332622	25.749	ng/ul	-0.01
92) Benzo(a)pyrene-d12	25.235	264	335247	27.543	ng/ul	-0.02
Target Compounds						
					Qvalue	
86) Bis(2-ethylhexyl)phtha...	21.846	149	592313	85.927	ng/ul#	97
89) Di-n-octyl phthalate	23.162	149	58759	4.716	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051638.D
Acq On : 18 Dec 2021 20:45
Operator : CG/JU
Sample : M5153-10
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL75

Quant Time: Dec 19 00:04:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 14 14:19:57 2021
Response via : Initial Calibration




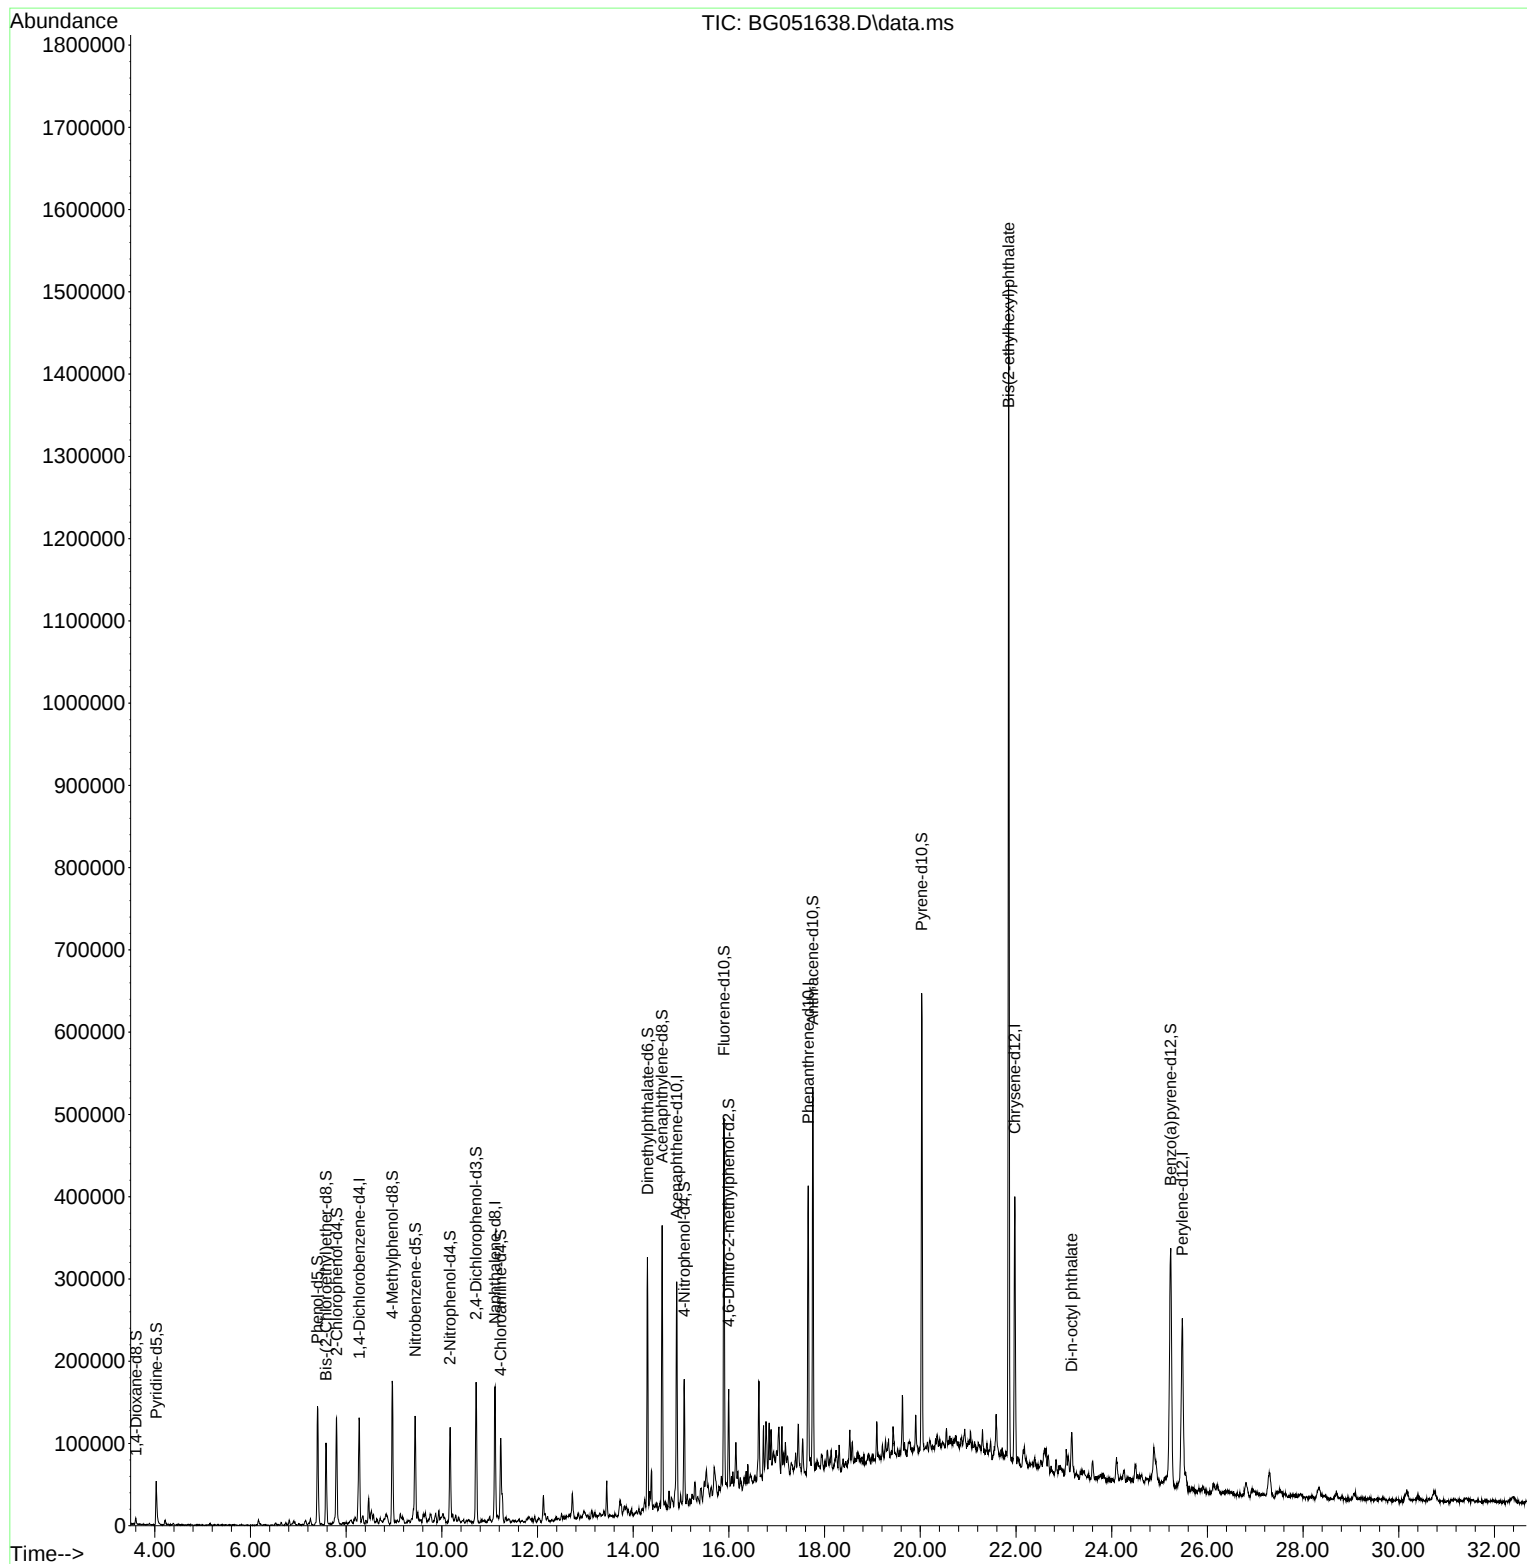


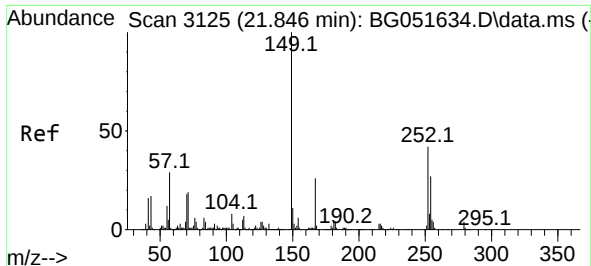

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 85.927 ng/ul
 RT: 21.846 min Scan# 3125
 Delta R.T. -0.022 min
 Lab File: BG051638.D
 Acq: 18 Dec 2021 20:45

Instrument :
 BNA_G
 ClientSampleId :
 BGL75

Tgt Ion:149 Resp: 592313
 Ion Ratio Lower Upper
 149 100
 167 27.6 21.1 31.7
 279 5.0 2.7 4.1#

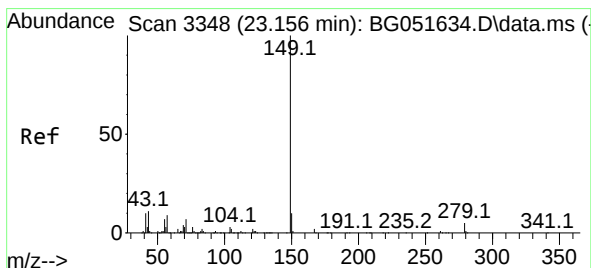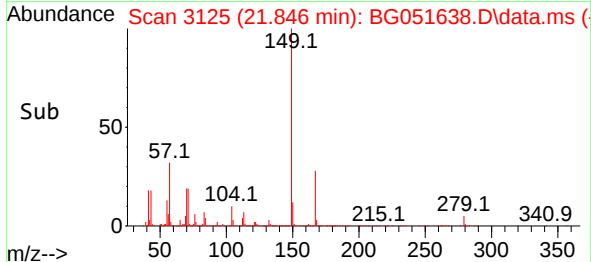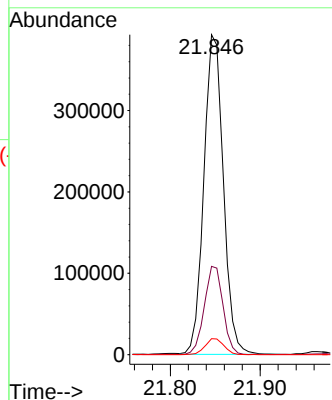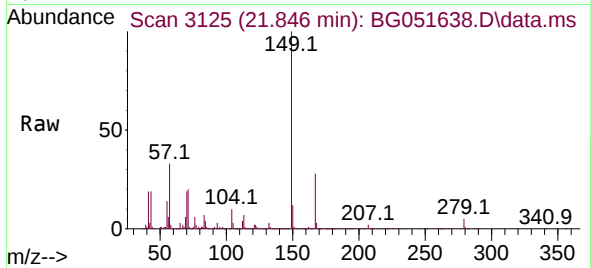

#89
 Di-n-octyl phthalate
 Concen: 4.716 ng/ul
 RT: 23.162 min Scan# 3349
 Delta R.T. -0.023 min
 Lab File: BG051638.D
 Acq: 18 Dec 2021 20:45

Tgt Ion:149 Resp: 58759

