

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051670.D
 Acq On : 19 Dec 2021 19:47
 Operator : CG/JU
 Sample : M5154-12
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL92

Quant Time: Dec 20 00:13:45 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Dec 14 14:19:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.270	152	41605	20.000	ng/u1	-0.02
20) Naphthalene-d8	11.107	136	178170	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.908	164	128829	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.651	188	295350	20.000	ng/u1	#-0.01
79) Chrysene-d12	21.969	240	285994	20.000	ng/u1	#-0.02
88) Perylene-d12	25.464	264	287703	20.000	ng/u1	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.600	96	5203	5.194	ng/uL	0.00
4) Pyridine-d5	4.023	84	59129	19.535	ng/u1	-0.02
7) Phenol-d5	7.400	99	102687	27.643	ng/u1	-0.02
9) Bis-(2-Chloroethyl)eth...	7.577	67	59304	26.854	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.794	132	71569	27.701	ng/u1	-0.02
15) 4-Methylphenol-d8	8.963	113	80085	27.890	ng/u1	-0.02
21) Nitrobenzene-d5	9.439	128	37048	28.362	ng/u1	-0.02
24) 2-Nitrophenol-d4	10.167	143	41410	28.999	ng/u1	-0.02
28) 2,4-Dichlorophenol-d3	10.713	165	80129	25.876	ng/u1	-0.02
31) 4-Chloroaniline-d4	11.230	131	102692	25.187	ng/u1	-0.01
46) Dimethylphthalate-d6	14.297	166	260476	25.261	ng/u1	-0.02
49) Acenaphthylene-d8	14.602	160	327532	25.576	ng/u1	-0.01
54) 4-Nitrophenol-d4	15.066	143	38068	22.702	ng/u1	-0.01
60) Fluorene-d10	15.895	176	229110	24.800	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.995	200	31874	20.714	ng/u1	-0.02
73) Anthracene-d10	17.751	188	367718	26.100	ng/u1	-0.01
81) Pyrene-d10	20.030	212	430875	25.033	ng/u1	-0.01
92) Benzo(a)pyrene-d12	25.223	264	391320	25.850	ng/u1	-0.03
Target Compounds						
					Qvalue	
8) Phenol	7.430	94	5909	1.600	ng/u1#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051670.D
Acq On : 19 Dec 2021 19:47
Operator : CG/JU
Sample : M5154-12
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL92

Quant Time: Dec 20 00:13:45 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 14 14:19:57 2021
Response via : Initial Calibration

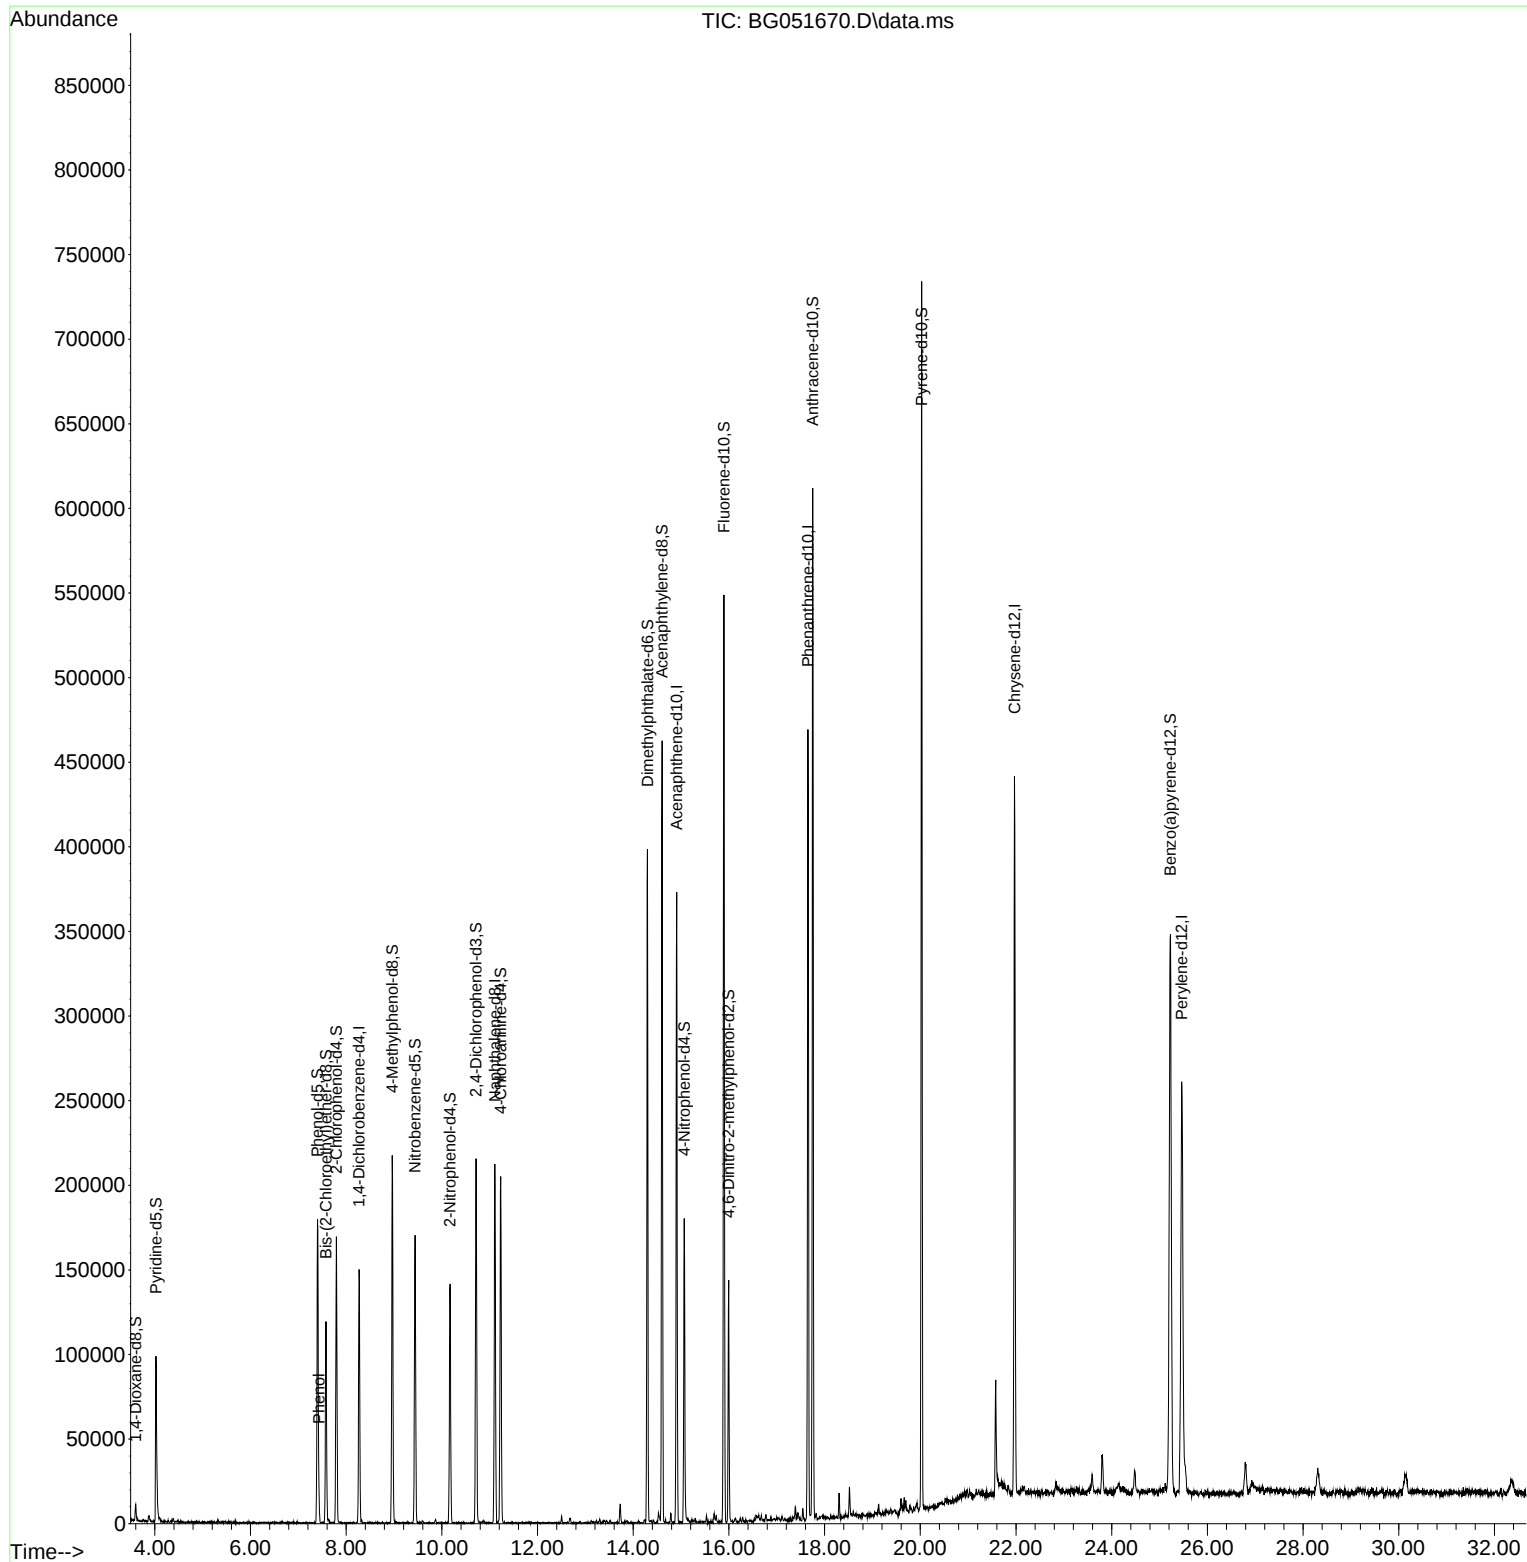

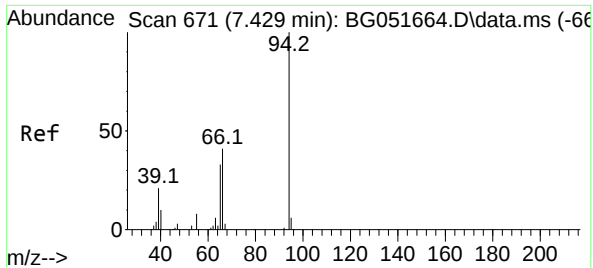

Phenol
 Concen: 1.600 ng/ul
 RT: 7.430 min Scan# 61
 Delta R.T. -0.011 min
 Lab File: BG051670.D
 Acq: 19 Dec 2021 19:47

Instrument :
 BNA_G
 ClientSampleId :
 BGL92

Tgt Ion: 94 Resp: 5909
 Ion Ratio Lower Upper
 94 100
 65 33.7 25.1 37.7
 66 49.8 31.6 47.4#

