

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051589.D
 Acq On : 17 Dec 2021 9:30
 Operator : CG/JU
 Sample : PB141447BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK447

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051589.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.603	15	19	24	rVV2	9150	13755	1.30%	0.142%
2	3.709	35	37	41	rVB3	1328	1632	0.15%	0.017%
3	4.038	89	93	104	rVB	21696	37288	3.53%	0.386%
4	4.385	148	152	158	rBV2	2308	3450	0.33%	0.036%
5	5.078	267	270	273	rBV	945	1122	0.11%	0.012%
6	5.689	371	374	376	rVB	1030	1076	0.10%	0.011%
7	7.404	658	666	674	rBV	162411	270220	25.56%	2.797%
8	7.580	689	696	704	rVB	105163	177890	16.83%	1.841%
9	7.798	726	733	740	rVV	141917	244166	23.09%	2.527%
10	8.273	808	814	822	rVB2	104279	183647	17.37%	1.901%
11	8.767	895	898	901	rBV	755	1202	0.11%	0.012%
12	8.967	925	932	939	rBV	185084	314744	29.77%	3.258%
13	9.442	1004	1013	1021	rBV	141658	253540	23.98%	2.624%
14	10.177	1131	1138	1145	rBV	119240	206984	19.58%	2.142%
15	10.717	1223	1230	1240	rVB	187150	332016	31.40%	3.436%
16	11.117	1288	1298	1305	rVB	149031	267930	25.34%	2.773%
17	11.293	1323	1328	1331	rBV2	645	1207	0.11%	0.012%
18	12.679	1559	1564	1570	rVB3	3379	4973	0.47%	0.051%
19	13.525	1704	1708	1711	rBV2	719	1070	0.10%	0.011%
20	13.895	1766	1771	1776	rBV3	1119	1618	0.15%	0.017%
21	14.301	1833	1840	1847	rVB	374149	540733	51.15%	5.597%
22	14.412	1857	1859	1863	rVB	1323	1164	0.11%	0.012%
23	14.606	1883	1892	1899	rBV	385321	607925	57.50%	6.292%
24	14.911	1937	1944	1951	rBV	252812	394973	37.36%	4.088%
25	15.070	1963	1971	1978	rBV	167754	268323	25.38%	2.777%
26	15.117	1978	1979	1981	rVV	2973	2128	0.20%	0.022%
27	15.898	2103	2112	2120	rVV	504621	765368	72.39%	7.922%
28	15.998	2123	2129	2138	rBV	141491	211916	20.04%	2.193%
29	16.151	2149	2155	2156	rBV3	1547	2476	0.23%	0.026%
30	16.351	2186	2189	2192	rBV2	1164	1540	0.15%	0.016%
31	16.480	2208	2211	2214	rVB4	1164	1242	0.12%	0.013%
32	17.085	2312	2314	2317	rBV	1007	1059	0.10%	0.011%
33	17.185	2328	2331	2333	rBV3	997	1161	0.11%	0.012%
34	17.408	2365	2369	2372	rBV2	920	1388	0.13%	0.014%
35	17.437	2372	2374	2379	rVB2	1604	1953	0.18%	0.020%
36	17.573	2395	2397	2401	rVV4	1267	1271	0.12%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051589.D
 Acq On : 17 Dec 2021 9:30
 Operator : CG/JU
 Sample : PB141447BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK447

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	17.661	2404	2412	2418	rBV	337719	518971	49.09%	5.372%
38	17.755	2422	2428	2438	rVB	574102	885508	83.76%	9.165%
39	17.948	2459	2461	2463	rBV2	1377	1248	0.12%	0.013%
40	18.019	2472	2473	2477	rBV2	1061	1146	0.11%	0.012%
41	18.189	2500	2502	2504	rVB2	1308	1061	0.10%	0.011%
42	18.295	2515	2520	2521	rBV3	1144	1570	0.15%	0.016%
43	18.501	2552	2555	2557	rBV2	2009	1909	0.18%	0.020%
44	18.777	2600	2602	2603	rBV	1784	1209	0.11%	0.013%
45	18.794	2603	2605	2609	rVV4	1598	1479	0.14%	0.015%
46	18.965	2632	2634	2637	rVB3	1777	1864	0.18%	0.019%
47	19.053	2648	2649	2651	rBV2	1998	1460	0.14%	0.015%
48	19.123	2660	2661	2663	rBV	1590	1418	0.13%	0.015%
49	19.159	2665	2667	2669	rBV3	1574	1959	0.19%	0.020%
50	19.294	2688	2690	2694	rBV5	1231	1783	0.17%	0.018%
51	19.405	2707	2709	2710	rBV2	2044	1632	0.15%	0.017%
52	19.540	2730	2732	2734	rVB4	1696	1223	0.12%	0.013%
53	19.599	2737	2742	2745	rBV4	9355	11908	1.13%	0.123%
54	19.664	2750	2753	2758	rBV4	6535	10390	0.98%	0.108%
55	19.905	2792	2794	2795	rBV2	2059	1333	0.13%	0.014%
56	19.922	2795	2797	2798	rVV2	2201	2013	0.19%	0.021%
57	19.958	2801	2803	2805	rVB	2828	1587	0.15%	0.016%
58	19.975	2805	2806	2809	rBV3	2547	2863	0.27%	0.030%
59	20.034	2809	2816	2822	rBV	746666	1057230	100.00%	10.943%
60	20.140	2832	2834	2836	rBV3	2631	1745	0.17%	0.018%
61	20.175	2838	2840	2841	rBV2	1963	1549	0.15%	0.016%
62	20.240	2849	2851	2852	rVB2	2776	1108	0.10%	0.011%
63	20.809	2946	2948	2949	rBV2	4041	2359	0.22%	0.024%
64	21.978	3140	3147	3154	rVB	314206	557593	52.74%	5.771%
65	25.233	3690	3701	3711	rVB2	323450	948190	89.69%	9.814%
66	25.474	3732	3742	3752	rBV	171892	508168	48.07%	5.260%
67	29.821	4480	4482	4484	rBV3	4652	3895	0.37%	0.040%




Sum of corrected areas: 9661521

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051589.D
Acq On : 17 Dec 2021 9:30
Operator : CG/JU
Sample : PB141447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

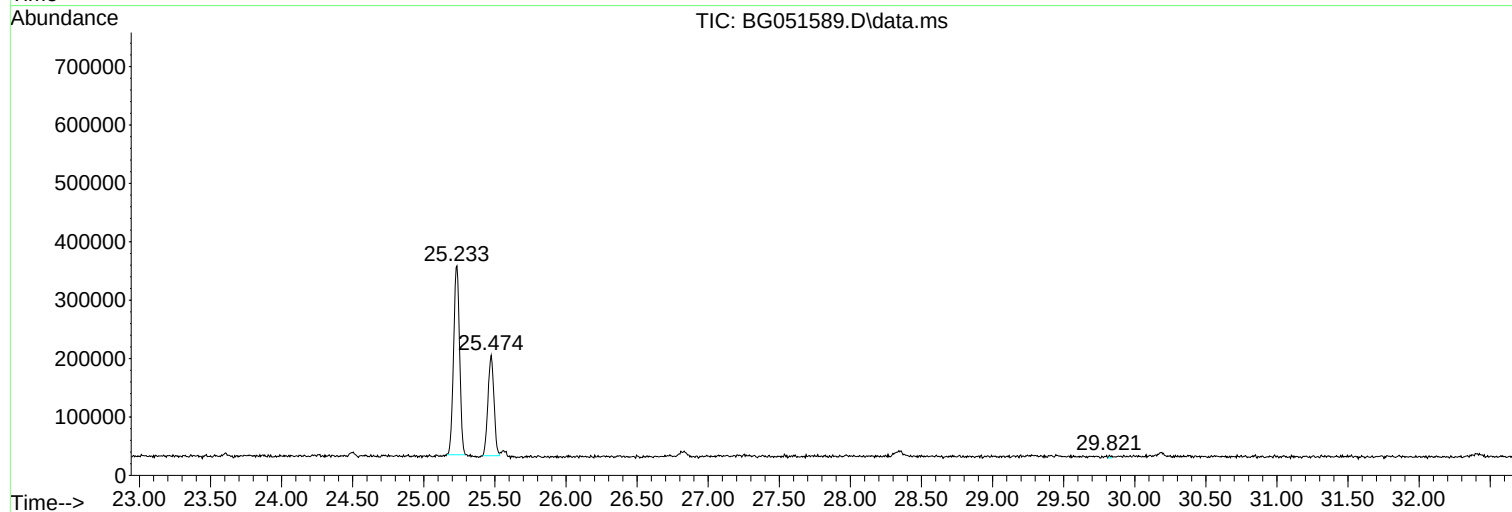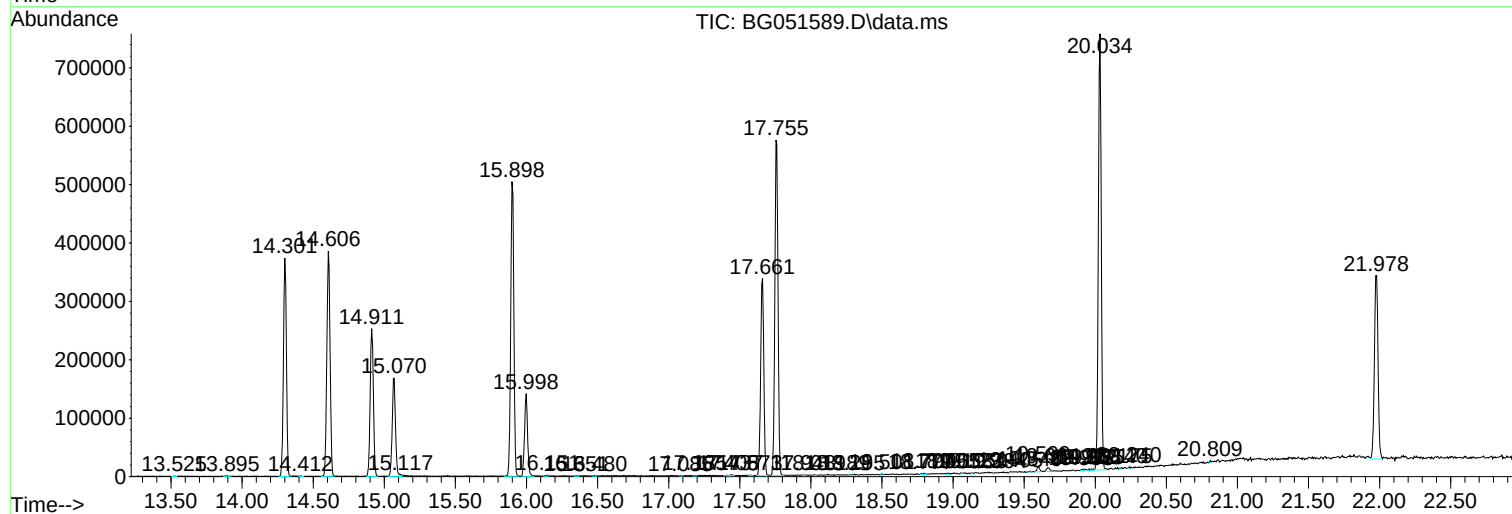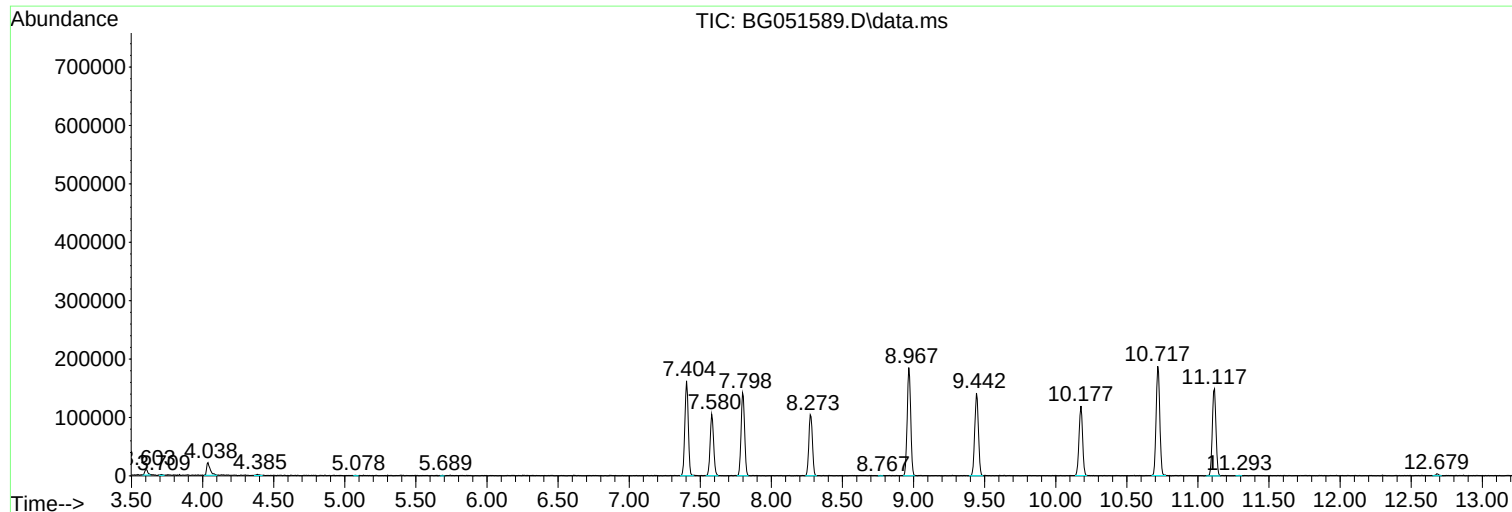

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051589.D
Acq On : 17 Dec 2021 9:30
Operator : CG/JU
Sample : PB141447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051589.D
Acq On : 17 Dec 2021 9:30
Operator : CG/JU
Sample : PB141447BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK447

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc