

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051591.D
 Acq On : 17 Dec 2021 10:51
 Operator : CG/JU
 Sample : M5037-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C00X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051591.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.602	15	19	24	rVV2	7095	11307	1.06%	0.122%
2	3.761	44	46	49	rVB2	1476	1258	0.12%	0.014%
3	4.002	83	87	89	rBV2	1148	1711	0.16%	0.018%
4	4.037	89	93	104	rVV2	14539	26654	2.50%	0.288%
5	4.237	124	127	128	rBV	1316	1410	0.13%	0.015%
6	4.389	148	153	159	rVB5	2808	5132	0.48%	0.055%
7	4.513	170	174	176	rBV3	963	1190	0.11%	0.013%
8	4.642	193	196	199	rVB3	1373	1827	0.17%	0.020%
9	5.482	337	339	342	rVB2	1300	1077	0.10%	0.012%
10	5.552	342	351	356	rBV3	7012	12214	1.15%	0.132%
11	5.993	422	426	430	rVB2	895	1158	0.11%	0.013%
12	6.956	587	590	595	rVB	922	1407	0.13%	0.015%
13	7.403	659	666	674	rVB2	41649	75115	7.06%	0.812%
14	7.579	689	696	706	rVB	99898	162684	15.29%	1.758%
15	7.796	726	733	741	rBV	108885	187186	17.59%	2.022%
16	8.161	792	795	803	rBV3	2484	4140	0.39%	0.045%
17	8.278	808	815	826	rVB	107189	191534	18.00%	2.069%
18	8.965	925	932	939	rBV	106207	177997	16.73%	1.923%
19	9.441	1005	1013	1022	rBV	133656	237420	22.31%	2.565%
20	9.524	1022	1027	1030	rVB	1019	1611	0.15%	0.017%
21	9.876	1084	1087	1092	rVB2	2046	2349	0.22%	0.025%
22	10.176	1127	1138	1148	rBV	108346	186823	17.55%	2.019%
23	10.716	1223	1230	1238	rBV2	161909	283018	26.59%	3.058%
24	10.974	1269	1274	1280	rVB2	11956	19190	1.80%	0.207%
25	11.115	1290	1298	1305	rVB	140063	258169	24.26%	2.789%
26	11.233	1310	1318	1326	rBV	124448	225587	21.20%	2.437%
27	11.503	1360	1364	1368	rVB3	3620	5466	0.51%	0.059%
28	11.879	1423	1428	1429	rBV	842	1180	0.11%	0.013%
29	12.514	1531	1536	1537	rVB2	937	1072	0.10%	0.012%
30	12.678	1561	1564	1568	rBV2	2560	3188	0.30%	0.034%
31	13.154	1640	1645	1648	rBV	1051	1153	0.11%	0.012%
32	13.730	1740	1743	1746	rVV2	1547	1529	0.14%	0.017%
33	14.299	1834	1840	1848	rVB	332749	491368	46.17%	5.309%
34	14.534	1877	1880	1885	rBV2	1177	1350	0.13%	0.015%
35	14.605	1885	1892	1899	rVV	346617	554276	52.08%	5.989%
36	14.910	1937	1944	1951	rVB	252816	387381	36.40%	4.185%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051591.D
 Acq On : 17 Dec 2021 10:51
 Operator : CG/JU
 Sample : M5037-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C00X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	15.063	1964	1970	1976	rVV2	45391	72316	6.80%	0.781%
38	15.286	2005	2008	2010	rBV	995	1293	0.12%	0.014%
39	15.504	2041	2045	2048	rVB2	929	1167	0.11%	0.013%
40	15.698	2074	2078	2081	rBV4	1712	2331	0.22%	0.025%
41	15.897	2105	2112	2123	rVB	482195	735252	69.09%	7.944%
42	15.997	2123	2129	2136	rBV	142829	223531	21.00%	2.415%
43	16.144	2150	2154	2157	rVB3	1948	2078	0.20%	0.022%
44	16.314	2180	2183	2187	rBV2	706	1278	0.12%	0.014%
45	16.461	2207	2208	2213	rVB3	1660	1676	0.16%	0.018%
46	16.579	2222	2228	2229	rVV2	1514	2153	0.20%	0.023%
47	16.596	2229	2231	2233	rVB2	1577	1365	0.13%	0.015%
48	17.137	2319	2323	2324	rBV2	1162	1176	0.11%	0.013%
49	17.331	2350	2356	2357	rBV2	1705	2252	0.21%	0.024%
50	17.395	2363	2367	2370	rBV4	1504	2530	0.24%	0.027%
51	17.554	2389	2394	2397	rVB3	1496	1990	0.19%	0.022%
52	17.589	2397	2400	2402	rVB2	1291	1370	0.13%	0.015%
53	17.654	2404	2411	2420	rBV	349596	522650	49.11%	5.647%
54	17.754	2421	2428	2437	rVV2	597794	896057	84.20%	9.682%
55	18.088	2483	2485	2486	rVB2	1892	1080	0.10%	0.012%
56	18.135	2490	2493	2495	rBV4	1685	1833	0.17%	0.020%
57	18.253	2510	2513	2517	rVB2	1265	1647	0.15%	0.018%
58	18.294	2519	2520	2522	rVV	1233	1255	0.12%	0.014%
59	18.312	2522	2523	2526	rVV2	2810	1927	0.18%	0.021%
60	18.341	2526	2528	2531	rVB2	1376	1070	0.10%	0.012%
61	18.453	2544	2547	2550	rVB4	1729	2244	0.21%	0.024%
62	18.523	2555	2559	2563	rVB4	4527	6205	0.58%	0.067%
63	18.605	2571	2573	2574	rVB2	2309	1584	0.15%	0.017%
64	18.682	2585	2586	2589	rVB	1658	1127	0.11%	0.012%
65	18.735	2593	2595	2598	rBV2	1690	1615	0.15%	0.017%
66	18.817	2607	2609	2612	rBV4	1523	1781	0.17%	0.019%
67	18.952	2630	2632	2635	rBV2	1961	2398	0.23%	0.026%
68	19.064	2649	2651	2657	rVB4	1358	2011	0.19%	0.022%
69	19.163	2666	2668	2669	rBV2	1589	1522	0.14%	0.016%
70	19.205	2673	2675	2678	rVB4	1194	1386	0.13%	0.015%
71	19.263	2684	2685	2687	rBV2	1913	1420	0.13%	0.015%
72	19.410	2708	2710	2712	rBV3	1270	1140	0.11%	0.012%
73	19.439	2713	2715	2716	rVV2	2702	1700	0.16%	0.018%
74	19.457	2716	2718	2719	rVB2	2978	1823	0.17%	0.020%
75	19.545	2731	2733	2736	rBV4	1920	1717	0.16%	0.019%
76	19.598	2739	2742	2746	rVV4	8646	10973	1.03%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051591.D
 Acq On : 17 Dec 2021 10:51
 Operator : CG/JU
 Sample : M5037-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C00X4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	19.663	2751	2753	2757	rVB2	7839	7732	0.73%	0.084%
78	19.745	2765	2767	2769	rBV3	2108	1105	0.10%	0.012%
79	19.821	2777	2780	2781	rBV2	2015	2009	0.19%	0.022%
80	19.968	2804	2805	2809	rBV4	2277	3042	0.29%	0.033%
81	20.033	2809	2816	2822	rVV	754248	1064244	100.00%	11.499%
82	20.080	2822	2824	2825	rVV2	3070	1894	0.18%	0.020%
83	20.097	2825	2827	2829	rVV3	3069	1876	0.18%	0.020%
84	20.115	2829	2830	2832	rVB2	3121	1497	0.14%	0.016%
85	20.162	2836	2838	2840	rBV2	2652	1697	0.16%	0.018%
86	20.227	2848	2849	2851	rBV2	3645	2709	0.25%	0.029%
87	20.685	2926	2927	2928	rBV	3202	1268	0.12%	0.014%
88	21.584	3078	3080	3085	rVB7	9210	12510	1.18%	0.135%
89	21.977	3140	3147	3155	rVB	313157	548742	51.56%	5.929%
90	23.599	3421	3423	3425	rBV3	5905	5907	0.56%	0.064%
91	24.909	3644	3646	3648	rBV3	5111	4031	0.38%	0.044%
92	25.232	3690	3701	3713	rVB	332862	1010623	94.96%	10.919%
93	25.473	3732	3742	3751	rVB	178153	503611	47.32%	5.441%
94	27.012	4002	4004	4007	rBV4	4849	4766	0.45%	0.051%
95	27.728	4124	4126	4128	rBV3	4858	4030	0.38%	0.044%
96	29.884	4491	4493	4495	rBV3	5563	5198	0.49%	0.056%
97	30.166	4536	4541	4543	rBV5	6852	14067	1.32%	0.152%
98	30.795	4646	4648	4650	rBV2	4413	3699	0.35%	0.040%




Sum of corrected areas: 9255311

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051591.D
Acq On : 17 Dec 2021 10:51
Operator : CG/JU
Sample : M5037-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C00X4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

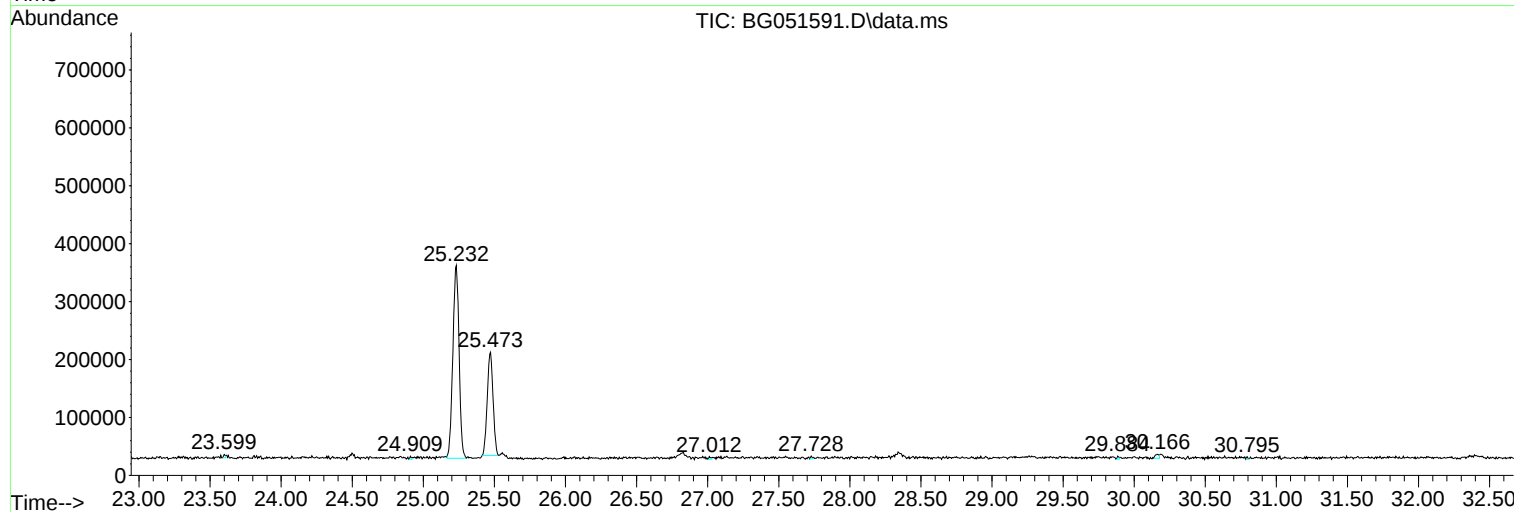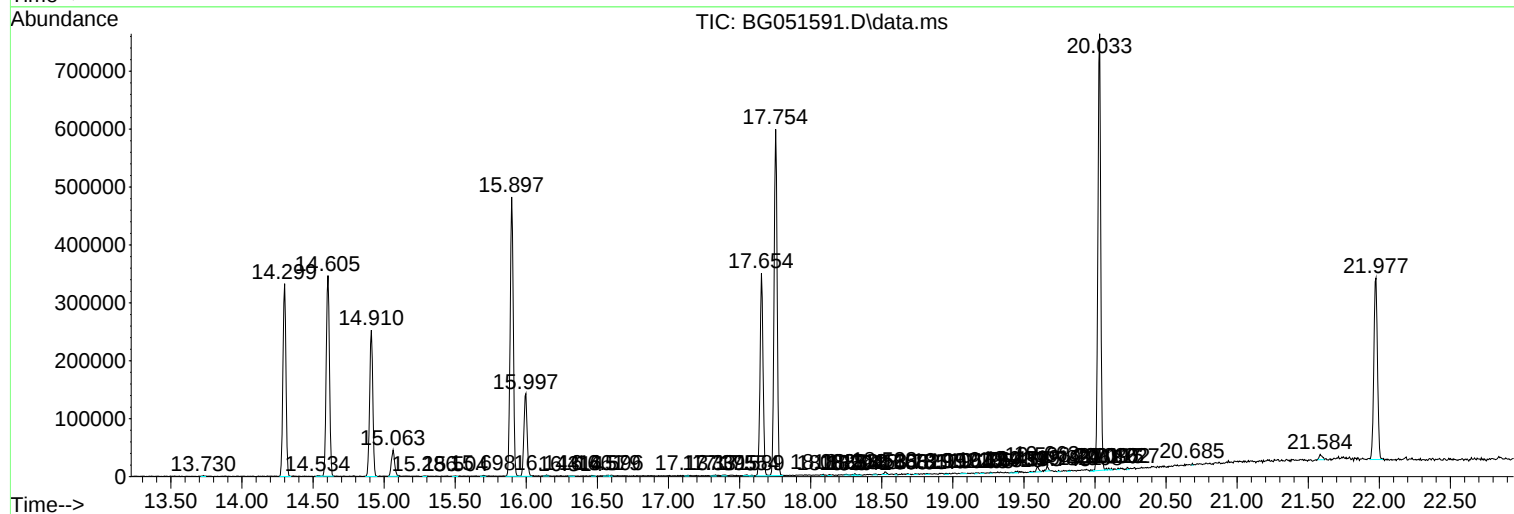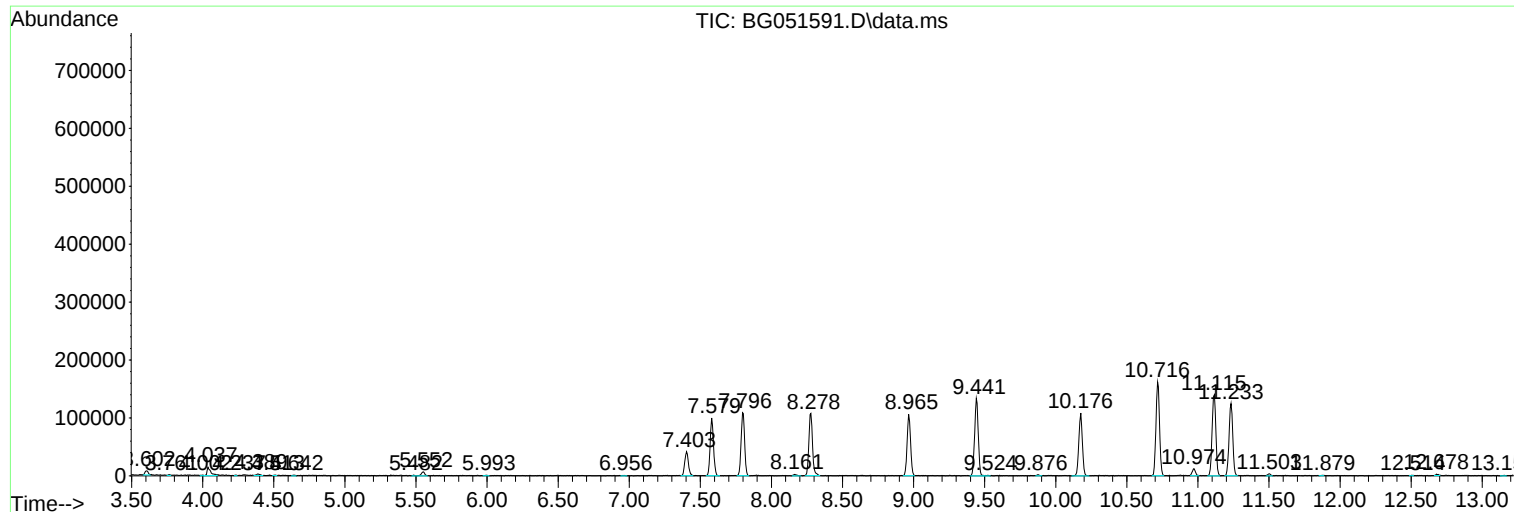

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051591.D
Acq On : 17 Dec 2021 10:51
Operator : CG/JU
Sample : M5037-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C00X4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051591.D
Acq On : 17 Dec 2021 10:51
Operator : CG/JU
Sample : M5037-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C00X4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc