

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051592.D
 Acq On : 17 Dec 2021 11:31
 Operator : CG/JU
 Sample : M5013-02DL3 250X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBLT1DL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051592.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.519	3	5	9	rBV3	851	929	0.15%	0.027%
2	3.602	15	19	20	rBV4	1029	1206	0.20%	0.036%
3	3.901	67	70	72	rBV2	983	1270	0.21%	0.038%
4	4.083	99	101	104	rVB	1176	937	0.15%	0.028%
5	4.136	108	110	112	rBV2	1348	1243	0.20%	0.037%
6	4.383	149	152	159	rVB3	1913	3548	0.58%	0.105%
7	4.583	180	186	187	rBV2	759	966	0.16%	0.029%
8	4.641	193	196	198	rVB	1010	995	0.16%	0.029%
9	4.671	198	201	204	rBV	990	1111	0.18%	0.033%
10	4.700	204	206	209	rBV2	574	814	0.13%	0.024%
11	4.853	230	232	235	rBV2	780	760	0.12%	0.022%
12	4.994	254	256	261	rBV	842	1223	0.20%	0.036%
13	5.029	261	262	267	rVB	691	901	0.15%	0.027%
14	5.199	288	291	294	rBV	690	845	0.14%	0.025%
15	5.323	309	312	316	rBV2	685	933	0.15%	0.028%
16	5.382	321	322	325	rVB	1486	951	0.15%	0.028%
17	5.411	325	327	330	rBV	638	833	0.14%	0.025%
18	5.540	347	349	351	rBB	1130	1017	0.16%	0.030%
19	5.575	351	355	357	rBV	959	1580	0.26%	0.047%
20	5.646	365	367	369	rVB	1018	796	0.13%	0.024%
21	5.875	402	406	407	rBV	648	772	0.13%	0.023%
22	5.951	418	419	424	rVB	941	1081	0.18%	0.032%
23	6.222	464	465	469	rBV	662	804	0.13%	0.024%
24	6.251	469	470	474	rBV2	969	914	0.15%	0.027%
25	6.339	484	485	489	rBV	722	834	0.14%	0.025%
26	6.551	518	521	522	rBV2	993	942	0.15%	0.028%
27	6.797	559	563	564	rBV	639	773	0.13%	0.023%
28	7.085	610	612	615	rVB	843	1024	0.17%	0.030%
29	7.115	615	617	620	rBB	727	875	0.14%	0.026%
30	7.332	651	654	656	rVB	808	812	0.13%	0.024%
31	7.350	656	657	660	rBV	990	999	0.16%	0.029%
32	7.479	675	679	686	rVB2	976	1953	0.32%	0.058%
33	7.549	688	691	694	rBV	596	962	0.16%	0.028%
34	7.725	715	721	722	rVB	737	977	0.16%	0.029%
35	7.919	750	754	756	rBV	1728	1529	0.25%	0.045%
36	8.278	808	815	822	rVB	113931	197200	31.98%	5.823%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051592.D
 Acq On : 17 Dec 2021 11:31
 Operator : CG/JU
 Sample : M5013-02DL3 250X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBLT1DL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	8.659	876	880	885	rVB2	4538	7017	1.14%	0.207%
38	9.482	1017	1020	1021	rBV2	1060	808	0.13%	0.024%
39	9.852	1081	1083	1086	rBV2	760	835	0.14%	0.025%
40	10.392	1169	1175	1177	rBV	582	1202	0.19%	0.035%
41	10.516	1194	1196	1201	rVB2	1229	1740	0.28%	0.051%
42	10.721	1227	1231	1234	rBV	904	1371	0.22%	0.040%
43	10.986	1274	1276	1279	rBV	1145	800	0.13%	0.024%
44	11.115	1290	1298	1302	rBV	155578	290632	47.14%	8.582%
45	11.168	1302	1307	1315	rVB	247660	453019	73.47%	13.377%
46	11.279	1322	1326	1331	rBV2	2386	4283	0.69%	0.126%
47	11.814	1414	1417	1419	rBV	776	812	0.13%	0.024%
48	11.949	1435	1440	1444	rVB2	463	910	0.15%	0.027%
49	12.249	1488	1491	1492	rBV	1126	977	0.16%	0.029%
50	12.384	1510	1514	1517	rBV2	532	788	0.13%	0.023%
51	12.472	1523	1529	1533	rVB3	3463	4501	0.73%	0.133%
52	12.754	1571	1577	1586	rVB	28871	49240	7.99%	1.454%
53	12.924	1602	1606	1607	rBB	1220	1278	0.21%	0.038%
54	12.971	1607	1614	1622	rBV	16221	26189	4.25%	0.773%
55	13.347	1676	1678	1684	rBV2	698	1235	0.20%	0.036%
56	13.659	1728	1731	1733	rBV2	676	790	0.13%	0.023%
57	13.747	1739	1746	1751	rBV2	9188	15043	2.44%	0.444%
58	14.087	1800	1804	1806	rBV	870	1090	0.18%	0.032%
59	14.228	1825	1828	1830	rVB2	1305	1234	0.20%	0.036%
60	14.281	1834	1837	1838	rVV2	1489	1184	0.19%	0.035%
61	14.305	1838	1841	1843	rVB	1428	1531	0.25%	0.045%
62	14.358	1848	1850	1854	rVB2	793	877	0.14%	0.026%
63	14.475	1869	1870	1873	rBV	920	950	0.15%	0.028%
64	14.540	1878	1881	1884	rVB	590	874	0.14%	0.026%
65	14.610	1889	1893	1900	rVB3	1851	3390	0.55%	0.100%
66	14.910	1938	1944	1952	rVV	264469	425036	68.93%	12.551%
67	14.980	1952	1956	1959	rVB2	1404	1649	0.27%	0.049%
68	15.033	1960	1965	1969	rBV2	4859	6462	1.05%	0.191%
69	15.080	1971	1973	1976	rVB	816	983	0.16%	0.029%
70	15.303	2006	2011	2016	rVB	18877	28751	4.66%	0.849%
71	15.556	2051	2054	2057	rBV2	921	1264	0.20%	0.037%
72	15.685	2072	2076	2079	rVB2	492	878	0.14%	0.026%
73	15.897	2108	2112	2119	rBV2	2171	3828	0.62%	0.113%
74	15.956	2119	2122	2127	rVB4	1291	2162	0.35%	0.064%
75	16.055	2137	2139	2141	rVB	953	859	0.14%	0.025%
76	16.085	2141	2144	2146	rBV2	977	1288	0.21%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051592.D
 Acq On : 17 Dec 2021 11:31
 Operator : CG/JU
 Sample : M5013-02DL3 250X
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBLT1DL3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	16.202	2159	2164	2166	rBV2	923	1243	0.20%	0.037%
78	16.378	2191	2194	2198	rBV3	812	1071	0.17%	0.032%
79	16.490	2210	2213	2215	rBV2	971	913	0.15%	0.027%
80	16.625	2229	2236	2239	rBV4	1826	2934	0.48%	0.087%
81	16.796	2262	2265	2268	rVB	1147	1652	0.27%	0.049%
82	16.819	2268	2269	2271	rBV	1332	1096	0.18%	0.032%
83	16.960	2290	2293	2295	rBV2	798	758	0.12%	0.022%
84	17.119	2318	2320	2323	rBV2	724	923	0.15%	0.027%
85	17.177	2326	2330	2331	rVB3	883	1034	0.17%	0.031%
86	17.301	2346	2351	2357	rVB3	5345	7994	1.30%	0.236%
87	17.424	2369	2372	2373	rBV3	1156	1203	0.20%	0.036%
88	17.442	2373	2375	2379	rVB2	1484	1788	0.29%	0.053%
89	17.559	2393	2395	2400	rBV3	741	1164	0.19%	0.034%
90	17.659	2405	2412	2418	rBV	364216	577758	93.70%	17.060%
91	17.753	2424	2428	2433	rBV3	4182	5491	0.89%	0.162%
92	17.947	2460	2461	2464	rVB2	1126	868	0.14%	0.026%
93	18.041	2475	2477	2478	rBV2	1029	1040	0.17%	0.031%
94	18.129	2487	2492	2495	rBV4	1158	2126	0.34%	0.063%
95	18.341	2525	2528	2531	rVB3	2113	2191	0.36%	0.065%
96	18.388	2534	2536	2537	rBV2	1631	1338	0.22%	0.040%
97	18.805	2605	2607	2608	rBV2	1854	981	0.16%	0.029%
98	19.069	2650	2652	2654	rVB2	1748	841	0.14%	0.025%
99	21.977	3140	3147	3153	rVB2	345499	616591	100.00%	18.207%
100	25.472	3732	3742	3752	rVB	194935	570518	92.53%	16.846%




Sum of corrected areas: 3386585

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051592.D
Acq On : 17 Dec 2021 11:31
Operator : CG/JU
Sample : M5013-02DL3 250X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBLT1DL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

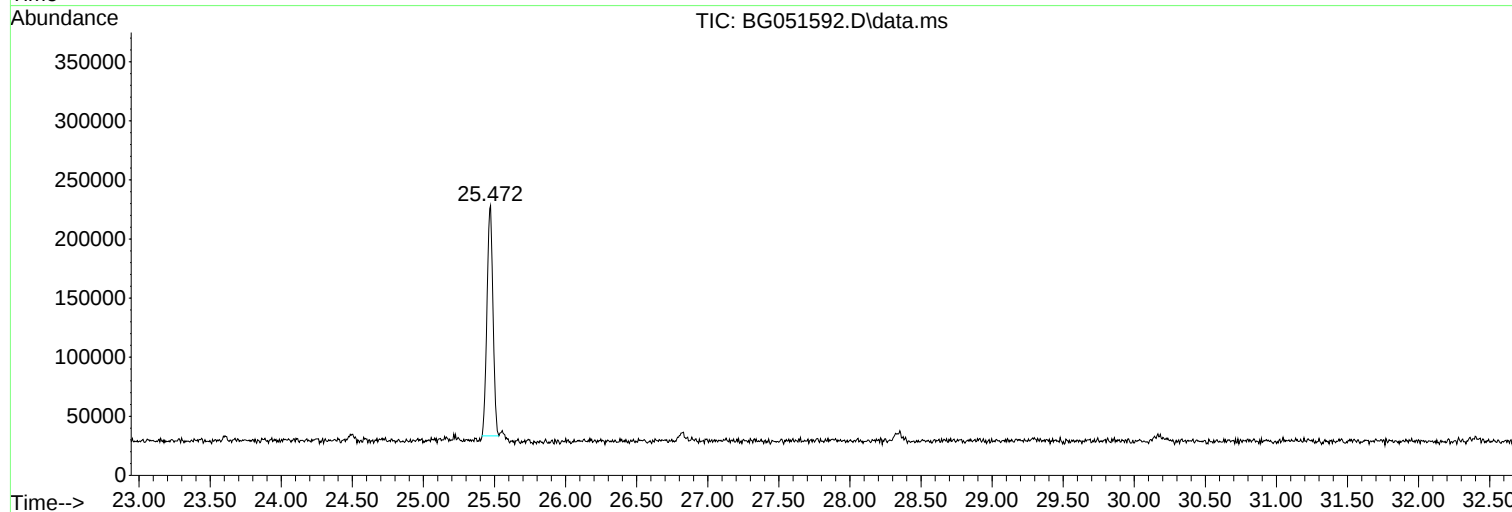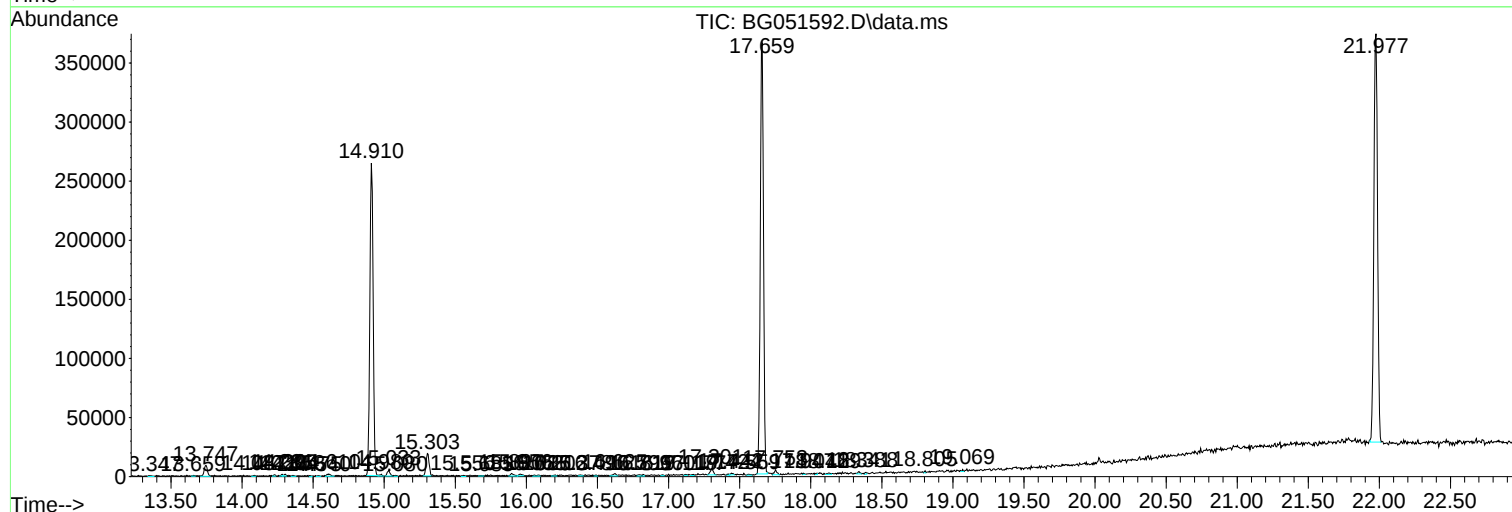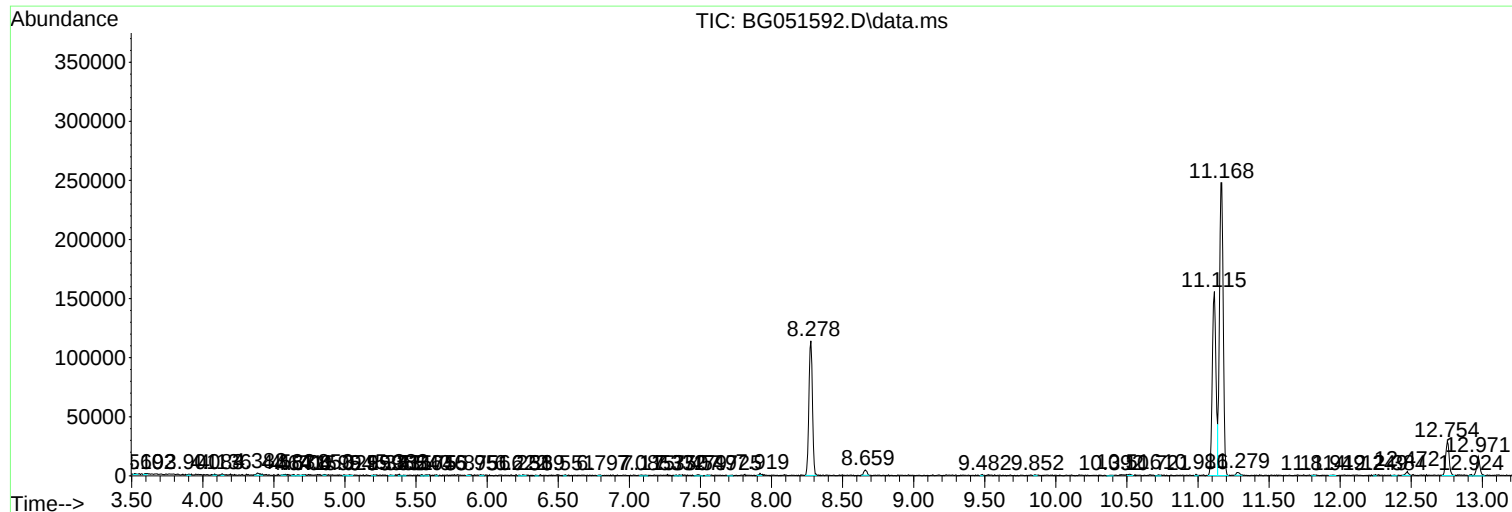

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051592.D
Acq On : 17 Dec 2021 11:31
Operator : CG/JU
Sample : M5013-02DL3 250X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBLT1DL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051592.D
Acq On : 17 Dec 2021 11:31
Operator : CG/JU
Sample : M5013-02DL3 250X
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBLT1DL3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc