

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051594.D
 Acq On : 17 Dec 2021 12:53
 Operator : CG/JU
 Sample : M5037-14
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C00X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051594.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.602	14	19	25	rVB2	9154	14455	1.20%	0.140%
2	3.673	25	31	35	rBV4	1055	2397	0.20%	0.023%
3	4.037	89	93	104	rBV	24055	44401	3.69%	0.431%
4	4.284	130	135	139	rBV4	2074	2516	0.21%	0.024%
5	4.378	147	151	154	rBV2	1806	2302	0.19%	0.022%
6	4.736	210	212	216	rVB2	1267	1604	0.13%	0.016%
7	4.801	220	223	225	rBV2	1374	1487	0.12%	0.014%
8	5.324	309	312	315	rVB2	2122	1907	0.16%	0.019%
9	5.747	380	384	389	rVV	770	1260	0.10%	0.012%
10	6.299	476	478	481	rBV	1183	1264	0.11%	0.012%
11	7.315	648	651	654	rVB	1087	1301	0.11%	0.013%
12	7.403	658	666	673	rBV3	44370	76544	6.37%	0.743%
13	7.579	690	696	705	rBV	108700	183219	15.24%	1.778%
14	7.797	724	733	741	rVB	119938	205840	17.12%	1.998%
15	8.079	779	781	785	rBV	991	1232	0.10%	0.012%
16	8.273	807	814	821	rBV	120726	212587	17.68%	2.063%
17	8.502	848	853	855	rBV	971	1669	0.14%	0.016%
18	8.966	925	932	939	rBV2	106744	181479	15.09%	1.761%
19	9.442	1005	1013	1021	rBV	147270	256412	21.32%	2.489%
20	9.547	1029	1031	1034	rBV	1199	1355	0.11%	0.013%
21	10.176	1130	1138	1146	rBV	113160	200919	16.71%	1.950%
22	10.716	1222	1230	1237	rBV	179092	307299	25.55%	2.983%
23	11.110	1289	1297	1305	rBV	163376	297243	24.72%	2.885%
24	11.233	1310	1318	1326	rVB	136928	249735	20.77%	2.424%
25	12.684	1559	1565	1571	rBV3	2694	4344	0.36%	0.042%
26	13.489	1697	1702	1705	rBV2	1234	1980	0.16%	0.019%
27	13.513	1705	1706	1711	rVV	989	1256	0.10%	0.012%
28	14.123	1808	1810	1814	rBV2	934	1545	0.13%	0.015%
29	14.300	1834	1840	1846	rBV	379187	540221	44.92%	5.243%
30	14.605	1885	1892	1902	rVB	400461	609932	50.72%	5.920%
31	14.911	1936	1944	1951	rVB	284763	448205	37.27%	4.350%
32	15.063	1962	1970	1976	rBV2	48712	77666	6.46%	0.754%
33	15.222	1994	1997	1999	rBV	1672	1579	0.13%	0.015%
34	15.316	2010	2013	2017	rVB	975	1251	0.10%	0.012%
35	15.698	2074	2078	2081	rBV3	1468	1819	0.15%	0.018%
36	15.898	2105	2112	2120	rBV	530199	796423	66.23%	7.730%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051594.D
 Acq On : 17 Dec 2021 12:53
 Operator : CG/JU
 Sample : M5037-14
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C00X6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	15.992	2122	2128	2136	rBV	152273	235766	19.61%	2.288%
38	16.133	2149	2152	2156	rBV2	1570	2181	0.18%	0.021%
39	16.679	2244	2245	2250	rVB2	2161	1626	0.14%	0.016%
40	16.884	2277	2280	2283	rBV3	1103	1626	0.14%	0.016%
41	16.926	2283	2287	2289	rBV	1126	1405	0.12%	0.014%
42	17.190	2330	2332	2334	rVB3	1727	1417	0.12%	0.014%
43	17.396	2365	2367	2371	rVB3	1896	1448	0.12%	0.014%
44	17.437	2371	2374	2376	rVV	1685	1606	0.13%	0.016%
45	17.478	2378	2381	2386	rVB4	1058	1498	0.12%	0.015%
46	17.654	2404	2411	2421	rBV	390060	593568	49.36%	5.761%
47	17.754	2421	2428	2435	rBV2	643427	986652	82.05%	9.576%
48	18.018	2470	2473	2476	rBV2	1395	1779	0.15%	0.017%
49	18.095	2484	2486	2488	rVB3	1683	1374	0.11%	0.013%
50	18.142	2491	2494	2497	rBV5	1563	2053	0.17%	0.020%
51	18.212	2503	2506	2507	rVV3	1918	1787	0.15%	0.017%
52	18.312	2519	2523	2526	rVV3	3051	4715	0.39%	0.046%
53	18.441	2540	2545	2549	rVB3	1340	2307	0.19%	0.022%
54	18.482	2549	2552	2554	rBV3	1897	2247	0.19%	0.022%
55	18.518	2554	2558	2563	rBV4	10818	17714	1.47%	0.172%
56	18.594	2567	2571	2575	rBV4	2015	3241	0.27%	0.031%
57	18.659	2581	2582	2584	rBV	1669	1462	0.12%	0.014%
58	18.800	2603	2606	2607	rBV2	1076	1240	0.10%	0.012%
59	18.940	2627	2630	2631	rVV2	1786	1666	0.14%	0.016%
60	18.982	2635	2637	2640	rVB4	1106	1214	0.10%	0.012%
61	19.140	2659	2664	2665	rBV5	2447	4036	0.34%	0.039%
62	19.199	2671	2674	2675	rBV2	3060	2282	0.19%	0.022%
63	19.234	2678	2680	2682	rBV3	2054	1322	0.11%	0.013%
64	19.264	2682	2685	2687	rBV3	2004	2190	0.18%	0.021%
65	19.358	2698	2701	2703	rBV3	1935	2097	0.17%	0.020%
66	19.375	2703	2704	2708	rVB2	1650	1474	0.12%	0.014%
67	19.410	2708	2710	2711	rBV	1756	1465	0.12%	0.014%
68	19.487	2722	2723	2725	rBV2	2316	1433	0.12%	0.014%
69	19.504	2725	2726	2729	rVB2	2120	1476	0.12%	0.014%
70	19.598	2739	2742	2748	rVB5	9339	13714	1.14%	0.133%
71	19.663	2748	2753	2757	rBV2	10386	16744	1.39%	0.163%
72	19.698	2757	2759	2760	rBV2	2093	1425	0.12%	0.014%
73	19.786	2770	2774	2775	rBV4	6138	6325	0.53%	0.061%
74	19.875	2787	2789	2791	rBV3	2283	2217	0.18%	0.022%
75	19.986	2807	2808	2809	rBV	2936	1604	0.13%	0.016%
76	20.033	2809	2816	2823	rVV	827959	1202555	100.00%	11.672%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051594.D
 Acq On : 17 Dec 2021 12:53
 Operator : CG/JU
 Sample : M5037-14
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C00X6

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	20.292	2858	2860	2861	rBV	2886	1761	0.15%	0.017%
78	20.403	2876	2879	2880	rBV2	4144	3658	0.30%	0.036%
79	20.574	2906	2908	2910	rVB2	3807	2362	0.20%	0.023%
80	20.867	2956	2958	2959	rBV2	4039	2742	0.23%	0.027%
81	21.578	3075	3079	3083	rBV5	16002	28138	2.34%	0.273%
82	21.972	3140	3146	3153	rVB2	361415	655493	54.51%	6.362%
83	23.564	3413	3417	3419	rBV3	8563	12185	1.01%	0.118%
84	25.232	3689	3701	3711	rVB2	378095	1112590	92.52%	10.798%
85	25.473	3732	3742	3752	rBV3	209215	601076	49.98%	5.834%
86	27.605	4103	4105	4107	rBV3	5447	4470	0.37%	0.043%
87	28.921	4327	4329	4332	rBV3	5308	4684	0.39%	0.045%
88	31.324	4736	4738	4739	rBV2	5139	3482	0.29%	0.034%




Sum of corrected areas: 10303240

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051594.D
Acq On : 17 Dec 2021 12:53
Operator : CG/JU
Sample : M5037-14
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C00X6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

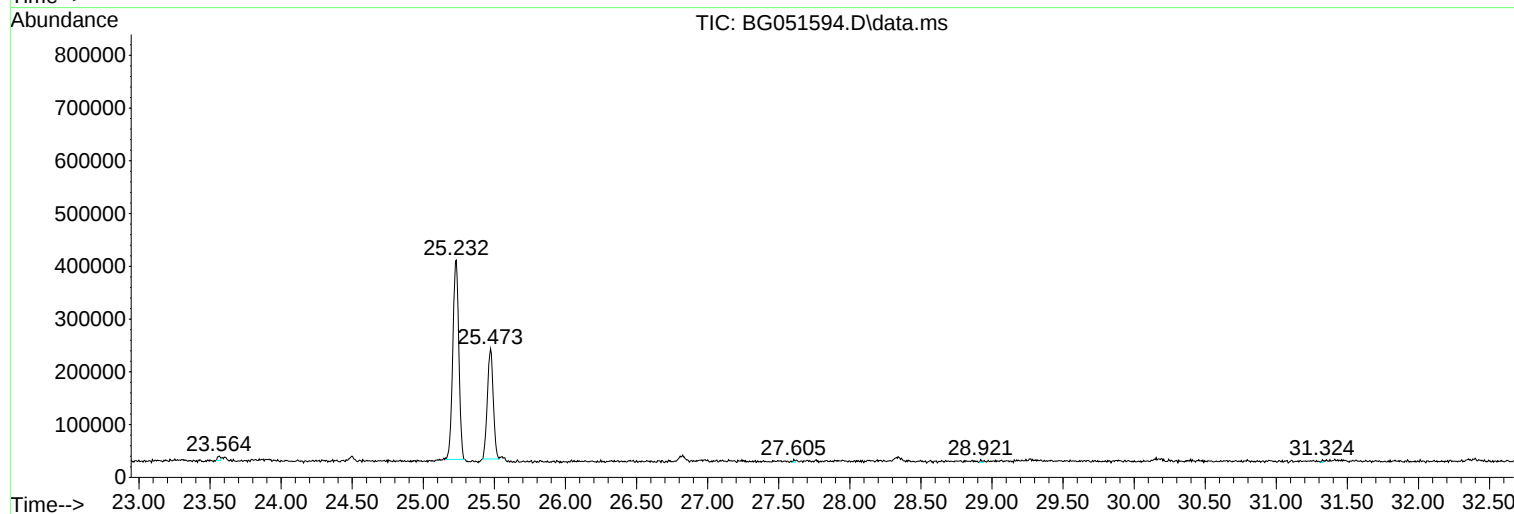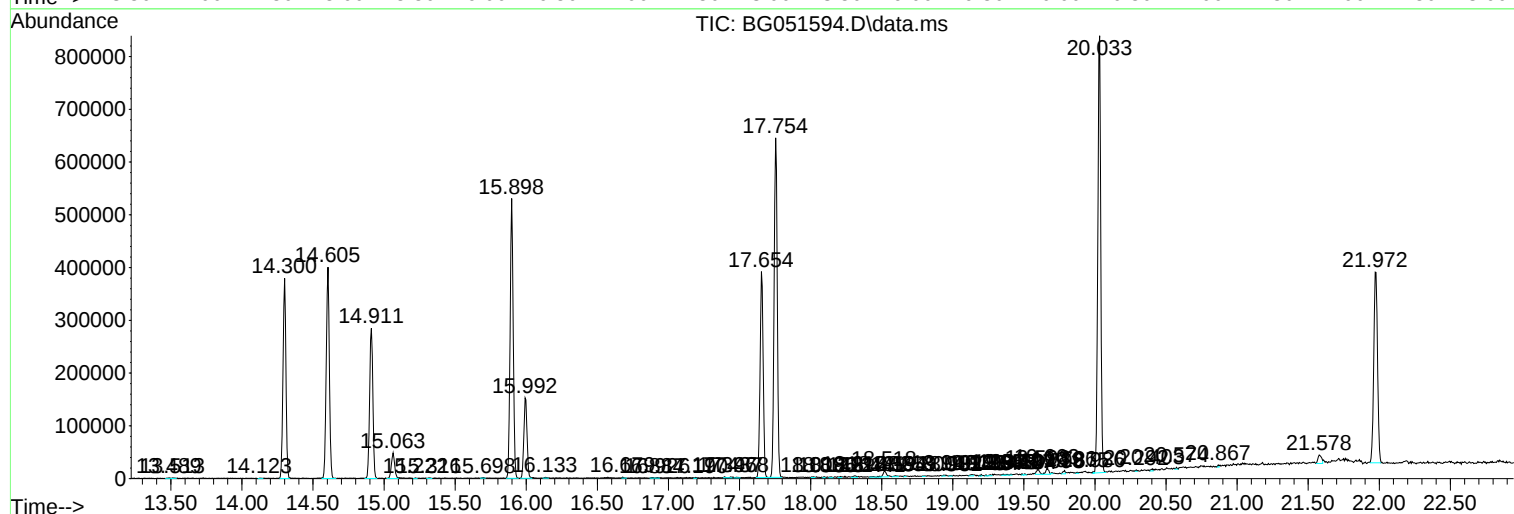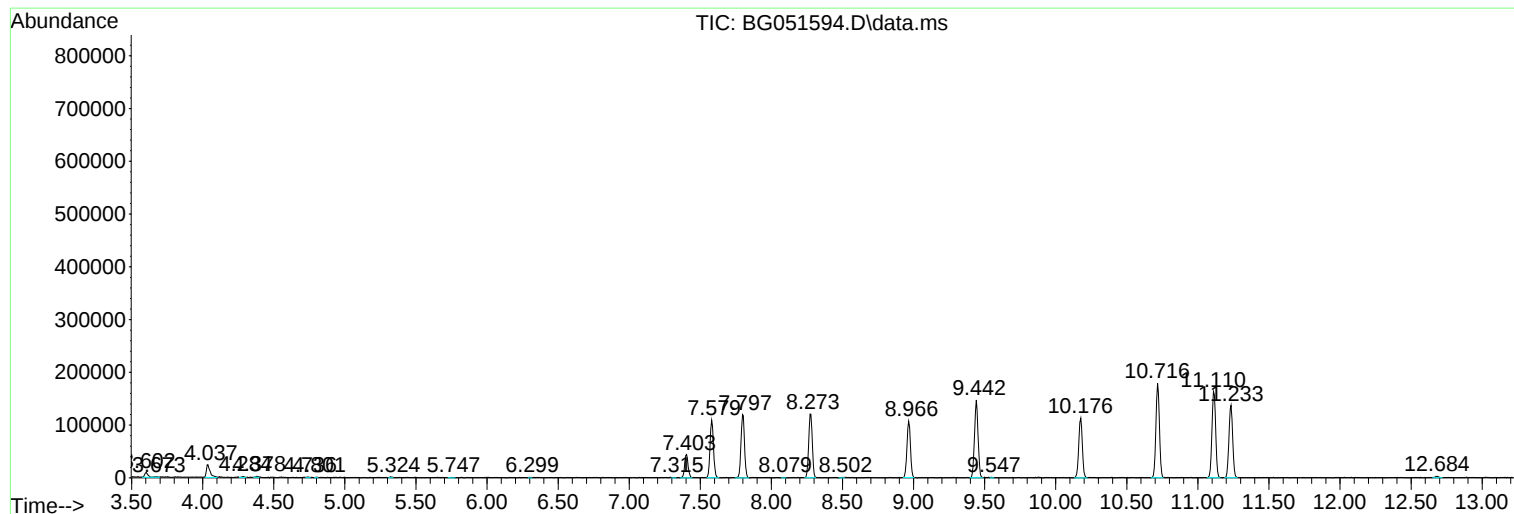

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051594.D
Acq On : 17 Dec 2021 12:53
Operator : CG/JU
Sample : M5037-14
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C00X6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051594.D
Acq On : 17 Dec 2021 12:53
Operator : CG/JU
Sample : M5037-14
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C00X6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc