

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051604.D
 Acq On : 17 Dec 2021 20:23
 Operator : CG/JU
 Sample : PB141493BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK493

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051604.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.526	3	6	9	rVB3	1029	1497	0.15%	0.015%
2	3.603	14	19	25	rBV4	8111	13913	1.38%	0.143%
3	3.697	33	35	38	rVV2	953	1011	0.10%	0.010%
4	3.761	42	46	49	rVB4	994	1100	0.11%	0.011%
5	3.996	82	86	87	rVB2	1413	1779	0.18%	0.018%
6	4.031	87	92	103	rBV	72119	127200	12.59%	1.309%
7	4.313	138	140	144	rVB	900	1109	0.11%	0.011%
8	4.384	148	152	159	rVB3	3435	5443	0.54%	0.056%
9	4.619	189	192	195	rVB2	1029	1227	0.12%	0.013%
10	4.666	195	200	203	rBV3	1296	1913	0.19%	0.020%
11	5.136	279	280	284	rVB	1484	1381	0.14%	0.014%
12	7.403	658	666	674	rBV	147465	250550	24.80%	2.578%
13	7.580	688	696	705	rVB	97834	169570	16.79%	1.745%
14	7.797	726	733	740	rBV	133682	227738	22.54%	2.343%
15	8.273	808	814	824	rVB	111247	189112	18.72%	1.946%
16	8.966	924	932	941	rVB2	170285	297573	29.46%	3.062%
17	9.283	984	986	991	rBV2	766	1097	0.11%	0.011%
18	9.442	1003	1013	1021	rVB	138147	242877	24.04%	2.499%
19	10.006	1105	1109	1111	rBV2	884	1031	0.10%	0.011%
20	10.176	1130	1138	1145	rVB2	108796	196887	19.49%	2.026%
21	10.405	1174	1177	1180	rBV	873	1194	0.12%	0.012%
22	10.716	1222	1230	1237	rBV	176203	306820	30.37%	3.157%
23	11.110	1290	1297	1307	rVB	149037	268672	26.60%	2.764%
24	11.228	1310	1317	1327	rBV	106647	198078	19.61%	2.038%
25	12.684	1558	1565	1568	rBV2	2689	4775	0.47%	0.049%
26	13.096	1628	1635	1638	rBV2	715	1395	0.14%	0.014%
27	13.195	1648	1652	1653	rBV	872	1091	0.11%	0.011%
28	13.366	1677	1681	1684	rBV	628	1020	0.10%	0.010%
29	13.877	1765	1768	1772	rVB	836	1024	0.10%	0.011%
30	14.300	1833	1840	1846	rBV	347399	498562	49.35%	5.130%
31	14.605	1885	1892	1900	rVB	360999	571538	56.58%	5.881%
32	14.911	1936	1944	1951	rVB	257284	405147	40.11%	4.169%
33	15.064	1964	1970	1977	rBV	165419	258345	25.57%	2.658%
34	15.216	1992	1996	1999	rVB3	802	1235	0.12%	0.013%
35	15.263	1999	2004	2006	rBV2	762	1175	0.12%	0.012%
36	15.898	2105	2112	2119	rVV	491687	723115	71.58%	7.440%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051604.D
 Acq On : 17 Dec 2021 20:23
 Operator : CG/JU
 Sample : PB141493BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK493

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	15.992	2122	2128	2139	rBV	139712	210644	20.85%	2.167%
38	16.133	2149	2152	2155	rVB2	2002	2236	0.22%	0.023%
39	16.215	2164	2166	2169	rVB2	1162	1064	0.11%	0.011%
40	16.667	2241	2243	2245	rBV2	1088	1070	0.11%	0.011%
41	16.820	2268	2269	2271	rBV	1425	1220	0.12%	0.013%
42	17.296	2345	2350	2353	rBV2	1336	1741	0.17%	0.018%
43	17.384	2362	2365	2368	rVB	812	1118	0.11%	0.012%
44	17.431	2370	2373	2375	rVV3	1338	1579	0.16%	0.016%
45	17.454	2375	2377	2379	rVB	1177	1187	0.12%	0.012%
46	17.531	2388	2390	2394	rVV3	1027	1199	0.12%	0.012%
47	17.607	2398	2403	2405	rBV3	1216	1891	0.19%	0.019%
48	17.654	2405	2411	2420	rVV	357334	529862	52.45%	5.452%
49	17.754	2421	2428	2435	rVV	534142	836521	82.81%	8.607%
50	17.965	2463	2464	2466	rBV	1319	1024	0.10%	0.011%
51	18.018	2470	2473	2476	rBV4	1656	1829	0.18%	0.019%
52	18.077	2479	2483	2485	rBV3	1525	1716	0.17%	0.018%
53	18.177	2496	2500	2503	rBV3	1173	1738	0.17%	0.018%
54	18.236	2507	2510	2512	rBV4	1103	1369	0.14%	0.014%
55	18.259	2512	2514	2516	rVB2	1383	1093	0.11%	0.011%
56	18.377	2531	2534	2538	rBV3	1214	1797	0.18%	0.018%
57	18.412	2538	2540	2543	rVB3	1765	2019	0.20%	0.021%
58	18.594	2570	2571	2573	rBV2	1881	1240	0.12%	0.013%
59	18.794	2603	2605	2608	rVB3	1454	1345	0.13%	0.014%
60	18.841	2610	2613	2615	rBV4	1356	1890	0.19%	0.019%
61	18.870	2615	2618	2620	rVB4	1140	1129	0.11%	0.012%
62	18.905	2620	2624	2629	rBV4	1496	3072	0.30%	0.032%
63	19.093	2653	2656	2657	rVB3	1663	1218	0.12%	0.013%
64	19.117	2659	2660	2663	rBV3	1306	1307	0.13%	0.013%
65	19.158	2665	2667	2670	rBV2	1478	1296	0.13%	0.013%
66	19.240	2679	2681	2684	rBV4	2016	2354	0.23%	0.024%
67	19.270	2684	2686	2688	rBV2	1539	1659	0.16%	0.017%
68	19.358	2699	2701	2706	rBV6	1743	2254	0.22%	0.023%
69	19.411	2708	2710	2712	rBV3	1571	1402	0.14%	0.014%
70	19.428	2712	2713	2716	rVV3	1987	2263	0.22%	0.023%
71	19.481	2720	2722	2724	rVB3	1207	1025	0.10%	0.011%
72	19.599	2738	2742	2745	rVB2	7346	9077	0.90%	0.093%
73	19.663	2748	2753	2756	rBV3	7421	12263	1.21%	0.126%
74	19.816	2777	2779	2780	rVB2	2232	1297	0.13%	0.013%
75	20.027	2809	2815	2821	rBV	736623	1010211	100.00%	10.395%
76	20.204	2844	2845	2848	rBV2	2669	2116	0.21%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051604.D
 Acq On : 17 Dec 2021 20:23
 Operator : CG/JU
 Sample : PB141493BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK493

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	20.362	2870	2872	2874	rBV3	2279	1717	0.17%	0.018%
78	20.409	2878	2880	2881	rBV2	2662	1538	0.15%	0.016%
79	20.533	2899	2901	2902	rBV2	3230	1711	0.17%	0.018%
80	20.691	2926	2928	2929	rBV	3485	3319	0.33%	0.034%
81	21.055	2988	2990	2995	rBV5	4321	6577	0.65%	0.068%
82	21.091	2995	2996	2997	rBV	3384	1328	0.13%	0.014%
83	21.108	2997	2999	3002	rBV3	3910	3212	0.32%	0.033%
84	21.273	3025	3027	3029	rBV3	4046	3357	0.33%	0.035%
85	21.972	3139	3146	3155	rVB	342568	580647	57.48%	5.975%
86	25.226	3689	3700	3713	rVB	326552	944512	93.50%	9.719%
87	25.467	3731	3741	3751	rBV2	170982	522426	51.71%	5.375%
88	27.459	4078	4080	4082	rBV2	4740	4339	0.43%	0.045%
89	29.990	4509	4511	4513	rBV3	4773	4452	0.44%	0.046%




Sum of corrected areas: 9718664

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051604.D
Acq On : 17 Dec 2021 20:23
Operator : CG/JU
Sample : PB141493BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

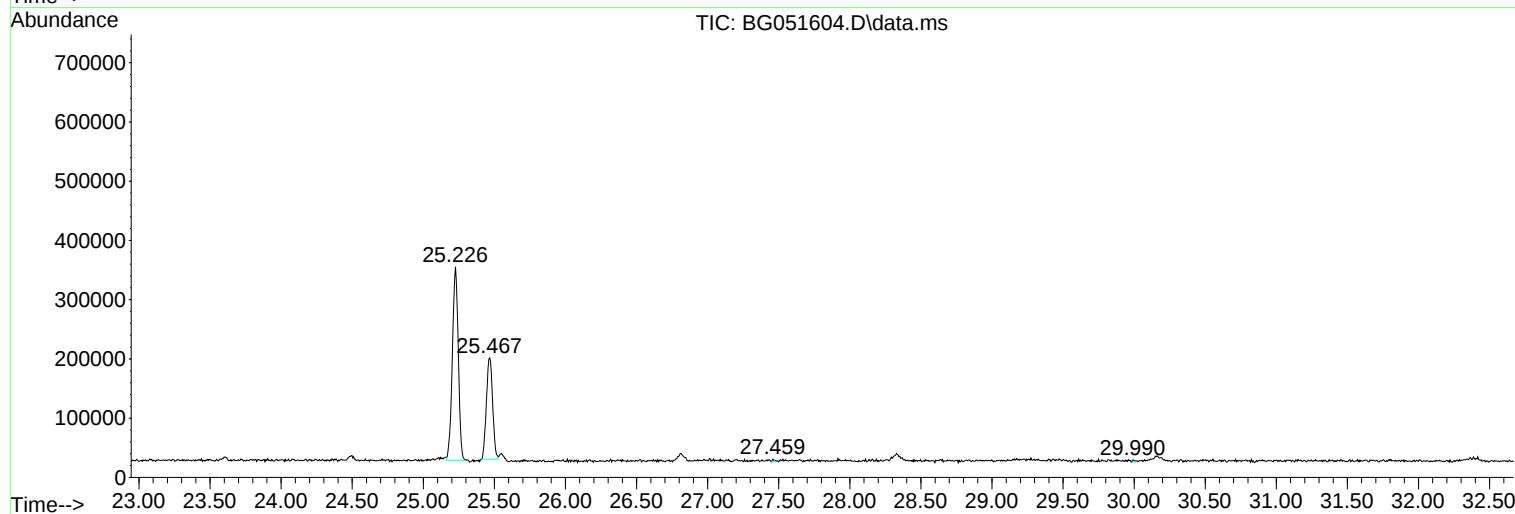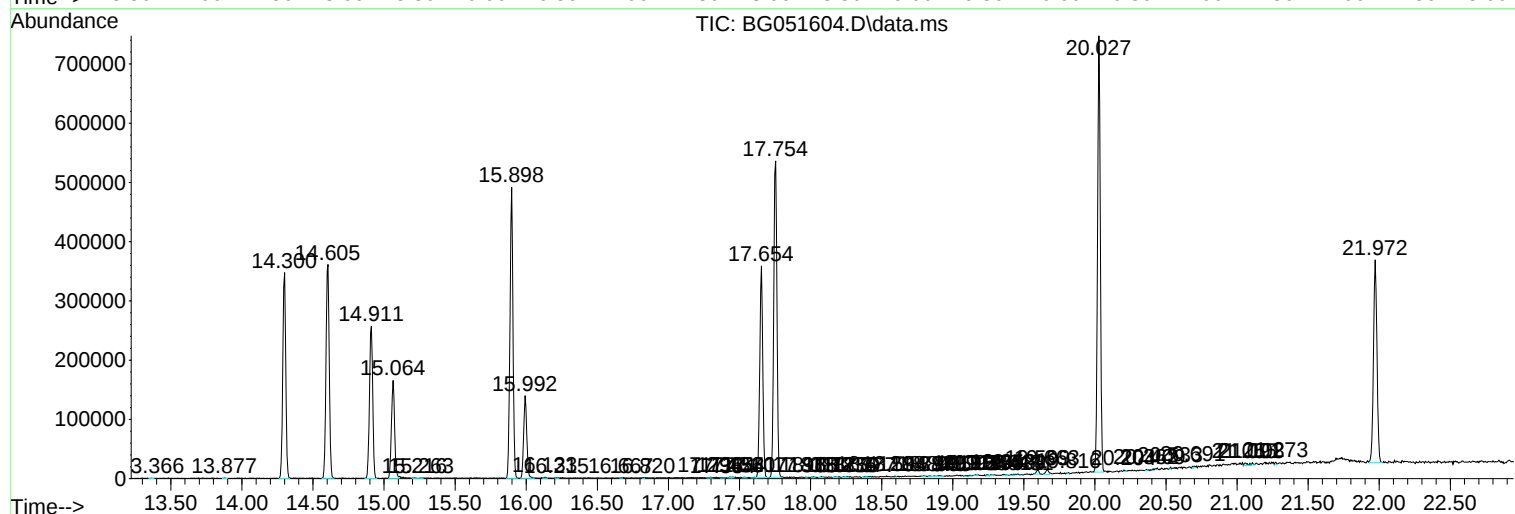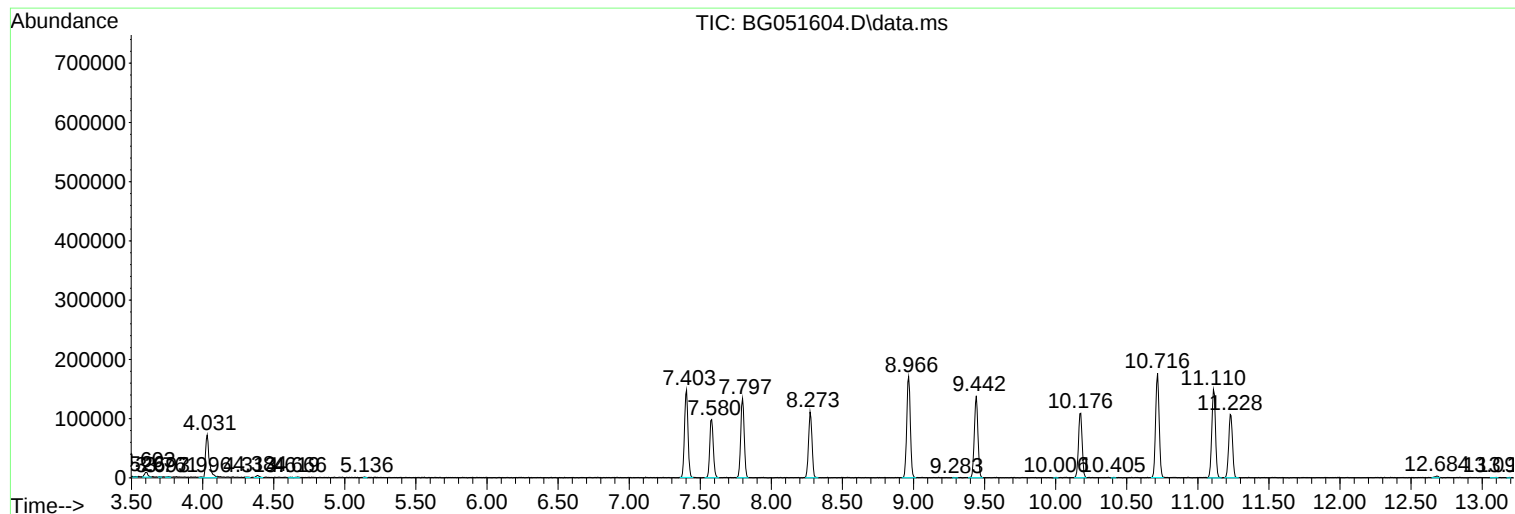

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051604.D
Acq On : 17 Dec 2021 20:23
Operator : CG/JU
Sample : PB141493BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051604.D
Acq On : 17 Dec 2021 20:23
Operator : CG/JU
Sample : PB141493BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK493

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc