

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051607.D
 Acq On : 17 Dec 2021 22:25
 Operator : CG/JU
 Sample : M5121-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.599	14	19	27	rVB3	7801	14604	1.77%	0.155%
2	3.781	49	50	55	rVB2	1567	2224	0.27%	0.024%
3	3.881	64	67	71	rBV3	3256	4766	0.58%	0.051%
4	4.034	88	93	106	rBV	34291	65459	7.94%	0.694%
5	4.386	150	153	158	rVV5	2643	4500	0.55%	0.048%
6	4.698	203	206	208	rBV2	1203	1758	0.21%	0.019%
7	5.320	307	312	317	rBV4	2157	3929	0.48%	0.042%
8	6.166	451	456	461	rBV2	4675	8402	1.02%	0.089%
9	6.325	478	483	486	rBV	1312	2075	0.25%	0.022%
10	6.813	562	566	568	rBV2	2461	3418	0.41%	0.036%
11	7.136	618	621	624	rBV2	1585	1847	0.22%	0.020%
12	7.406	659	667	678	rVB	167407	300196	36.43%	3.184%
13	7.582	688	697	712	rBV	113290	200432	24.33%	2.126%
14	7.752	723	726	727	rBV	2771	2498	0.30%	0.026%
15	7.799	727	734	743	rVB	153945	270584	32.84%	2.870%
16	7.888	745	749	752	rVV2	1469	1766	0.21%	0.019%
17	8.275	807	815	822	rVV	137034	233464	28.34%	2.476%
18	8.469	843	848	853	rVV4	5599	11112	1.35%	0.118%
19	8.516	853	856	857	rVV3	3410	3958	0.48%	0.042%
20	8.534	857	859	861	rVV2	3263	3056	0.37%	0.032%
21	8.863	913	915	921	rVB2	1606	2175	0.26%	0.023%
22	8.968	926	933	943	rBV	194969	345611	41.95%	3.666%
23	9.174	964	968	971	rVV2	1648	3350	0.41%	0.036%
24	9.444	1007	1014	1021	rVV	153943	271025	32.89%	2.875%
25	9.609	1038	1042	1043	rBV	2461	3184	0.39%	0.034%
26	9.879	1084	1088	1092	rVB4	4350	6843	0.83%	0.073%
27	10.179	1131	1139	1146	rBV	126684	227756	27.64%	2.416%
28	10.719	1224	1231	1239	rVB	197168	352250	42.75%	3.736%
29	10.866	1251	1256	1259	rBV4	2363	3368	0.41%	0.036%
30	11.113	1291	1298	1305	rBV	181870	337394	40.95%	3.579%
31	11.160	1305	1306	1312	rVV2	8362	11559	1.40%	0.123%
32	11.236	1312	1319	1331	rVB2	136116	257668	31.27%	2.733%
33	12.123	1467	1470	1474	rVB4	4253	6026	0.73%	0.064%
34	12.505	1531	1535	1540	rBV3	6218	9506	1.15%	0.101%
35	12.581	1544	1548	1552	rBV2	1829	3220	0.39%	0.034%
36	12.646	1558	1559	1562	rVV3	1849	1825	0.22%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051607.D
 Acq On : 17 Dec 2021 22:25
 Operator : CG/JU
 Sample : M5121-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	12.687	1562	1566	1570	rVV4	3956	6325	0.77%	0.067%
38	12.740	1570	1575	1580	rVB6	4636	9122	1.11%	0.097%
39	12.863	1594	1596	1601	rVB4	4470	5244	0.64%	0.056%
40	12.922	1604	1606	1609	rBV2	1863	1789	0.22%	0.019%
41	12.975	1609	1615	1619	rVB3	6557	13431	1.63%	0.142%
42	13.010	1619	1621	1623	rBV2	1962	2207	0.27%	0.023%
43	13.081	1630	1633	1635	rBV3	2040	1750	0.21%	0.019%
44	13.128	1638	1641	1644	rBV4	3375	3837	0.47%	0.041%
45	13.239	1658	1660	1663	rVB4	2645	3277	0.40%	0.035%
46	13.274	1663	1666	1667	rBV	2797	2165	0.26%	0.023%
47	13.304	1667	1671	1676	rVV5	4241	7932	0.96%	0.084%
48	13.357	1678	1680	1683	rVV3	1804	2458	0.30%	0.026%
49	13.392	1683	1686	1689	rVV4	3005	4654	0.56%	0.049%
50	13.415	1689	1690	1692	rVV	2668	2071	0.25%	0.022%
51	13.451	1692	1696	1700	rVV4	6395	9215	1.12%	0.098%
52	13.656	1729	1731	1734	rVB3	2540	2231	0.27%	0.024%
53	13.733	1737	1744	1751	rBV3	15553	24811	3.01%	0.263%
54	13.809	1755	1757	1759	rBV3	2161	2010	0.24%	0.021%
55	13.879	1767	1769	1773	rVB4	2424	2537	0.31%	0.027%
56	14.079	1800	1803	1804	rVV3	3085	3526	0.43%	0.037%
57	14.120	1807	1810	1813	rVV5	2315	3450	0.42%	0.037%
58	14.203	1822	1824	1825	rVV	2488	1828	0.22%	0.019%
59	14.232	1825	1829	1832	rVV5	5013	8289	1.01%	0.088%
60	14.302	1834	1841	1846	rVV	338294	505042	61.30%	5.357%
61	14.349	1846	1849	1852	rVV5	4171	6770	0.82%	0.072%
62	14.385	1852	1855	1860	rVV5	7068	9317	1.13%	0.099%
63	14.432	1862	1863	1866	rVV2	2001	1844	0.22%	0.020%
64	14.531	1875	1880	1883	rVV7	7177	10575	1.28%	0.112%
65	14.608	1886	1893	1900	rVB	389449	624699	75.82%	6.626%
66	14.655	1900	1901	1903	rBV2	3475	2171	0.26%	0.023%
67	14.719	1910	1912	1914	rVB2	2761	2503	0.30%	0.027%
68	14.743	1914	1916	1919	rBV2	3764	5088	0.62%	0.054%
69	14.790	1921	1924	1930	rBV8	7844	16309	1.98%	0.173%
70	14.860	1934	1936	1937	rBV2	3499	3261	0.40%	0.035%
71	14.913	1937	1945	1952	rVB	290433	465387	56.48%	4.936%
72	14.966	1952	1954	1956	rBV3	2877	1861	0.23%	0.020%
73	14.990	1956	1958	1959	rVB2	3896	2370	0.29%	0.025%
74	15.066	1964	1971	1979	rVV	146215	233097	28.29%	2.472%
75	15.137	1979	1983	1985	rBV5	2911	3558	0.43%	0.038%
76	15.189	1990	1992	1994	rVV3	4352	3883	0.47%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051607.D
 Acq On : 17 Dec 2021 22:25
 Operator : CG/JU
 Sample : M5121-03
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL52

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	15.219	1994	1997	2000	rVV5	4469	5710	0.69%	0.061%
78	15.301	2006	2011	2016	rVB8	7683	14681	1.78%	0.156%
79	15.460	2037	2038	2039	rBV	5226	2741	0.33%	0.029%
80	15.489	2039	2043	2045	rVV4	9272	15431	1.87%	0.164%
81	15.536	2047	2051	2055	rVB6	11579	19971	2.42%	0.212%
82	15.612	2062	2064	2066	rVB3	4004	2009	0.24%	0.021%
83	15.630	2066	2067	2070	rBV3	4485	3834	0.47%	0.041%
84	15.700	2075	2079	2081	rVV5	13677	19270	2.34%	0.204%
85	15.736	2084	2085	2087	rVV2	7998	6018	0.73%	0.064%
86	15.789	2091	2094	2095	rBV3	6250	5847	0.71%	0.062%
87	15.847	2102	2104	2105	rBV2	4905	3646	0.44%	0.039%
88	15.900	2107	2113	2121	rVB	475599	717872	87.13%	7.614%
89	15.959	2121	2123	2124	rBV2	4424	2730	0.33%	0.029%
90	16.000	2124	2130	2136	rBV2	95162	144386	17.52%	1.531%
91	16.182	2159	2161	2164	rBV4	5513	5065	0.61%	0.054%
92	16.529	2218	2220	2221	rBV2	9101	6762	0.82%	0.072%
93	16.629	2233	2237	2241	rVB7	12362	19869	2.41%	0.211%
94	17.657	2407	2412	2417	rBV	318965	473228	57.43%	5.019%
95	17.757	2423	2429	2436	rBV2	447522	731499	88.78%	7.759%
96	18.526	2558	2560	2562	rVB2	41491	30463	3.70%	0.323%
97	20.036	2812	2817	2822	rBV	518875	823941	100.00%	8.739%
98	21.851	3122	3126	3129	rBV	177416	229602	27.87%	2.435%
99	21.980	3143	3148	3154	rVB	287379	484523	58.81%	5.139%
100	25.235	3697	3702	3711	rVB2	248432	654242	79.40%	6.939%




Sum of corrected areas: 9428042

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051607.D
Acq On : 17 Dec 2021 22:25
Operator : CG/JU
Sample : M5121-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL52

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

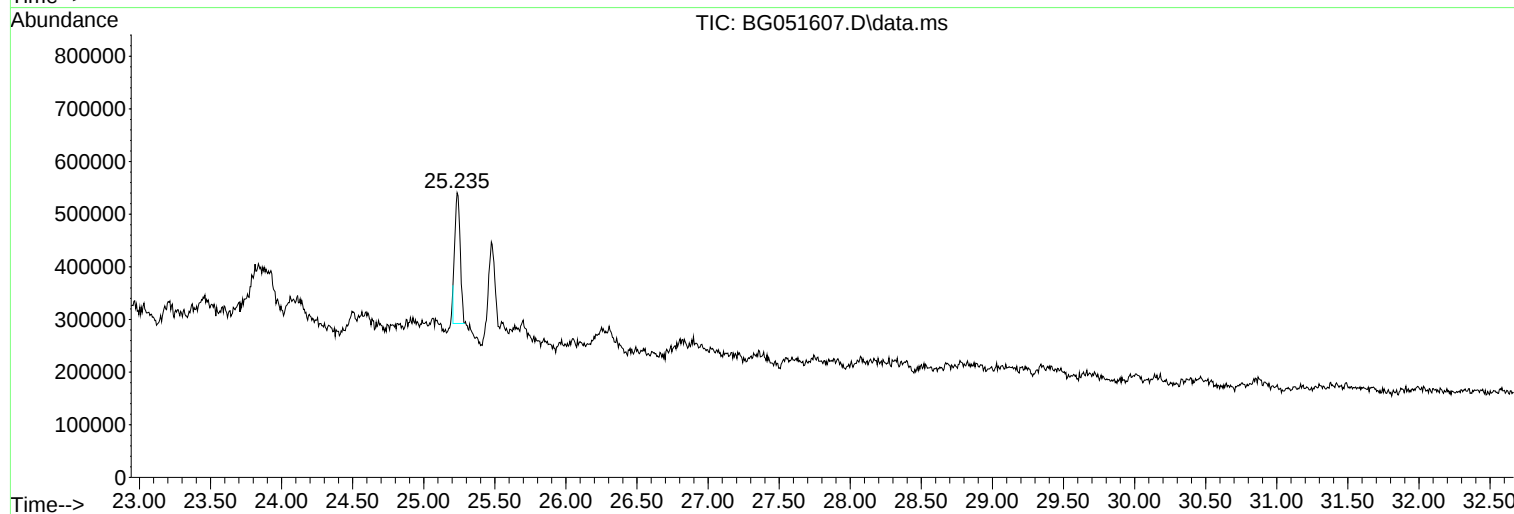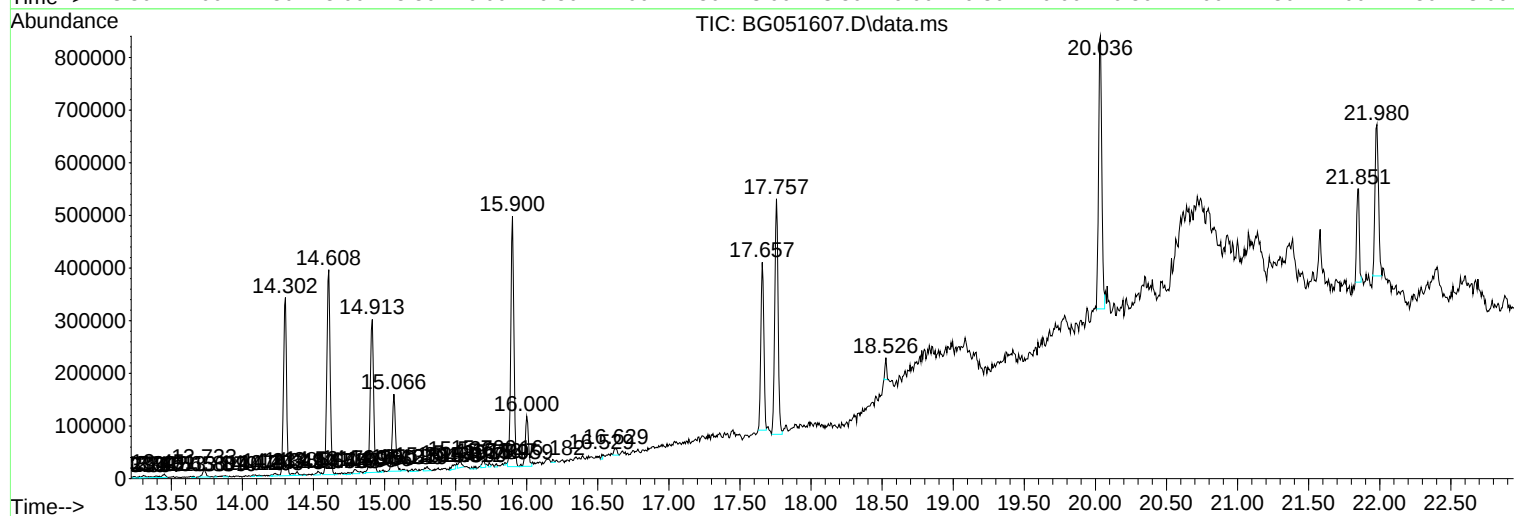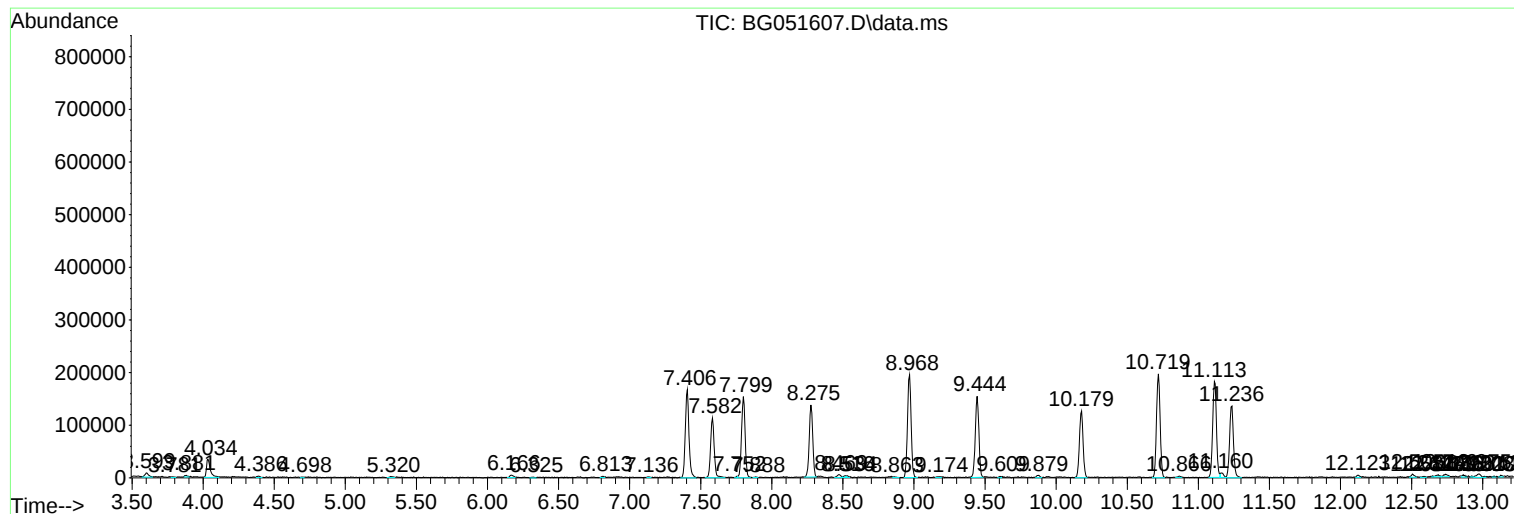

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051607.D
Acq On : 17 Dec 2021 22:25
Operator : CG/JU
Sample : M5121-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL52

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051607.D
Acq On : 17 Dec 2021 22:25
Operator : CG/JU
Sample : M5121-03
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL52

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc