

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051609.D
 Acq On : 17 Dec 2021 23:47
 Operator : CG/JU
 Sample : M5121-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051609.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.606	16	20	25	rVB3	8019	12677	1.39%	0.114%
2	3.882	64	67	71	rVV3	3209	4975	0.55%	0.045%
3	4.029	88	92	105	rVV	61967	106165	11.64%	0.959%
4	4.381	147	152	154	rBV3	3347	4134	0.45%	0.037%
5	4.816	223	226	230	rVB2	1355	1843	0.20%	0.017%
6	5.321	309	312	314	rBV	2136	2388	0.26%	0.022%
7	5.891	407	409	413	rBV	1235	1793	0.20%	0.016%
8	6.337	481	485	487	rVB3	1543	1850	0.20%	0.017%
9	6.666	539	541	544	rBV2	1879	1652	0.18%	0.015%
10	7.406	659	667	677	rVV	165483	305972	33.56%	2.763%
11	7.583	690	697	704	rBV	110316	189573	20.79%	1.712%
12	7.630	704	705	710	rVB4	3270	3554	0.39%	0.032%
13	7.800	727	734	741	rBV	155357	267310	29.32%	2.414%
14	8.276	808	815	822	rBV	138005	232057	25.45%	2.095%
15	8.329	822	824	826	rVV2	2698	2157	0.24%	0.019%
16	8.969	926	933	941	rBV	198005	351734	38.58%	3.176%
17	9.445	1006	1014	1022	rVV	154088	278943	30.59%	2.519%
18	9.874	1081	1087	1091	rVB2	4306	7046	0.77%	0.064%
19	10.179	1131	1139	1146	rVV	126717	234537	25.72%	2.118%
20	10.719	1222	1231	1240	rBV	204662	368295	40.40%	3.325%
21	10.855	1250	1254	1255	rBV	3792	3390	0.37%	0.031%
22	11.113	1287	1298	1306	rBV	194143	344958	37.84%	3.115%
23	11.231	1311	1318	1325	rVV	116365	217123	23.81%	1.960%
24	11.865	1423	1426	1429	rVB2	1524	2301	0.25%	0.021%
25	12.106	1463	1467	1469	rBV3	1522	1745	0.19%	0.016%
26	12.382	1511	1514	1519	rVB	1002	1784	0.20%	0.016%
27	12.505	1530	1535	1540	rBV4	7663	11200	1.23%	0.101%
28	12.687	1561	1566	1572	rVB3	4048	7360	0.81%	0.066%
29	13.134	1640	1642	1645	rVV2	2797	3066	0.34%	0.028%
30	13.240	1656	1660	1665	rVB5	1903	2858	0.31%	0.026%
31	13.310	1669	1672	1675	rVB4	3973	4800	0.53%	0.043%
32	13.398	1682	1687	1692	rVV7	2280	4812	0.53%	0.043%
33	13.439	1692	1694	1695	rVV	2288	1897	0.21%	0.017%
34	13.457	1695	1697	1700	rVV2	2772	3043	0.33%	0.027%
35	13.522	1702	1708	1712	rVB5	1977	2589	0.28%	0.023%
36	13.616	1718	1724	1727	rBV4	824	1848	0.20%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051609.D
 Acq On : 17 Dec 2021 23:47
 Operator : CG/JU
 Sample : M5121-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	13.733	1736	1744	1751	rVB4	16454	29450	3.23%	0.266%
38	13.856	1763	1765	1770	rBV4	1662	2312	0.25%	0.021%
39	14.074	1799	1802	1806	rBV3	1454	2374	0.26%	0.021%
40	14.209	1823	1825	1829	rBV3	1501	2403	0.26%	0.022%
41	14.297	1833	1840	1847	rBV	352125	529289	58.05%	4.779%
42	14.385	1853	1855	1858	rVB4	1911	1889	0.21%	0.017%
43	14.497	1871	1874	1876	rBV2	2318	2566	0.28%	0.023%
44	14.532	1876	1880	1881	rBV2	5772	5588	0.61%	0.050%
45	14.608	1886	1893	1901	rVB	409402	648519	71.13%	5.855%
46	14.667	1901	1903	1905	rBV2	2438	2807	0.31%	0.025%
47	14.685	1905	1906	1910	rVB3	1491	1701	0.19%	0.015%
48	14.785	1921	1923	1930	rBV2	5993	8912	0.98%	0.080%
49	14.914	1937	1945	1954	rVB	303133	495490	54.35%	4.474%
50	14.990	1954	1958	1960	rBV3	2051	2306	0.25%	0.021%
51	15.008	1960	1961	1964	rBV3	1780	1719	0.19%	0.016%
52	15.066	1964	1971	1980	rBV	169537	272454	29.88%	2.460%
53	15.125	1980	1981	1987	rVV4	2760	3424	0.38%	0.031%
54	15.231	1996	1999	2000	rVV3	2730	1815	0.20%	0.016%
55	15.254	2000	2003	2006	rVV4	1867	2088	0.23%	0.019%
56	15.290	2006	2009	2016	rVB8	4000	8981	0.99%	0.081%
57	15.431	2030	2033	2034	rVB3	3237	2540	0.28%	0.023%
58	15.536	2046	2051	2056	rVB4	5847	9289	1.02%	0.084%
59	15.589	2059	2060	2064	rBV4	3421	3339	0.37%	0.030%
60	15.636	2066	2068	2071	rBV3	1481	1735	0.19%	0.016%
61	15.695	2071	2078	2082	rVV7	3895	9050	0.99%	0.082%
62	15.742	2082	2086	2088	rVB4	4665	4806	0.53%	0.043%
63	15.789	2092	2094	2097	rBV2	1966	2444	0.27%	0.022%
64	15.901	2105	2113	2119	rBV2	543184	845398	92.72%	7.633%
65	16.001	2124	2130	2138	rVV2	115467	178070	19.53%	1.608%
66	16.089	2140	2145	2150	rBV6	3714	7114	0.78%	0.064%
67	16.142	2150	2154	2159	rVB7	5499	8450	0.93%	0.076%
68	16.183	2159	2161	2163	rVB3	1895	1827	0.20%	0.016%
69	16.241	2167	2171	2173	rBV5	2983	3849	0.42%	0.035%
70	16.265	2173	2175	2177	rVB4	2491	1702	0.19%	0.015%
71	16.288	2177	2179	2183	rBV5	3331	4075	0.45%	0.037%
72	16.335	2183	2187	2188	rBV3	3228	3668	0.40%	0.033%
73	16.418	2197	2201	2203	rBV5	3021	3987	0.44%	0.036%
74	16.470	2209	2210	2213	rBV3	2363	1692	0.19%	0.015%
75	16.523	2217	2219	2222	rVV3	2392	1952	0.21%	0.018%
76	16.564	2224	2226	2230	rVV5	4250	5064	0.56%	0.046%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051609.D
 Acq On : 17 Dec 2021 23:47
 Operator : CG/JU
 Sample : M5121-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	16.600	2230	2232	2233	rVV2	3687	3496	0.38%	0.032%
78	16.623	2235	2236	2241	rVB4	12444	13468	1.48%	0.122%
79	16.676	2241	2245	2247	rBV5	3875	4756	0.52%	0.043%
80	16.723	2249	2253	2257	rBV	14887	20181	2.21%	0.182%
81	16.782	2258	2263	2269	rVB6	20636	33994	3.73%	0.307%
82	16.841	2269	2273	2277	rBV2	16676	22387	2.46%	0.202%
83	16.888	2277	2281	2285	rBV5	13053	17407	1.91%	0.157%
84	16.935	2287	2289	2292	rVB4	4353	4612	0.51%	0.042%
85	17.040	2304	2307	2312	rBV5	14914	25864	2.84%	0.234%
86	17.111	2314	2319	2323	rBV	18048	31000	3.40%	0.280%
87	17.240	2339	2341	2342	rBV2	3236	2290	0.25%	0.021%
88	17.387	2363	2366	2371	rBV6	8475	16125	1.77%	0.146%
89	17.428	2371	2373	2374	rBV2	4807	4514	0.50%	0.041%
90	17.551	2390	2394	2398	rBV6	11497	16794	1.84%	0.152%
91	17.657	2406	2412	2418	rBV	360172	548018	60.11%	4.948%
92	17.757	2420	2429	2438	rBV	501220	809222	88.76%	7.306%
93	17.874	2447	2449	2451	rBV3	6208	6481	0.71%	0.059%
94	18.521	2557	2559	2564	rVB5	22193	26726	2.93%	0.241%
95	20.030	2811	2816	2822	rBV	524185	787989	86.43%	7.115%
96	21.575	3077	3079	3089	rVB6	59056	128937	14.14%	1.164%
97	21.846	3122	3125	3141	rVB2	239676	537581	58.96%	4.854%
98	21.975	3143	3147	3157	rVB	306639	518934	56.92%	4.685%
99	25.235	3695	3702	3717	rVB2	288321	911728	100.00%	8.232%
100	25.476	3737	3743	3752	rVB3	162392	463400	50.83%	4.184%




Sum of corrected areas: 11075471

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051609.D
Acq On : 17 Dec 2021 23:47
Operator : CG/JU
Sample : M5121-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL59

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

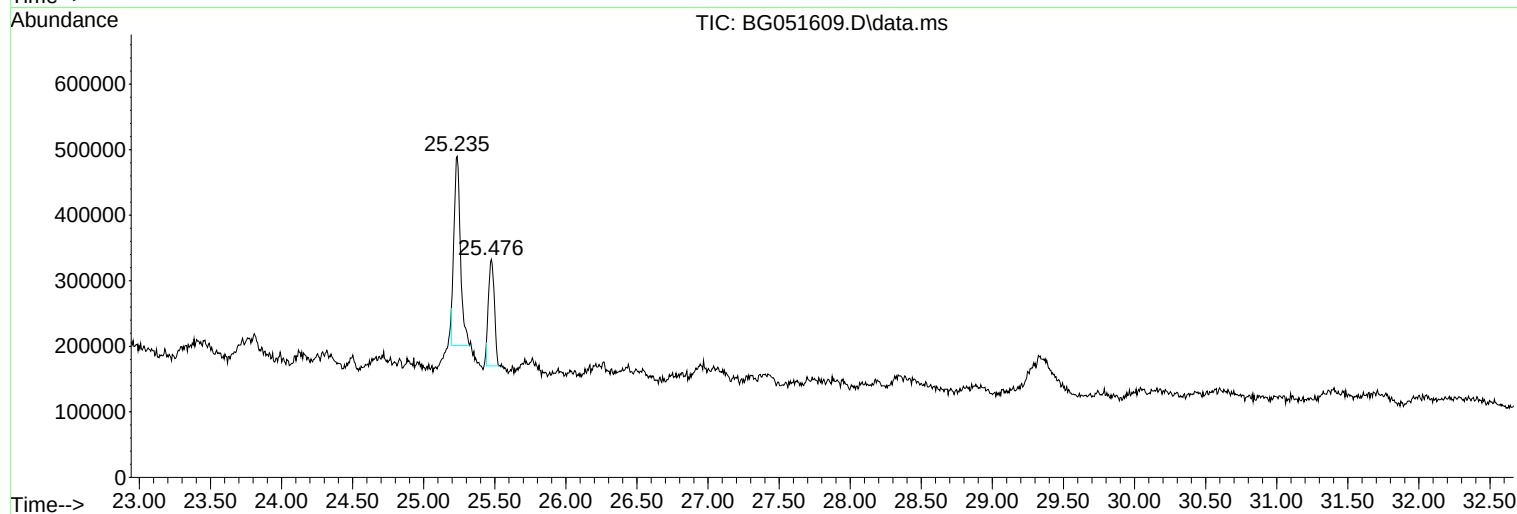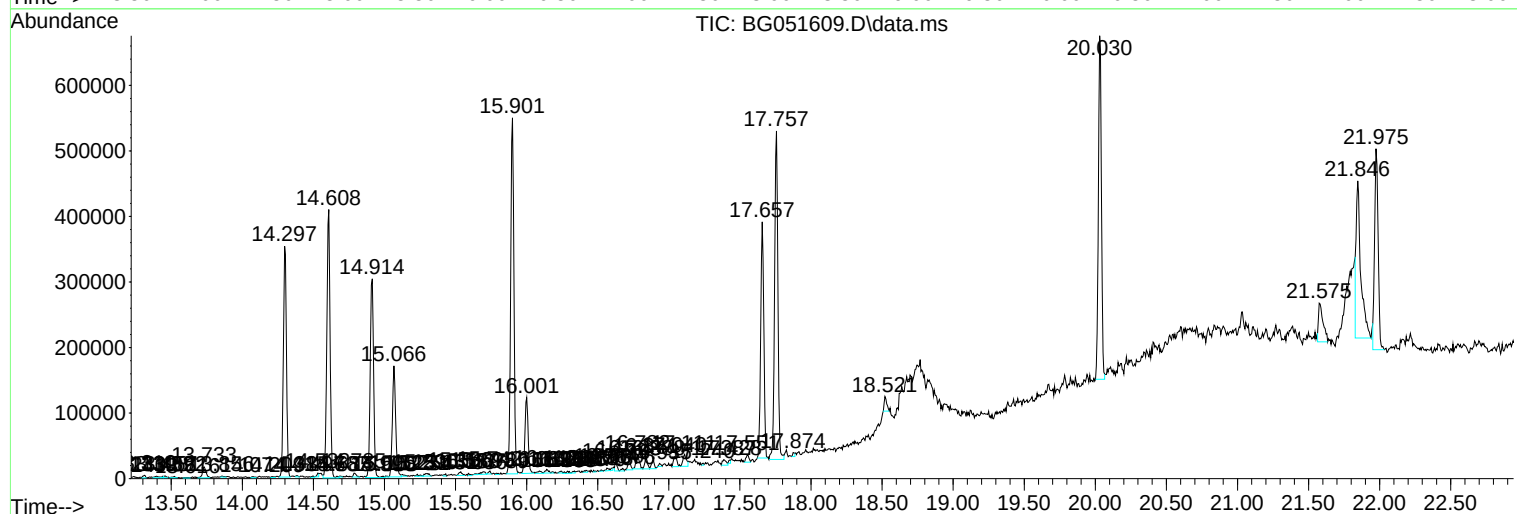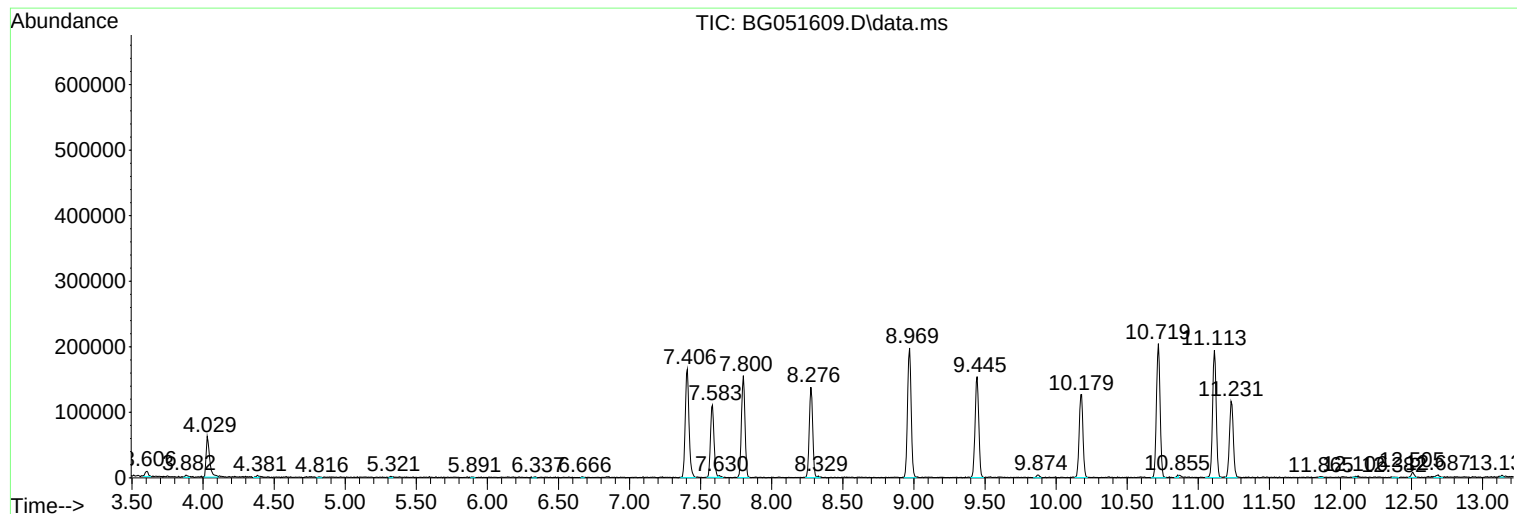

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051609.D
Acq On : 17 Dec 2021 23:47
Operator : CG/JU
Sample : M5121-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL59










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.575	4.97 ng/ul	128937	Chrysene-d12	21.975

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Eicosene, (E)-		280	C20H40	074685-33-9	89
2	3-Hexadecene, (Z)-		224	C16H32	034303-81-6	89
3	Cetene		224	C16H32	000629-73-2	76
4	Oleyl alcohol, trifluoroacetate		364	C20H35F3O2	1000352-68-4	68
5	7-Tetradecene		196	C14H28	010374-74-0	68

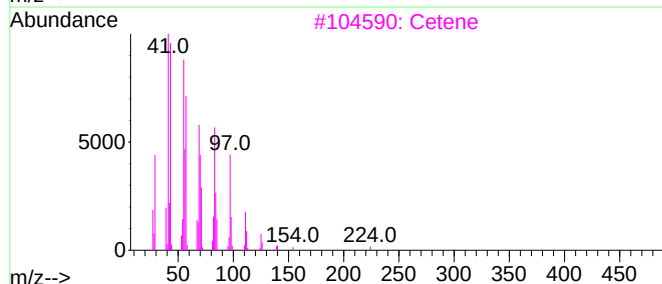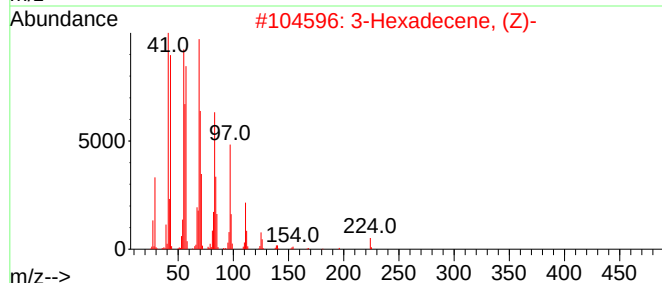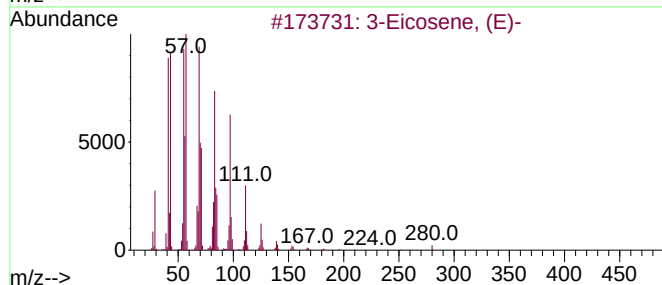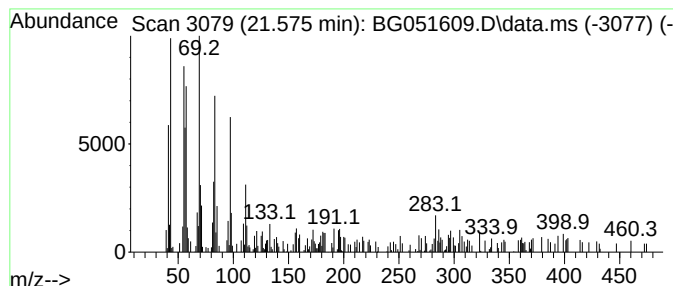

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051609.D
Acq On : 17 Dec 2021 23:47
Operator : CG/JU
Sample : M5121-07
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL59

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.575	5.0	ng/u1	128937	5	21.975	518934	20.0