

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051612.D
 Acq On : 18 Dec 2021 1:49
 Operator : CG/JU
 Sample : M5121-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.564	12	13	16	rBV2	1534	1349	0.18%	0.016%
2	3.599	16	19	26	rVV4	7532	11097	1.46%	0.135%
3	3.892	66	69	70	rBV2	1345	1306	0.17%	0.016%
4	3.939	74	77	79	rVB2	1566	1707	0.23%	0.021%
5	4.033	90	93	101	rBV	27905	44158	5.83%	0.535%
6	4.327	140	143	144	rBV	1761	1789	0.24%	0.022%
7	4.392	149	154	157	rVV3	2597	3349	0.44%	0.041%
8	5.320	308	312	313	rBV2	1524	1397	0.18%	0.017%
9	6.330	481	484	487	rVB2	1340	1550	0.20%	0.019%
10	6.559	521	523	529	rVB	992	1551	0.20%	0.019%
11	6.818	565	567	570	rBV	1029	1213	0.16%	0.015%
12	6.877	575	577	582	rVB2	1188	1478	0.19%	0.018%
13	7.405	659	667	678	rVB	149300	267267	35.26%	3.241%
14	7.582	690	697	704	rBV	102299	170962	22.55%	2.073%
15	7.799	727	734	741	rBV	136992	235363	31.05%	2.854%
16	8.275	808	815	821	rBV	144363	237385	31.31%	2.879%
17	8.322	821	823	825	rVB2	1686	1209	0.16%	0.015%
18	8.968	925	933	942	rBV	180984	305839	40.35%	3.709%
19	9.062	944	949	950	rVV2	1646	1380	0.18%	0.017%
20	9.444	1006	1014	1022	rBV	137520	245203	32.35%	2.973%
21	9.520	1025	1027	1032	rBV2	1325	1689	0.22%	0.020%
22	9.867	1082	1086	1093	rVB2	3417	5948	0.78%	0.072%
23	9.978	1102	1105	1109	rBV	1177	1697	0.22%	0.021%
24	10.119	1124	1129	1130	rBV3	1136	1417	0.19%	0.017%
25	10.172	1130	1138	1147	rVB	109528	201858	26.63%	2.448%
26	10.296	1157	1159	1164	rVB	933	1273	0.17%	0.015%
27	10.378	1168	1173	1176	rBV2	1699	2553	0.34%	0.031%
28	10.719	1224	1231	1241	rVB	176601	314003	41.42%	3.808%
29	10.854	1250	1254	1255	rBV	1418	1419	0.19%	0.017%
30	10.871	1255	1257	1260	rVB	1705	1910	0.25%	0.023%
31	10.959	1270	1272	1275	rBV	898	1199	0.16%	0.015%
32	11.112	1291	1298	1307	rBV	190444	347635	45.86%	4.216%
33	11.230	1311	1318	1328	rVB2	100201	188209	24.83%	2.282%
34	11.864	1420	1426	1428	rBV2	1849	2986	0.39%	0.036%
35	12.111	1465	1468	1474	rVB6	1314	2430	0.32%	0.029%
36	12.504	1531	1535	1541	rVB3	6375	9098	1.20%	0.110%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051612.D
 Acq On : 18 Dec 2021 1:49
 Operator : CG/JU
 Sample : M5121-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	12.681	1560	1565	1568	rBV3	2963	3922	0.52%	0.048%
38	12.792	1578	1584	1586	rBV	1572	2110	0.28%	0.026%
39	12.939	1607	1609	1613	rVB2	1410	1258	0.17%	0.015%
40	13.133	1637	1642	1645	rBV2	2118	3127	0.41%	0.038%
41	13.162	1645	1647	1652	rVV3	1426	1561	0.21%	0.019%
42	13.239	1657	1660	1663	rVB3	1888	1794	0.24%	0.022%
43	13.280	1663	1667	1669	rBV2	1775	2216	0.29%	0.027%
44	13.309	1670	1672	1675	rVB2	2976	2258	0.30%	0.027%
45	13.356	1677	1680	1683	rVB2	1617	1700	0.22%	0.021%
46	13.397	1683	1687	1689	rBV	2687	3648	0.48%	0.044%
47	13.444	1691	1695	1698	rBV3	2630	3838	0.51%	0.047%
48	13.515	1703	1707	1708	rBV2	2096	1910	0.25%	0.023%
49	13.726	1738	1743	1750	rVB3	14570	22528	2.97%	0.273%
50	13.885	1767	1770	1773	rVB3	1389	1899	0.25%	0.023%
51	14.038	1794	1796	1800	rVB2	1302	1333	0.18%	0.016%
52	14.108	1806	1808	1810	rVV2	1568	1460	0.19%	0.018%
53	14.132	1810	1812	1815	rVB2	1610	1379	0.18%	0.017%
54	14.184	1819	1821	1827	rBV2	1621	2964	0.39%	0.036%
55	14.243	1827	1831	1832	rBV2	1621	1874	0.25%	0.023%
56	14.296	1834	1840	1846	rBV	317849	460594	60.76%	5.585%
57	14.378	1851	1854	1858	rVV3	1934	2683	0.35%	0.033%
58	14.414	1858	1860	1864	rVB2	1370	1787	0.24%	0.022%
59	14.496	1869	1874	1876	rBV4	2104	2934	0.39%	0.036%
60	14.531	1876	1880	1886	rBV6	5175	10421	1.37%	0.126%
61	14.607	1886	1893	1900	rVV	361209	583333	76.95%	7.074%
62	14.690	1903	1907	1910	rVB	1911	2155	0.28%	0.026%
63	14.789	1920	1924	1927	rBV3	5234	7305	0.96%	0.089%
64	14.913	1939	1945	1952	rVB	323156	518259	68.37%	6.285%
65	15.066	1965	1971	1979	rBV	124378	203151	26.80%	2.463%
66	15.189	1990	1992	1993	rBV2	1701	1232	0.16%	0.015%
67	15.230	1996	1999	2000	rVV	1805	1278	0.17%	0.015%
68	15.295	2006	2010	2013	rBV4	3180	4461	0.59%	0.054%
69	15.406	2027	2029	2030	rBV2	2290	1316	0.17%	0.016%
70	15.465	2037	2039	2044	rVV5	1136	1804	0.24%	0.022%
71	15.530	2047	2050	2054	rVB4	3221	4694	0.62%	0.057%
72	15.671	2071	2074	2075	rBV3	1427	1894	0.25%	0.023%
73	15.700	2075	2079	2082	rVV4	5095	7745	1.02%	0.094%
74	15.735	2082	2085	2088	rVV3	4833	5776	0.76%	0.070%
75	15.771	2089	2091	2093	rVB3	2093	1557	0.21%	0.019%
76	15.900	2106	2113	2119	rBV	454611	703613	92.82%	8.532%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051612.D
 Acq On : 18 Dec 2021 1:49
 Operator : CG/JU
 Sample : M5121-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL64

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	16.000	2121	2130	2135	rBV	82535	123350	16.27%	1.496%
78	16.135	2149	2153	2157	rVV6	4136	7122	0.94%	0.086%
79	16.199	2160	2164	2165	rVB4	1884	1580	0.21%	0.019%
80	16.240	2168	2171	2173	rVV4	2398	2359	0.31%	0.029%
81	16.287	2177	2179	2181	rBV3	3674	3401	0.45%	0.041%
82	16.534	2215	2221	2223	rBV5	3448	6098	0.80%	0.074%
83	16.622	2234	2236	2243	rVB4	8366	12751	1.68%	0.155%
84	16.716	2249	2252	2258	rBV2	12230	17064	2.25%	0.207%
85	16.781	2258	2263	2269	rBV4	16583	30449	4.02%	0.369%
86	16.840	2269	2273	2278	rBV3	12648	17318	2.28%	0.210%
87	16.887	2278	2281	2286	rVB6	9184	12442	1.64%	0.151%
88	16.928	2286	2288	2291	rBV3	4987	6755	0.89%	0.082%
89	17.045	2304	2308	2314	rVB7	11192	20815	2.75%	0.252%
90	17.110	2314	2319	2323	rBV2	16096	28966	3.82%	0.351%
91	17.180	2328	2331	2338	rVB4	7571	12552	1.66%	0.152%
92	17.392	2363	2367	2370	rBV5	5593	8277	1.09%	0.100%
93	17.433	2372	2374	2377	rBV4	5131	7454	0.98%	0.090%
94	17.550	2391	2394	2398	rVB4	7508	8342	1.10%	0.101%
95	17.656	2406	2412	2419	rBV	406288	616395	81.31%	7.475%
96	17.756	2423	2429	2435	rVV2	478878	745418	98.33%	9.039%
97	17.821	2438	2440	2446	rVB7	6859	11842	1.56%	0.144%
98	18.520	2556	2559	2565	rVB5	26197	36725	4.84%	0.445%
99	20.029	2811	2816	2823	rVB	514435	758057	100.00%	9.192%
100	21.980	3142	3148	3154	rVB2	310577	538330	71.01%	6.528%




Sum of corrected areas: 8246509

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051612.D
Acq On : 18 Dec 2021 1:49
Operator : CG/JU
Sample : M5121-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

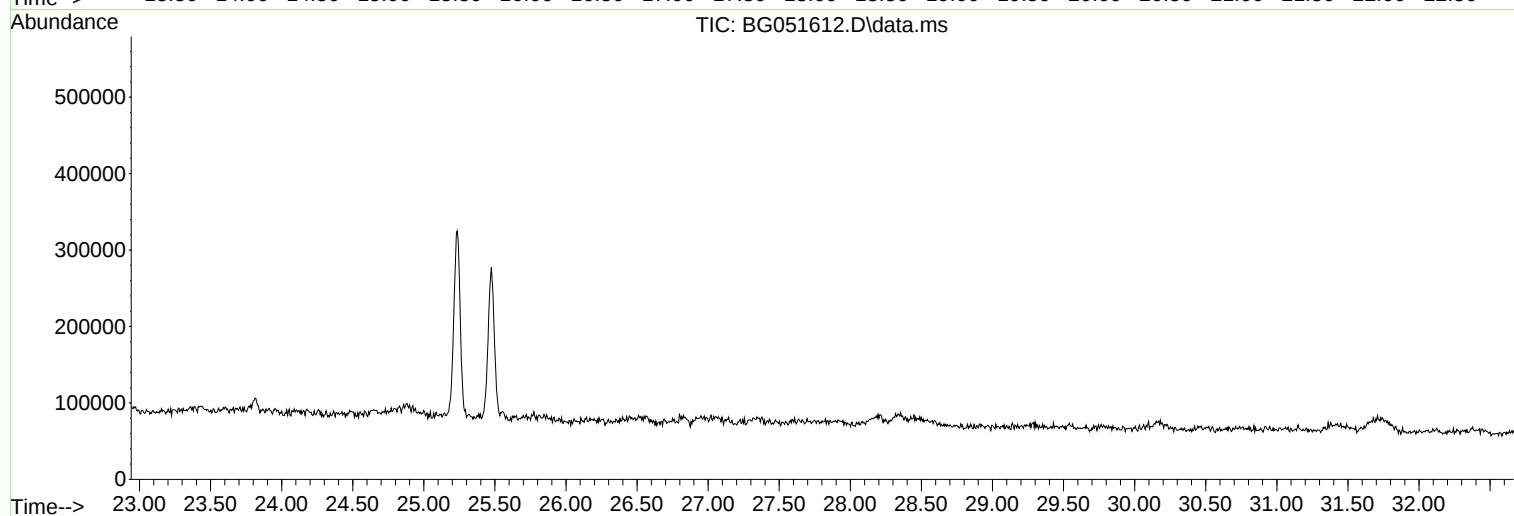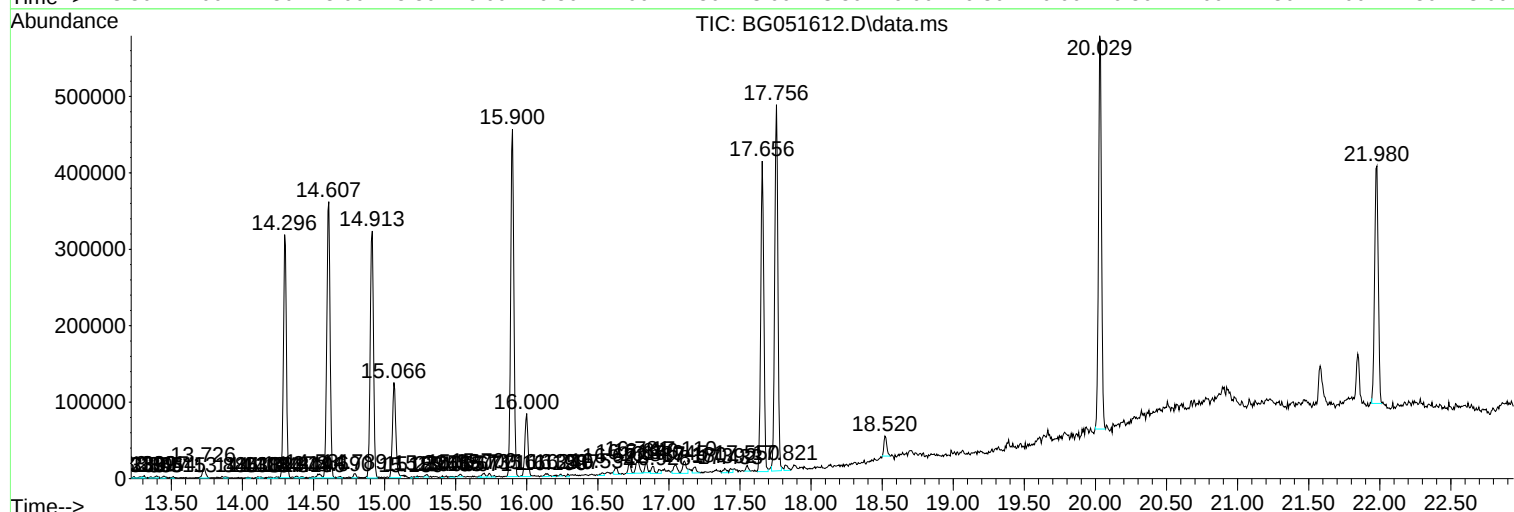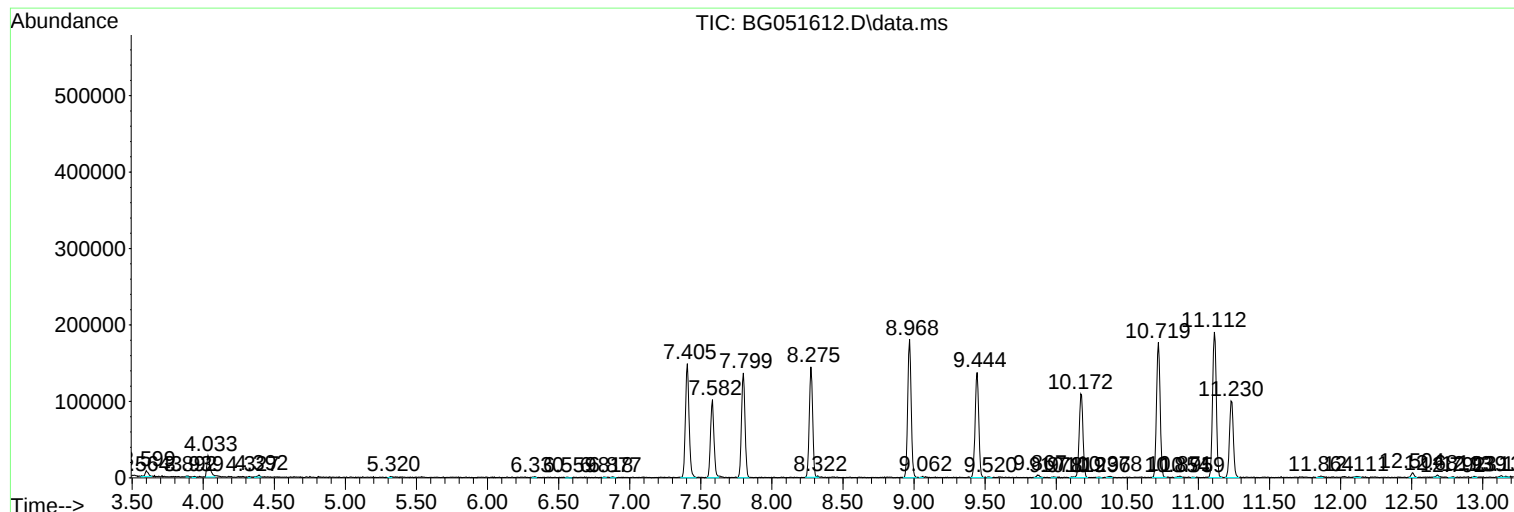

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051612.D
Acq On : 18 Dec 2021 1:49
Operator : CG/JU
Sample : M5121-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051612.D
Acq On : 18 Dec 2021 1:49
Operator : CG/JU
Sample : M5121-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL64

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc