

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051616.D
 Acq On : 18 Dec 2021 4:30
 Operator : CG/JU
 Sample : M5121-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051616.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.600	16	19	22	rVB4	3575	4930	0.38%	0.057%
2	4.035	89	93	103	rVB	14121	26200	2.01%	0.301%
3	4.217	121	124	131	rBV3	2024	4677	0.36%	0.054%
4	4.281	131	135	140	rVB3	5612	7906	0.61%	0.091%
5	5.315	307	311	315	rBV2	5168	7136	0.55%	0.082%
6	6.514	511	515	520	rBV4	2248	4836	0.37%	0.056%
7	6.643	532	537	538	rBV3	3102	4591	0.35%	0.053%
8	6.737	549	553	557	rBV3	3918	4851	0.37%	0.056%
9	6.807	559	565	570	rBV3	7660	12243	0.94%	0.141%
10	6.896	577	580	583	rBV4	2550	3482	0.27%	0.040%
11	6.931	583	586	589	rVB3	3482	4345	0.33%	0.050%
12	7.136	618	621	626	rVB3	3615	5089	0.39%	0.058%
13	7.401	658	666	676	rVB2	77461	146509	11.26%	1.682%
14	7.583	689	697	705	rBV2	52534	97877	7.52%	1.124%
15	7.659	705	710	714	rVB5	1736	3625	0.28%	0.042%
16	7.800	724	734	746	rVB	70861	135782	10.43%	1.559%
17	8.000	764	768	769	rBV4	2735	2684	0.21%	0.031%
18	8.270	806	814	821	rVB	133149	249483	19.17%	2.865%
19	8.347	821	827	834	rVB3	5278	12124	0.93%	0.139%
20	8.470	842	848	853	rVV4	11349	20935	1.61%	0.240%
21	8.523	853	857	866	rVB7	8528	19815	1.52%	0.228%
22	8.634	872	876	883	rVB7	2130	5337	0.41%	0.061%
23	8.717	887	890	895	rVB5	2466	5013	0.39%	0.058%
24	8.834	905	910	912	rBV3	5420	9533	0.73%	0.109%
25	8.963	926	932	940	rBV	90571	158164	12.15%	1.816%
26	9.128	958	960	967	rVB6	2769	4250	0.33%	0.049%
27	9.328	989	994	995	rVB4	3002	4277	0.33%	0.049%
28	9.439	1003	1013	1020	rBV	68312	133011	10.22%	1.527%
29	9.610	1037	1042	1044	rBV4	4788	6786	0.52%	0.078%
30	9.727	1057	1062	1065	rBV3	2328	4559	0.35%	0.052%
31	9.868	1080	1086	1091	rVB4	5482	9806	0.75%	0.113%
32	9.933	1091	1097	1103	rBV4	5831	11729	0.90%	0.135%
33	10.027	1109	1113	1116	rBV6	3828	6755	0.52%	0.078%
34	10.173	1130	1138	1145	rBV2	61784	117651	9.04%	1.351%
35	10.279	1152	1156	1157	rBV2	4450	4058	0.31%	0.047%
36	10.297	1157	1159	1164	rVB4	5374	5436	0.42%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051616.D
 Acq On : 18 Dec 2021 4:30
 Operator : CG/JU
 Sample : M5121-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	10.367	1164	1171	1174	rVB3	1521	3085	0.24%	0.035%
38	10.514	1191	1196	1198	rBV3	2435	4603	0.35%	0.053%
39	10.720	1222	1231	1239	rVB	87581	157044	12.07%	1.803%
40	11.113	1290	1298	1304	rBV	184461	337711	25.95%	3.878%
41	11.231	1312	1318	1322	rBV2	28656	55464	4.26%	0.637%
42	11.577	1372	1377	1379	rBV3	2398	3829	0.29%	0.044%
43	11.765	1405	1409	1411	rBV4	2594	3002	0.23%	0.034%
44	11.859	1422	1425	1429	rBV4	1832	2806	0.22%	0.032%
45	11.948	1434	1440	1444	rBV6	2537	5194	0.40%	0.060%
46	12.118	1464	1469	1474	rVV	13662	19807	1.52%	0.227%
47	12.159	1474	1476	1480	rVB3	3256	2967	0.23%	0.034%
48	12.300	1498	1500	1504	rVB2	2410	2781	0.21%	0.032%
49	12.394	1511	1516	1519	rBV4	3032	5267	0.40%	0.060%
50	12.506	1530	1535	1538	rBV3	4358	6993	0.54%	0.080%
51	12.594	1548	1550	1554	rBV2	1877	2806	0.22%	0.032%
52	12.729	1567	1573	1581	rVB4	11135	23939	1.84%	0.275%
53	12.864	1590	1596	1599	rBV4	5968	9576	0.74%	0.110%
54	12.976	1611	1615	1618	rVB3	5590	8841	0.68%	0.102%
55	13.140	1639	1643	1646	rBV6	2709	3973	0.31%	0.046%
56	13.446	1691	1695	1701	rVB3	14179	22329	1.72%	0.256%
57	13.722	1736	1742	1751	rVB7	10833	25062	1.93%	0.288%
58	13.810	1751	1757	1761	rBV4	3262	6819	0.52%	0.078%
59	13.968	1781	1784	1788	rVB5	3377	4387	0.34%	0.050%
60	14.062	1797	1800	1805	rVB5	5525	8951	0.69%	0.103%
61	14.227	1825	1828	1833	rVB5	11907	16969	1.30%	0.195%
62	14.297	1834	1840	1845	rVV	177175	261665	20.10%	3.005%
63	14.338	1845	1847	1850	rVV3	6453	9194	0.71%	0.106%
64	14.380	1851	1854	1859	rVB4	18722	24517	1.88%	0.282%
65	14.526	1878	1879	1882	rBV2	2426	2823	0.22%	0.032%
66	14.603	1886	1892	1899	rVV	185597	285224	21.91%	3.275%
67	14.744	1914	1916	1921	rVB6	8210	10954	0.84%	0.126%
68	14.791	1921	1924	1925	rBV2	3901	3744	0.29%	0.043%
69	14.867	1935	1937	1938	rBV2	3099	2681	0.21%	0.031%
70	14.908	1938	1944	1950	rVV	306625	492984	37.88%	5.661%
71	15.067	1964	1971	1977	rBV	76876	126713	9.74%	1.455%
72	15.178	1988	1990	1994	rBV4	4350	7657	0.59%	0.088%
73	15.296	2005	2010	2016	rVB6	20907	36485	2.80%	0.419%
74	15.372	2019	2023	2025	rBV5	4020	4718	0.36%	0.054%
75	15.484	2038	2042	2043	rBV4	3734	4095	0.31%	0.047%
76	15.525	2046	2049	2053	rVV6	6738	9952	0.76%	0.114%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051616.D
 Acq On : 18 Dec 2021 4:30
 Operator : CG/JU
 Sample : M5121-02
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	15.690	2073	2077	2082	rBV5	18324	34403	2.64%	0.395%
78	15.842	2099	2103	2107	rBV4	8673	11201	0.86%	0.129%
79	15.895	2107	2112	2118	rVB	246686	375380	28.84%	4.311%
80	15.995	2125	2129	2136	rVB	52398	71890	5.52%	0.826%
81	16.083	2141	2144	2148	rVB2	11022	13493	1.04%	0.155%
82	16.148	2151	2155	2158	rBV4	15588	20981	1.61%	0.241%
83	16.230	2168	2169	2173	rVB4	6221	6360	0.49%	0.073%
84	16.394	2194	2197	2201	rVB3	13277	15311	1.18%	0.176%
85	16.624	2233	2236	2240	rVB2	34471	46953	3.61%	0.539%
86	16.723	2250	2253	2256	rBV	13468	16977	1.30%	0.195%
87	16.876	2276	2279	2282	rVB2	13373	15469	1.19%	0.178%
88	17.446	2374	2376	2380	rVB4	19669	24500	1.88%	0.281%
89	17.657	2406	2412	2417	rBV	367877	588586	45.22%	6.759%
90	17.751	2423	2428	2434	rVB2	275934	425816	32.72%	4.890%
91	18.057	2476	2480	2481	rBV4	9112	11757	0.90%	0.135%
92	18.298	2519	2521	2527	rVB7	17648	24005	1.84%	0.276%
93	19.091	2652	2656	2661	rBV7	18964	27788	2.14%	0.319%
94	19.625	2744	2747	2751	rVB3	25713	30432	2.34%	0.349%
95	20.031	2811	2816	2822	rVB	354143	493031	37.88%	5.662%
96	21.846	3120	3125	3134	rVB	844449	1301531	100.00%	14.946%
97	21.975	3141	3147	3155	rVB2	331583	590861	45.40%	6.785%
98	23.162	3346	3349	3362	rVB	68944	177214	13.62%	2.035%
99	25.224	3693	3700	3715	rVB4	154719	486953	37.41%	5.592%
100	25.470	3735	3742	3759	rVB2	195533	604052	46.41%	6.937%




Sum of corrected areas: 8708040

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051616.D
Acq On : 18 Dec 2021 4:30
Operator : CG/JU
Sample : M5121-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL51

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

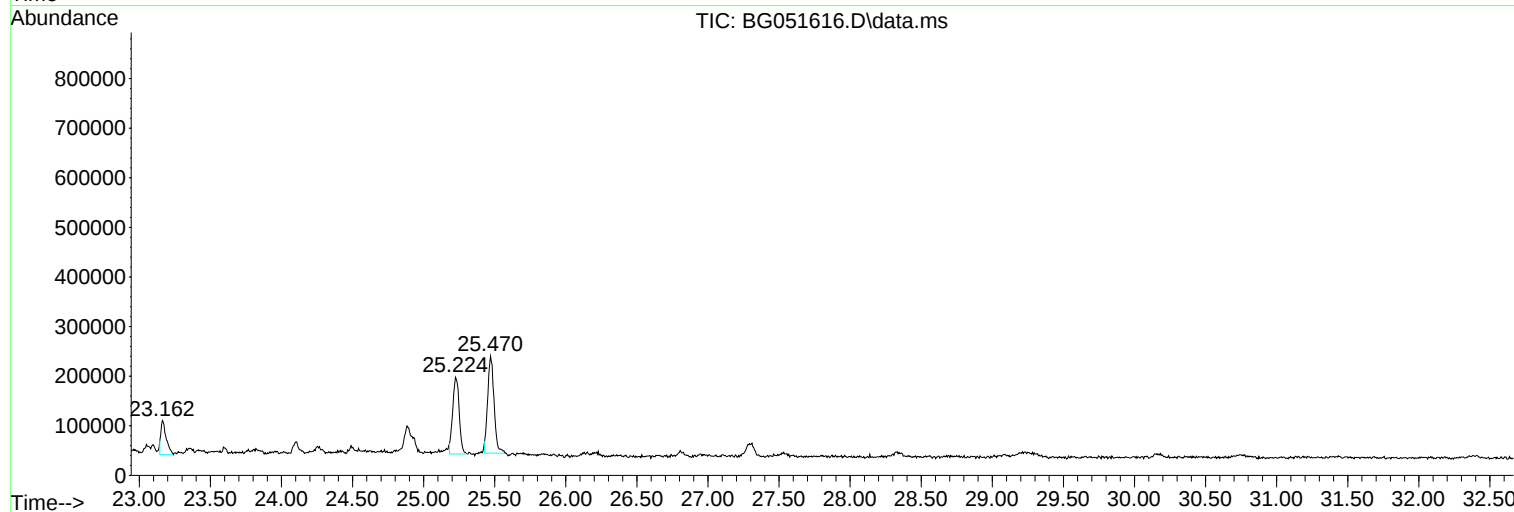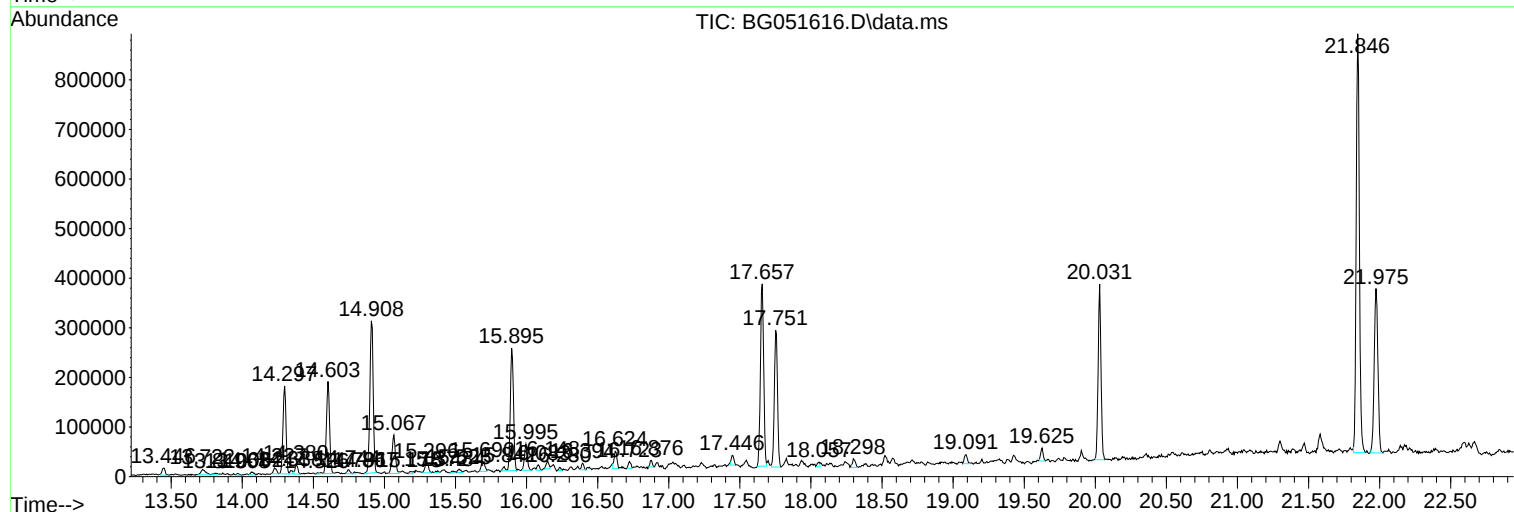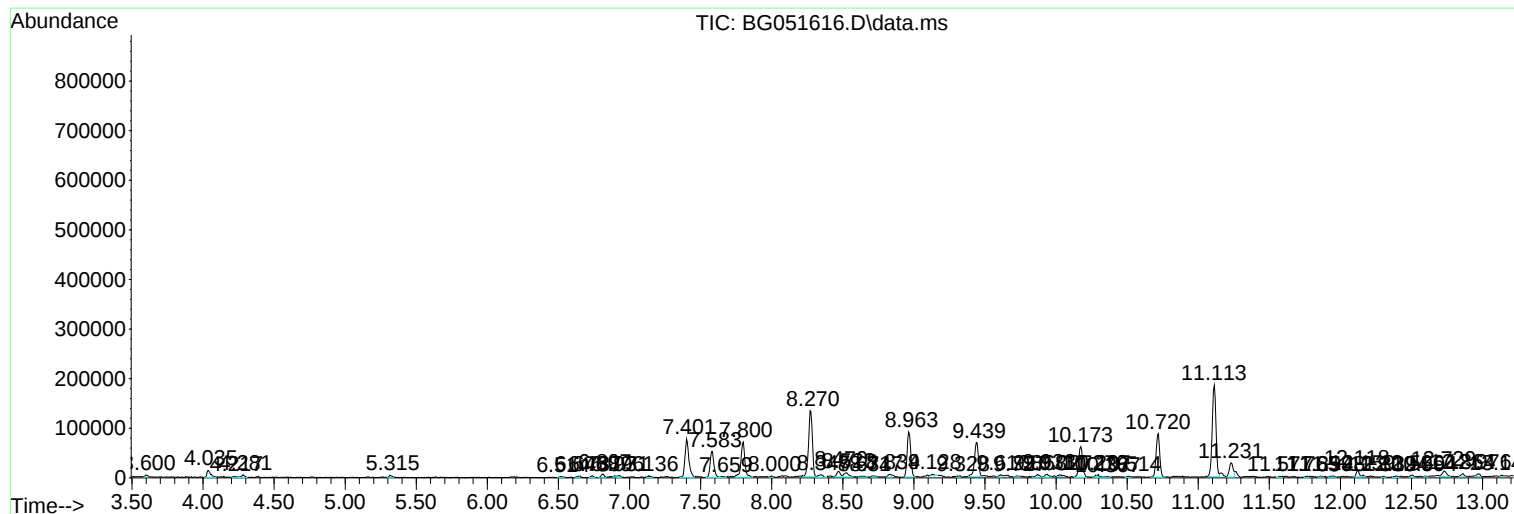

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051616.D
Acq On : 18 Dec 2021 4:30
Operator : CG/JU
Sample : M5121-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL51

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051616.D
Acq On : 18 Dec 2021 4:30
Operator : CG/JU
Sample : M5121-02
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL51

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc