

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051619.D
 Acq On : 18 Dec 2021 7:12
 Operator : CG/JU
 Sample : PB141449BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK449

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051619.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.603	13	19	24	rBV	10305	16868	1.42%	0.144%
2	3.779	44	49	52	rVB3	724	1201	0.10%	0.010%
3	3.838	56	59	62	rBV2	1461	1307	0.11%	0.011%
4	3.867	62	64	69	rBV4	773	1375	0.12%	0.012%
5	3.973	79	82	88	rBV3	1704	2209	0.19%	0.019%
6	4.032	88	92	102	rBV	34409	61133	5.15%	0.524%
7	4.102	102	104	108	rVB4	1868	1621	0.14%	0.014%
8	4.214	122	123	128	rVB3	1125	1408	0.12%	0.012%
9	4.279	130	134	136	rBV2	944	1209	0.10%	0.010%
10	4.384	148	152	156	rBV4	2287	4221	0.36%	0.036%
11	5.976	419	423	424	rBV	1570	1493	0.13%	0.013%
12	7.404	659	666	674	rBV	197728	337319	28.41%	2.889%
13	7.580	689	696	704	rVB	135063	226347	19.07%	1.938%
14	7.797	726	733	740	rBV	182414	309697	26.09%	2.652%
15	8.273	807	814	821	rVB	139832	232476	19.58%	1.991%
16	8.966	925	932	941	rBV	228004	400388	33.72%	3.429%
17	9.442	1005	1013	1020	rVB	186973	322091	27.13%	2.758%
18	10.177	1130	1138	1145	rBV	149014	270784	22.81%	2.319%
19	10.365	1165	1170	1176	rBV2	648	1442	0.12%	0.012%
20	10.717	1221	1230	1238	rBV	235220	419164	35.31%	3.590%
21	11.111	1290	1297	1307	rVB	176664	330013	27.80%	2.826%
22	12.673	1559	1563	1571	rBV3	3469	6316	0.53%	0.054%
23	14.300	1833	1840	1847	rBV	444613	640362	53.94%	5.484%
24	14.606	1885	1892	1900	rVB	464358	739189	62.26%	6.330%
25	14.911	1936	1944	1953	rVB	299114	482670	40.66%	4.133%
26	15.064	1964	1970	1981	rBV	215173	339572	28.60%	2.908%
27	15.317	2009	2013	2015	rVB2	944	1395	0.12%	0.012%
28	15.534	2046	2050	2052	rBV3	826	1383	0.12%	0.012%
29	15.898	2105	2112	2121	rVB	619107	917797	77.31%	7.860%
30	15.998	2123	2129	2137	rVV	180385	265690	22.38%	2.275%
31	16.139	2149	2153	2157	rBV3	2616	3360	0.28%	0.029%
32	16.327	2180	2185	2187	rBV2	1363	1760	0.15%	0.015%
33	16.398	2194	2197	2199	rBV2	1508	1632	0.14%	0.014%
34	16.462	2202	2208	2210	rBV2	1294	1982	0.17%	0.017%
35	17.443	2369	2375	2376	rBV3	2020	2399	0.20%	0.021%
36	17.655	2405	2411	2418	rBV	412964	603144	50.80%	5.165%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051619.D
 Acq On : 18 Dec 2021 7:12
 Operator : CG/JU
 Sample : PB141449BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK449

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	17.755	2420	2428	2435	rVV	698998	1024062	86.26%	8.770%
38	17.807	2435	2437	2441	rVB2	1304	1577	0.13%	0.014%
39	18.060	2479	2480	2485	rBV4	1568	1413	0.12%	0.012%
40	18.125	2489	2491	2493	rBV2	962	1205	0.10%	0.010%
41	18.236	2509	2510	2514	rBV	1135	1213	0.10%	0.010%
42	18.348	2527	2529	2532	rVB4	1128	1233	0.10%	0.011%
43	18.536	2560	2561	2566	rVB3	1432	1552	0.13%	0.013%
44	18.583	2566	2569	2570	rBV2	1440	1318	0.11%	0.011%
45	18.630	2574	2577	2580	rBV4	1155	1734	0.15%	0.015%
46	18.706	2588	2590	2592	rBV3	2113	1206	0.10%	0.010%
47	18.771	2595	2601	2602	rBV3	1503	1937	0.16%	0.017%
48	18.824	2605	2610	2612	rBV3	1832	3243	0.27%	0.028%
49	18.847	2612	2614	2618	rVB2	1512	1808	0.15%	0.015%
50	18.929	2626	2628	2630	rBV2	1887	2148	0.18%	0.018%
51	18.982	2635	2637	2641	rBV4	1671	2194	0.18%	0.019%
52	19.018	2641	2643	2646	rVB2	1378	1428	0.12%	0.012%
53	19.123	2658	2661	2662	rBV3	1435	1221	0.10%	0.010%
54	19.270	2683	2686	2687	rBV2	2027	1549	0.13%	0.013%
55	19.435	2712	2714	2717	rVB3	2413	2396	0.20%	0.021%
56	19.464	2717	2719	2720	rBV	2665	2107	0.18%	0.018%
57	19.540	2728	2732	2733	rBV3	1381	1941	0.16%	0.017%
58	19.593	2736	2741	2746	rBV3	10017	16663	1.40%	0.143%
59	19.664	2749	2753	2759	rVV2	8541	14091	1.19%	0.121%
60	19.722	2762	2763	2765	rBV2	2467	1736	0.15%	0.015%
61	19.934	2797	2799	2803	rVB5	2525	2628	0.22%	0.023%
62	19.963	2803	2804	2805	rBV	2711	1277	0.11%	0.011%
63	20.028	2809	2815	2823	rVV	822653	1187225	100.00%	10.167%
64	20.122	2827	2831	2833	rBV5	3925	4079	0.34%	0.035%
65	20.157	2835	2837	2838	rBV2	1948	1230	0.10%	0.011%
66	20.204	2843	2845	2846	rBV2	2801	2246	0.19%	0.019%
67	20.322	2863	2865	2867	rVB3	2602	1313	0.11%	0.011%
68	20.427	2881	2883	2888	rBV5	2731	3861	0.33%	0.033%
69	20.521	2898	2899	2900	rBV	3234	2085	0.18%	0.018%
70	20.774	2940	2942	2943	rVB2	3742	1535	0.13%	0.013%
71	20.950	2970	2972	2974	rBV3	5771	5244	0.44%	0.045%
72	21.062	2989	2991	2992	rBV2	4606	2429	0.20%	0.021%
73	21.126	3000	3002	3004	rVB3	5318	3496	0.29%	0.030%
74	21.226	3017	3019	3023	rVB5	5782	4566	0.38%	0.039%
75	21.291	3028	3030	3033	rBV4	3701	3427	0.29%	0.029%
76	21.356	3039	3041	3044	rBV4	5374	4613	0.39%	0.040%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051619.D
 Acq On : 18 Dec 2021 7:12
 Operator : CG/JU
 Sample : PB141449BL
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK449

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	21.702	3098	3100	3102	rBV3	5745	4003	0.34%	0.034%
78	21.972	3139	3146	3153	rBV	363159	621156	52.32%	5.319%
79	22.525	3236	3240	3241	rBV4	5639	6055	0.51%	0.052%
80	22.906	3303	3305	3306	rBV2	5278	2786	0.23%	0.024%
81	24.481	3571	3573	3582	rVB7	12899	22467	1.89%	0.192%
82	24.833	3632	3633	3635	rVB2	5380	2278	0.19%	0.020%
83	25.227	3690	3700	3714	rVB2	371106	1117706	94.14%	9.572%
84	25.468	3730	3741	3750	rBV2	187279	613991	51.72%	5.258%
85	27.471	4080	4082	4086	rVB6	5442	6035	0.51%	0.052%
86	28.299	4222	4223	4225	rBV2	7240	6047	0.51%	0.052%




Sum of corrected areas: 11677170

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051619.D
Acq On : 18 Dec 2021 7:12
Operator : CG/JU
Sample : PB141449BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

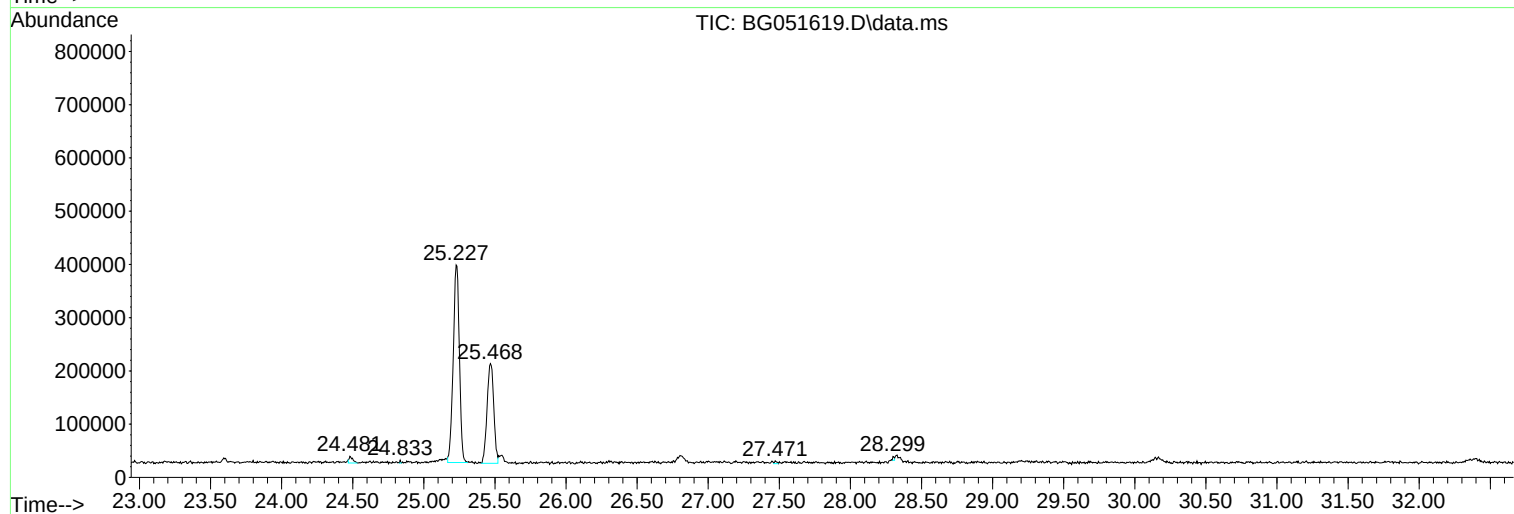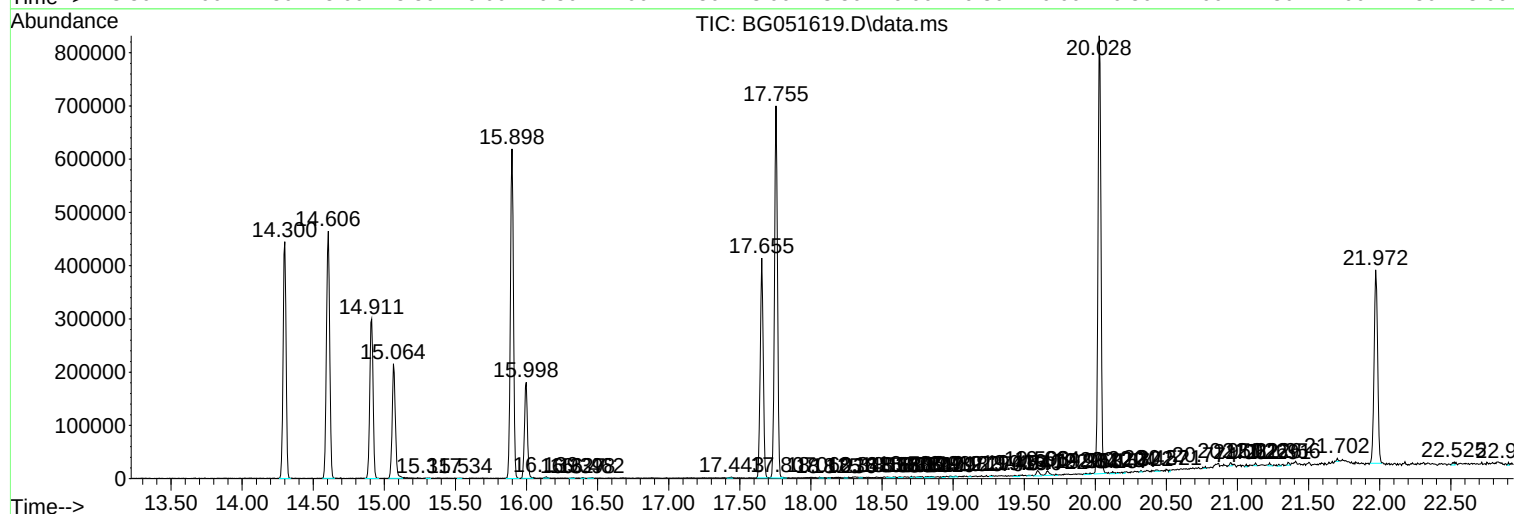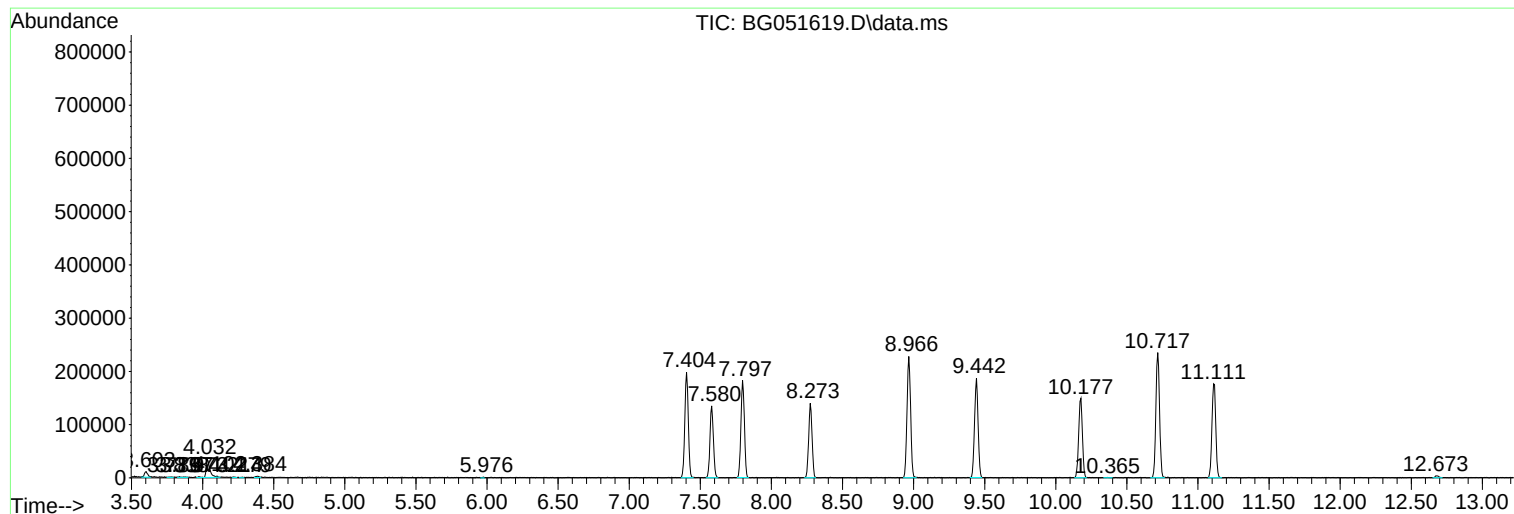

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051619.D
Acq On : 18 Dec 2021 7:12
Operator : CG/JU
Sample : PB141449BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051619.D
Acq On : 18 Dec 2021 7:12
Operator : CG/JU
Sample : PB141449BL
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK449

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc