

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051620.D
 Acq On : 18 Dec 2021 7:52
 Operator : CG/JU
 Sample : PB141497BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK497

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051620.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.600	14	19	26	rVB	10338	15949	1.38%	0.141%
2	3.823	55	57	60	rBV3	1143	1307	0.11%	0.012%
3	3.888	66	68	71	rBV2	1210	1364	0.12%	0.012%
4	4.029	88	92	105	rBV	87133	154847	13.44%	1.366%
5	4.140	109	111	116	rVB3	1566	2385	0.21%	0.021%
6	4.181	116	118	125	rVB3	1024	1500	0.13%	0.013%
7	4.387	146	153	158	rVB4	2553	4898	0.43%	0.043%
8	4.604	187	190	193	rVV2	1022	1374	0.12%	0.012%
9	5.515	343	345	351	rVB	804	1357	0.12%	0.012%
10	5.568	351	354	357	rBV	956	1203	0.10%	0.011%
11	7.400	659	666	674	rBV	184243	319265	27.71%	2.817%
12	7.577	690	696	708	rVB	122177	211174	18.33%	1.863%
13	7.688	714	715	719	rBV	1243	1208	0.10%	0.011%
14	7.800	727	734	741	rVB	169861	286264	24.85%	2.526%
15	8.276	808	815	825	rVB	132006	221769	19.25%	1.957%
16	8.969	925	933	940	rBV2	206014	371489	32.25%	3.278%
17	9.439	1004	1013	1022	rBV	168336	297653	25.84%	2.627%
18	10.173	1128	1138	1147	rVB	142824	259755	22.55%	2.292%
19	10.267	1153	1154	1160	rVB	1367	1263	0.11%	0.011%
20	10.373	1168	1172	1175	rBV	885	1376	0.12%	0.012%
21	10.719	1222	1231	1241	rVB	214071	392328	34.05%	3.462%
22	11.113	1288	1298	1305	rBV	174153	312354	27.11%	2.756%
23	11.231	1310	1318	1326	rVV	114263	202900	17.61%	1.790%
24	12.682	1558	1565	1570	rBV2	3316	5988	0.52%	0.053%
25	13.363	1677	1681	1684	rBV2	836	1400	0.12%	0.012%
26	14.297	1832	1840	1848	rBV	410285	589771	51.19%	5.204%
27	14.367	1848	1852	1856	rVB	863	1418	0.12%	0.013%
28	14.602	1884	1892	1900	rBV	442443	702252	60.96%	6.197%
29	14.908	1938	1944	1951	rVB	295949	457255	39.69%	4.035%
30	15.067	1964	1971	1979	rVV	206551	324015	28.12%	2.859%
31	15.119	1979	1980	1986	rVV2	3447	4043	0.35%	0.036%
32	15.196	1990	1993	1995	rVB2	1229	1293	0.11%	0.011%
33	15.536	2049	2051	2055	rBV2	900	1186	0.10%	0.010%
34	15.895	2104	2112	2119	rBV	570371	861353	74.77%	7.601%
35	15.995	2123	2129	2140	rVB	175962	260697	22.63%	2.300%
36	16.142	2149	2154	2156	rVB4	1749	2518	0.22%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051620.D
 Acq On : 18 Dec 2021 7:52
 Operator : CG/JU
 Sample : PB141497BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK497

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	17.651	2404	2411	2418	rBV	369480	578556	50.22%	5.105%
38	17.751	2421	2428	2437	rBV	625461	995400	86.40%	8.784%
39	18.010	2469	2472	2473	rBV2	1308	1535	0.13%	0.014%
40	18.162	2494	2498	2501	rBV3	1019	1535	0.13%	0.014%
41	18.491	2552	2554	2557	rBV2	1633	2105	0.18%	0.019%
42	18.568	2565	2567	2569	rBV	1357	1258	0.11%	0.011%
43	18.650	2580	2581	2586	rBV2	1747	2130	0.18%	0.019%
44	18.697	2586	2589	2591	rVB3	1427	1289	0.11%	0.011%
45	18.779	2600	2603	2605	rVV2	1579	1867	0.16%	0.016%
46	18.803	2605	2607	2610	rVB3	1898	1193	0.10%	0.011%
47	18.867	2616	2618	2620	rBV2	1289	1164	0.10%	0.010%
48	18.955	2631	2633	2636	rVB2	1644	1354	0.12%	0.012%
49	19.132	2660	2663	2665	rVB4	2119	2083	0.18%	0.018%
50	19.155	2665	2667	2669	rBV3	1777	1699	0.15%	0.015%
51	19.208	2674	2676	2679	rVB3	1225	1346	0.12%	0.012%
52	19.243	2681	2682	2686	rBV3	1322	1755	0.15%	0.015%
53	19.308	2689	2693	2695	rBV4	1787	2181	0.19%	0.019%
54	19.372	2703	2704	2708	rBV4	1565	1399	0.12%	0.012%
55	19.496	2723	2725	2727	rBV2	1738	1339	0.12%	0.012%
56	19.525	2727	2730	2731	rVV3	1897	1488	0.13%	0.013%
57	19.602	2738	2743	2747	rVB3	9178	12452	1.08%	0.110%
58	19.660	2750	2753	2758	rVB2	9747	13428	1.17%	0.118%
59	19.889	2789	2792	2793	rVB3	1789	1569	0.14%	0.014%
60	19.901	2793	2794	2796	rBV2	1736	1532	0.13%	0.014%
61	19.960	2802	2804	2805	rBV	1656	1162	0.10%	0.010%
62	20.030	2809	2816	2824	rVV	813875	1152065	100.00%	10.166%
63	20.089	2824	2826	2827	rVV2	2182	1524	0.13%	0.013%
64	20.119	2830	2831	2835	rVV4	2857	2369	0.21%	0.021%
65	20.160	2835	2838	2839	rVB3	2462	2156	0.19%	0.019%
66	20.306	2862	2863	2865	rBV2	2903	1737	0.15%	0.015%
67	20.706	2929	2931	2932	rVB2	4454	2614	0.23%	0.023%
68	20.724	2932	2934	2935	rBV2	2477	1563	0.14%	0.014%
69	20.741	2935	2937	2939	rBV3	2823	2957	0.26%	0.026%
70	20.765	2939	2941	2942	rVB2	3290	2052	0.18%	0.018%
71	20.953	2972	2973	2974	rBV	4405	2134	0.19%	0.019%
72	20.970	2974	2976	2978	rVB3	3832	2876	0.25%	0.025%
73	21.975	3140	3147	3157	rVB2	343264	598523	51.95%	5.281%
74	23.596	3420	3423	3426	rBV5	6742	8577	0.74%	0.076%
75	24.871	3638	3640	3641	rBV2	4683	2941	0.26%	0.026%
76	25.229	3691	3701	3712	rVB2	360920	1074051	93.23%	9.478%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051620.D
Acq On : 18 Dec 2021 7:52
Operator : CG/JU
Sample : PB141497BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK497

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Title : SVOA CALIBRATION

77	25.470	3732	3742	3752	rBV	189713	552611	47.97%	4.876%
78	28.419	4242	4244	4245	rBV2	4117	2347	0.20%	0.021%
79	29.800	4478	4479	4480	rBV	4303	2084	0.18%	0.018%
80	30.363	4574	4575	4578	rBV3	4402	3188	0.28%	0.028%
81	31.891	4833	4835	4838	rBV3	4172	3087	0.27%	0.027%




Sum of corrected areas: 11332446

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051620.D
Acq On : 18 Dec 2021 7:52
Operator : CG/JU
Sample : PB141497BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK497

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

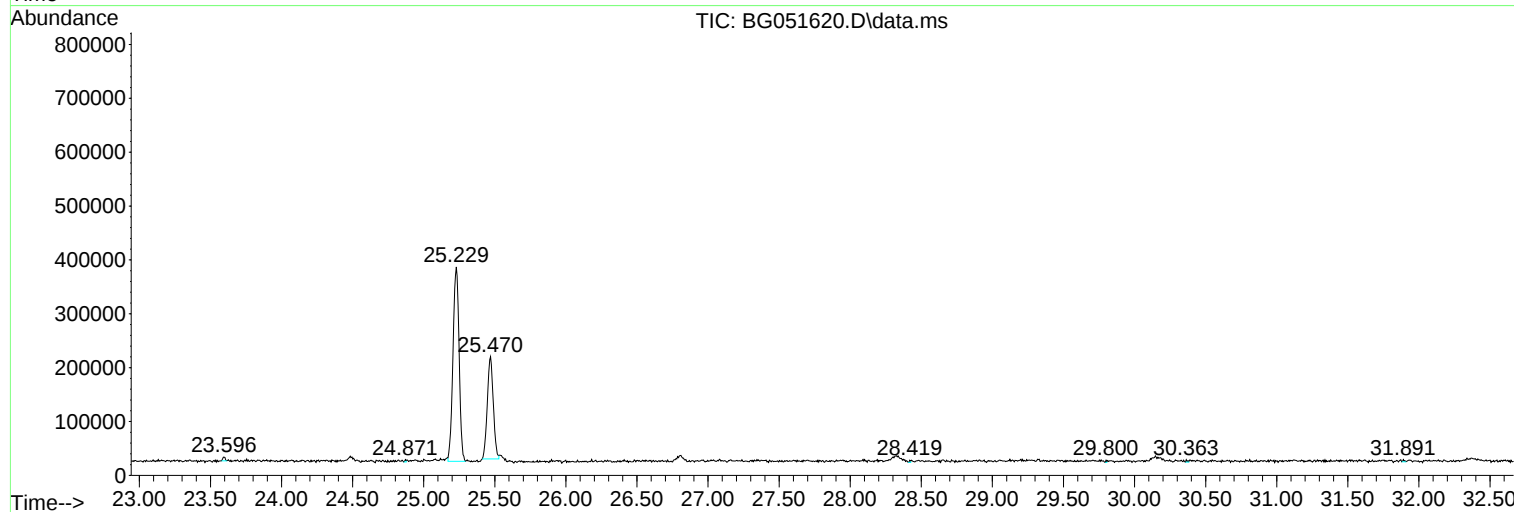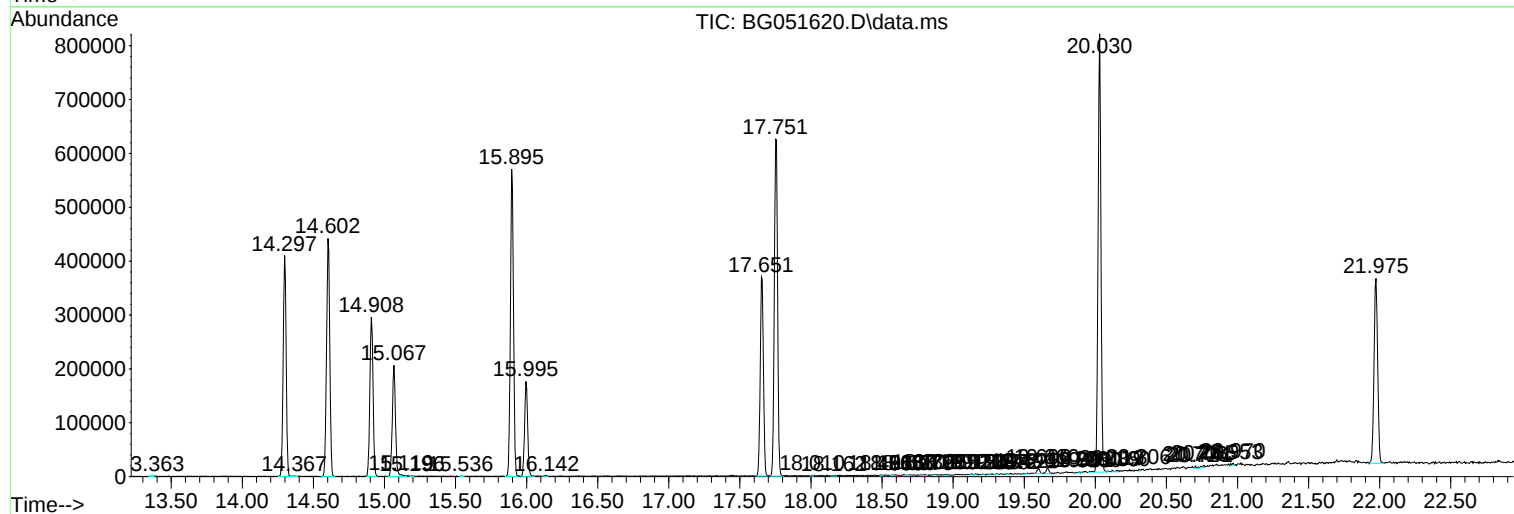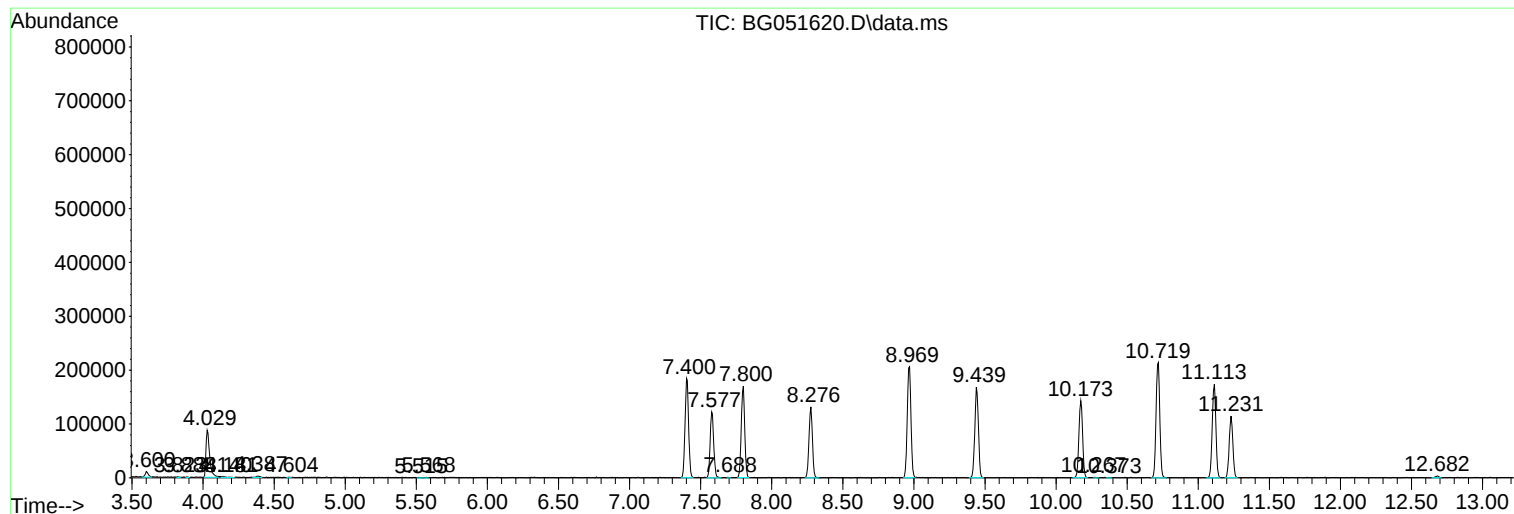

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051620.D
Acq On : 18 Dec 2021 7:52
Operator : CG/JU
Sample : PB141497BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK497

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051620.D
Acq On : 18 Dec 2021 7:52
Operator : CG/JU
Sample : PB141497BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK497

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc