

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051621.D
 Acq On : 18 Dec 2021 8:33
 Operator : CG/JU
 Sample : PB141486BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK486

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051621.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.596	14	18	24	rBV2	12298	18559	1.36%	0.131%
2	3.772	45	48	51	rBV4	1269	1457	0.11%	0.010%
3	4.025	87	91	107	rBV	102720	180747	13.23%	1.275%
4	4.383	148	152	159	rVB2	3681	5825	0.43%	0.041%
5	5.394	322	324	328	rBV2	1365	1964	0.14%	0.014%
6	7.403	658	666	675	rVB	218964	374031	27.37%	2.638%
7	7.579	689	696	703	rBV	144589	247750	18.13%	1.748%
8	7.796	726	733	740	rBV	200922	344751	25.23%	2.432%
9	8.272	806	814	821	rBV	171029	294737	21.57%	2.079%
10	8.965	923	932	942	rVB	260466	446505	32.68%	3.150%
11	9.441	1005	1013	1023	rVB	202346	362064	26.50%	2.554%
12	10.170	1130	1137	1145	rVB	169065	309611	22.66%	2.184%
13	10.716	1221	1230	1242	rBV	268263	466075	34.11%	3.288%
14	11.110	1288	1297	1306	rVB	233310	437111	31.99%	3.083%
15	11.233	1310	1318	1326	rVV	145522	273519	20.02%	1.929%
16	12.678	1559	1564	1570	rVB	3643	6752	0.49%	0.048%
17	13.318	1671	1673	1676	rBV	994	1551	0.11%	0.011%
18	14.299	1832	1840	1847	rBV	507418	719131	52.63%	5.073%
19	14.605	1884	1892	1899	rBV	534423	843560	61.73%	5.951%
20	14.910	1936	1944	1951	rBV	405786	644435	47.16%	4.546%
21	15.069	1962	1971	1979	rBV	243422	390835	28.60%	2.757%
22	15.275	2002	2006	2010	rVB2	1178	2049	0.15%	0.014%
23	15.897	2105	2112	2120	rBV	708972	1046031	76.55%	7.379%
24	15.997	2123	2129	2136	rBV	213050	321968	23.56%	2.271%
25	16.132	2148	2152	2157	rBV3	2167	3156	0.23%	0.022%
26	17.425	2371	2372	2375	rVV	1990	2377	0.17%	0.017%
27	17.448	2375	2376	2379	rVV	2032	1740	0.13%	0.012%
28	17.654	2404	2411	2419	rVB	534595	810883	59.34%	5.720%
29	17.754	2421	2428	2436	rVV2	765194	1189190	87.03%	8.389%
30	18.012	2470	2472	2478	rVB3	1503	2637	0.19%	0.019%
31	18.417	2538	2541	2543	rBV3	1269	1639	0.12%	0.012%
32	18.870	2616	2618	2621	rVB	2111	1877	0.14%	0.013%
33	19.069	2650	2652	2654	rBV3	1627	1749	0.13%	0.012%
34	19.204	2673	2675	2678	rBV3	1210	1466	0.11%	0.010%
35	19.316	2692	2694	2698	rVB4	1976	1715	0.13%	0.012%
36	19.398	2706	2708	2711	rBV3	1573	1586	0.12%	0.011%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051621.D
 Acq On : 18 Dec 2021 8:33
 Operator : CG/JU
 Sample : PB141486BL
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK486

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	19.457	2716	2718	2720	rBV3	1625	1389	0.10%	0.010%
38	19.481	2720	2722	2725	rBV3	1555	2288	0.17%	0.016%
39	19.516	2727	2728	2731	rBV2	2115	2419	0.18%	0.017%
40	19.539	2731	2732	2734	rVV2	1836	1490	0.11%	0.011%
41	19.598	2737	2742	2746	rVV3	10468	15243	1.12%	0.108%
42	19.669	2746	2754	2758	rVV2	9223	15861	1.16%	0.112%
43	19.933	2797	2799	2804	rVB5	4158	4798	0.35%	0.034%
44	20.027	2809	2815	2822	rVV	927079	1366439	100.00%	9.639%
45	20.150	2834	2836	2837	rVB2	2698	1592	0.12%	0.011%
46	20.168	2837	2839	2840	rBV	2905	1819	0.13%	0.013%
47	20.197	2842	2844	2845	rVV	2996	1671	0.12%	0.012%
48	20.215	2845	2847	2852	rVB6	2755	3847	0.28%	0.027%
49	20.338	2866	2868	2870	rVB2	2752	1678	0.12%	0.012%
50	20.403	2877	2879	2881	rBV3	3397	2223	0.16%	0.016%
51	21.231	3019	3020	3023	rBV3	4644	4485	0.33%	0.032%
52	21.413	3049	3051	3052	rBV2	4322	3306	0.24%	0.023%
53	21.466	3058	3060	3062	rVB3	3978	2248	0.16%	0.016%
54	21.537	3070	3072	3074	rBV3	3350	2853	0.21%	0.020%
55	21.701	3098	3100	3105	rBV6	4770	9075	0.66%	0.064%
56	21.877	3128	3130	3131	rBV2	3742	1951	0.14%	0.014%
57	21.971	3139	3146	3155	rVB	500574	840833	61.53%	5.931%
58	23.082	3333	3335	3336	rVB2	4369	2042	0.15%	0.014%
59	23.722	3442	3444	3445	rBV	5438	4001	0.29%	0.028%
60	24.133	3512	3514	3516	rBV3	3988	3008	0.22%	0.021%
61	24.480	3569	3573	3574	rBV4	10323	13907	1.02%	0.098%
62	25.232	3689	3701	3712	rVB2	423146	1270250	92.96%	8.960%
63	25.472	3730	3742	3752	rBV3	266810	815888	59.71%	5.755%
64	26.442	3905	3907	3908	rVB2	4226	1819	0.13%	0.013%
65	26.894	3982	3984	3985	rBV2	4633	2993	0.22%	0.021%
66	27.564	4096	4098	4100	rBV3	5279	3330	0.24%	0.023%
67	29.491	4424	4426	4428	rBV3	4888	4398	0.32%	0.031%
68	31.629	4788	4790	4791	rBV2	4019	2716	0.20%	0.019%
69	32.328	4907	4909	4911	rBV3	4653	3384	0.25%	0.024%




Sum of corrected areas: 14176277

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051621.D
Acq On : 18 Dec 2021 8:33
Operator : CG/JU
Sample : PB141486BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

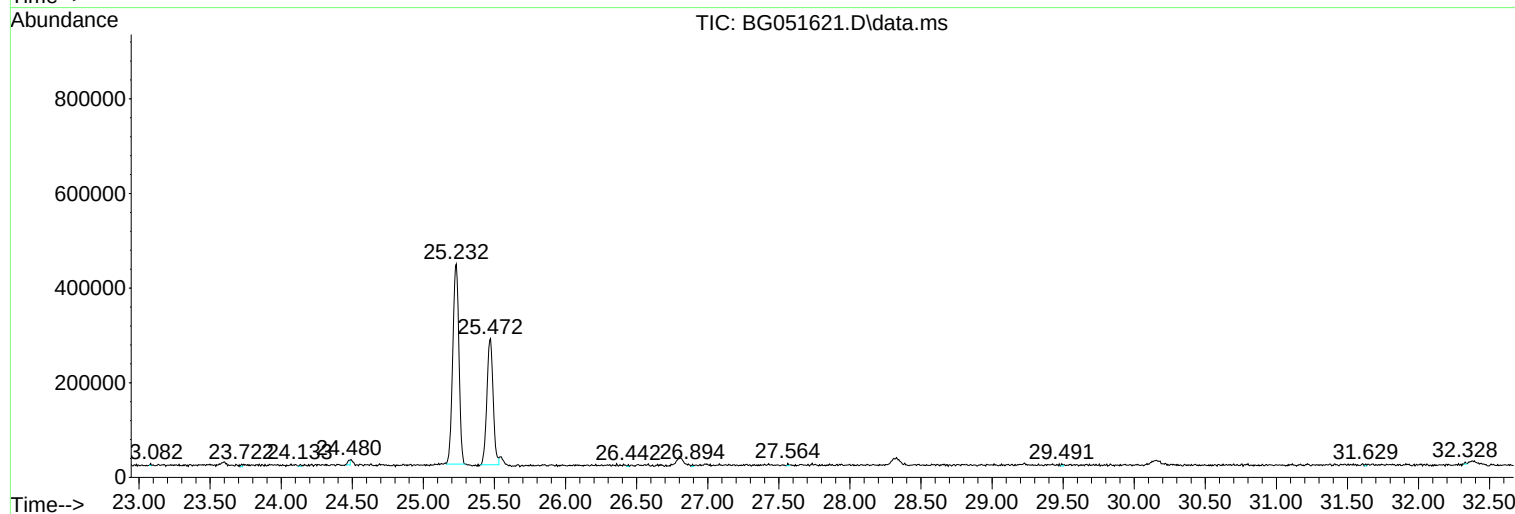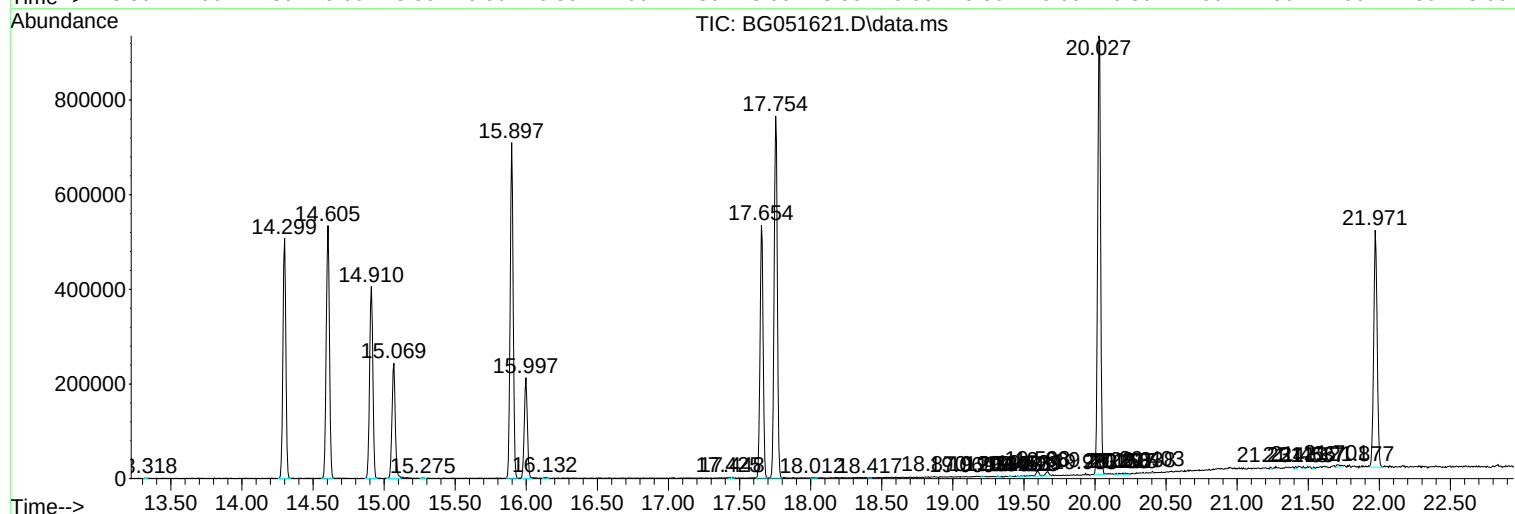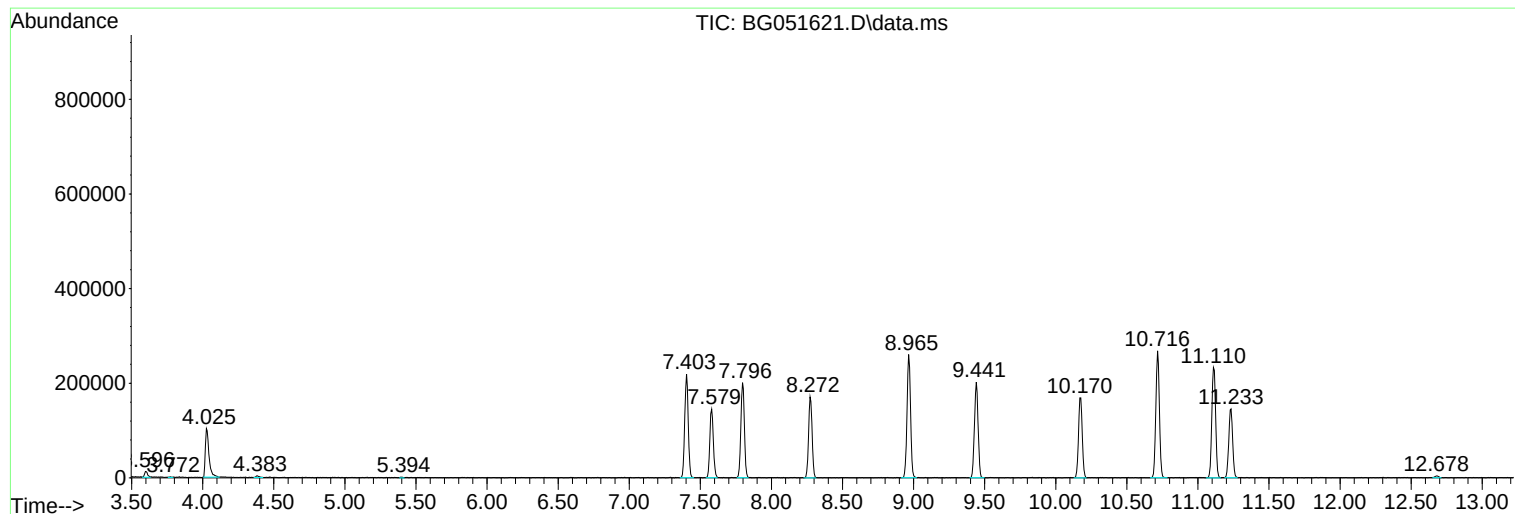

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051621.D
Acq On : 18 Dec 2021 8:33
Operator : CG/JU
Sample : PB141486BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051621.D
Acq On : 18 Dec 2021 8:33
Operator : CG/JU
Sample : PB141486BL
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK486

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc