

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051635.D
 Acq On : 18 Dec 2021 18:43
 Operator : CG/JU
 Sample : PB141535BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK535

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051635.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.603	15	19	25	rVB	10372	16367	1.41%	0.134%
2	3.673	28	31	32	rVB2	1382	1265	0.11%	0.010%
3	3.714	35	38	39	rVB2	1500	1426	0.12%	0.012%
4	4.026	86	91	107	rBV	136436	236921	20.41%	1.936%
5	4.378	148	151	157	rVB2	3116	4364	0.38%	0.036%
6	4.472	164	167	169	rBV2	930	1229	0.11%	0.010%
7	4.519	173	175	179	rVV3	907	1171	0.10%	0.010%
8	4.842	229	230	234	rVB2	1129	1171	0.10%	0.010%
9	4.960	247	250	254	rVB2	884	1206	0.10%	0.010%
10	5.071	266	269	272	rBV2	1129	1205	0.10%	0.010%
11	5.230	292	296	299	rBV	875	1376	0.12%	0.011%
12	5.512	342	344	349	rVB	735	1174	0.10%	0.010%
13	5.594	353	358	360	rVB	953	1301	0.11%	0.011%
14	5.741	378	383	384	rBV	1093	1383	0.12%	0.011%
15	7.403	658	666	673	rBV	194207	323457	27.86%	2.644%
16	7.580	689	696	705	rVB	130628	214761	18.50%	1.755%
17	7.797	724	733	740	rVV	170442	298172	25.68%	2.437%
18	8.108	782	786	789	rBV2	1026	1517	0.13%	0.012%
19	8.273	807	814	822	rVB	138890	235912	20.32%	1.928%
20	8.966	925	932	946	rBV	225387	385551	33.21%	3.151%
21	9.442	1005	1013	1021	rBV	177002	311626	26.84%	2.547%
22	10.176	1129	1138	1148	rBV2	146121	267228	23.02%	2.184%
23	10.717	1222	1230	1240	rBV	228442	400539	34.50%	3.274%
24	11.110	1290	1297	1307	rVB	191526	350929	30.23%	2.868%
25	11.233	1310	1318	1326	rBV	215258	396037	34.11%	3.237%
26	12.679	1560	1564	1569	rVB3	3475	5790	0.50%	0.047%
27	13.613	1719	1723	1726	rVB	913	1263	0.11%	0.010%
28	13.883	1762	1769	1772	rBV2	798	1975	0.17%	0.016%
29	14.300	1831	1840	1847	rBV	413811	615324	53.00%	5.029%
30	14.605	1884	1892	1903	rVB	464309	725039	62.45%	5.926%
31	14.911	1937	1944	1951	rVB	333747	517692	44.59%	4.231%
32	15.064	1964	1970	1984	rBV	190984	311427	26.83%	2.545%
33	15.539	2048	2051	2052	rBV	1150	1213	0.10%	0.010%
34	15.898	2104	2112	2119	rVB	612573	894404	77.04%	7.310%
35	15.998	2123	2129	2138	rBV	157474	231869	19.97%	1.895%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051635.D
 Acq On : 18 Dec 2021 18:43
 Operator : CG/JU
 Sample : PB141535BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK535

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

36	16.139	2150	2153	2158	rVB3	2420	3315	0.29%	0.027%
37	16.679	2242	2245	2249	rVB2	928	1181	0.10%	0.010%
38	17.437	2370	2374	2379	rBV2	1628	2872	0.25%	0.023%
39	17.595	2396	2401	2404	rVB3	1166	1434	0.12%	0.012%
40	17.654	2404	2411	2419	rBV	424051	653532	56.29%	5.342%
41	17.754	2421	2428	2437	rBV2	676525	998113	85.97%	8.158%
42	18.277	2516	2517	2522	rVV3	1263	1220	0.11%	0.010%
43	18.447	2541	2546	2547	rVB	1514	1983	0.17%	0.016%
44	18.459	2547	2548	2551	rBV2	1538	1302	0.11%	0.011%
45	18.488	2551	2553	2556	rBV2	1243	1344	0.12%	0.011%
46	18.706	2587	2590	2591	rBV	1546	1362	0.12%	0.011%
47	18.729	2591	2594	2596	rVB2	1017	1185	0.10%	0.010%
48	18.788	2600	2604	2605	rBV2	1438	1768	0.15%	0.014%
49	18.882	2618	2620	2624	rVB3	1130	1279	0.11%	0.010%
50	18.994	2635	2639	2641	rVB3	2136	2064	0.18%	0.017%
51	19.082	2651	2654	2655	rBV2	1404	1237	0.11%	0.010%
52	19.164	2665	2668	2669	rBV3	1812	1901	0.16%	0.016%
53	19.211	2675	2676	2681	rVB4	1188	1336	0.12%	0.011%
54	19.328	2694	2696	2700	rBV3	1076	1430	0.12%	0.012%
55	19.546	2731	2733	2735	rBV2	1563	1304	0.11%	0.011%
56	19.575	2735	2738	2739	rBV3	1646	1979	0.17%	0.016%
57	19.599	2739	2742	2748	rVB5	8537	12127	1.04%	0.099%
58	19.663	2750	2753	2760	rVB2	8663	11039	0.95%	0.090%
59	19.892	2790	2792	2794	rBV2	1183	1238	0.11%	0.010%
60	19.945	2796	2801	2803	rBV6	2506	3366	0.29%	0.028%
61	19.969	2803	2805	2807	rBV3	2942	1810	0.16%	0.015%
62	20.027	2807	2815	2822	rBV	791695	1160936	100.00%	9.489%
63	20.204	2843	2845	2850	rBV5	2483	2412	0.21%	0.020%
64	20.239	2850	2851	2852	rBV	2491	1321	0.11%	0.011%
65	20.333	2863	2867	2869	rBV5	2451	3646	0.31%	0.030%
66	20.356	2869	2871	2874	rVV3	2032	2112	0.18%	0.017%
67	20.433	2882	2884	2887	rVB4	2363	1723	0.15%	0.014%
68	20.539	2901	2902	2905	rBV3	2741	1693	0.15%	0.014%
69	20.615	2912	2915	2918	rBV5	3386	5107	0.44%	0.042%
70	20.674	2923	2925	2926	rBV2	2403	1410	0.12%	0.012%
71	20.756	2938	2939	2943	rBV4	3536	3222	0.28%	0.026%
72	20.897	2960	2963	2965	rBV2	4036	5083	0.44%	0.042%
73	21.978	3139	3147	3155	rBV	390404	701974	60.47%	5.738%
74	22.765	3279	3281	3283	rBV3	3241	3554	0.31%	0.029%
75	22.835	3288	3293	3295	rBV4	6220	9567	0.82%	0.078%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051635.D
 Acq On : 18 Dec 2021 18:43
 Operator : CG/JU
 Sample : PB141535BL
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK535

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

76	23.587	3419	3421	3422	rBV	4448	3203	0.28%	0.026%
77	23.840	3462	3464	3465	rVB2	3947	1969	0.17%	0.016%
78	24.492	3569	3575	3582	rBV7	12055	30066	2.59%	0.246%
79	24.621	3596	3597	3598	rBV	3484	1442	0.12%	0.012%
80	25.232	3691	3701	3713	rVB2	371925	1078447	92.89%	8.815%
81	25.473	3731	3742	3753	rBV2	214007	672504	57.93%	5.497%
82	26.818	3965	3971	3977	rVB7	12011	26914	2.32%	0.220%
83	27.276	4047	4049	4053	rBV4	3428	3644	0.31%	0.030%
84	28.017	4173	4175	4176	rBV	3393	1984	0.17%	0.016%
85	28.316	4222	4226	4228	rBV5	8156	12095	1.04%	0.099%
86	28.475	4251	4253	4254	rVB2	3735	1908	0.16%	0.016%
87	28.751	4298	4300	4301	rBV	3085	1347	0.12%	0.011%
88	30.026	4513	4517	4521	rBV5	3980	7543	0.65%	0.062%
89	30.484	4593	4595	4596	rBV2	4398	3132	0.27%	0.026%
90	31.130	4703	4705	4709	rBV4	3567	3251	0.28%	0.027%
91	31.494	4765	4767	4768	rBV2	4790	2676	0.23%	0.022%
92	31.530	4771	4773	4775	rBV3	3539	2704	0.23%	0.022%




Sum of corrected areas: 12234594

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051635.D
Acq On : 18 Dec 2021 18:43
Operator : CG/JU
Sample : PB141535BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK535

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

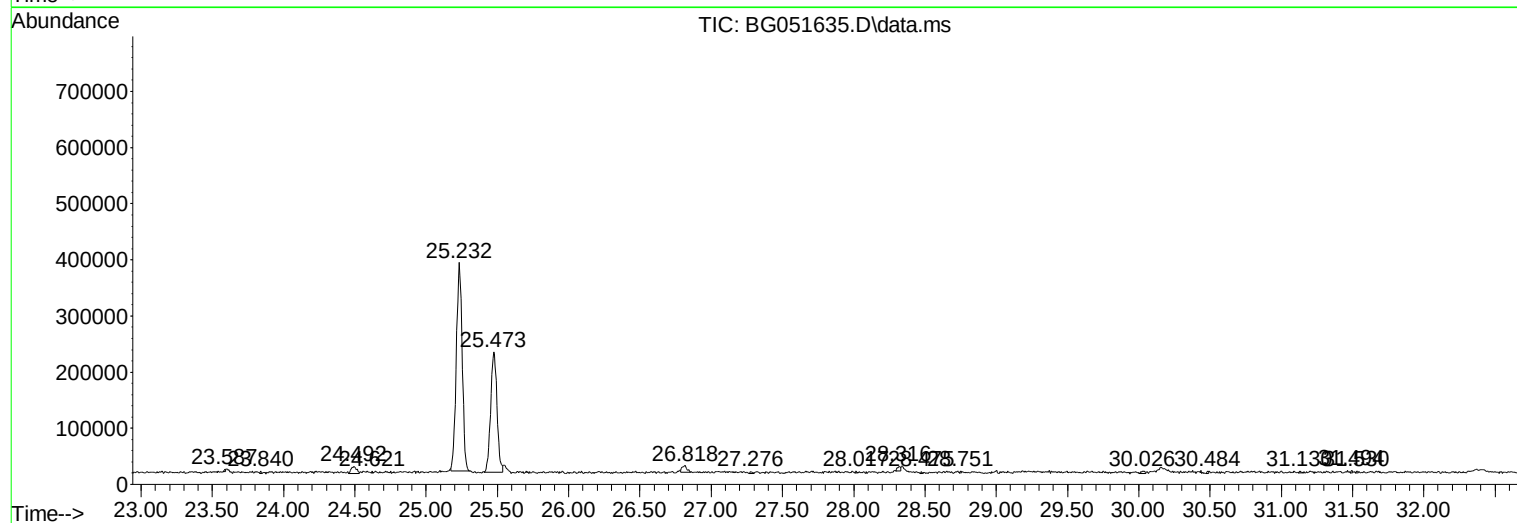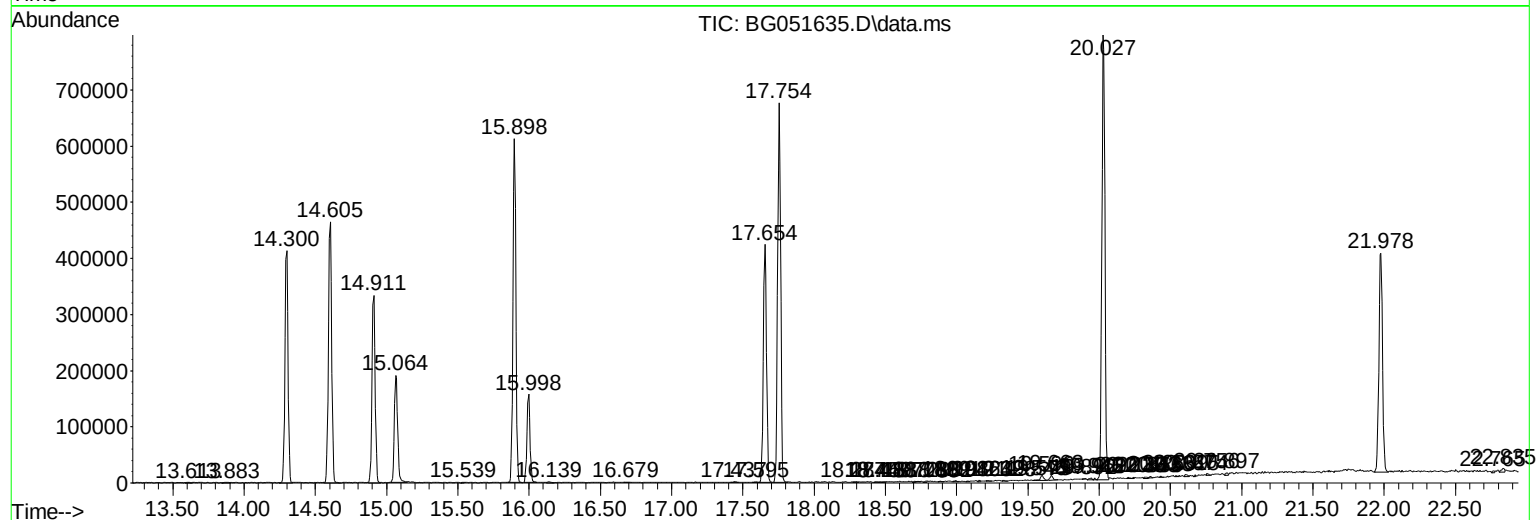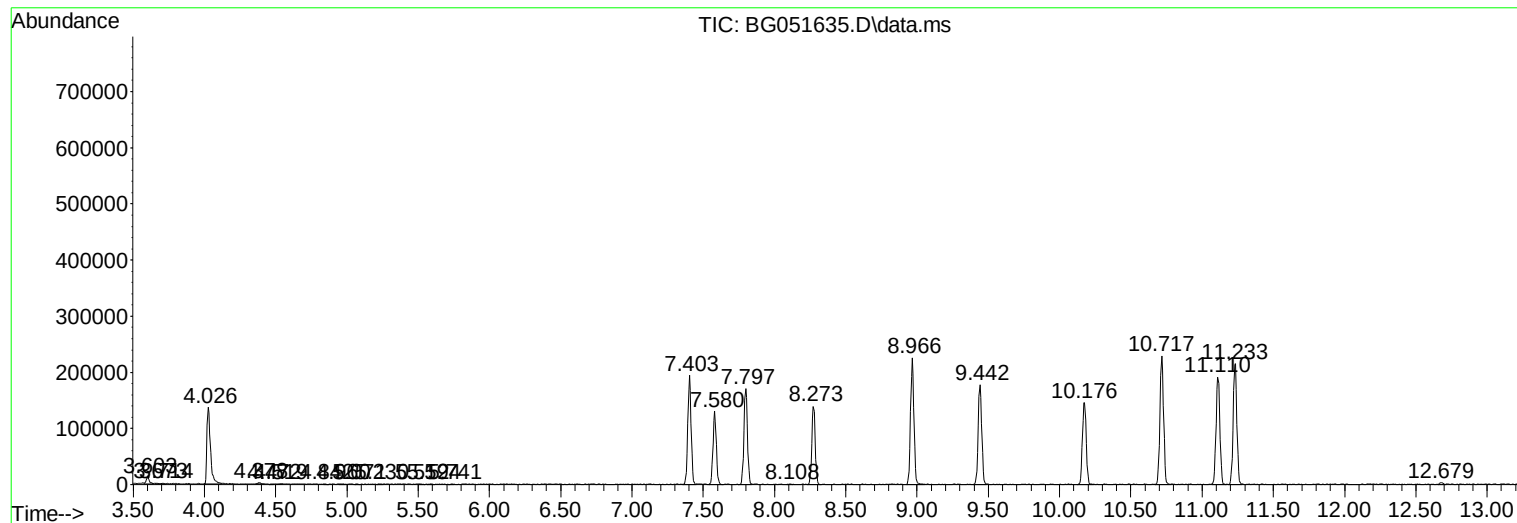

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051635.D
Acq On : 18 Dec 2021 18:43
Operator : CG/JU
Sample : PB141535BL
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK535

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected
