

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051644.D
 Acq On : 19 Dec 2021 00:53
 Operator : CG/JU
 Sample : M5153-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.602	12	19	24	rVB3	4846	8966	1.47%	0.136%
2	3.649	26	27	29	rBV	1449	1272	0.21%	0.019%
3	3.831	56	58	61	rVB2	1191	1126	0.18%	0.017%
4	3.890	65	68	70	rBV3	1337	1208	0.20%	0.018%
5	3.943	75	77	79	rVB2	2210	1246	0.20%	0.019%
6	4.043	91	94	100	rBV2	6003	9825	1.61%	0.149%
7	4.143	109	111	117	rVV3	3031	4179	0.68%	0.063%
8	4.195	119	120	123	rVB3	1677	1108	0.18%	0.017%
9	4.284	130	135	139	rBV7	4287	7213	1.18%	0.109%
10	4.389	149	153	156	rBV2	2343	3417	0.56%	0.052%
11	4.442	158	162	164	rVB2	1344	1361	0.22%	0.021%
12	4.759	213	216	217	rBV	1290	1076	0.18%	0.016%
13	5.118	275	277	278	rBV	1366	1102	0.18%	0.017%
14	5.171	282	286	288	rVB	876	1172	0.19%	0.018%
15	5.323	306	312	318	rBV3	8369	13270	2.17%	0.201%
16	6.146	448	452	453	rBV	798	1101	0.18%	0.017%
17	7.009	597	599	605	rVB	1143	1301	0.21%	0.020%
18	7.403	660	666	678	rVB	80074	146057	23.88%	2.208%
19	7.579	689	696	704	rBV	57422	96360	15.76%	1.457%
20	7.796	727	733	740	rBV	71161	124090	20.29%	1.876%
21	7.890	745	749	757	rVV3	1513	2687	0.44%	0.041%
22	8.061	776	778	784	rVB2	768	1290	0.21%	0.020%
23	8.272	807	814	827	rVB	126413	221425	36.21%	3.347%
24	8.965	925	932	940	rVB	96336	161580	26.42%	2.443%
25	9.101	948	955	958	rVB3	2571	3905	0.64%	0.059%
26	9.365	996	1000	1002	rBV2	780	1122	0.18%	0.017%
27	9.441	1004	1013	1023	rVV	79057	144920	23.70%	2.191%
28	9.541	1027	1030	1034	rVB	1208	1656	0.27%	0.025%
29	9.594	1034	1039	1041	rBV	1016	1522	0.25%	0.023%
30	9.870	1084	1086	1090	rVB3	1285	1639	0.27%	0.025%
31	10.176	1129	1138	1145	rBV2	64196	117671	19.24%	1.779%
32	10.716	1223	1230	1241	rVB2	91075	169014	27.64%	2.555%
33	10.869	1249	1256	1260	rBV3	1608	3585	0.59%	0.054%
34	11.110	1291	1297	1308	rVV	187421	334569	54.71%	5.058%
35	11.233	1310	1318	1325	rBV2	36792	68997	11.28%	1.043%
36	11.362	1339	1340	1345	rVB	974	1074	0.18%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051644.D
 Acq On : 19 Dec 2021 00:53
 Operator : CG/JU
 Sample : M5153-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	11.527	1364	1368	1372	rBV2	1326	1958	0.32%	0.030%
38	11.738	1398	1404	1406	rBV2	765	1155	0.19%	0.017%
39	11.867	1421	1426	1429	rBV5	1398	2160	0.35%	0.033%
40	12.508	1529	1535	1538	rBV4	1041	2138	0.35%	0.032%
41	12.543	1538	1541	1547	rVB3	1938	3185	0.52%	0.048%
42	12.678	1559	1564	1568	rBV2	1448	2765	0.45%	0.042%
43	12.743	1571	1575	1580	rVB2	7143	10942	1.79%	0.165%
44	12.854	1590	1594	1597	rVB2	778	1092	0.18%	0.017%
45	13.389	1682	1685	1692	rVB2	1077	1626	0.27%	0.025%
46	13.448	1692	1695	1699	rBV2	830	1253	0.20%	0.019%
47	13.524	1704	1708	1710	rVB2	874	1156	0.19%	0.017%
48	13.730	1738	1743	1748	rBV3	7174	9240	1.51%	0.140%
49	13.853	1759	1764	1770	rVB2	1045	1981	0.32%	0.030%
50	13.994	1785	1788	1791	rBV2	940	1165	0.19%	0.018%
51	14.294	1832	1839	1847	rBV	189703	281321	46.00%	4.253%
52	14.534	1874	1880	1881	rBV2	2395	2594	0.42%	0.039%
53	14.605	1886	1892	1898	rVB	187169	294921	48.22%	4.458%
54	14.787	1918	1923	1927	rBV3	3076	4564	0.75%	0.069%
55	14.910	1937	1944	1951	rVB	318520	497627	81.37%	7.522%
56	15.069	1964	1971	1977	rBV	64878	110035	17.99%	1.663%
57	15.298	2003	2010	2015	rVB3	7369	11501	1.88%	0.174%
58	15.533	2047	2050	2057	rVV3	2068	2754	0.45%	0.042%
59	15.621	2060	2065	2067	rBV	1616	2050	0.34%	0.031%
60	15.692	2073	2077	2082	rVV3	3765	5979	0.98%	0.090%
61	15.733	2082	2084	2088	rVB2	2788	3111	0.51%	0.047%
62	15.897	2104	2112	2119	rBV	260199	390292	63.82%	5.900%
63	15.997	2123	2129	2136	rBV	59528	90440	14.79%	1.367%
64	16.291	2171	2179	2182	rVV2	1208	2736	0.45%	0.041%
65	16.426	2199	2202	2203	rBV	1467	1665	0.27%	0.025%
66	16.532	2219	2220	2224	rBV2	1362	1122	0.18%	0.017%
67	16.590	2228	2230	2233	rBV2	1733	2488	0.41%	0.038%
68	16.684	2243	2246	2248	rVB2	2123	2390	0.39%	0.036%
69	16.726	2250	2253	2255	rBV3	1195	1197	0.20%	0.018%
70	16.778	2258	2262	2265	rVB4	3089	4411	0.72%	0.067%
71	16.890	2276	2281	2283	rVB4	1624	2275	0.37%	0.034%
72	16.949	2288	2291	2295	rVV3	1258	1724	0.28%	0.026%
73	17.113	2317	2319	2322	rVB4	1708	1455	0.24%	0.022%
74	17.172	2326	2329	2331	rBV3	1126	1257	0.21%	0.019%
75	17.342	2355	2358	2362	rBV2	1125	1575	0.26%	0.024%
76	17.389	2362	2366	2369	rBV2	3781	5082	0.83%	0.077%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051644.D
 Acq On : 19 Dec 2021 00:53
 Operator : CG/JU
 Sample : M5153-01
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BGL66

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

77	17.436	2372	2374	2377	rBV3	2929	3048	0.50%	0.046%
78	17.501	2383	2385	2388	rBV	1411	1381	0.23%	0.021%
79	17.548	2390	2393	2396	rVB3	4978	4159	0.68%	0.063%
80	17.654	2405	2411	2418	rVV	400335	609175	99.61%	9.209%
81	17.754	2421	2428	2434	rVV2	255773	397588	65.01%	6.010%
82	17.818	2437	2439	2445	rVB5	6986	7945	1.30%	0.120%
83	17.918	2452	2456	2457	rBV2	2553	2815	0.46%	0.043%
84	18.047	2476	2478	2480	rBV3	1617	1130	0.18%	0.017%
85	18.065	2480	2481	2485	rVB2	1430	1319	0.22%	0.020%
86	18.306	2518	2522	2527	rBV2	11031	12617	2.06%	0.191%
87	18.370	2531	2533	2536	rBV4	1261	1227	0.20%	0.019%
88	18.400	2536	2538	2541	rBV3	1275	1190	0.19%	0.018%
89	18.517	2554	2558	2563	rBV4	21702	30017	4.91%	0.454%
90	18.740	2594	2596	2597	rVB2	2126	1124	0.18%	0.017%
91	18.811	2607	2608	2613	rBV3	1967	1822	0.30%	0.028%
92	19.304	2688	2692	2694	rBV5	2785	3636	0.59%	0.055%
93	19.669	2751	2754	2755	rBV3	7329	6418	1.05%	0.097%
94	19.780	2770	2773	2778	rBV6	7007	7676	1.26%	0.116%
95	20.027	2809	2815	2825	rVB	296705	439940	71.93%	6.650%
96	20.233	2848	2850	2851	rBV2	3378	2273	0.37%	0.034%
97	21.578	3075	3079	3086	rBV5	37942	77571	12.68%	1.173%
98	21.971	3140	3146	3155	rVB	349144	611581	100.00%	9.245%
99	25.226	3692	3700	3711	rVB	133128	367880	60.15%	5.561%
100	25.473	3732	3742	3753	rBV3	193252	590282	96.52%	8.923%




Sum of corrected areas: 6615302

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051644.D
Acq On : 19 Dec 2021 00:53
Operator : CG/JU
Sample : M5153-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

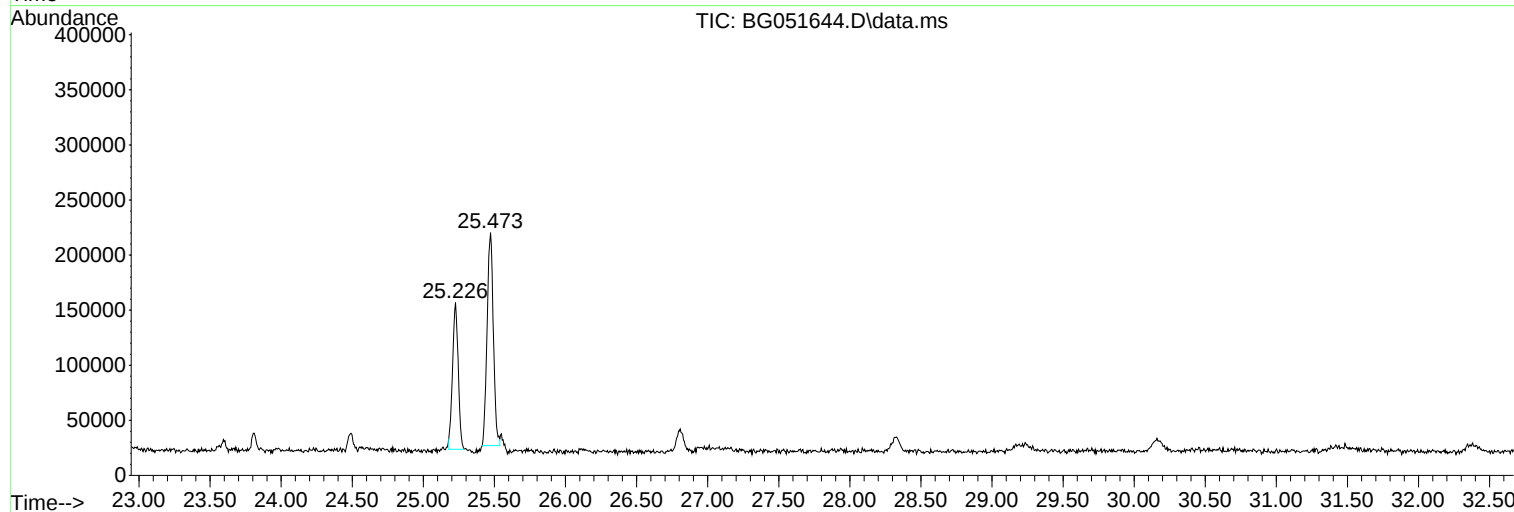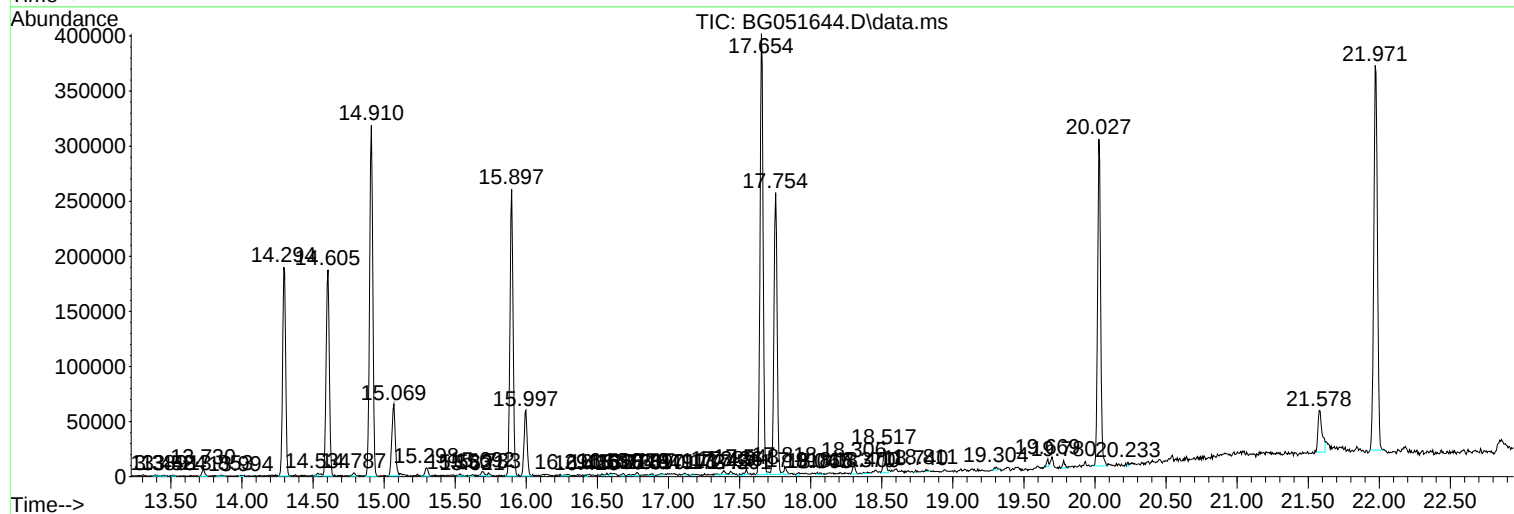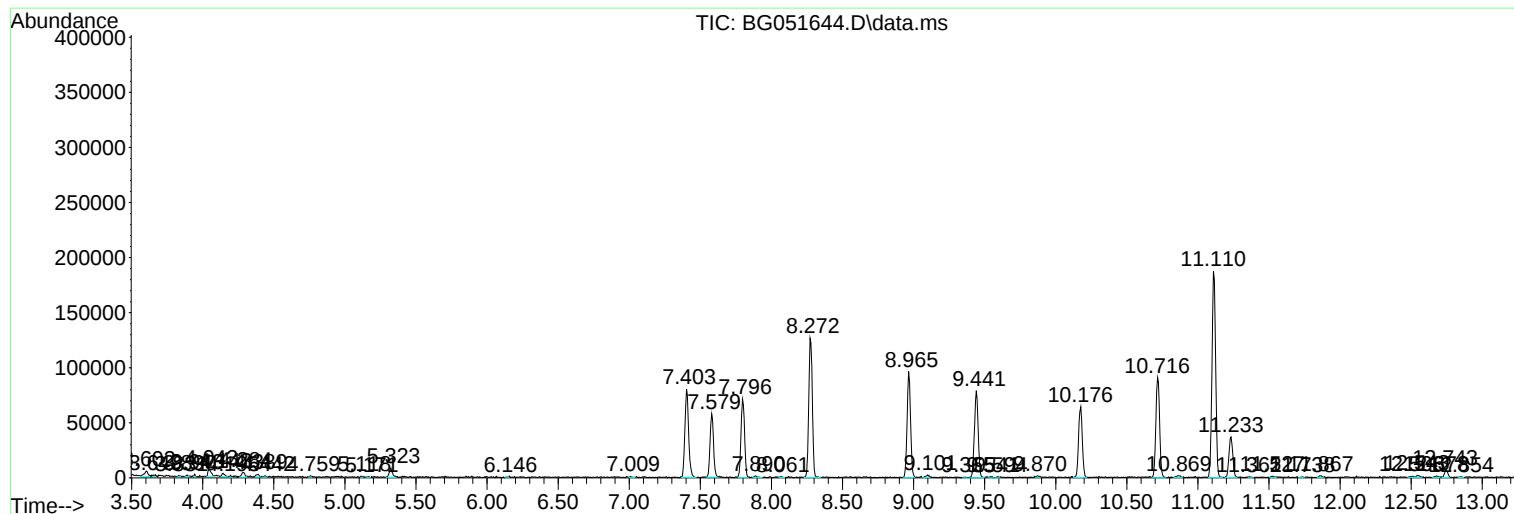

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051644.D
Acq On : 19 Dec 2021 00:53
Operator : CG/JU
Sample : M5153-01
Misc :
ALS Vial : 60 Sample Multiplier: 1










Instrument :
BNA_G
ClientSampleId :
BGL66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.	
21.578	2.54 ng/ul	77571	Chrysene-d12		21.971	
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	17-Pentatriacontene		491	C35H70	006971-40-0	87
2	Tetracosyl heptafluorobutyrate		550	C28H49F7O2	1000351-83-7	76
3	Octacosyl trifluoroacetate		506	C30H57F3O2	1000351-74-9	76
4	Hexacosyl pentafluoropropionate		528	C29H53F5O2	1000351-81-2	76
5	Tricosyl trifluoroacetate		436	C25H47F3O2	1000351-75-1	76

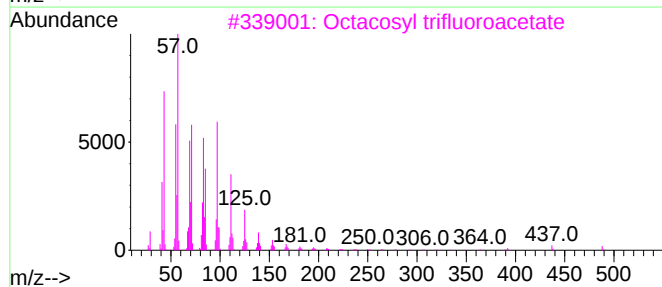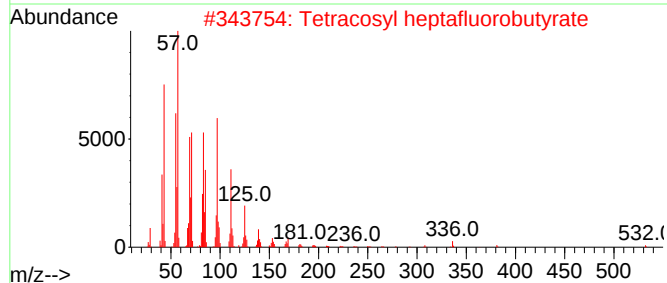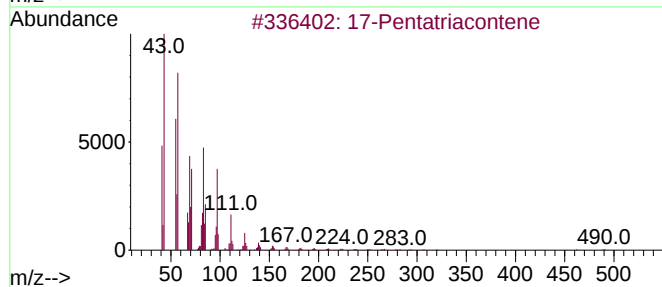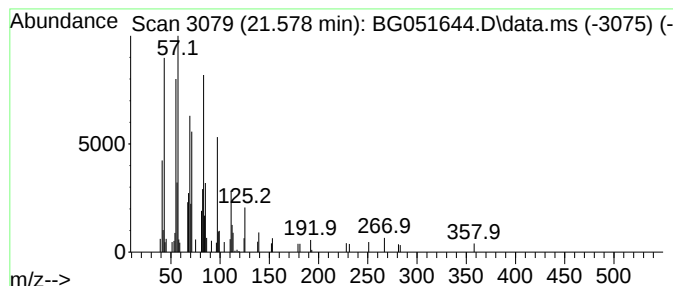

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051644.D
Acq On : 19 Dec 2021 00:53
Operator : CG/JU
Sample : M5153-01
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BGL66

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	21.578	2.5	ng/u1	77571	5	21.971	611581	20.0