

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051650.D
 Acq On : 19 Dec 2021 5:40
 Operator : CG/JU
 Sample : PB141536BL
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK536

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051650.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.599	15	19	29	rVB2	11930	19362	1.45%	0.140%
2	4.028	87	92	101	rBV	154063	266008	19.91%	1.930%
3	4.381	148	152	156	rBV3	3671	4525	0.34%	0.033%
4	4.710	205	208	211	rBV	971	1347	0.10%	0.010%
5	5.732	379	382	390	rVB2	1001	2035	0.15%	0.015%
6	7.400	659	666	681	rVB	211988	371375	27.80%	2.695%
7	7.576	689	696	707	rBV	140935	241835	18.10%	1.755%
8	7.799	727	734	741	rVB	193630	334575	25.04%	2.428%
9	8.275	806	815	822	rBV	155195	254740	19.07%	1.848%
10	8.968	923	933	941	rBV	245023	437139	32.72%	3.172%
11	9.438	1002	1013	1021	rBV	194369	353823	26.48%	2.567%
12	10.173	1129	1138	1148	rBV	168037	305042	22.83%	2.213%
13	10.719	1223	1231	1238	rBV	252505	450299	33.70%	3.267%
14	11.113	1288	1298	1306	rBV	202692	373379	27.95%	2.709%
15	11.230	1310	1318	1326	rBV	251738	451838	33.82%	3.279%
16	12.675	1561	1564	1570	rVB3	3965	6427	0.48%	0.047%
17	14.297	1834	1840	1848	rBV	482935	701559	52.51%	5.091%
18	14.602	1885	1892	1904	rVB	518618	825088	61.75%	5.987%
19	14.907	1937	1944	1952	rVB	363529	554876	41.53%	4.026%
20	15.066	1964	1971	1985	rBV2	225771	361861	27.08%	2.626%
21	15.160	1985	1987	1991	rVV3	1714	2138	0.16%	0.016%
22	15.894	2105	2112	2121	rBV	677865	1029543	77.06%	7.470%
23	15.994	2124	2129	2136	rVV	164021	259487	19.42%	1.883%
24	16.129	2149	2152	2158	rBV3	2383	3732	0.28%	0.027%
25	17.328	2353	2356	2363	rVB4	1340	2111	0.16%	0.015%
26	17.439	2371	2375	2380	rVB	1842	2755	0.21%	0.020%
27	17.657	2405	2412	2422	rBV	463504	710405	53.17%	5.155%
28	17.757	2422	2429	2436	rBV	763237	1151186	86.16%	8.353%
29	18.015	2471	2473	2476	rVB3	1346	1486	0.11%	0.011%
30	18.755	2597	2599	2603	rVB3	1357	1633	0.12%	0.012%
31	18.914	2623	2626	2630	rBV2	1158	1698	0.13%	0.012%
32	19.536	2728	2732	2734	rBV4	1734	2175	0.16%	0.016%
33	19.601	2738	2743	2748	rVV5	11898	17468	1.31%	0.127%
34	19.666	2748	2754	2759	rVV2	8531	14198	1.06%	0.103%
35	19.742	2765	2767	2769	rBV3	1314	1341	0.10%	0.010%
36	19.936	2795	2800	2802	rBV5	2486	2889	0.22%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
 Data File : BG051650.D
 Acq On : 19 Dec 2021 5:40
 Operator : CG/JU
 Sample : PB141536BL
 Misc :
 ALS Vial : 67 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK536

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	20.030	2810	2816	2823	rVV2	915799	1336073	100.00%	9.695%
38	20.118	2829	2831	2833	rBV3	1656	1499	0.11%	0.011%
39	20.241	2850	2852	2855	rBV4	1638	1801	0.13%	0.013%
40	20.488	2893	2894	2896	rBV2	2064	1773	0.13%	0.013%
41	20.600	2911	2913	2915	rBV3	2572	2448	0.18%	0.018%
42	20.776	2941	2943	2944	rBV2	2349	2207	0.17%	0.016%
43	20.911	2964	2966	2967	rBV2	4557	3243	0.24%	0.024%
44	20.929	2967	2969	2970	rVV2	2617	1628	0.12%	0.012%
45	20.976	2975	2977	2980	rVV4	4401	5134	0.38%	0.037%
46	21.363	3041	3043	3044	rBV2	2698	2426	0.18%	0.018%
47	21.681	3095	3097	3099	rVB3	3041	1651	0.12%	0.012%
48	21.974	3139	3147	3157	rBV	457052	761930	57.03%	5.529%
49	22.292	3199	3201	3202	rBV2	2855	2694	0.20%	0.020%
50	22.574	3247	3249	3251	rBV3	4406	3226	0.24%	0.023%
51	22.715	3271	3273	3277	rBV5	2785	4015	0.30%	0.029%
52	23.414	3391	3392	3395	rBV3	4494	4654	0.35%	0.034%
53	24.083	3505	3506	3509	rBV2	3481	2323	0.17%	0.017%
54	24.195	3523	3525	3529	rBV5	4105	5710	0.43%	0.041%
55	24.236	3531	3532	3533	rBV	4570	2122	0.16%	0.015%
56	24.494	3572	3576	3580	rVB5	10359	16610	1.24%	0.121%
57	24.624	3596	3598	3601	rBV3	2787	2786	0.21%	0.020%
58	25.235	3690	3702	3713	rVB2	416727	1263879	94.60%	9.171%
59	25.470	3732	3742	3753	rBV2	239756	713993	53.44%	5.181%
60	26.004	3831	3833	3835	rBV3	3262	2470	0.18%	0.018%
61	26.791	3963	3967	3970	rBV6	8902	15524	1.16%	0.113%
62	27.626	4107	4109	4110	rBV2	2821	1472	0.11%	0.011%
63	28.090	4186	4188	4189	rBV2	3173	1663	0.12%	0.012%
64	28.195	4205	4206	4207	rBV	3576	1547	0.12%	0.011%
65	28.330	4221	4229	4238	rVB8	11562	38855	2.91%	0.282%
66	29.088	4356	4358	4359	rBV2	3304	2273	0.17%	0.016%
67	29.147	4366	4368	4370	rVB2	3398	2188	0.16%	0.016%
68	29.276	4388	4390	4391	rBV2	2902	2310	0.17%	0.017%
69	29.588	4441	4443	4446	rBV4	3256	3099	0.23%	0.022%
70	29.805	4478	4480	4481	rBV2	2956	1713	0.13%	0.012%
71	30.152	4535	4539	4542	rBV6	6629	12251	0.92%	0.089%
72	30.240	4552	4554	4557	rVB4	3148	2975	0.22%	0.022%
73	30.334	4568	4570	4573	rVB2	5400	3279	0.25%	0.024%
74	30.574	4609	4611	4615	rBV4	3670	6511	0.49%	0.047%
75	30.692	4630	4631	4632	rBV	4077	2638	0.20%	0.019%
76	31.027	4687	4688	4690	rBV2	3065	2289	0.17%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051650.D
Acq On : 19 Dec 2021 5:40
Operator : CG/JU
Sample : PB141536BL
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK536

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Title : SVOA CALIBRATION

77	31.150	4707	4709	4711	rBV3	3161	1901	0.14%	0.014%
78	31.285	4730	4732	4736	rVB4	3619	3677	0.28%	0.027%
79	32.043	4859	4861	4864	rVB3	2845	2265	0.17%	0.016%
80	32.149	4878	4879	4881	rBV2	3496	2410	0.18%	0.017%
81	32.208	4887	4889	4890	rBV	3040	3082	0.23%	0.022%




Sum of corrected areas: 13781595

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051650.D
Acq On : 19 Dec 2021 5:40
Operator : CG/JU
Sample : PB141536BL
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK536

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

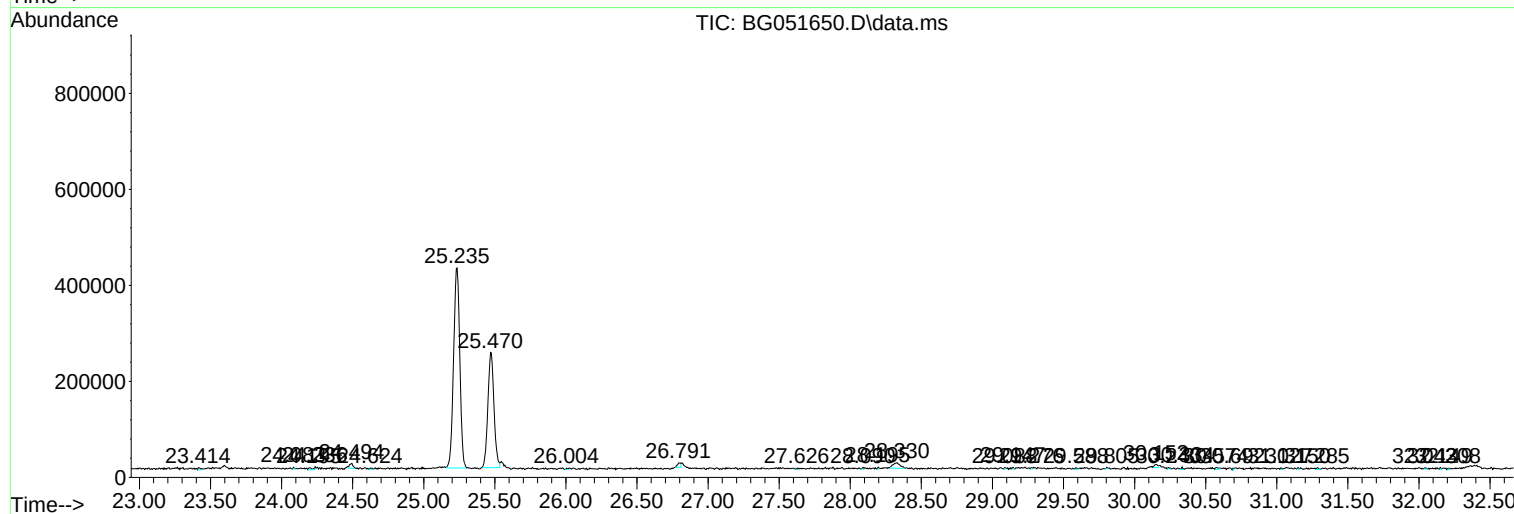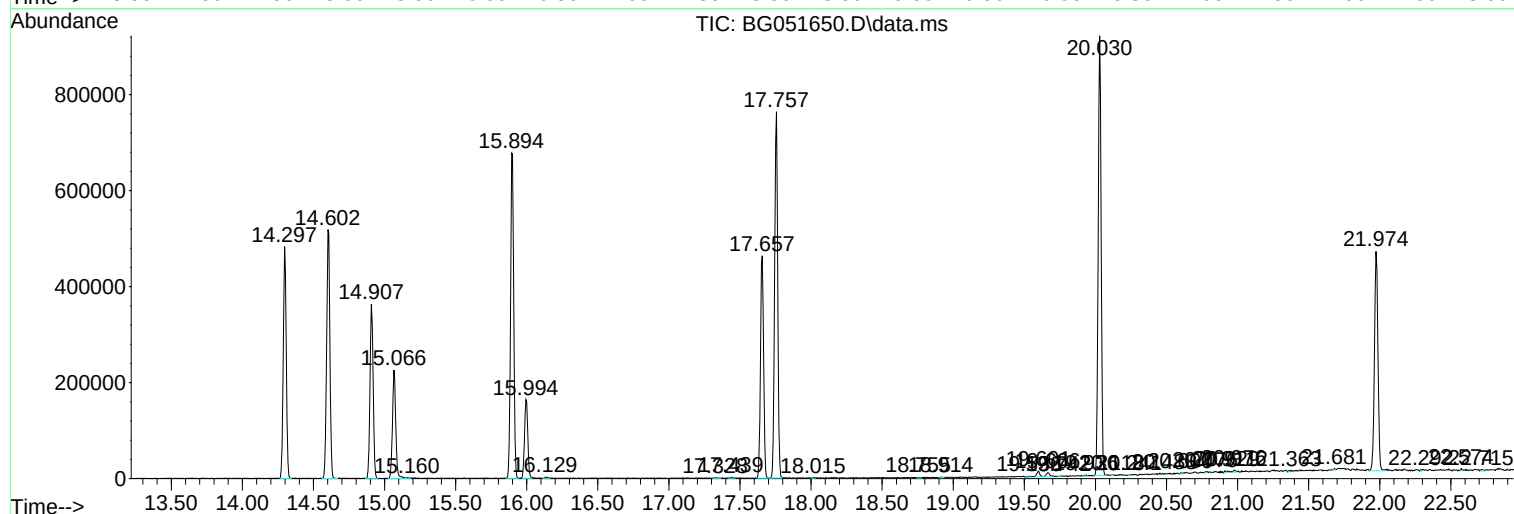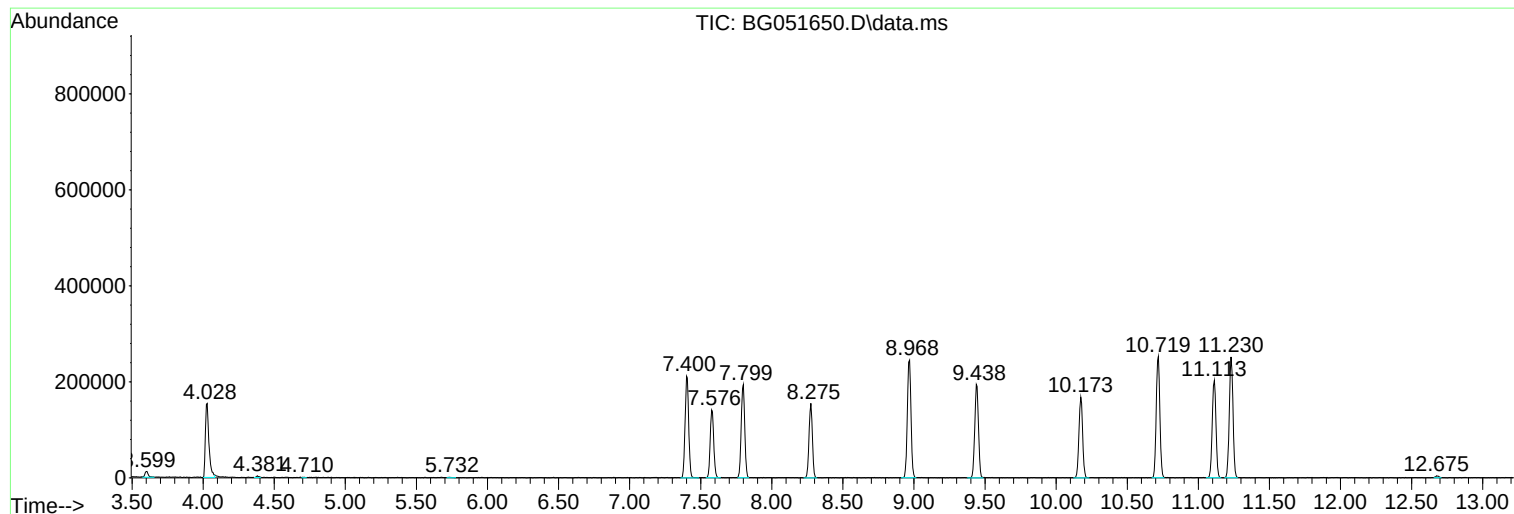

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051650.D
Acq On : 19 Dec 2021 5:40
Operator : CG/JU
Sample : PB141536BL
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK536

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG121721\
Data File : BG051650.D
Acq On : 19 Dec 2021 5:40
Operator : CG/JU
Sample : PB141536BL
Misc :
ALS Vial : 67 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK536

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc