


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG010218\
 Data File : BG031869.D
 Acq On : 2 Jan 2018 13:39
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 29 15:51:46 2017

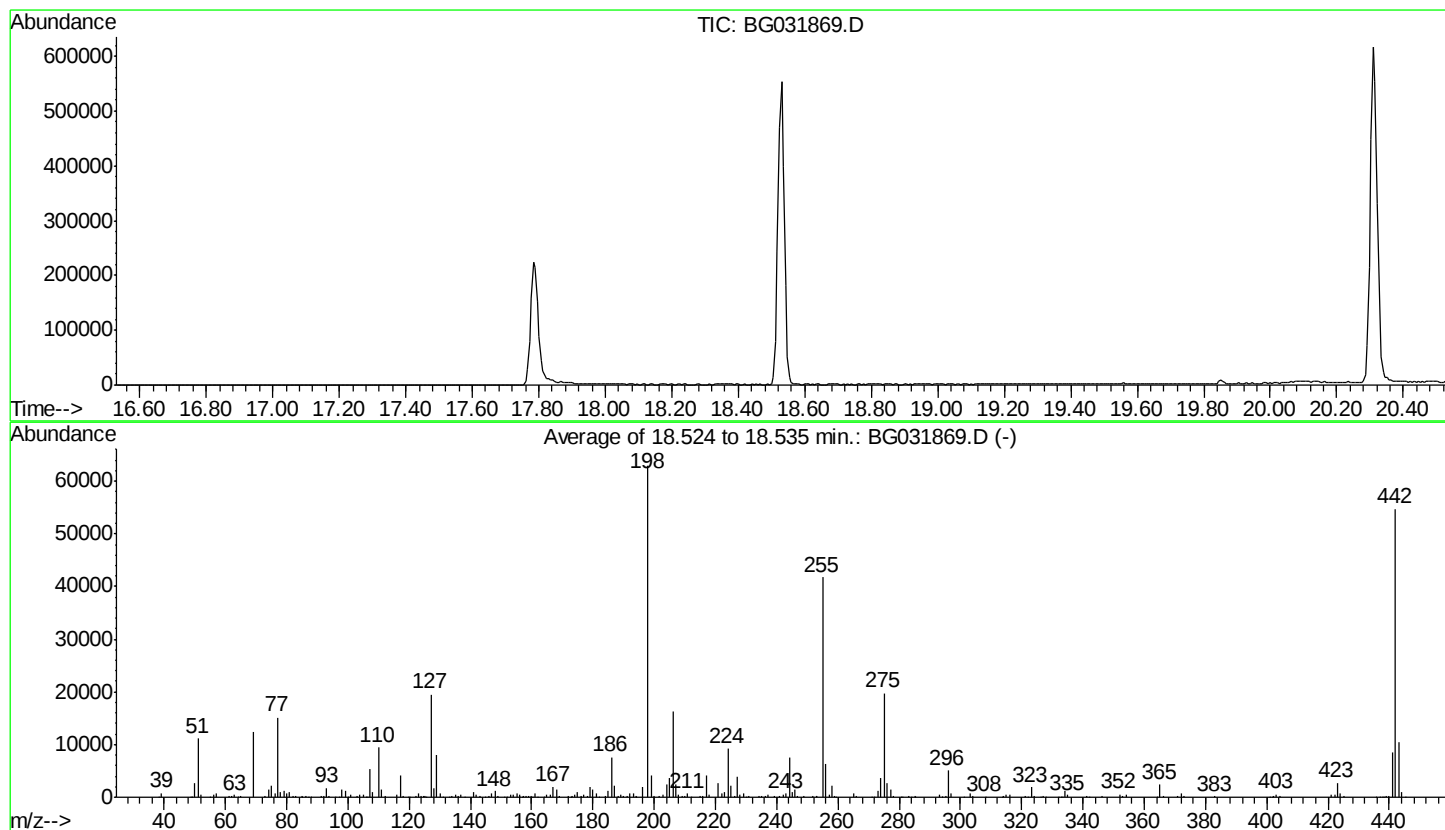

AutoFind: Scans 2593, 2594, 2595; Background Corrected with Scan 2586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.7	11155	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	19.8	12475	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	30.9	19461	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	62949	PASS
199	198	5	9	6.5	4115	PASS
275	198	10	60	31.4	19770	PASS
365	198	1	100	3.7	2337	PASS
441	442	0.01	24	15.4	8435	PASS
442	198	50	100	86.9	54704	PASS
443	442	15	24	19.1	10438	PASS