
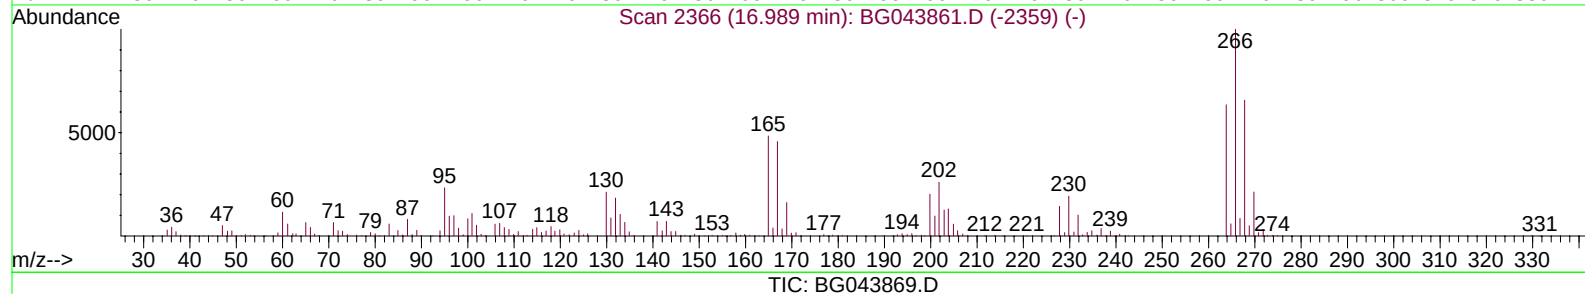
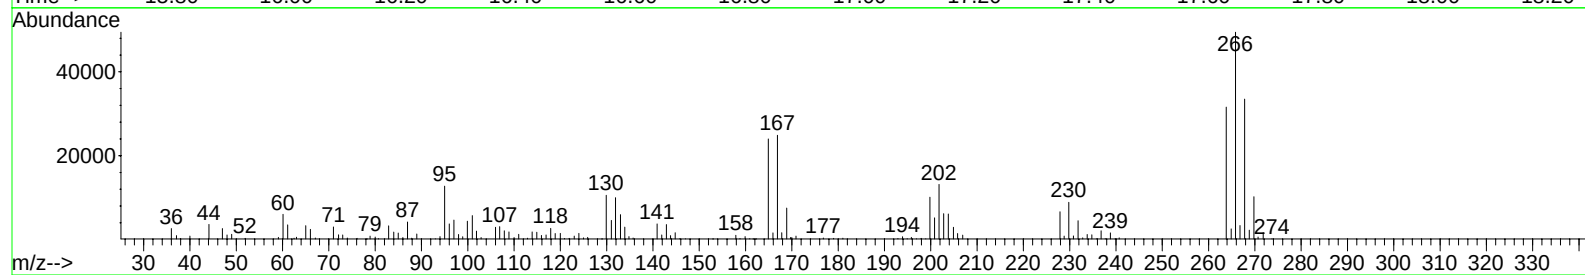


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010220\
Data File : BG043869.D
Acq On : 2 Jan 2020 10:01
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 18:26:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

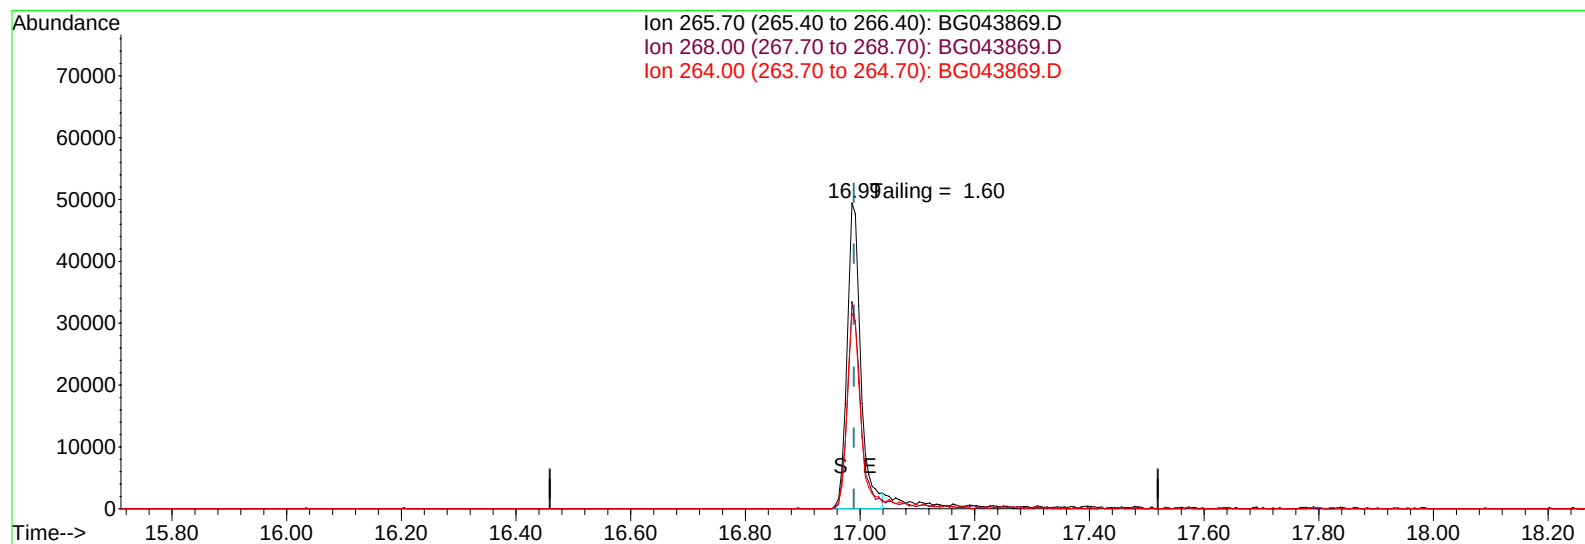

(70) Pentachlorophenol (C)




16.986min (-0.003) 193638.01ng

response 86672

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	67.72
264.00	63.50	63.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010220\
Data File : BG043869.D
Acq On : 2 Jan 2020 10:01
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 18:26:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

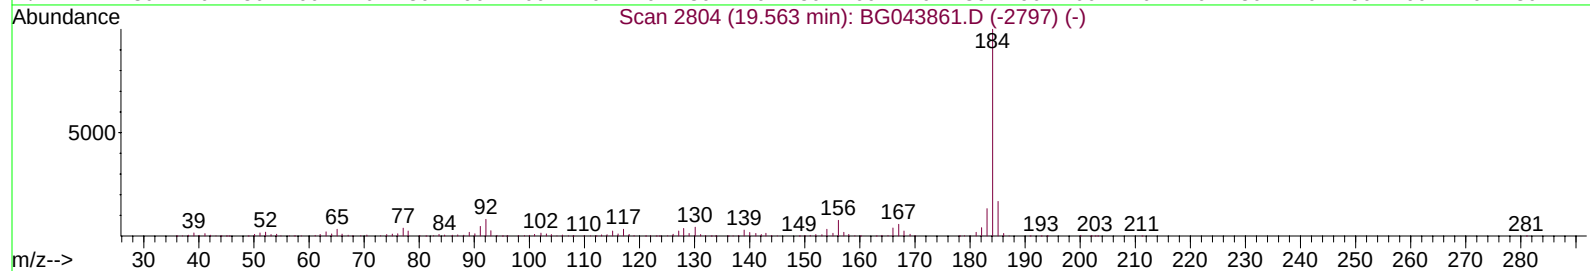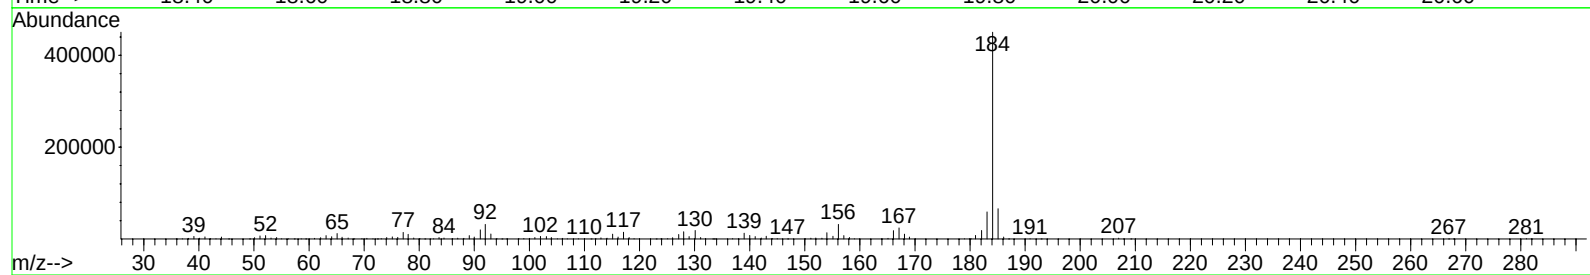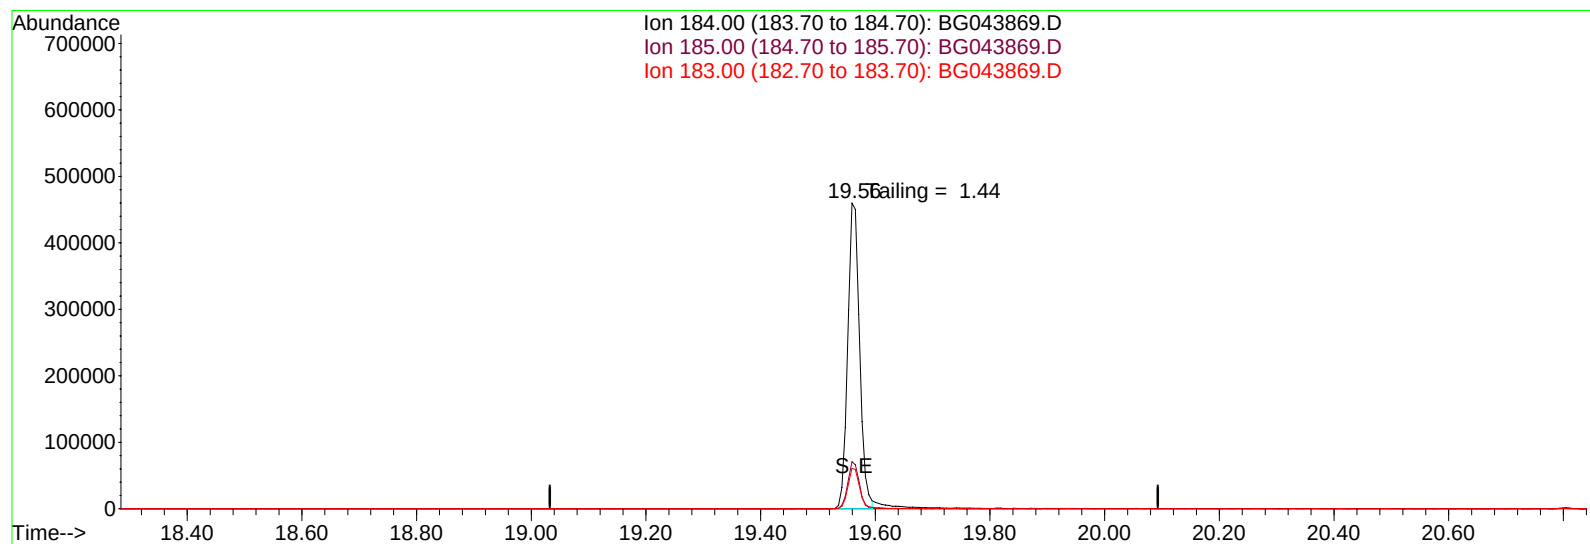

(77) Benzidine

19.563min (-19.563) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	16.70	0.00#
183.00	13.20	0.00#
0.00	0.00	0.00