
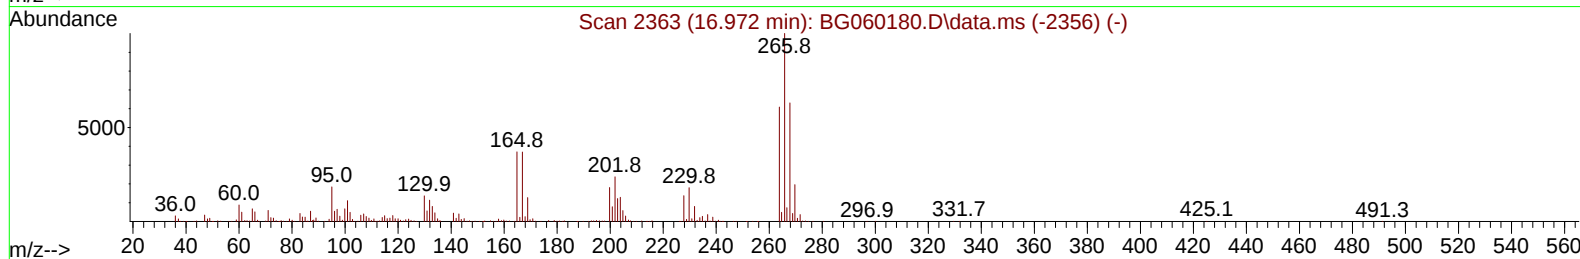
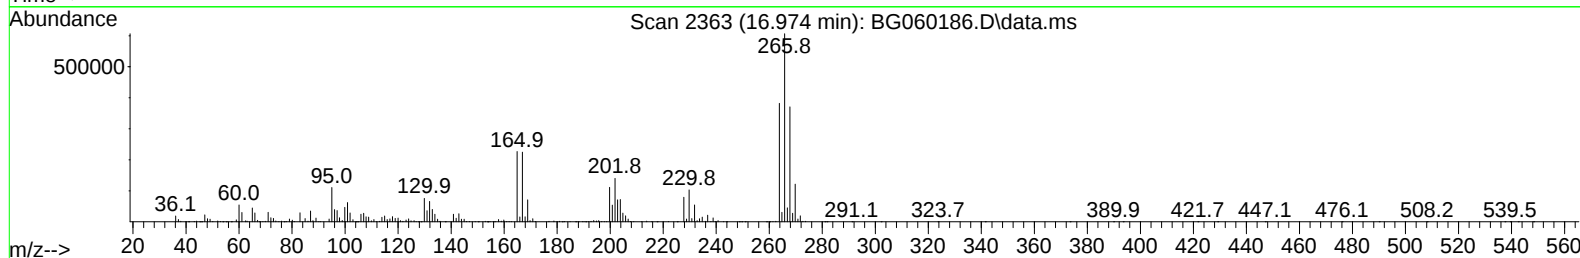


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
Data File : BG060186.D
Acq On : 2 Jan 2024 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 10:59:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

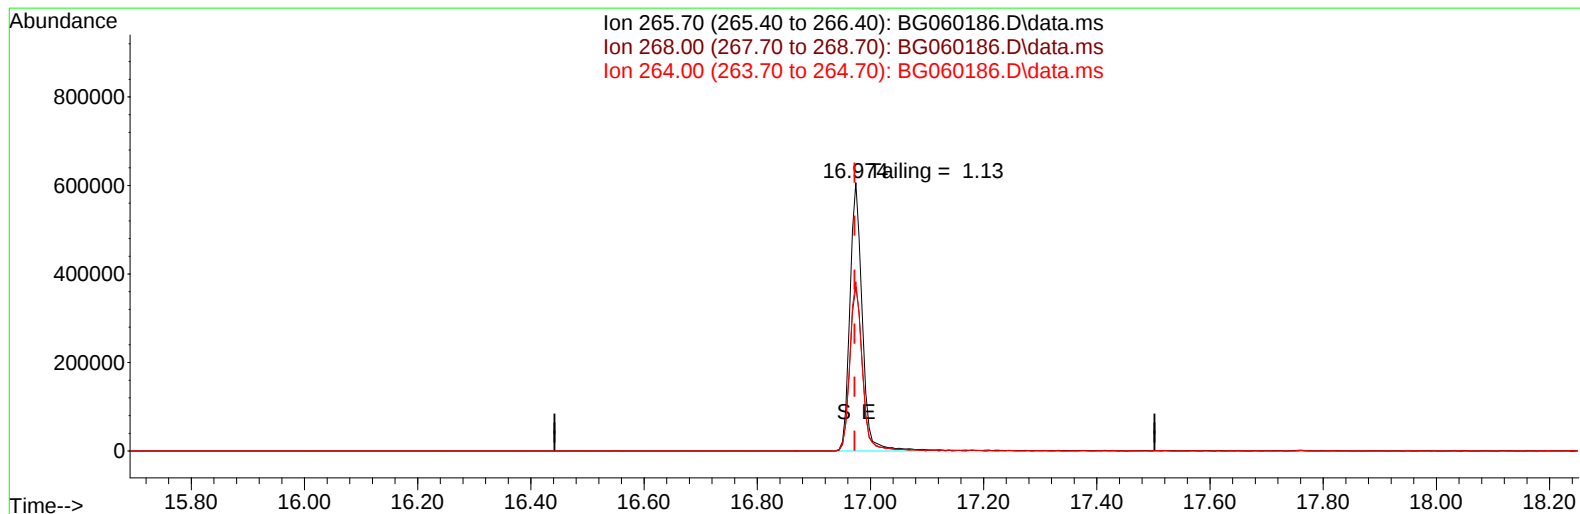




TIC: BG060186.D\data.ms

(70) Pentachlorophenol (C)**16.974min (+ 0.002) 618388.76 ng****response 916356**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	61.11
264.00	65.80	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
 Data File : BG060186.D
 Acq On : 2 Jan 2024 9:09
 Operator : MA/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 02 10:59:36 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 30 03:14:04 2023
 Response via : Initial Calibration

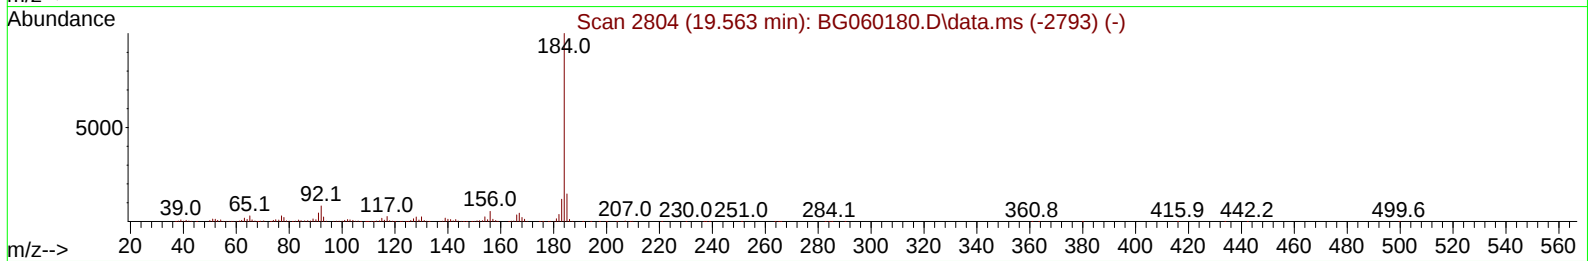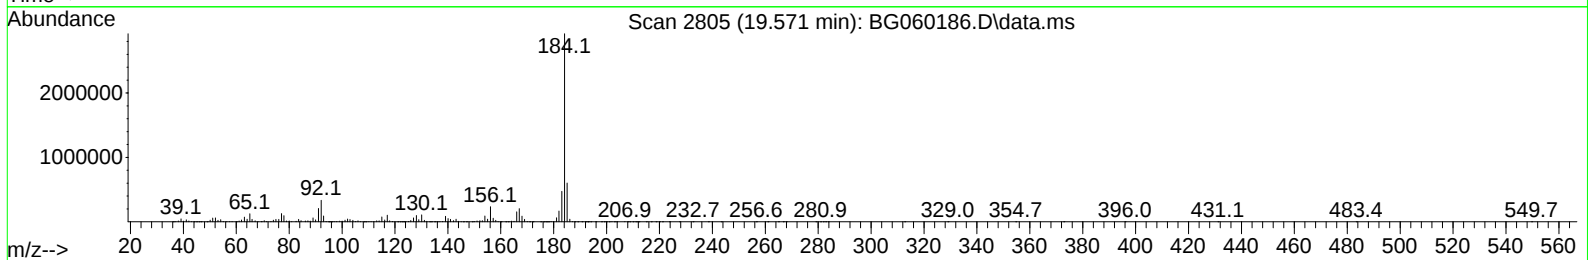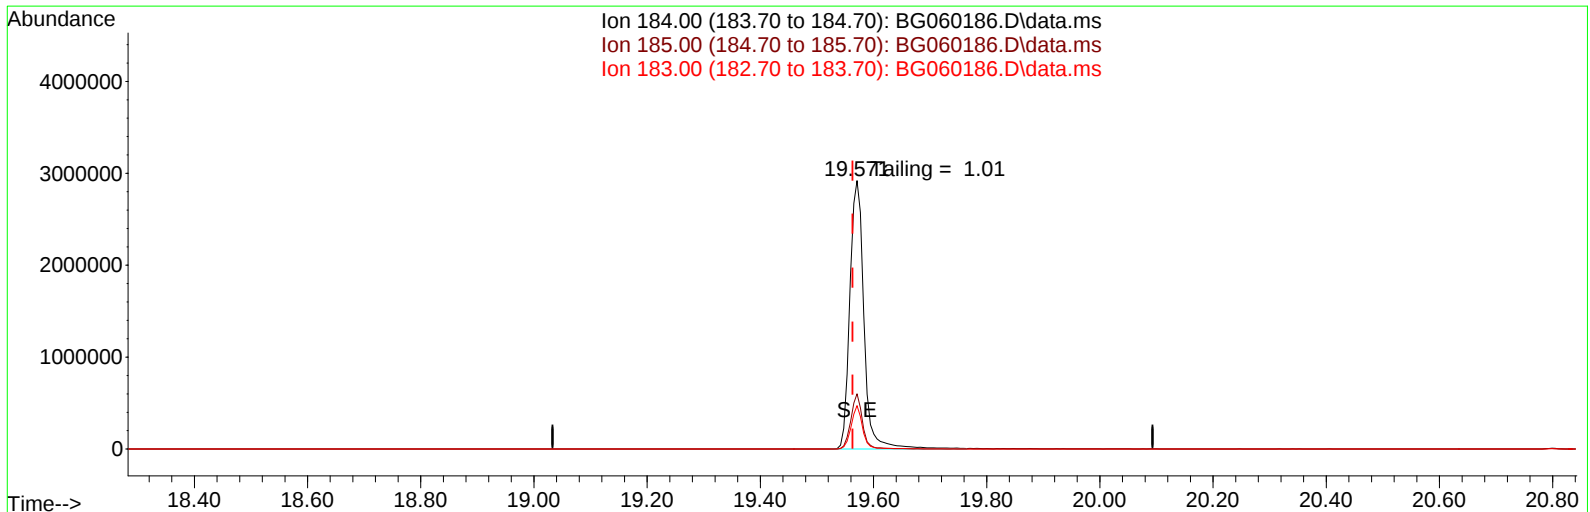

TIC: BG060186.D\data.ms

(77) Benzidine

19.571min (+ 0.008) 5724.17 ng m

response 5079606

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	20.61#
183.00	11.80	16.17#
0.00	0.00	0.00