
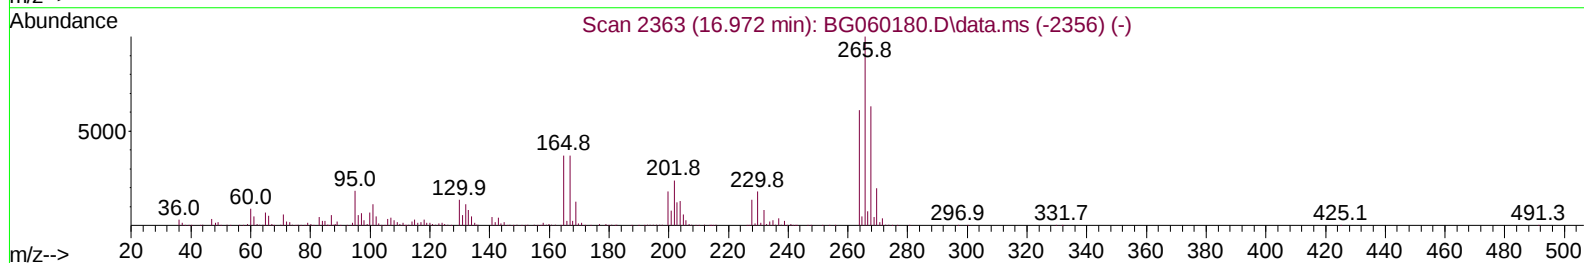
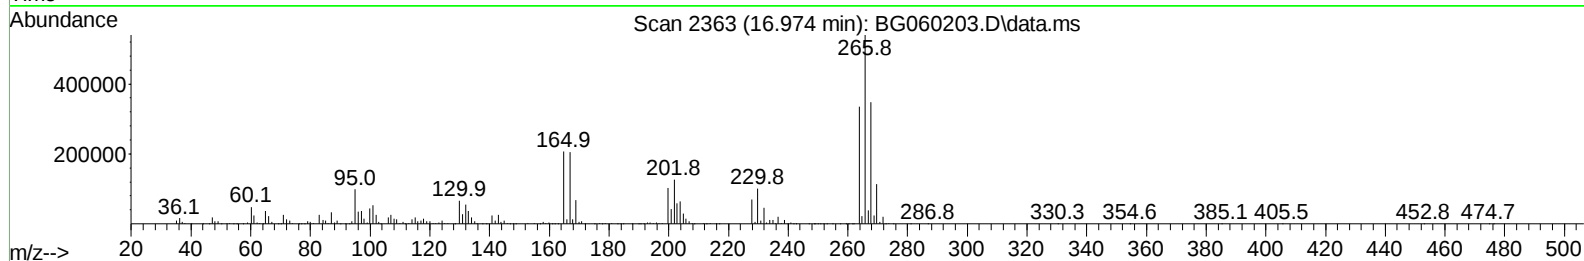


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG010224\  
Data File : BG060203.D  
Acq On : 2 Jan 2024 21:12  
Operator : MA/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 01:09:23 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 30 03:14:04 2023  
Response via : Initial Calibration



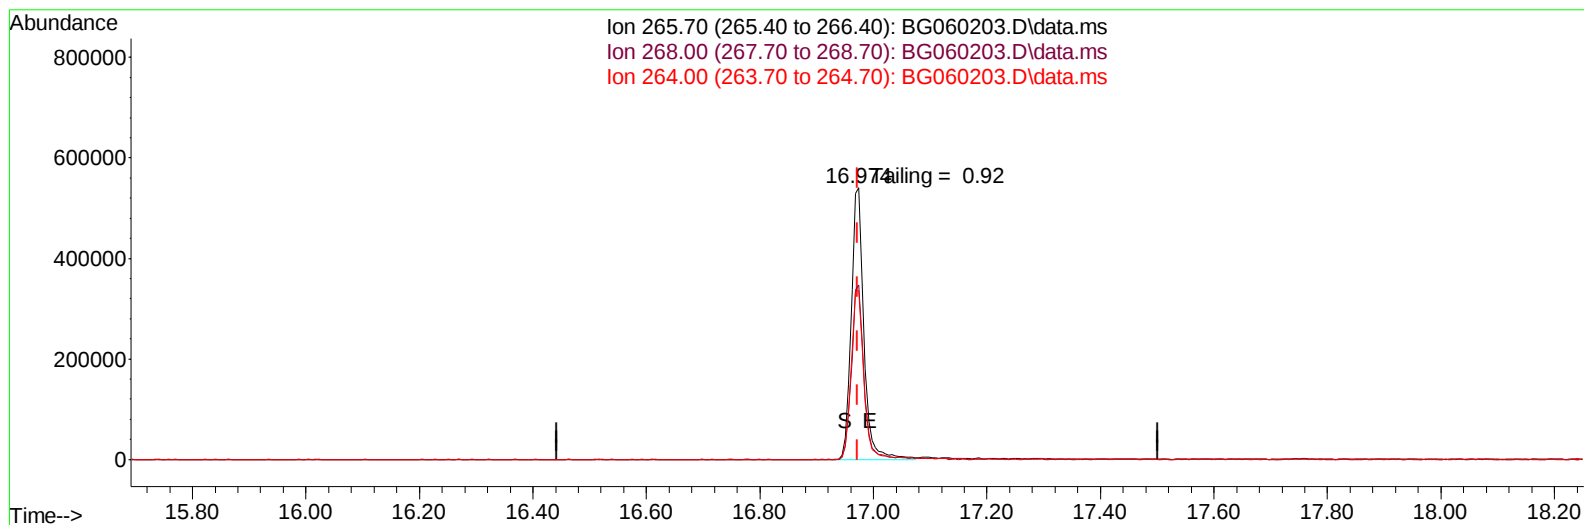


TIC: BG060203.D\data.ms

**(70) Pentachlorophenol (C)****16.974min (+ 0.002) 826206.53 ng****response 840655**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.00  | 64.34  |
| 264.00 | 65.80  | 66.41  |
| 0.00   | 0.00   | 0.00   |

Quant Time: Jan 03 01:09:23 2024  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG122923.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Sat Dec 30 03:14:04 2023  
Response via : Initial Calibration

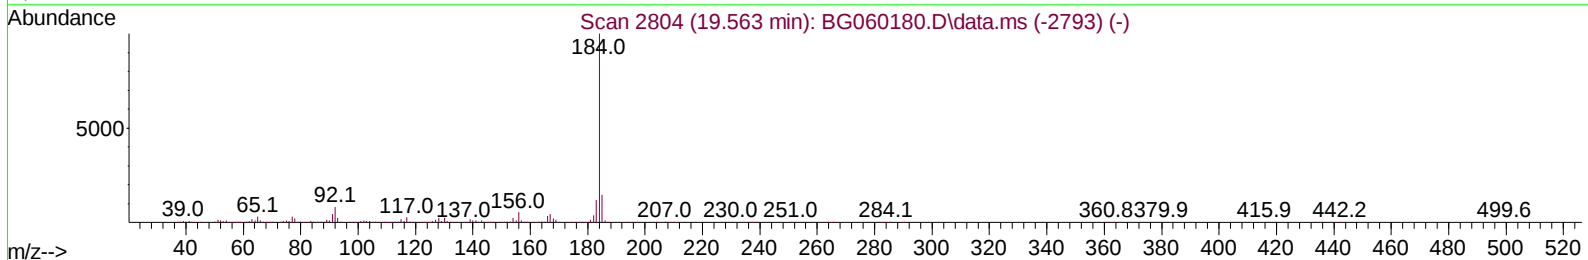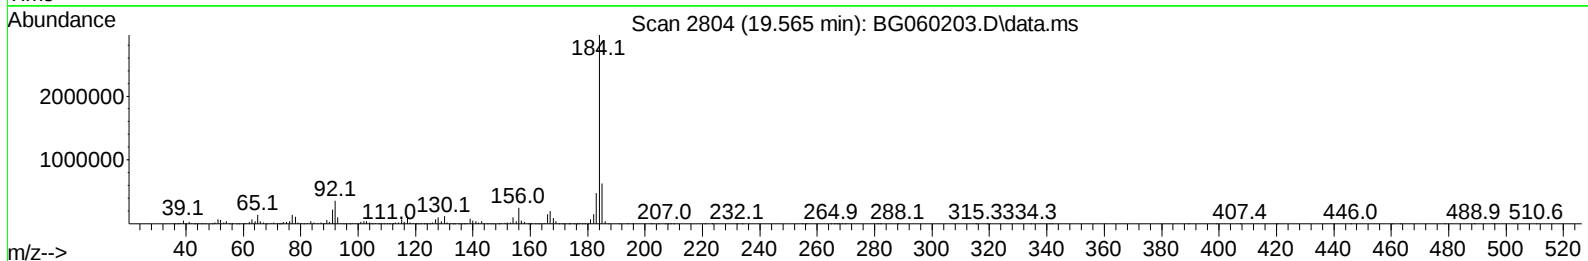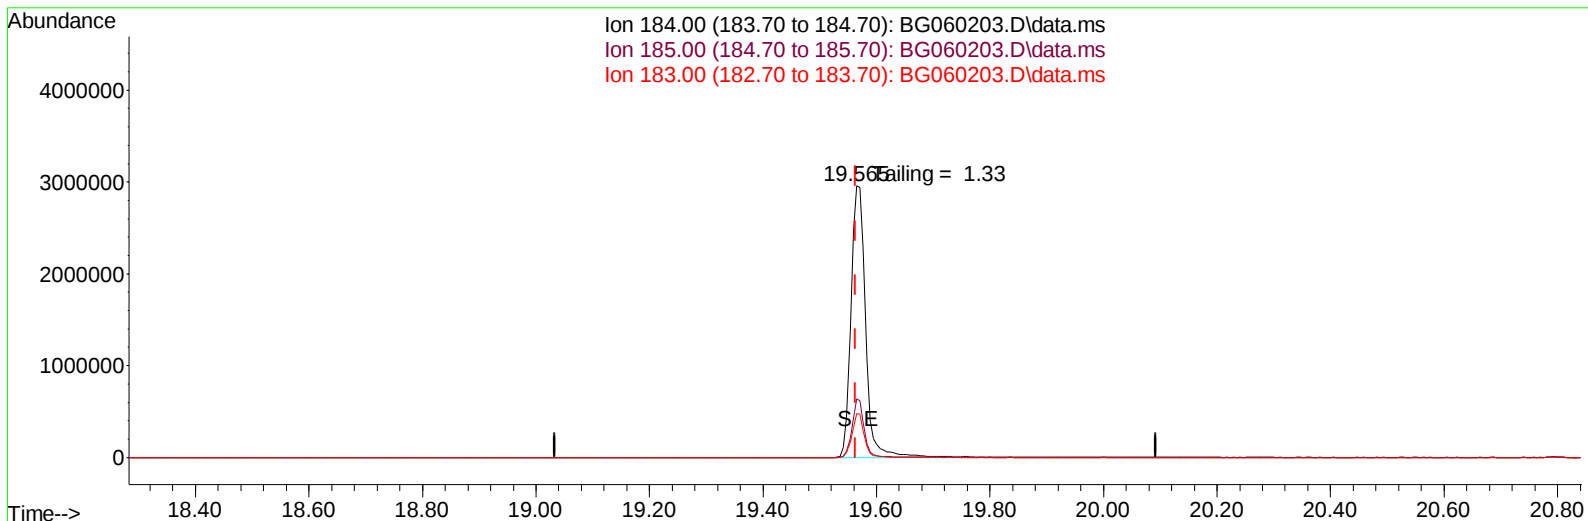

TIC: BG060203.D\data.ms

(77) Benzidine

19.565min (+ 0.002) 2708070.08 ng

**response**      **5321467**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.60  | 21.52# |
| 183.00 | 11.80  | 16.15# |
| 0.00   | 0.00   | 0.00   |