

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
 Data File : BG060214.D
 Acq On : 3 Jan 2024 5:18
 Operator : MA/JU
 Sample : 05899-20
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GHL-SS-07-2-4

Quant Time: Jan 03 05:52:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 30 03:14:04 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.935	152	238643	20.000	ng	0.00
21) Naphthalene-d8	10.743	136	998635	20.000	ng	0.00
39) Acenaphthene-d10	14.574	164	796501	20.000	ng	0.00
64) Phenanthrene-d10	17.324	188	1912028	20.000	ng	0.00
76) Chrysene-d12	21.589	240	1568413	20.000	ng	0.00
86) Perylene-d12	24.762	264	1784365	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.508	112	1558438	98.566	ng	0.00
7) Phenol-d6	7.100	99	2128078	90.650	ng	0.00
23) Nitrobenzene-d5	9.098	82	1254801	58.038	ng	0.00
42) 2,4,6-Tribromophenol	16.066	330	924726	86.731	ng	0.00
45) 2-Fluorobiphenyl	13.199	172	3129136	56.463	ng	0.00
79) Terphenyl-d14	19.944	244	4348176	53.298	ng	0.00
Target Compounds						
72) Anthracene	17.453	178	279822	2.981	ng	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
Data File : BG060214.D
Acq On : 3 Jan 2024 5:18
Operator : MA/JU
Sample : 05899-20
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GHL-SS-07-2-4

Quant Time: Jan 03 05:52:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration




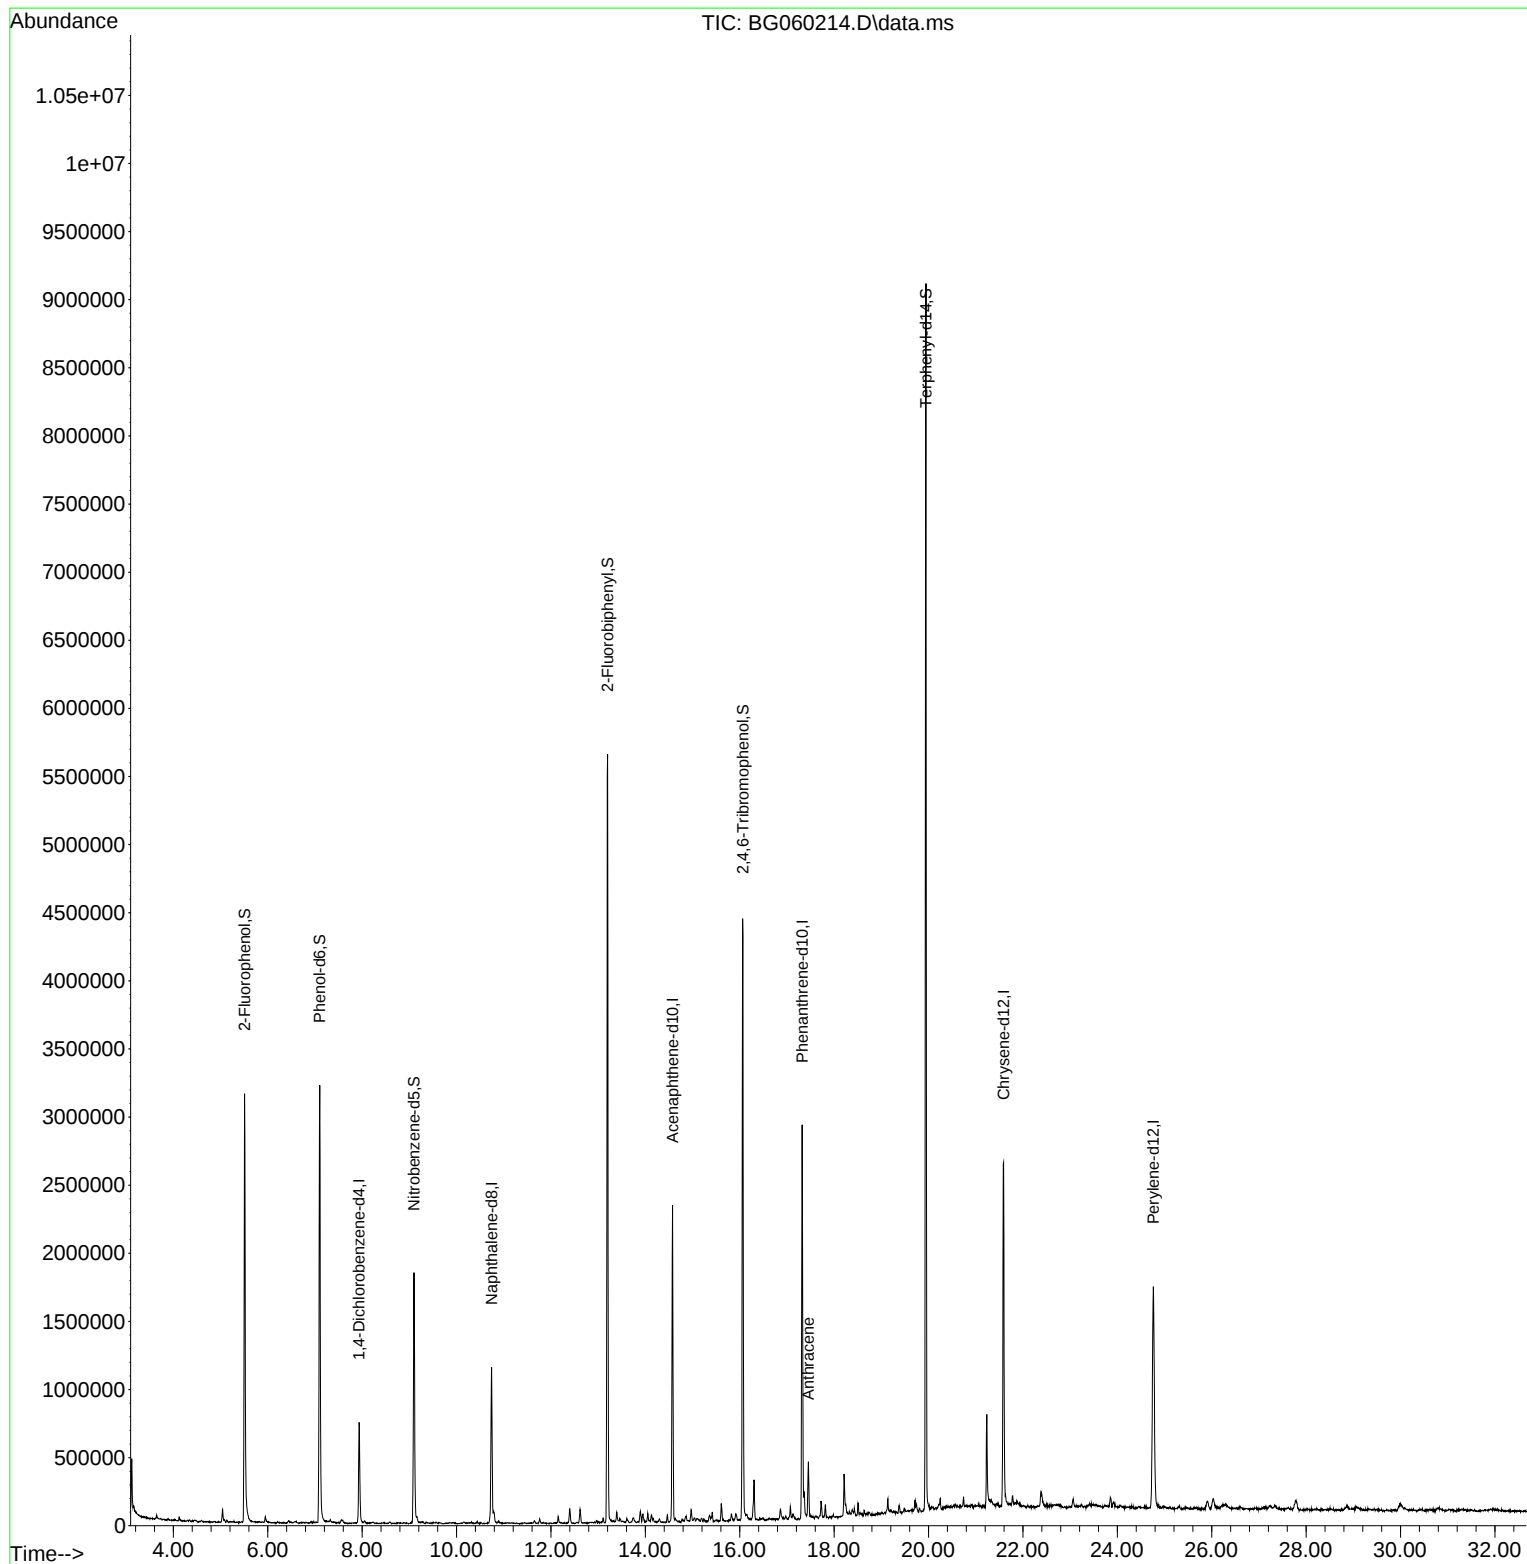




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.935 min Scan# 81
Delta R.T. -0.006 min
Lab File: BG060214.D
Acq: 3 Jan 2024 5:18




Instrument :
BNA_G
ClientSampleId :
GHL-SS-07-2-4


Tgt Ion:152 Resp: 238643
Ion Ratio Lower Upper
152 100
150 152.7 123.4 185.0
115 53.2 45.4 68.0

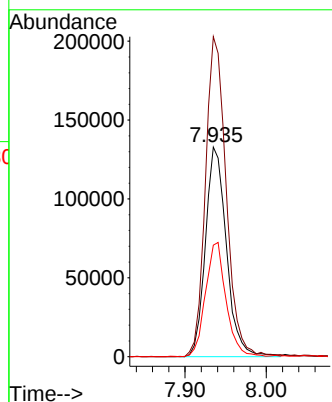

#5
2-Fluorophenol
Concen: 98.566 ng
RT: 5.508 min Scan# 412
Delta R.T. -0.000 min
Lab File: BG060214.D
Acq: 3 Jan 2024 5:18

Tgt Ion:112 Resp: 1558438
Ion Ratio Lower Upper
112 100
64 64.2 52.2 78.4
63 33.5 25.4 38.0

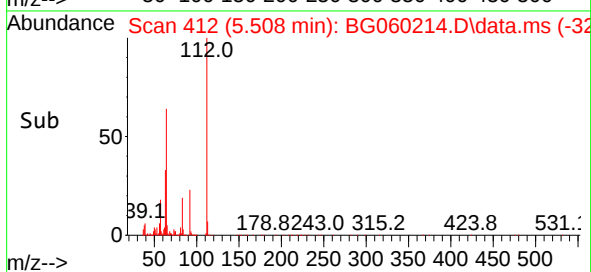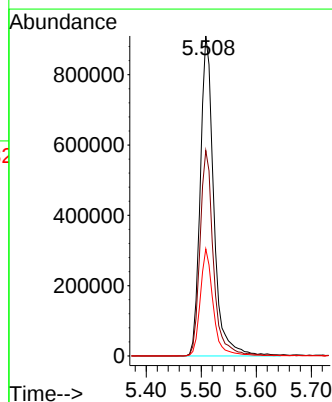







#7
Phenol-d6
Concen: 90.650 ng
RT: 7.100 min Scan# 61
Delta R.T. -0.000 min
Lab File: BG060214.D
Acq: 3 Jan 2024 5:18

Instrument :
BNA_G
ClientSampleId :
GHL-SS-07-2-4

Tgt Ion: 99 Resp: 2128078




Ion	Ratio	Lower	Upper
99	100		
42	15.4	12.5	18.7
71	29.0	24.1	36.1

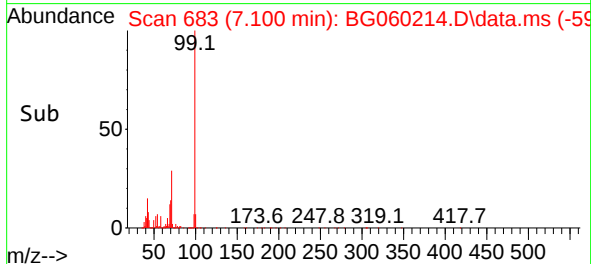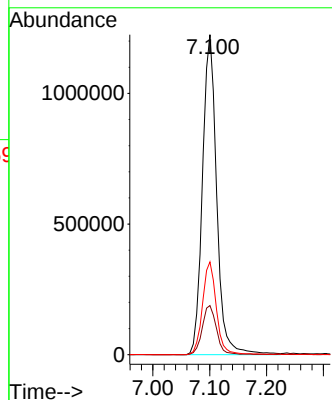


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.743 min Scan# 1303
Delta R.T. -0.000 min
Lab File: BG060214.D
Acq: 3 Jan 2024 5:18

Tgt Ion:136 Resp: 998635

Ion	Ratio	Lower	Upper
136	100		
137	10.4	9.4	14.0
54	9.0	7.4	11.2
68	7.8	6.2	9.4

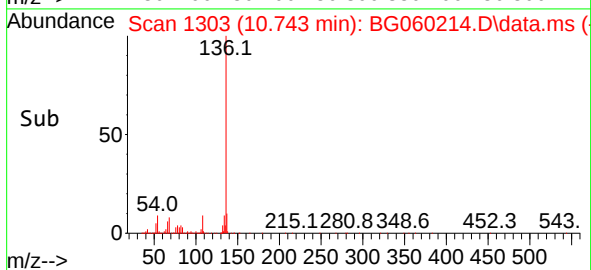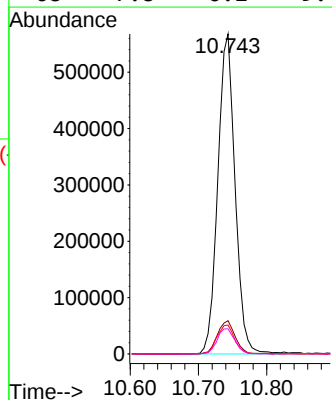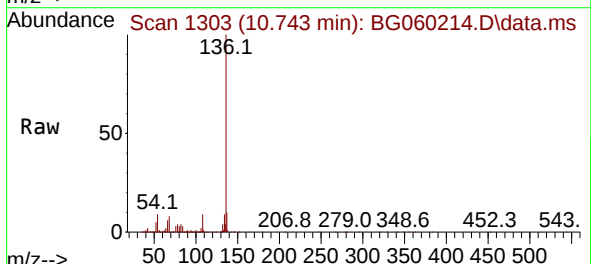



#23

Nitrobenzene-d5

Concen: 58.038 ng

RT: 9.098 min Scan# 1024

Delta R.T. -0.006 min

Lab File: BG060214.D

Acq: 3 Jan 2024 5:18

Instrument :





BNA_G

ClientSampleId :

GHL-SS-07-2-4

Tgt Ion: 82 Resp: 1254801

Ion	Ratio	Lower	Upper
82	100		
128	37.3	28.7	43.1
54	47.4	36.9	55.3

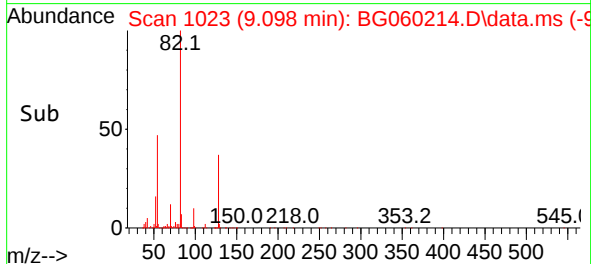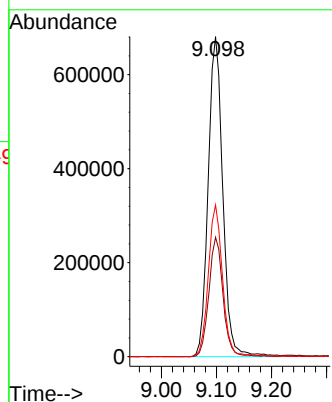

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.574 min Scan# 1955




Delta R.T. -0.000 min


Lab File: BG060214.D

Acq: 3 Jan 2024 5:18

Tgt Ion: 164 Resp: 796501

Ion	Ratio	Lower	Upper
164	100		
162	104.4	83.9	125.9
160	41.9	34.2	51.4


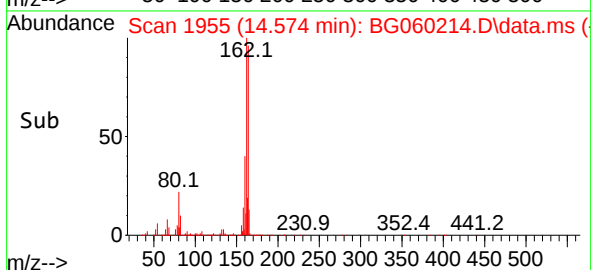
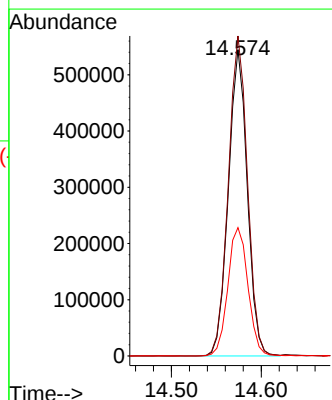





#42
2,4,6-Tribromophenol
Concen: 86.731 ng
RT: 16.066 min Scan# 21
Delta R.T. -0.000 min
Lab File: BG060214.D
Acq: 3 Jan 2024 5:18




Instrument :
BNA_G
ClientSampleId :
GHL-SS-07-2-4


Tgt Ion	330	Resp	924726
Ion Ratio	100		
Lower			
Upper			
332	97.3	76.7	115.1
141	26.9	21.0	31.4

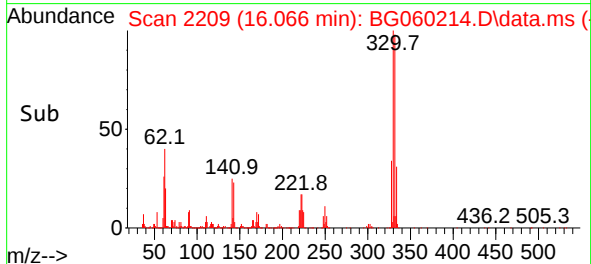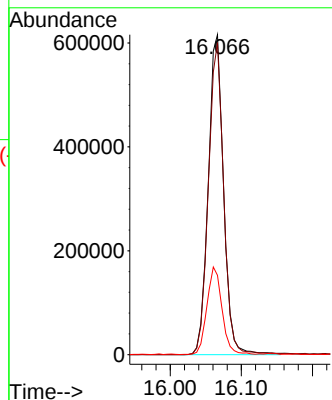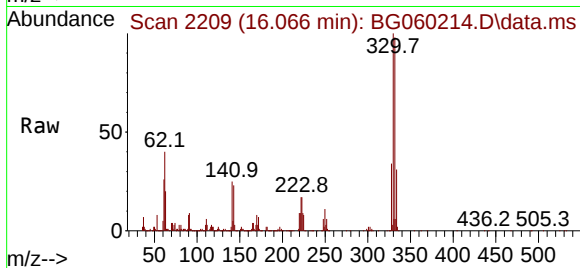

#45
2-Fluorobiphenyl
Concen: 56.463 ng
RT: 13.199 min Scan# 1721
Delta R.T. -0.000 min
Lab File: BG060214.D
Acq: 3 Jan 2024 5:18

Tgt Ion	172	Resp	3129136
Ion Ratio <td>100</td> <td></td> <td></td>	100		
Lower			
Upper			
171	38.7	32.6	48.8
170	27.1	21.8	32.6


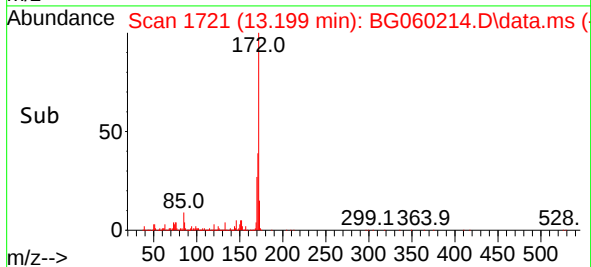
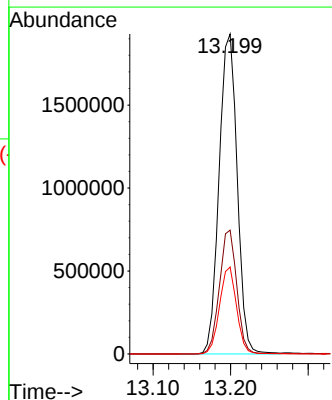
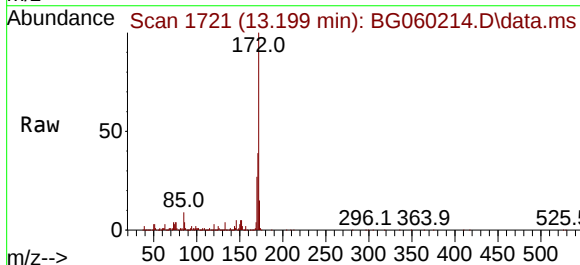




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.324 min Scan# 2423
Delta R.T. -0.000 min
Lab File: BG060214.D
Acq: 3 Jan 2024 5:18




Instrument :
BNA_G
ClientSampleId :
GHL-SS-07-2-4


Tgt Ion:188 Resp: 1912028
Ion Ratio Lower Upper
188 100
94 10.1 7.8 11.6
80 10.8 8.6 13.0

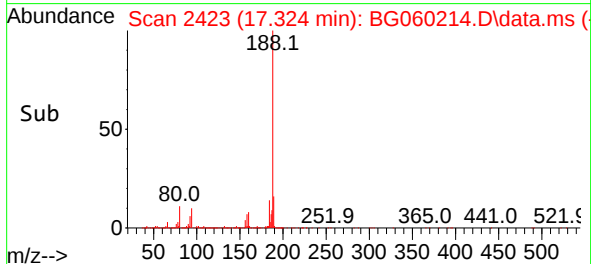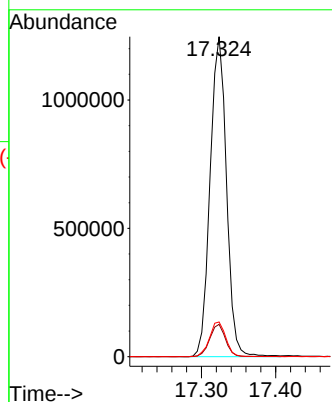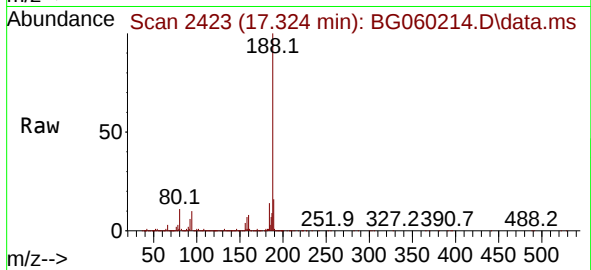

#72
Anthracene
Concen: 2.981 ng
RT: 17.453 min Scan# 2445
Delta R.T. -0.006 min
Lab File: BG060214.D
Acq: 3 Jan 2024 5:18

Tgt Ion:178 Resp: 279822
Ion Ratio Lower Upper
178 100
176 16.9 16.2 24.2
179 14.2 14.0 21.0

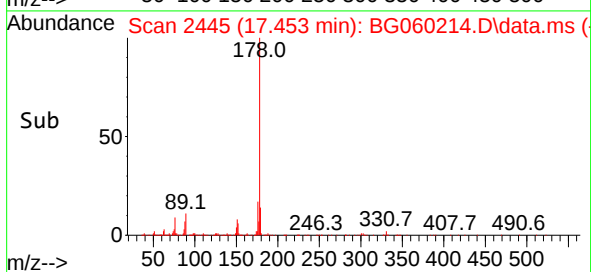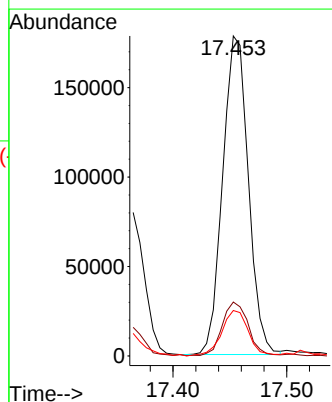



#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.589 min Scan# 3149

Delta R.T. -0.000 min

Lab File: BG060214.D

Acq: 3 Jan 2024 5:18

Instrument :

BNA_G

ClientSampleId :

GHL-SS-07-2-4





Tgt Ion:240 Resp: 1568413

Ion Ratio Lower Upper

240 100

120 10.2 8.5 12.7

236 24.5 21.4 32.2

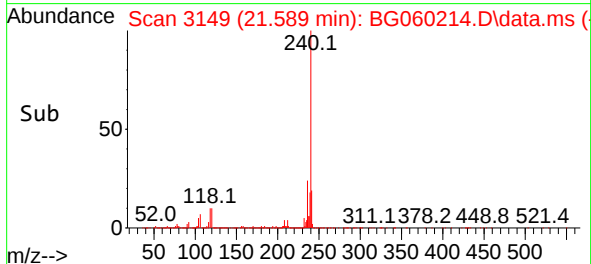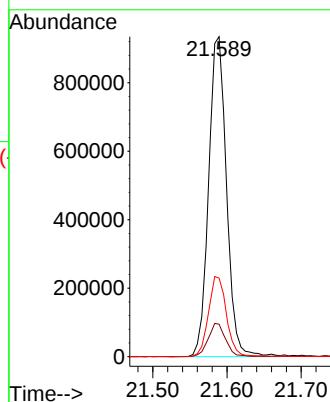

#79

Terphenyl-d14

Concen: 53.298 ng

RT: 19.944 min Scan# 2869

Delta R.T. -0.001 min

Lab File: BG060214.D

Acq: 3 Jan 2024 5:18




Tgt Ion:244 Resp: 4348176


Ion Ratio Lower Upper

244 100

212 10.3 9.5 14.3

122 13.2 11.4 17.2

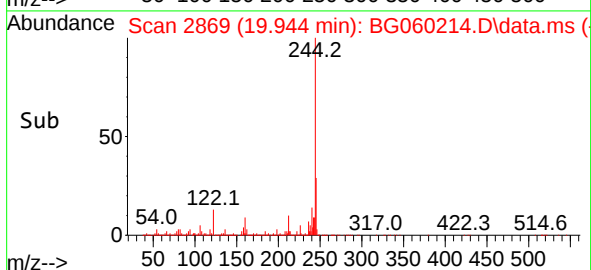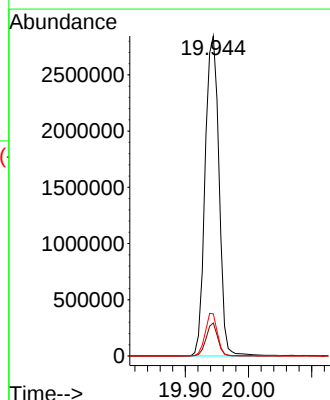



#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.762 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: BG060214.D
 Acq: 3 Jan 2024 5:18

Instrument :
 BNA_G
 ClientSampleId :
 GHL-SS-07-2-4

Tgt Ion:264 Resp: 1784365

Ion	Ratio	Lower	Upper
264	100		
260	23.0	18.0	27.0
265	21.9	17.4	26.0

