

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
 Data File : BG060205.D
 Acq On : 2 Jan 2024 23:13
 Operator : MA/JU
 Sample : PB158126BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB158126BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG060205.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.509	405	412	427	rBV	6049573	9731065	41.84%	9.810%
2	7.101	675	683	698	rBV	5390356	9401673	40.42%	9.478%
3	7.936	817	825	837	rBV	872992	1520283	6.54%	1.533%
4	9.099	1015	1023	1037	rBV	3256971	5780948	24.85%	5.828%
5	10.738	1294	1302	1312	rBV	1230064	2200830	9.46%	2.219%
6	13.200	1712	1721	1738	rBV	9184040	15002063	64.50%	15.125%
7	14.575	1948	1955	1966	rBV	2362750	3645632	15.67%	3.675%
8	16.067	2200	2209	2226	rBV	7162912	11433316	49.15%	11.527%
9	17.325	2414	2423	2436	rBV	3239277	4930007	21.20%	4.970%
10	19.945	2862	2869	2885	rBV	16090449	23259966	100.00%	23.450%
11	21.590	3141	3149	3161	rBV	3173550	5372146	23.10%	5.416%
12	24.763	3677	3689	3703	rBV2	1992653	5888118	25.31%	5.936%
13	25.903	3873	3883	3893	rBV3	121394	369554	1.59%	0.373%
14	27.243	4103	4111	4124	rVB4	101764	373238	1.60%	0.376%
15	28.864	4376	4387	4400	rVB5	69669	281520	1.21%	0.284%




Sum of corrected areas: 99190359

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
Data File : BG060205.D
Acq On : 2 Jan 2024 23:13
Operator : MA/JU
Sample : PB158126BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB158126BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

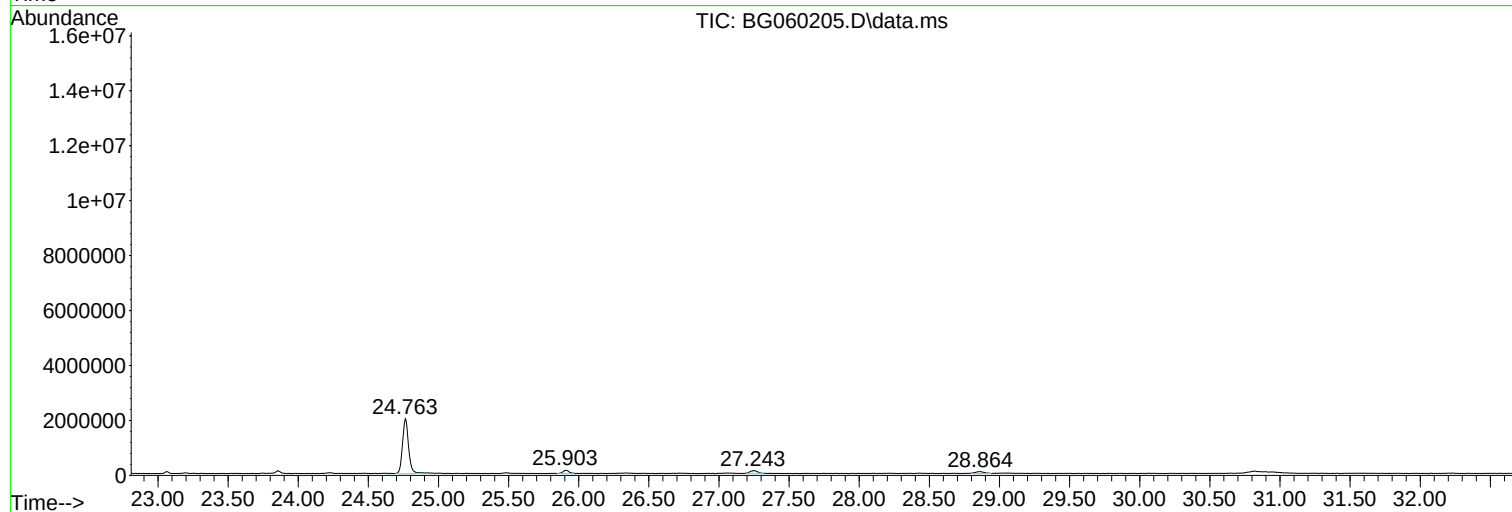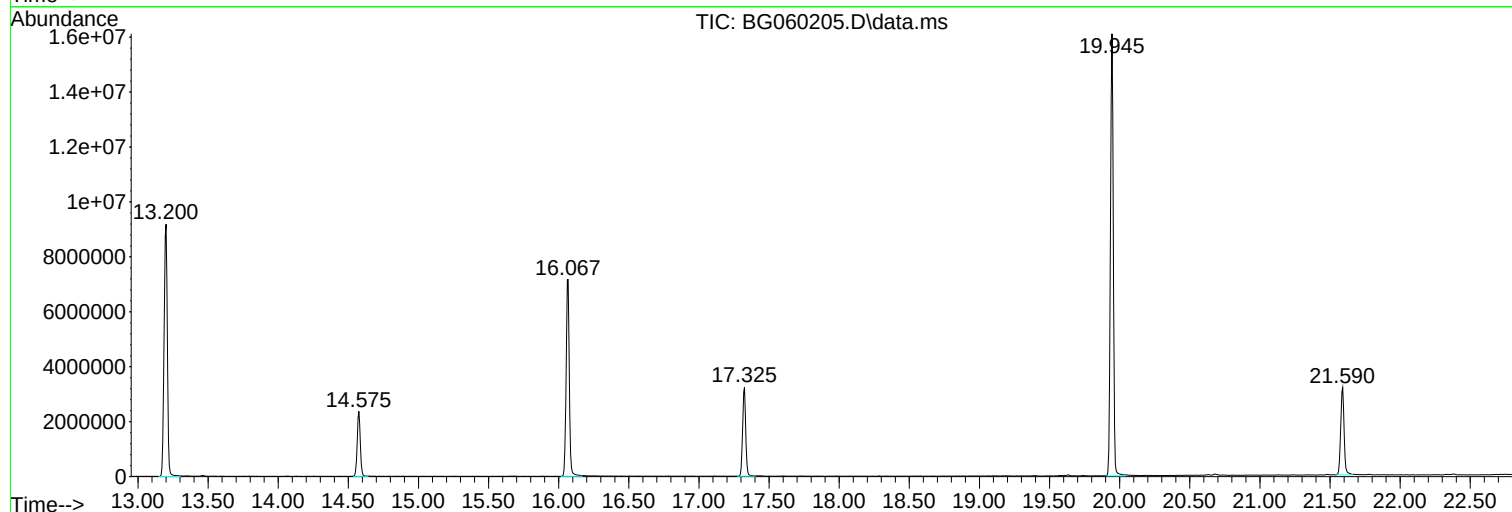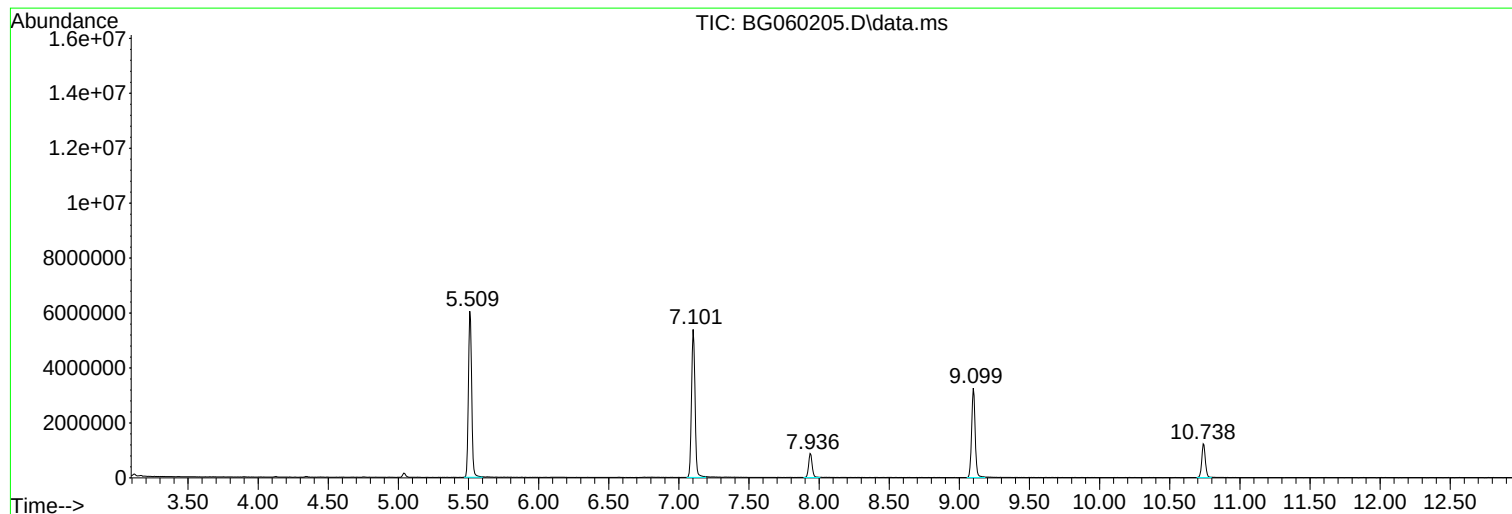

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
Data File : BG060205.D
Acq On : 2 Jan 2024 23:13
Operator : MA/JU
Sample : PB158126BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB158126BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
Data File : BG060205.D
Acq On : 2 Jan 2024 23:13
Operator : MA/JU
Sample : PB158126BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB158126BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------