
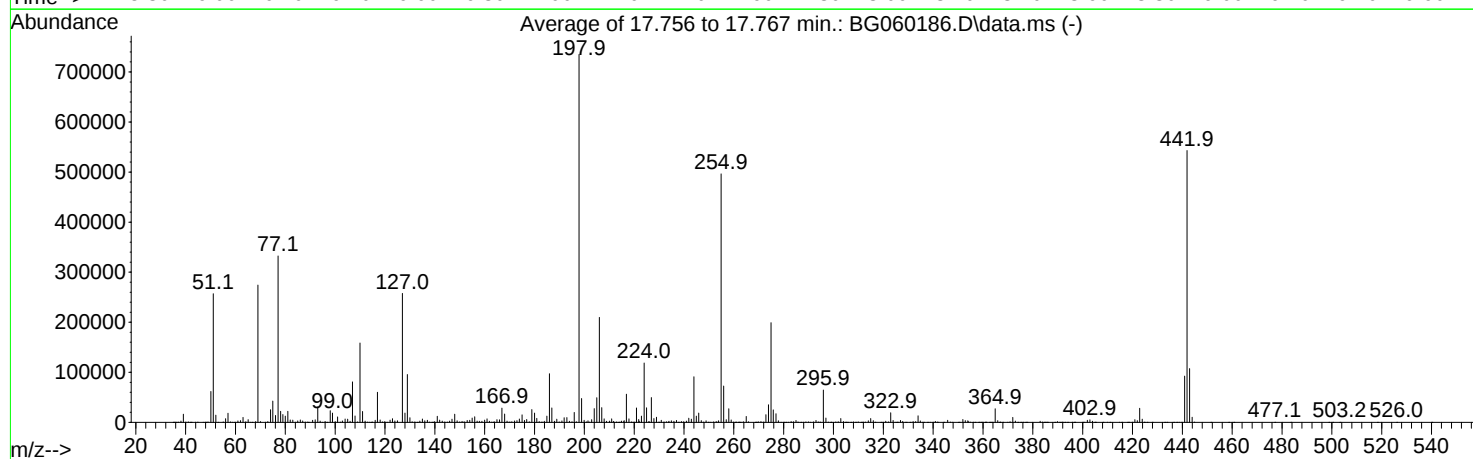


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
Data File : BG060186.D
Acq On : 2 Jan 2024 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Dec 30 03:14:04 2023

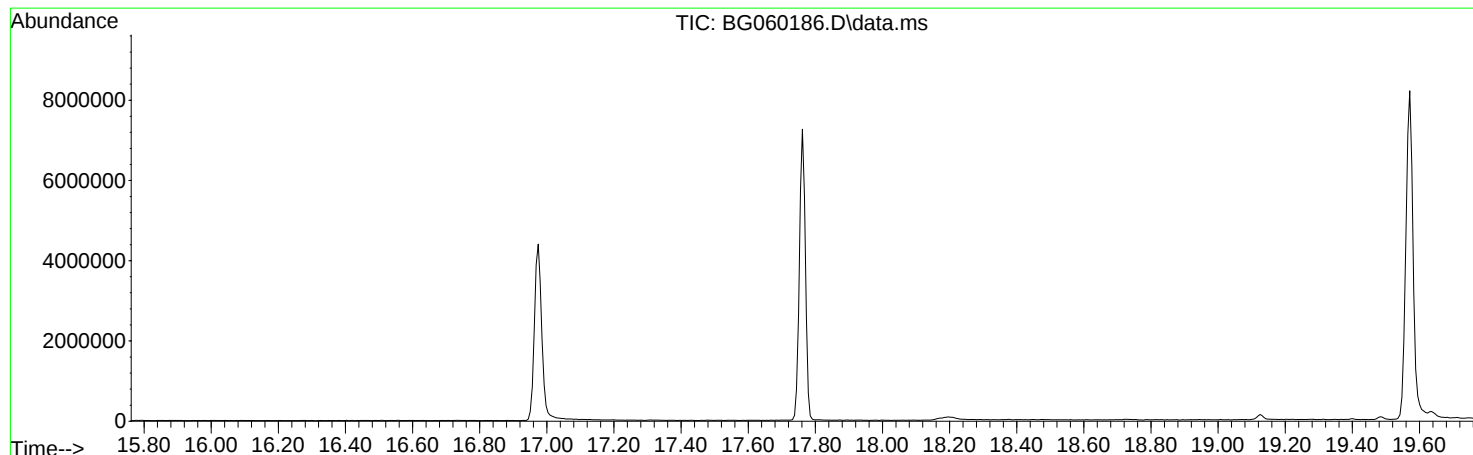




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2489

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	257088	PASS
68	69	0.00	2	0.6	1519	PASS
69	198	0.00	100	37.3	274295	PASS
70	69	0.00	2	0.6	1682	PASS
127	198	10	80	35.1	257579	PASS
197	198	0.00	2	0.2	1445	PASS
198	198	100	100	100.0	734848	PASS
199	198	5	9	6.5	47504	PASS
275	198	10	60	27.1	199211	PASS
365	198	1	100	3.7	27157	PASS
441	198	0.01	100	12.6	92224	PASS
442	442	50	100	100.0	542912	PASS
443	442	15	24	19.8	107515	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
Data File : BG060186.D
Acq On : 2 Jan 2024 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 02 10:59:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

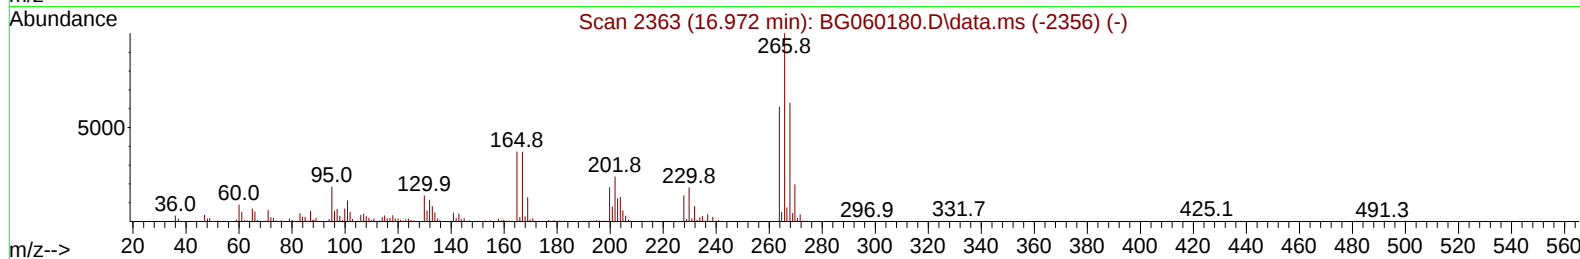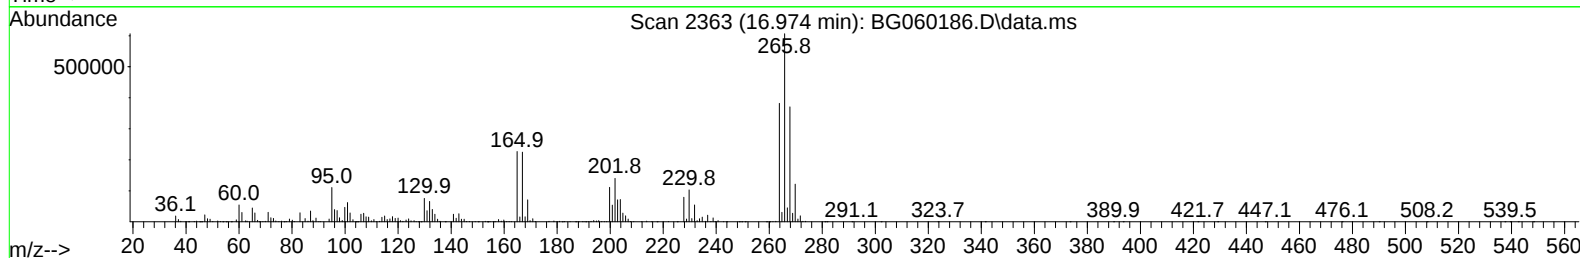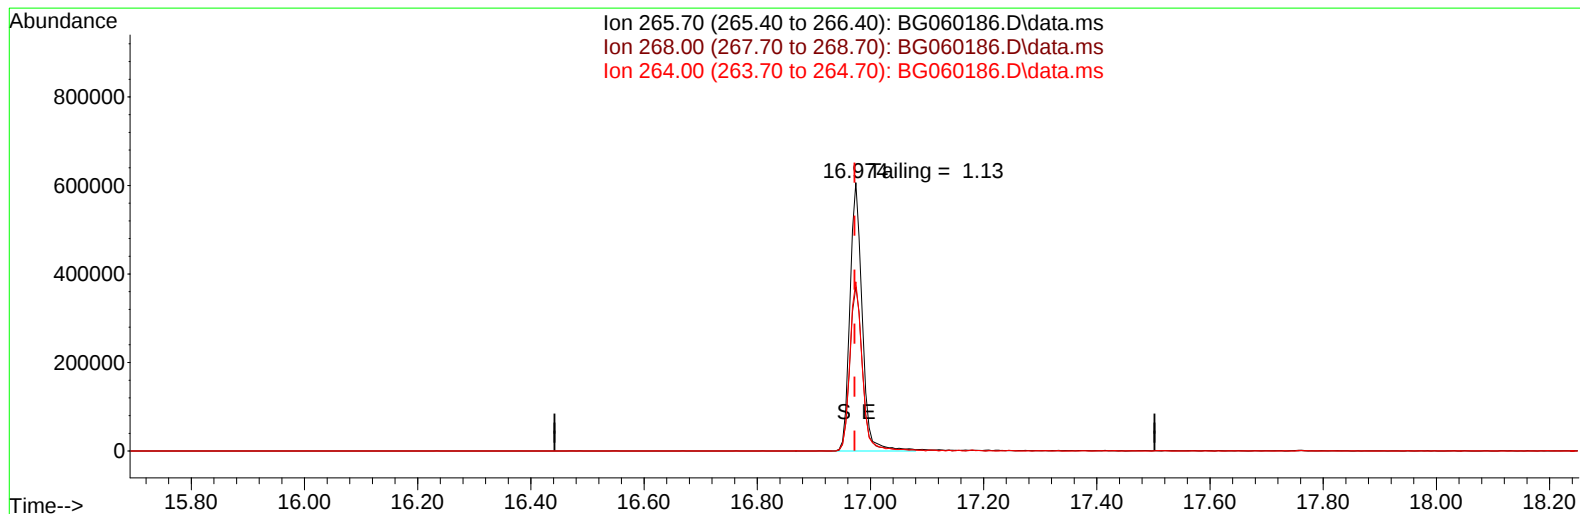

TIC: BG060186.D\data.ms

(70) Pentachlorophenol (C)

16.974min (+ 0.002) 618388.76 ng




response 916356

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	61.11
264.00	65.80	63.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
Data File : BG060186.D
Acq On : 2 Jan 2024 9:09
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 02 10:59:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

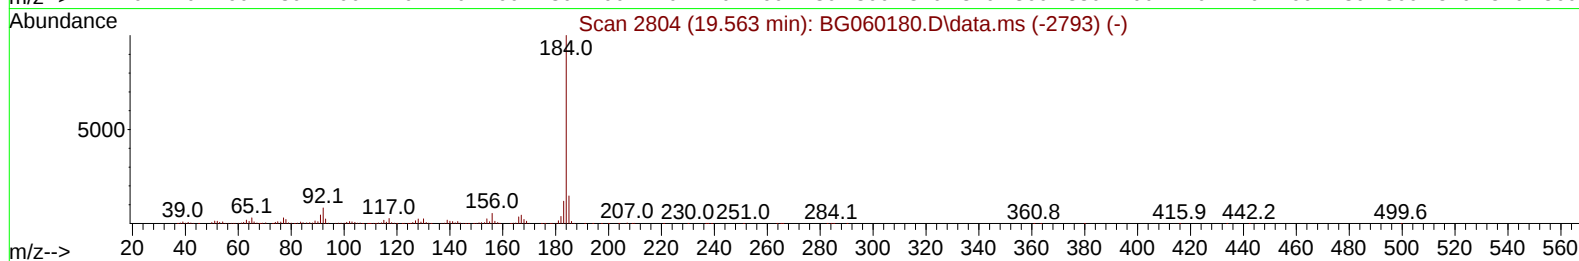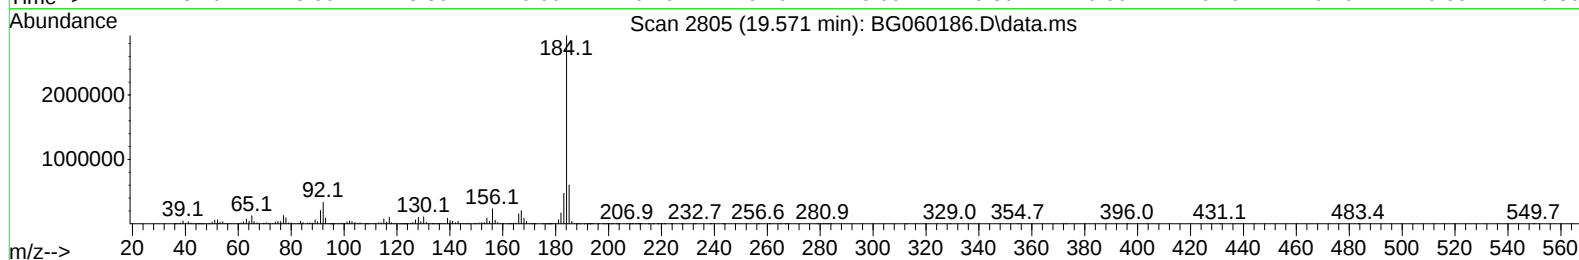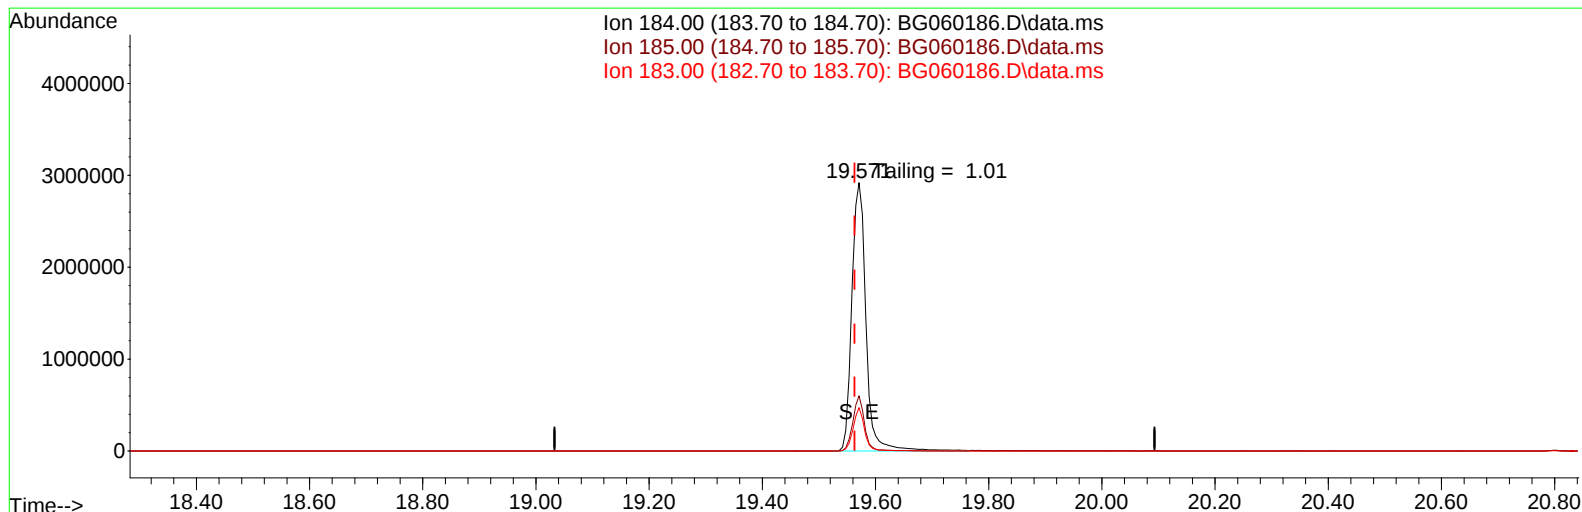

TIC: BG060186.D\data.ms

(77) Benzidine

19.571min (+ 0.008) 5724.17 ng m

response 5079606

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	20.61#
183.00	11.80	16.17#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/2/2024	BNA_G	<u>BG060186.D</u>
Compound Name	Response	Retention Time
DDT	2238567	20.799
DDD	36222	20.358
DDE	838	19.853
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37060	2275627	1.63

Instrument :
BNA_G
ClientSampleId :
DFTPP