
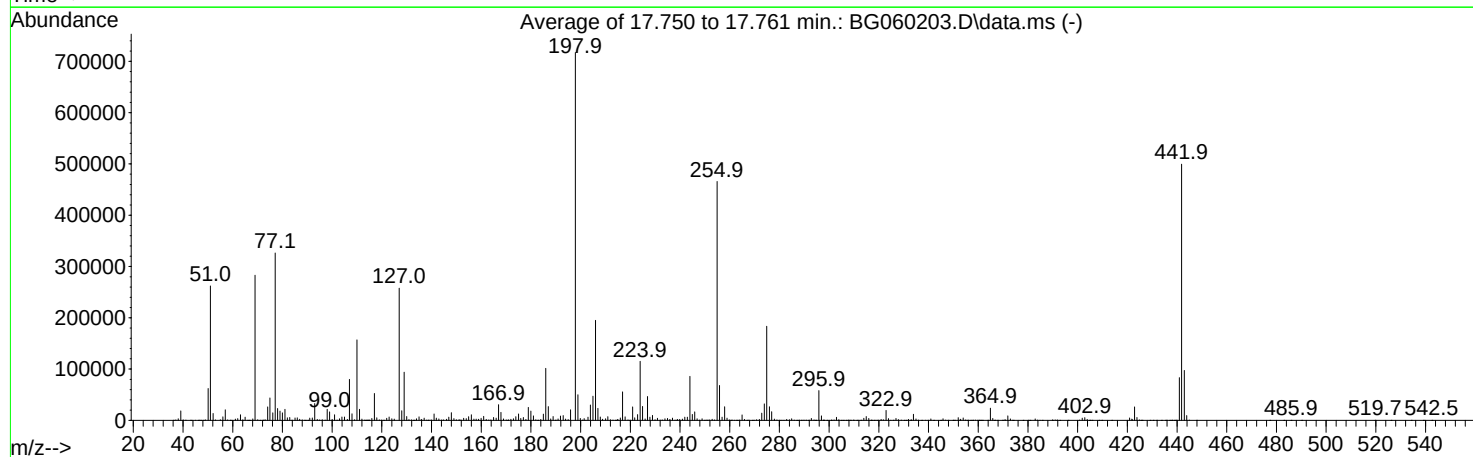


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
Data File : BG060203.D
Acq On : 2 Jan 2024 21:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Dec 30 03:14:04 2023

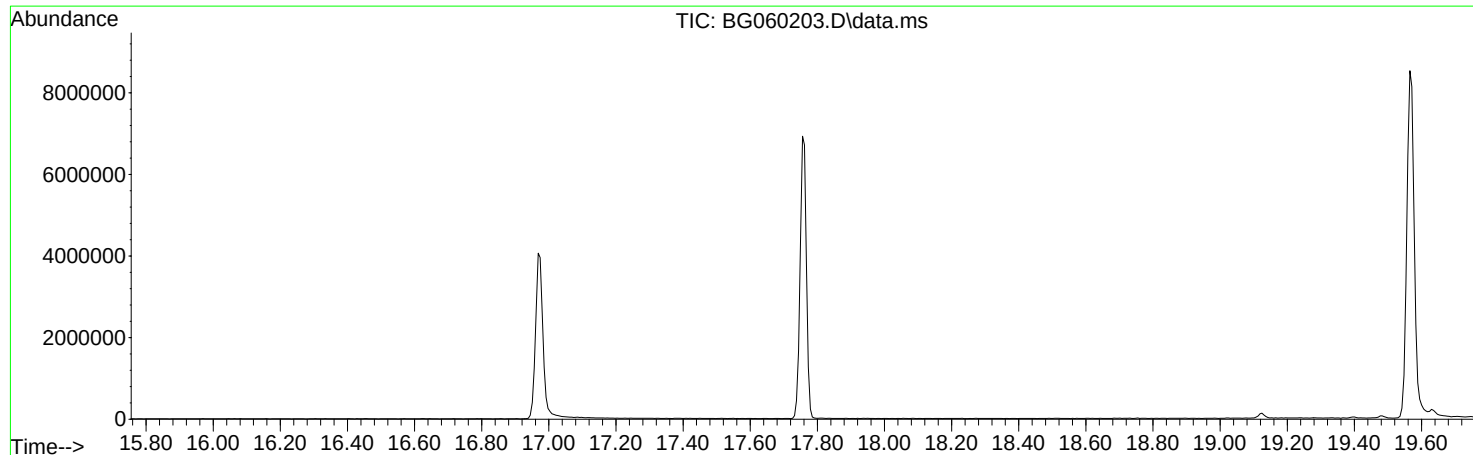




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	262118	PASS
68	69	0.00	2	1.0	2788	PASS
69	198	0.00	100	39.4	282837	PASS
70	69	0.00	2	0.5	1306	PASS
127	198	10	80	35.9	257698	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	717227	PASS
199	198	5	9	7.0	50091	PASS
275	198	10	60	25.6	183419	PASS
365	198	1	100	3.3	23828	PASS
441	198	0.01	100	11.6	83413	PASS
442	442	50	100	100.0	499400	PASS
443	442	15	24	19.5	97333	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010224\
Data File : BG060203.D
Acq On : 2 Jan 2024 21:12
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 03 01:09:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG122923.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 30 03:14:04 2023
Response via : Initial Calibration

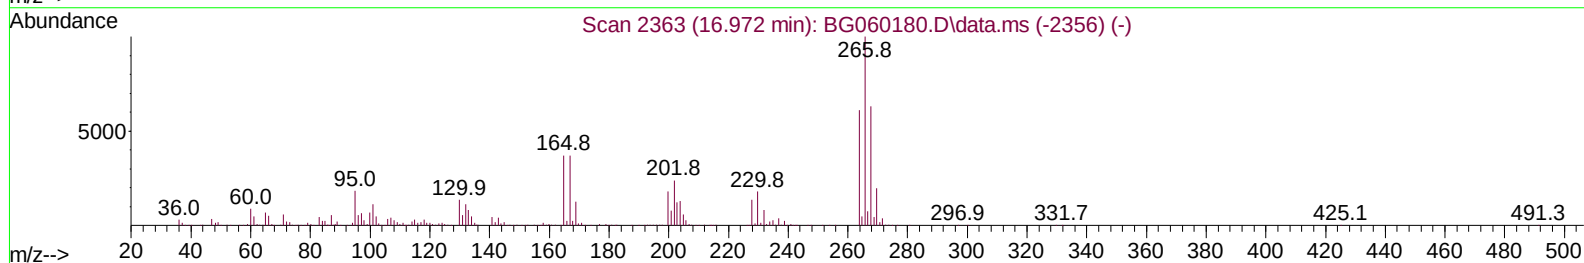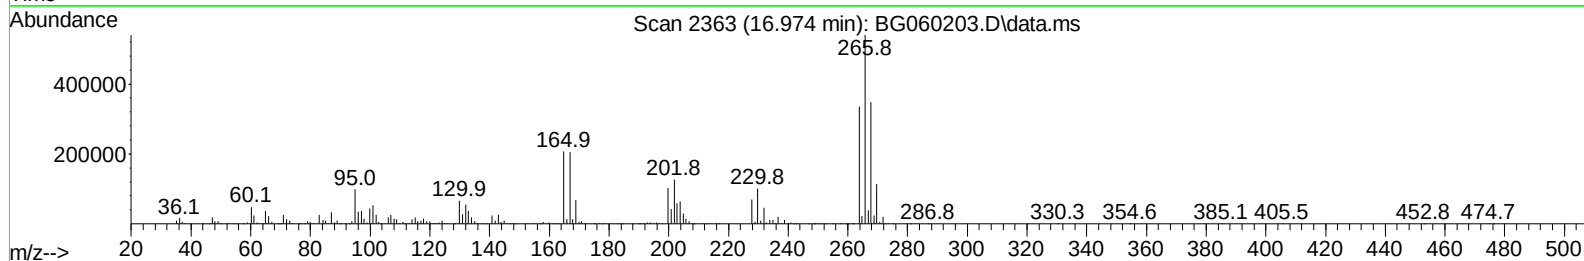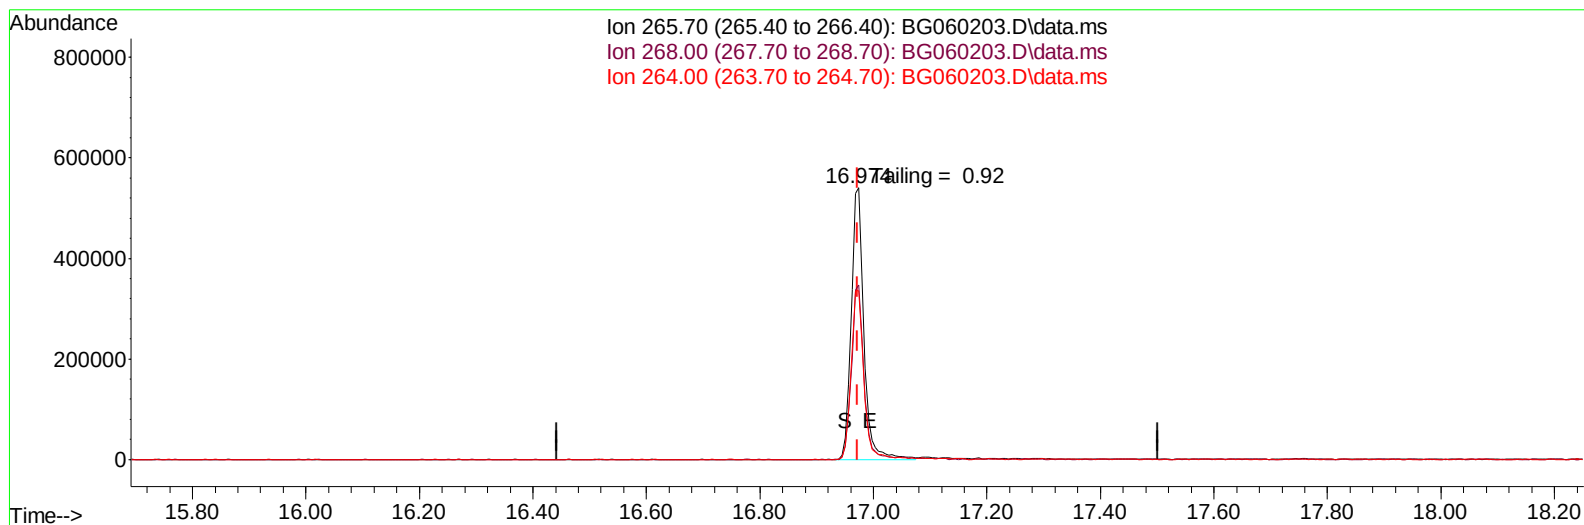

TIC: BG060203.D\data.ms

(70) Pentachlorophenol (C)

16.974min (+ 0.002) 826206.53 ng

response 840655

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	64.34
264.00	65.80	66.41
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/2/2024	BNA_G	<u>BG060203.D</u>
Compound Name	Response	Retention Time
DDT	2508461	20.799
DDD	79807	20.352
DDE	1306	19.853
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
81113	2589574	3.13

Instrument :
BNA_G
ClientSampleId :
DFTPP