
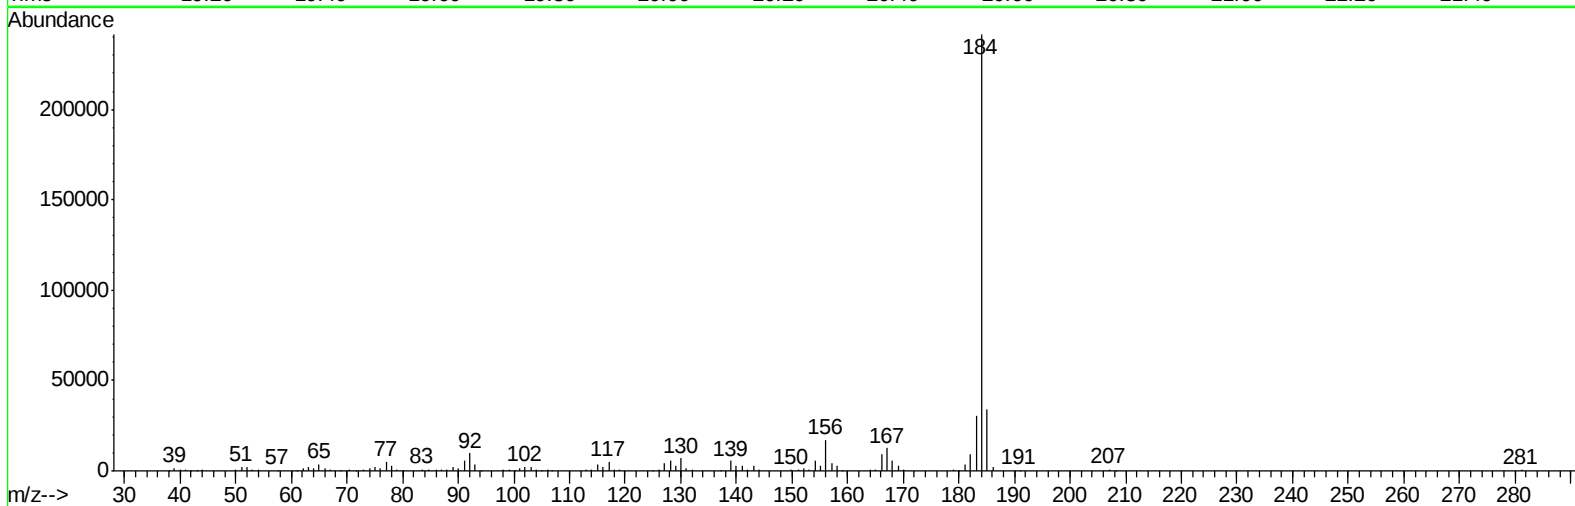


Data Path : Z:\HPCHEM1\BNA G\Data\BG010318\
Data File : BG031900.D
Acq On : 3 Jan 2018 21:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 08:38:13 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 15:51:46 2017
Response via : Initial Calibration

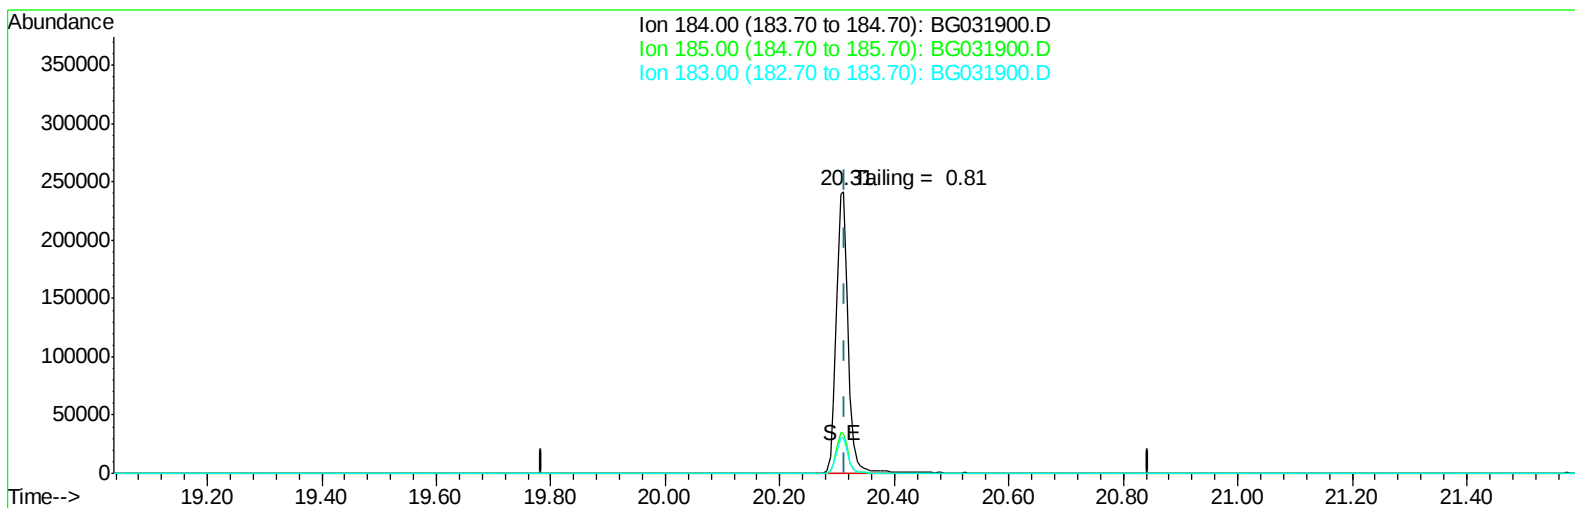

TIC: BG031900.D

(76) Benzidine



20.311min (-0.003) 0.00ng

response 348230

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.07
183.00	13.30	12.61
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG010318\
Data File : BG031900.D
Acq On : 3 Jan 2018 21:37
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 04 08:38:13 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 15:51:46 2017
Response via : Initial Calibration

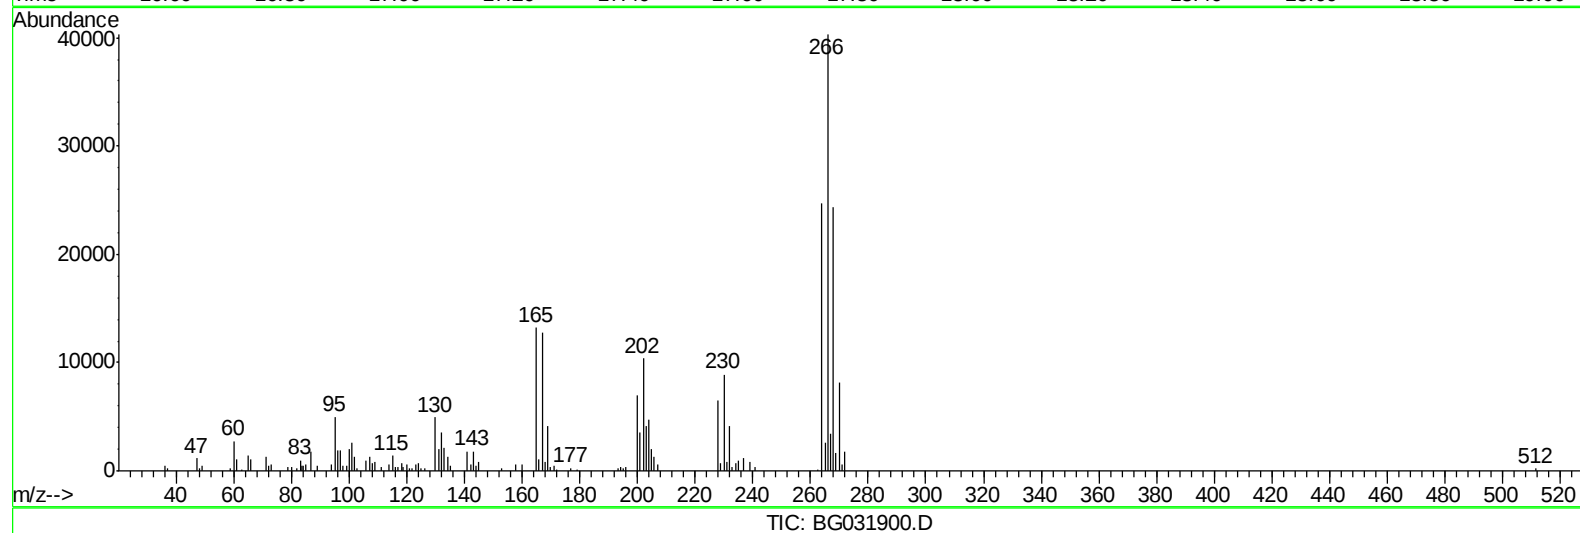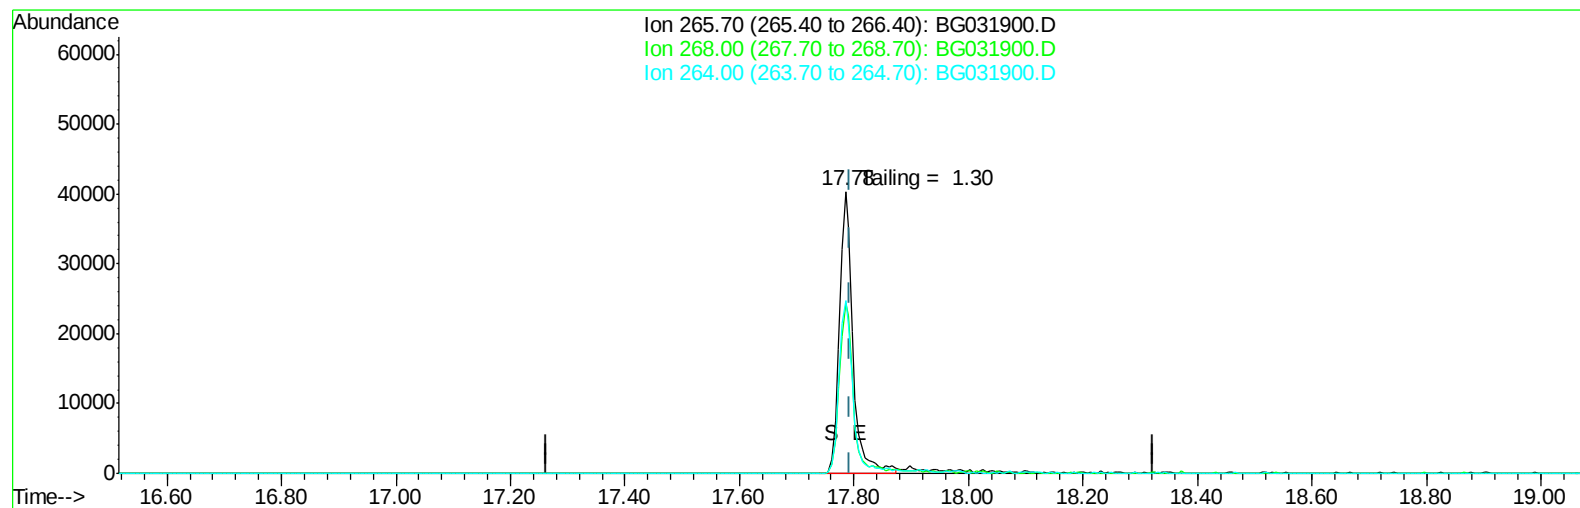

TIC: BG031900.D

(69) Pentachlorophenol (C)

17.785min (-0.009) 23425.10ng

response 64785

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.54
264.00	62.00	61.33
0.00	0.00	0.00