

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG010318\
 Data File : BG031898.D
 Acq On : 3 Jan 2018 19:45
 Operator : SJ/JU
 Sample : PB105460BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB105460BL

Quant Time: Jan 04 06:48:08 2018
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 29 15:51:46 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.79	152	43942	20.00	ng	0.00
21) Naphthalene-d8	11.67	136	175339	20.00	ng	-0.01
38) Acenaphthene-d10	15.41	164	120813	20.00	ng	-0.01
63) Phenanthrene-d10	18.15	188	350836	20.00	ng	-0.01
75) Chrysene-d12	22.49	240	428631	20.00	ng	-0.02
86) Perylene-d12	26.22	264	450760	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	6.21	112	303895	125.96	ng	0.00
7) Phenol-d6	7.89	99	391521	124.99	ng	0.00
23) Nitrobenzene-d5	9.98	82	206175	88.79	ng	0.00
41) 2,4,6-Tribromophenol	16.89	330	270467	146.72	ng	0.00
44) 2-Fluorobiphenyl	14.05	172	764592	79.43	ng	0.00
78) Terphenyl-d14	20.68	244	1601132	85.34	ng	-0.01


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_G\DATA\BG010318\
Data File : BG031898.D
Acq On : 3 Jan 2018 19:45
Operator : SJ/JU
Sample : PB105460BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB105460BL

Quant Time: Jan 04 06:48:08 2018
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 15:51:46 2017
Response via : Initial Calibration

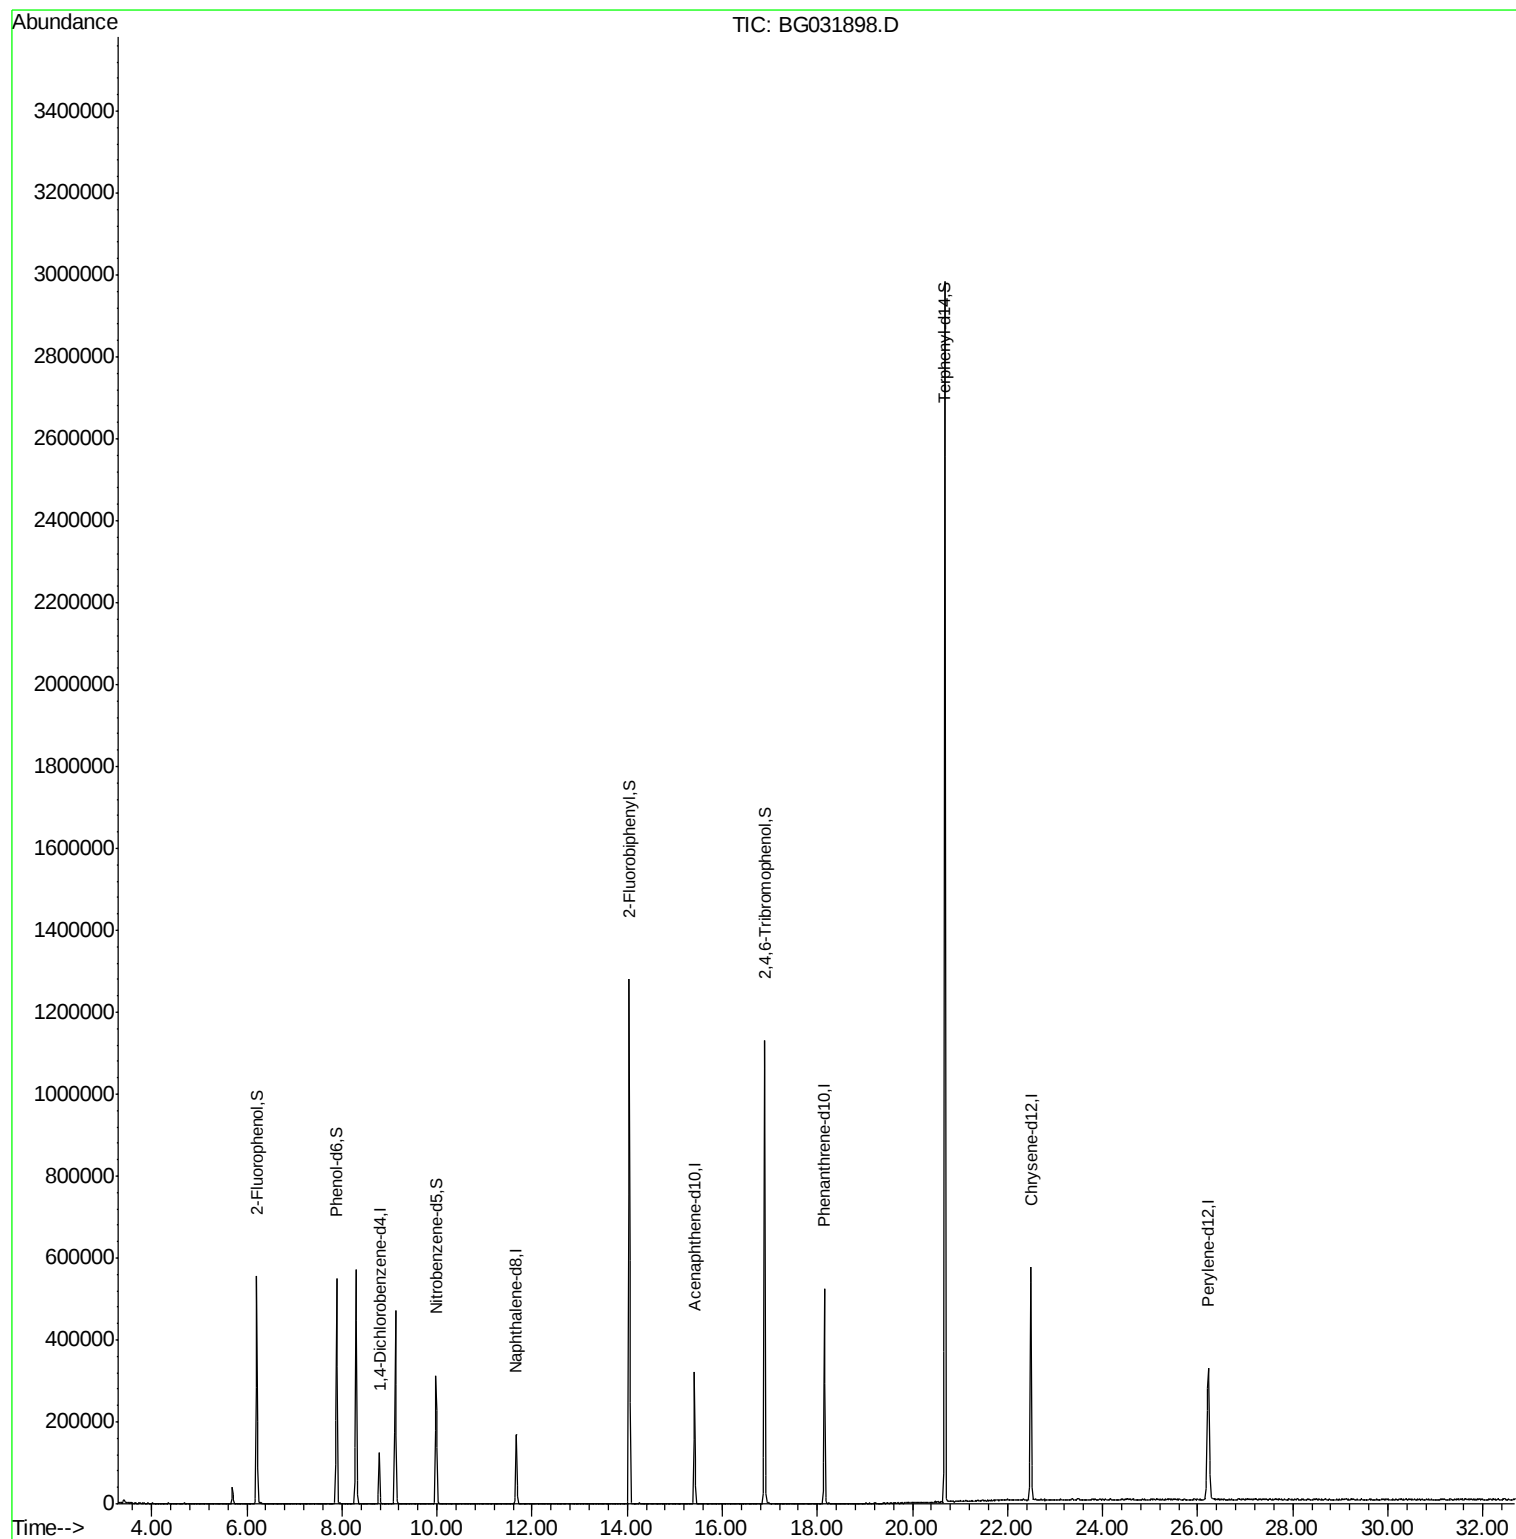




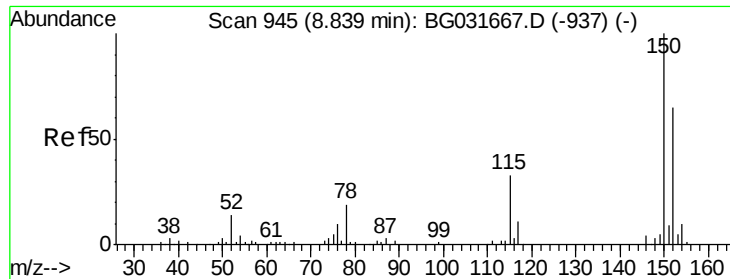


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 8.79 min Scan# 936
 Delta R.T. -0.01 min
 Lab File: BG031898.D
 Acq: 3 Jan 2018 19:45

Instrument :
 BNA_G
 ClientSampleID :
 PB105460BL




Tgt Ion:152 Resp: 43942
 Ion Ratio Lower Upper
 152 100
 150 168.5 126.6 189.8
 115 50.0 53.0 79.4#

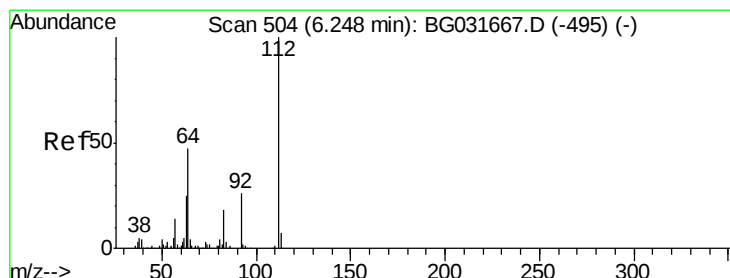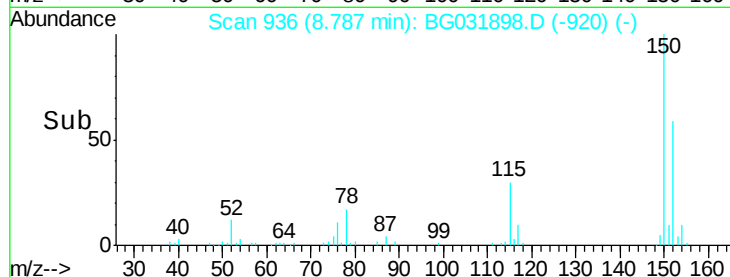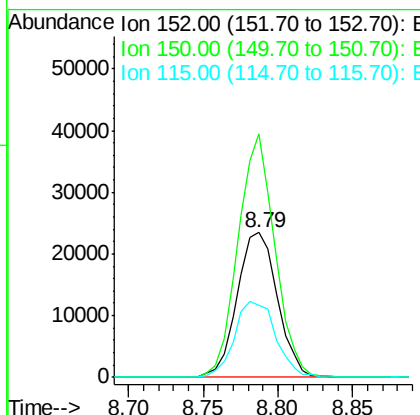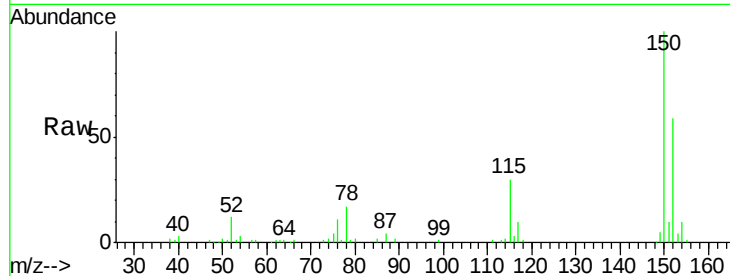

#5

2-Fluorophenol
 Concen: 125.964 ng
 RT: 6.21 min Scan# 497
 Delta R.T. -0.01 min
 Lab File: BG031898.D
 Acq: 3 Jan 2018 19:45

Tgt Ion:112 Resp: 303895
 Ion Ratio Lower Upper
 112 100
 64 51.0 56.3 84.5#
 63 26.9 30.1 45.1#

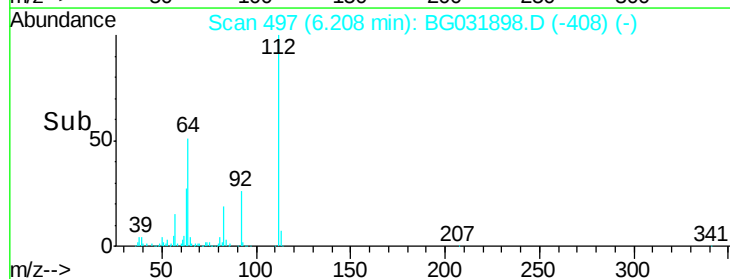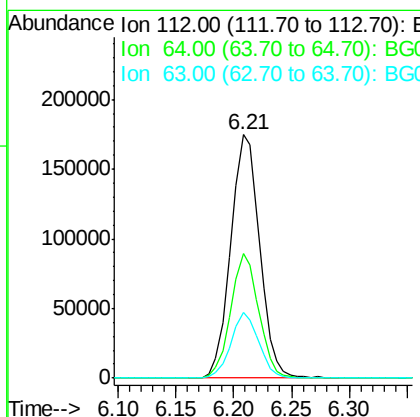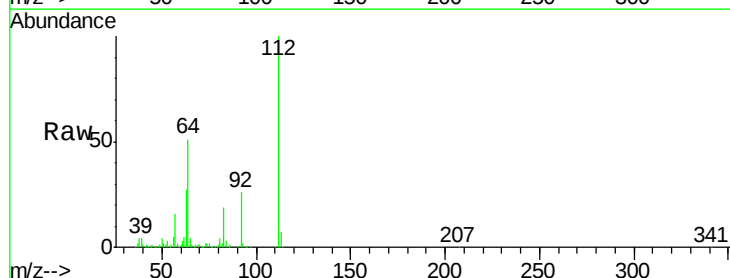



#7

Phenol-d6

Concen: 124.995 ng

RT: 7.89 min Scan# 783

Delta R.T. -0.01 min

Lab File: BG031898.D

Acq: 3 Jan 2018 19:45

Instrument :

BNA_G

ClientSampleId :

PB105460BL


Tgt Ion: 99 Resp: 391521

Ion Ratio Lower Upper




99 100

42 13.6 14.1 21.1#

71 33.4 26.1 39.1

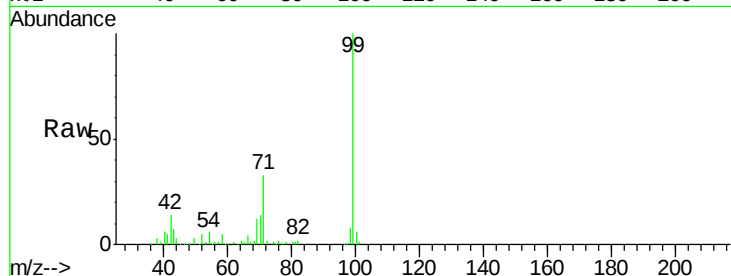

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

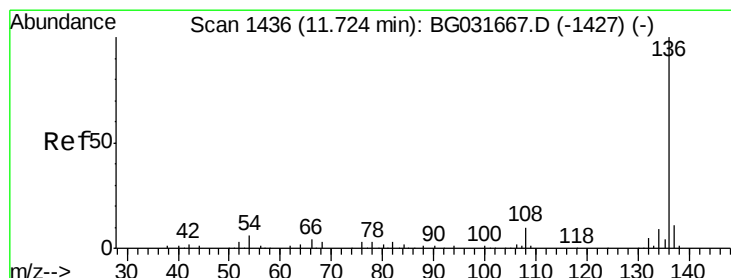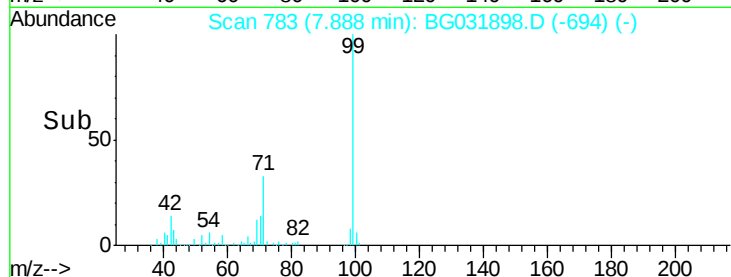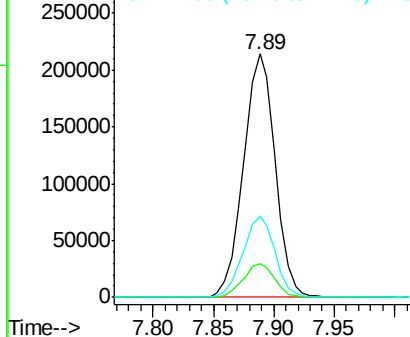

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.67 min Scan# 1426

Delta R.T. -0.01 min

Lab File: BG031898.D

Acq: 3 Jan 2018 19:45

Tgt Ion: 136 Resp: 175339


Ion Ratio Lower Upper

136 100



137 10.3 9.2 13.8


54 5.9 10.3 15.5#

68 4.4 4.5 6.7#

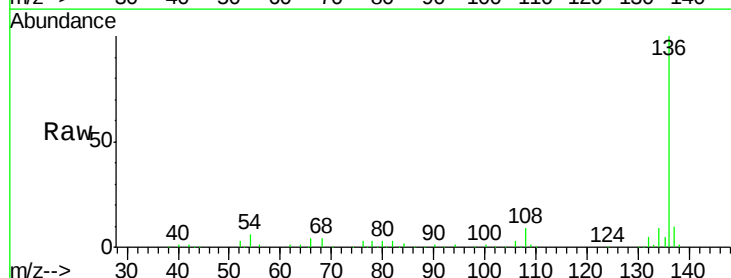

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

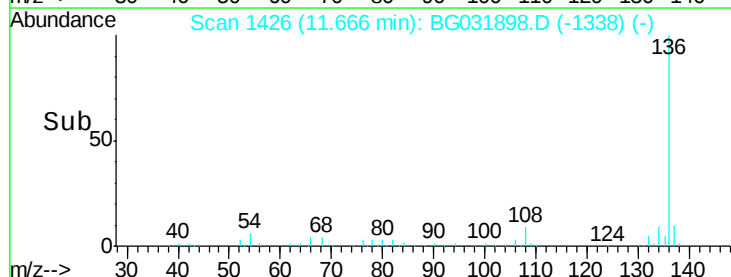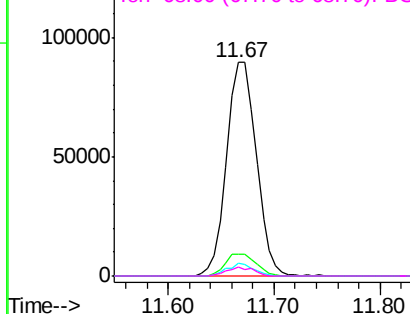


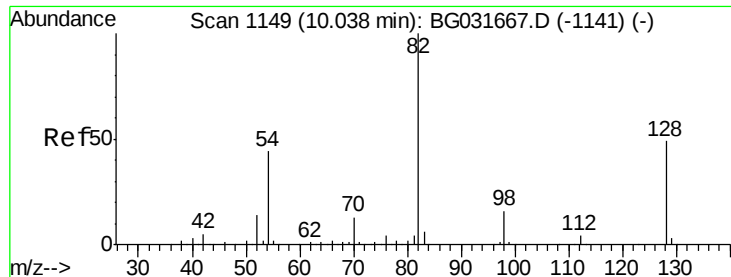




#23
 Nitrobenzene-d5
 Concen: 88.792 ng
 RT: 9.98 min Scan# 1139
 Delta R.T. -0.01 min
 Lab File: BG031898.D
 Acq: 3 Jan 2018 19:45

Instrument :
 BNA_G
 ClientSampleID :
 PB105460BL

Tgt Ion: 82 Resp: 206175
 Ion Ratio Lower Upper
 82 100
 128 51.2 29.7 44.5#
 54 44.0 43.1 64.7

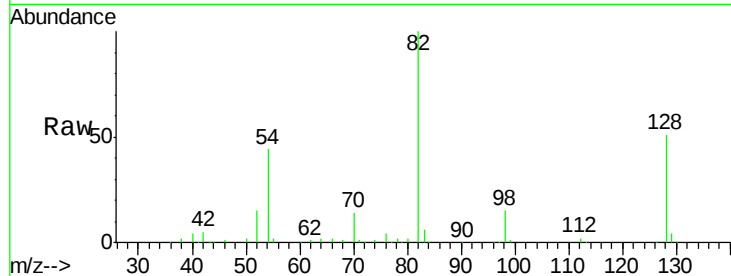


Abundance Ion 82.00 (81.70 to 82.70): BGC
 Ion 128.00 (127.70 to 128.70): BGC
 Ion 54.00 (53.70 to 54.70): BGC

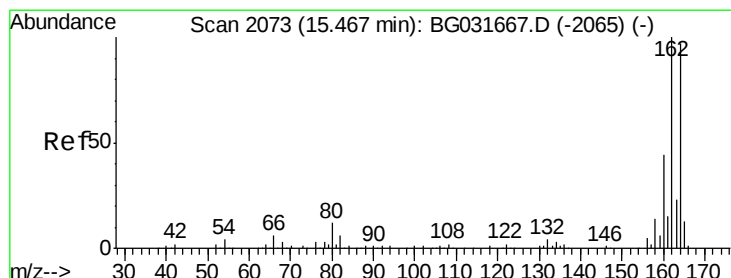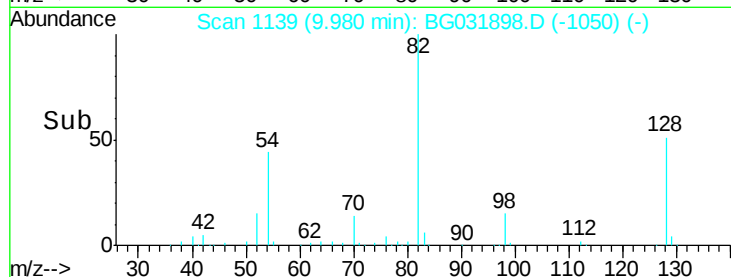
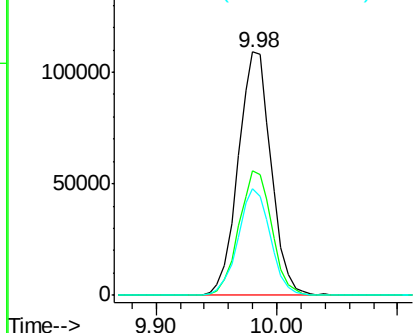



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 15.41 min Scan# 2064
 Delta R.T. -0.01 min
 Lab File: BG031898.D
 Acq: 3 Jan 2018 19:45

Tgt Ion: 164 Resp: 120813
 Ion Ratio Lower Upper
 164 100
 162 106.1 78.8 118.2
 160 47.7 35.4 53.0

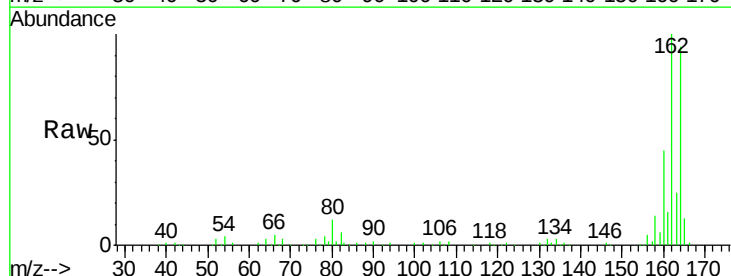

Abundance Ion 164.00 (163.70 to 164.70): BGC
 Ion 162.00 (161.70 to 162.70): BGC
 Ion 160.00 (159.70 to 160.70): BGC

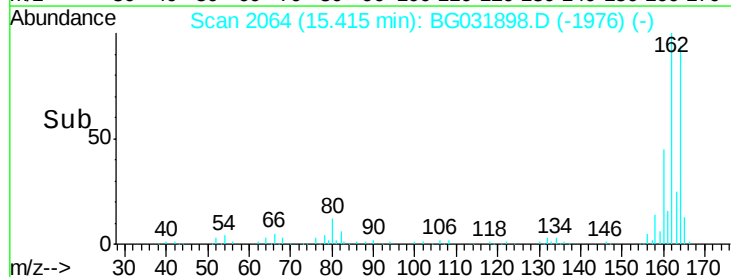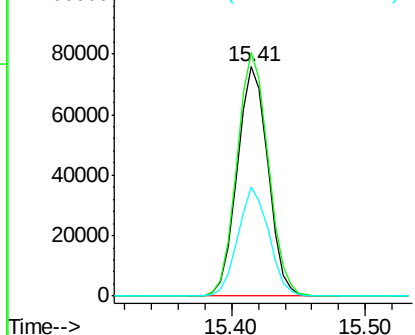


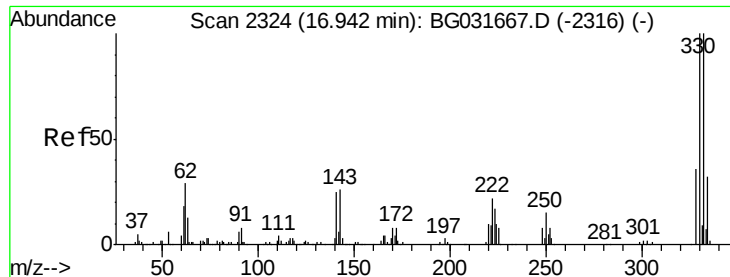




#41
 2,4,6-Tribromophenol
 Concen: 146.719 ng
 RT: 16.89 min Scan# 2315
 Delta R.T. -0.01 min
 Lab File: BG031898.D
 Acq: 3 Jan 2018 19:45

Instrument :
 BNA_G
 ClientSampleId :
 PB105460BL

Tgt Ion:330 Resp: 270467
 Ion Ratio Lower Upper
 330 100
 332 96.4 77.0 115.6
 141 26.8 25.2 37.8

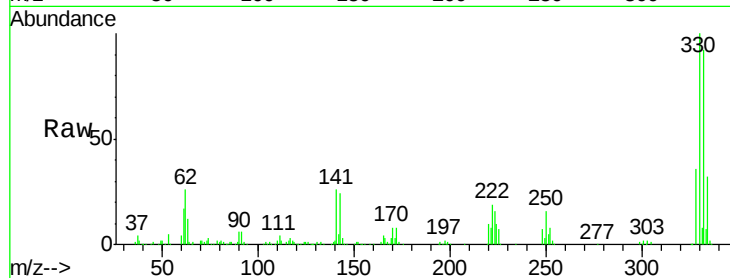


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

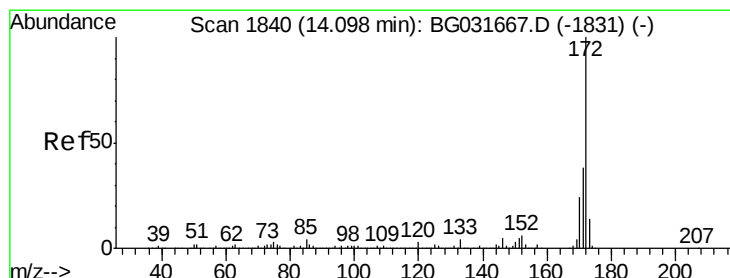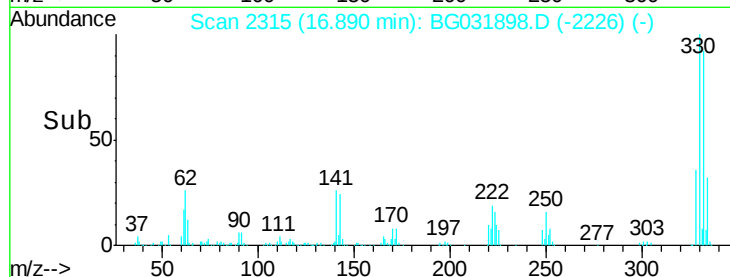
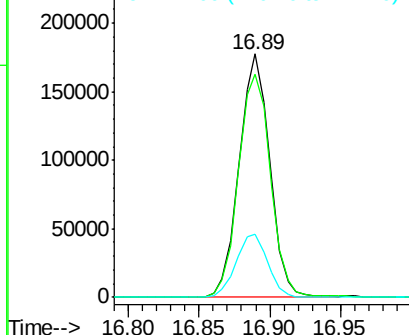



#44
 2-Fluorobiphenyl
 Concen: 79.434 ng
 RT: 14.05 min Scan# 1831
 Delta R.T. -0.01 min
 Lab File: BG031898.D
 Acq: 3 Jan 2018 19:45

Tgt Ion:172 Resp: 764592
 Ion Ratio Lower Upper
 172 100
 171 36.6 30.0 45.0
 170 23.8 19.5 29.3

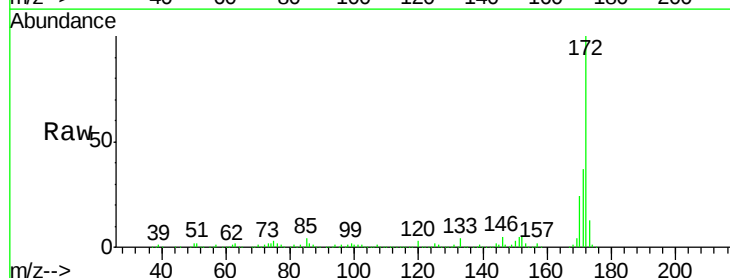

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



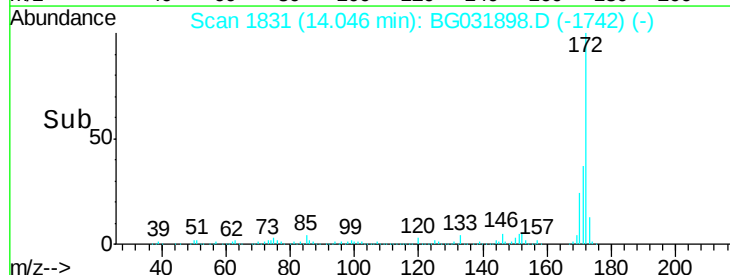
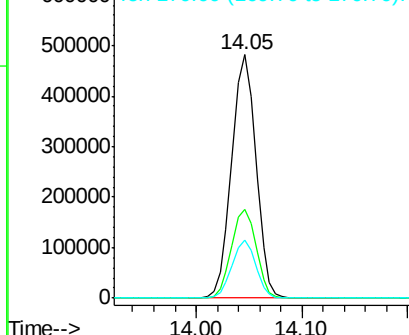


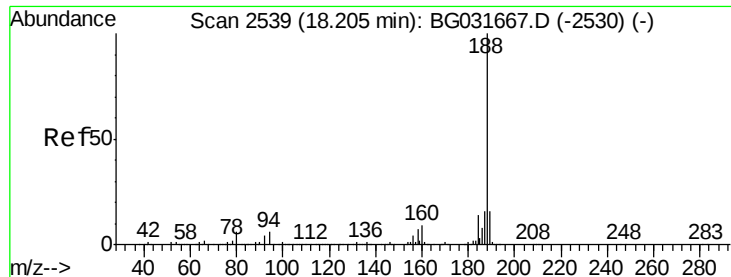

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.15 min Scan# 2529
Delta R.T. -0.01 min
Lab File: BG031898.D
Acq: 3 Jan 2018 19:45




Instrument :
BNA_G
ClientSampleId :
PB105460BL


Tgt Ion:188 Resp: 350836
Ion Ratio Lower Upper
188 100
94 5.6 6.9 10.3#
80 6.2 7.7 11.5#

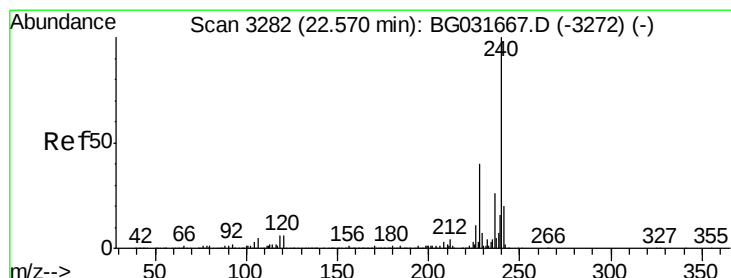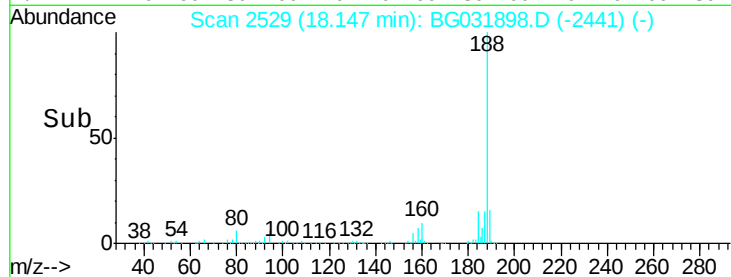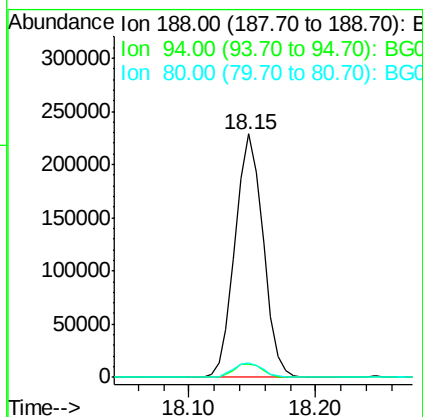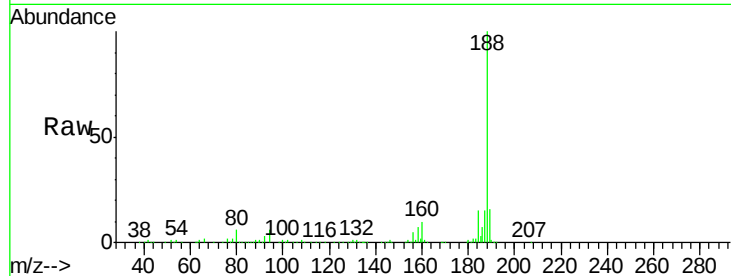

#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.49 min Scan# 3268
Delta R.T. -0.02 min
Lab File: BG031898.D
Acq: 3 Jan 2018 19:45

Tgt Ion:240 Resp: 428631
Ion Ratio Lower Upper
240 100
120 6.0 6.8 10.2#
236 25.9 20.9 31.3

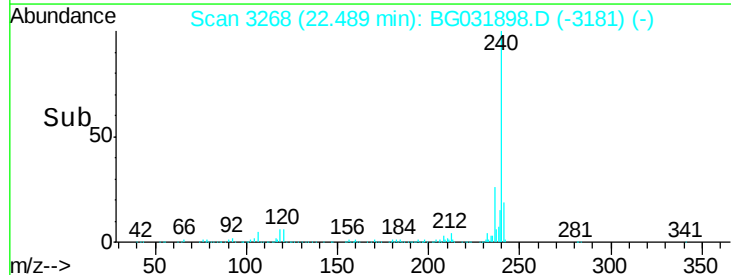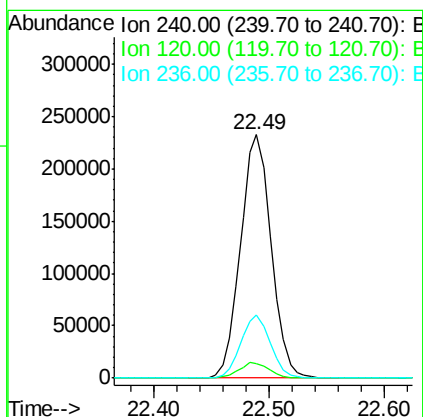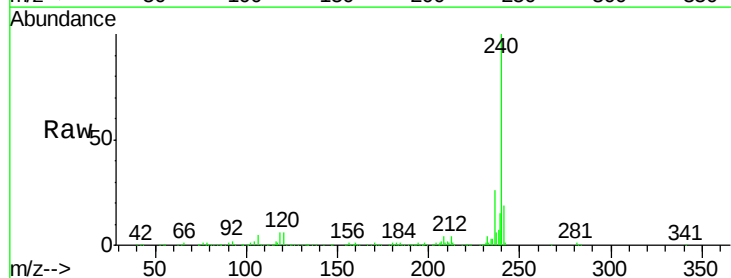

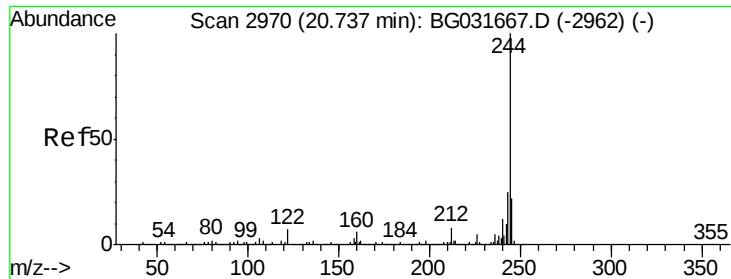

#78

Terphenyl-d14

Concen: 85.342 ng

RT: 20.68 min Scan# 2960

Delta R.T. -0.01 min

Lab File: BG031898.D

Acq: 3 Jan 2018 19:45

Instrument :

BNA_G

ClientSampleId :

PB105460BL


Tgt Ion:244 Resp: 1601132

Ion Ratio Lower Upper

244 100

212 7.2 5.8 8.8




122 7.1 7.0 10.4

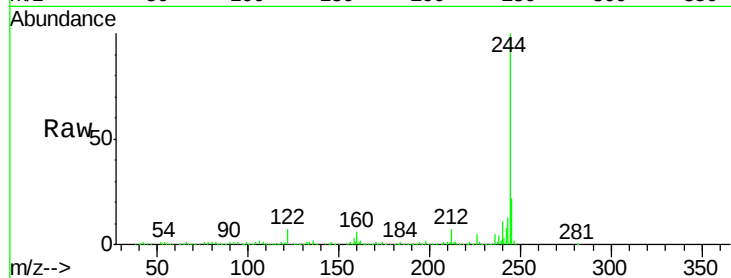

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

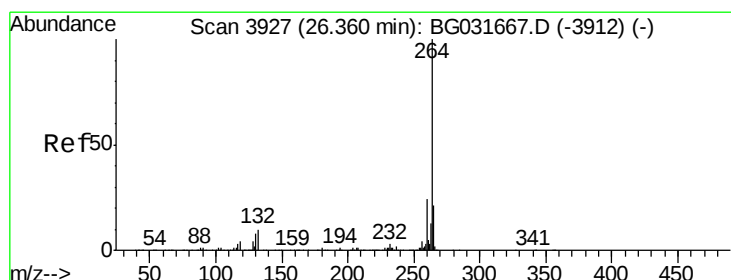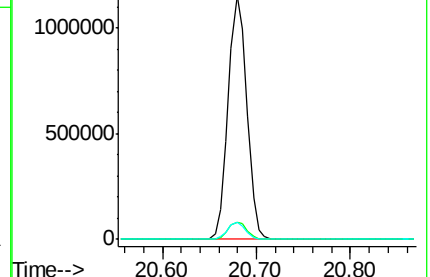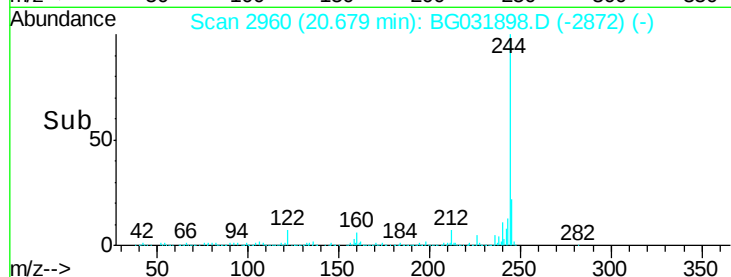

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.22 min Scan# 3903

Delta R.T. -0.03 min

Lab File: BG031898.D

Acq: 3 Jan 2018 19:45


Tgt Ion:264 Resp: 450760

Ion Ratio Lower Upper

264 100

260 23.0 17.4 26.0

265 21.8 17.7 26.5

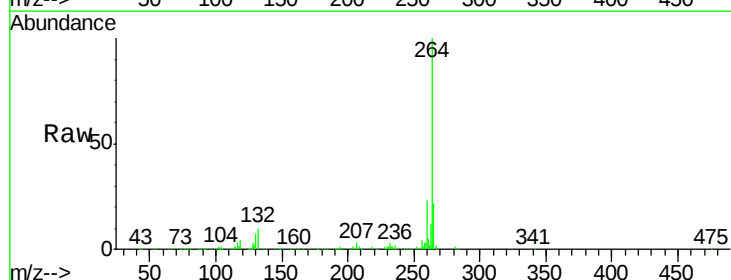

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

