


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA_G\Data\BG010318\
 Data File : BG031900.D
 Acq On : 3 Jan 2018 21:37
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG122117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 29 15:51:46 2017

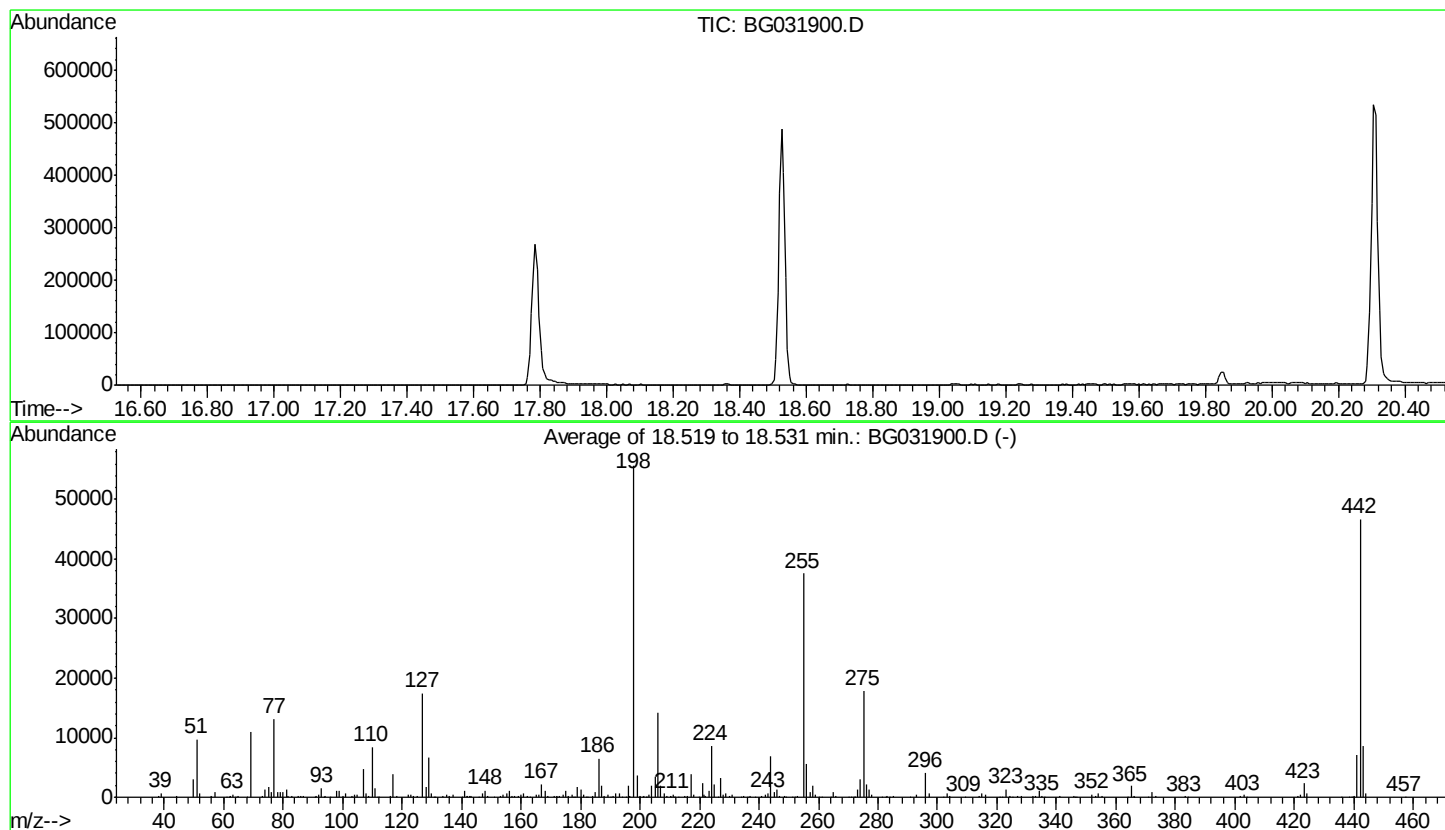

AutoFind: Scans 2592, 2593, 2594; Background Corrected with Scan 2586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	17.4	9718	PASS
68	69	0.00	2	0.7	73	PASS
69	198	0.00	100	19.8	11017	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	31.3	17455	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	55693	PASS
199	198	5	9	6.6	3666	PASS
275	198	10	60	32.1	17901	PASS
365	198	1	100	3.3	1843	PASS
441	442	0.01	24	15.2	7091	PASS
442	198	50	100	83.9	46706	PASS
443	442	15	24	18.6	8709	PASS