

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010319\
 Data File : BG038914.D
 Acq On : 3 Jan 2019 21:59
 Operator : JU/SJ
 Sample : K1016-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Jan 04 04:13:43 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	26976	20.00	ng	-0.02
21) Naphthalene-d8	10.86	136	108158	20.00	ng	-0.02
39) Acenaphthene-d10	14.68	164	78549	20.00	ng	-0.02
64) Phenanthrene-d10	17.43	188	202179	20.00	ng	-0.01
76) Chrysene-d12	21.71	240	204205	20.00	ng	-0.02
87) Perylene-d12	25.01	264	214177	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	170359	112.01	ng	0.00
7) Phenol-d6	7.21	99	199213	95.41	ng	0.00
23) Nitrobenzene-d5	9.22	82	170276	80.43	ng	-0.02
42) 2,4,6-Tribromophenol	16.17	330	146410	135.25	ng	-0.02
45) 2-Fluorobiphenyl	13.30	172	456212	79.68	ng	-0.02
79) Terphenyl-d14	20.03	244	920281	98.08	ng	-0.01
Target Compounds						
19) n-Nitroso-di-n-propylamine	9.22	70	22753	15.516	ng	# 67
51) 2,6-Dinitrotoluene	14.69	165	10479	7.209	ng	# 21
57) 2,4-Dinitrotoluene	14.69	165	10479	5.118	ng	# 23
67) 4-Bromophenyl-phenylether	16.17	248	9349	3.786	ng	# 1
77) Benzidine	20.03	184	15252	2.526	ng	# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG010319\
Data File : BG038914.D
Acq On : 3 Jan 2019 21:59
Operator : JU/SJ
Sample : K1016-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Jan 04 04:13:43 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

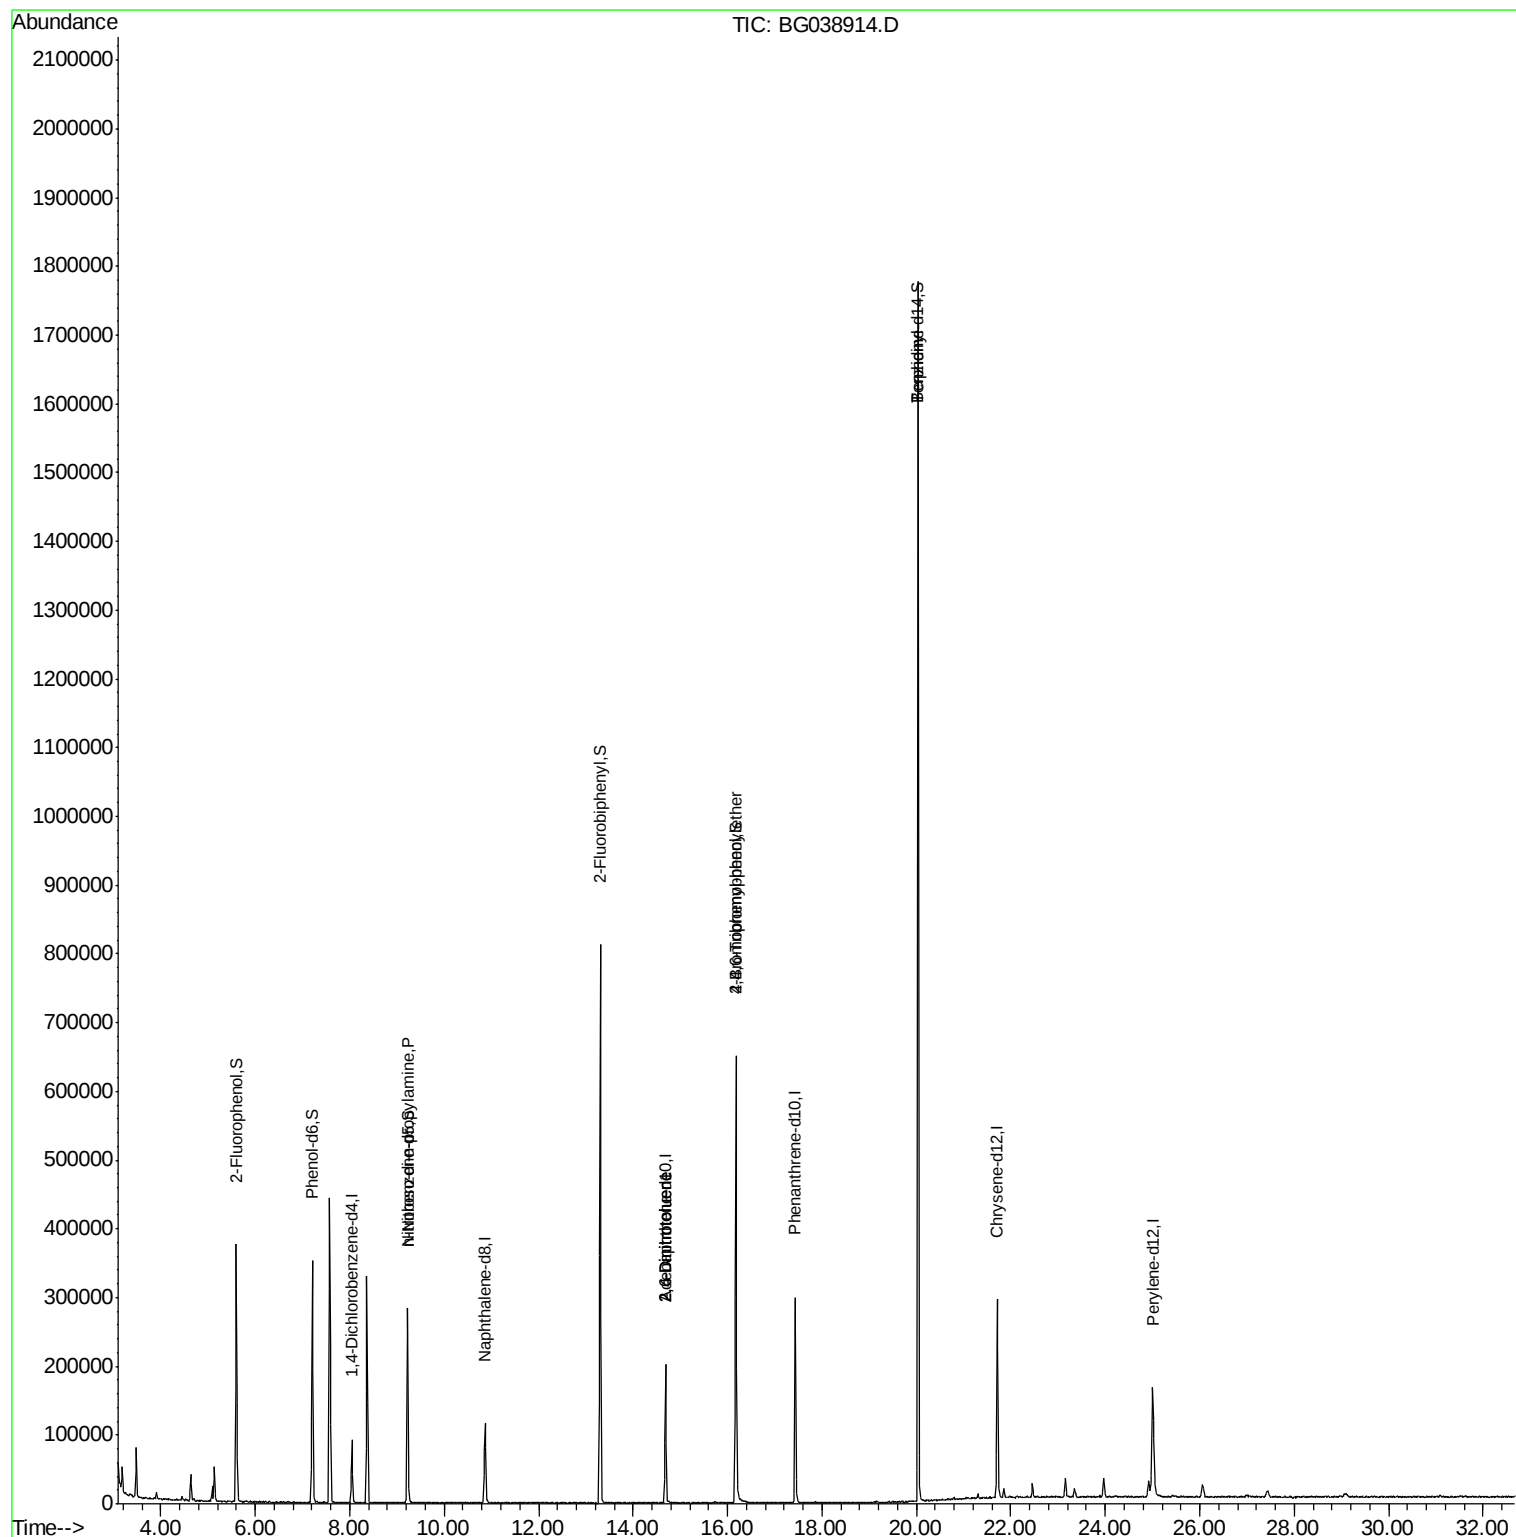




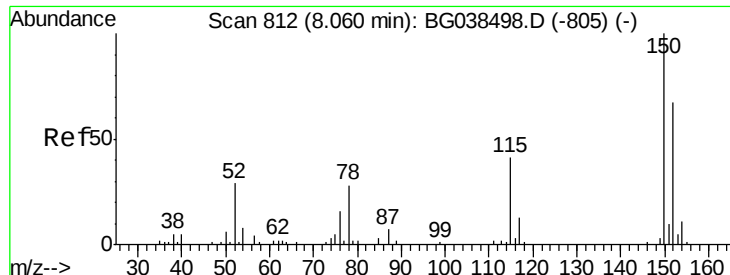


#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.04 min Scan# 843
Delta R.T. -0.02 min
Lab File: BG038914.D
Acq: 3 Jan 2019 21:59

Instrument :
BNA_G
ClientSampleId :




Tot Ion:152 Resp: 26976
Ion Ratio Lower Upper
152 100
150 157.1 119.5 179.3
115 59.5 49.6 74.4

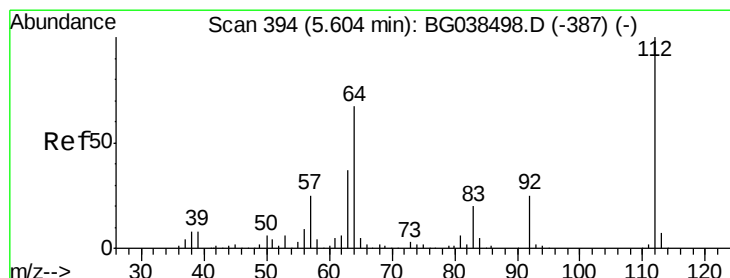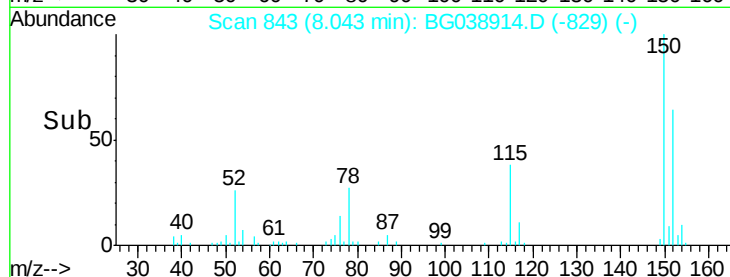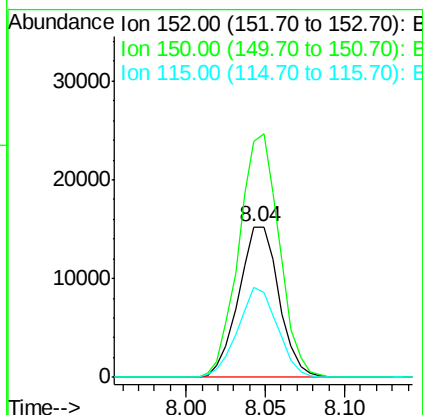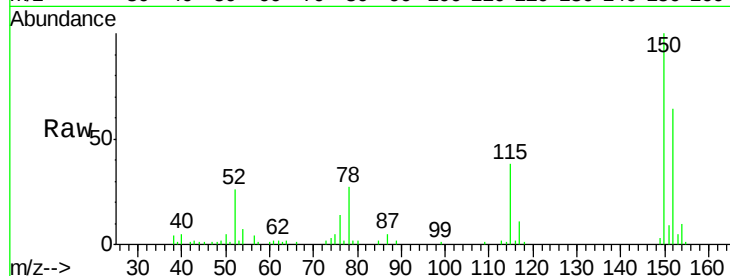


#5

2-Fluorophenol
Concen: 112.010 ng
RT: 5.60 min Scan# 428
Delta R.T. 0.00 min
Lab File: BG038914.D
Acq: 3 Jan 2019 21:59

Tgt Ion:112 Resp: 170359
Ion Ratio Lower Upper
112 100
64 61.1 53.4 80.2
63 34.8 29.3 43.9

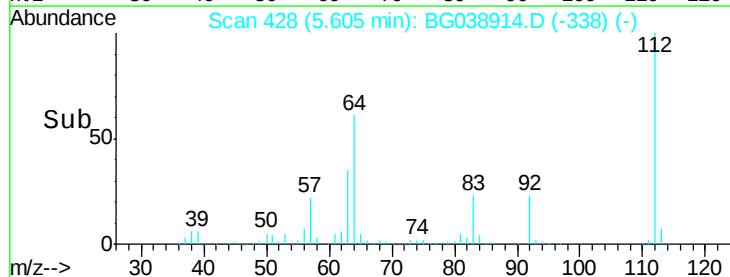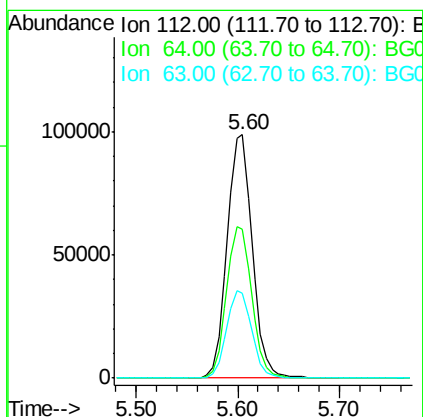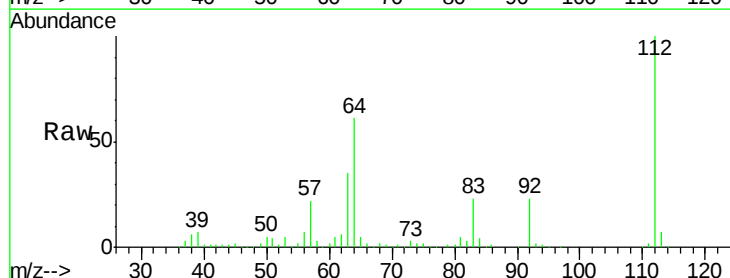

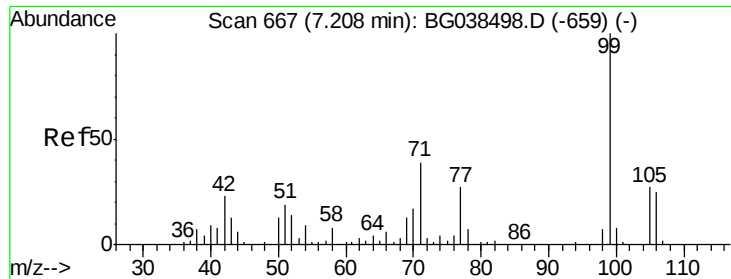

#7

Phenol-d6

Concen: 95.411 ng

RT: 7.21 min Scan# 701

Delta R.T. 0.00 min

Lab File: BG038914.D

Acq: 3 Jan 2019 21:59

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 199213

Ion Ratio Lower Upper




99 100

42 21.6 18.5 27.7

71 37.2 31.1 46.7

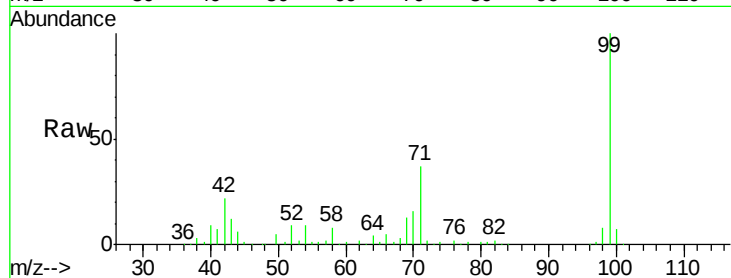

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

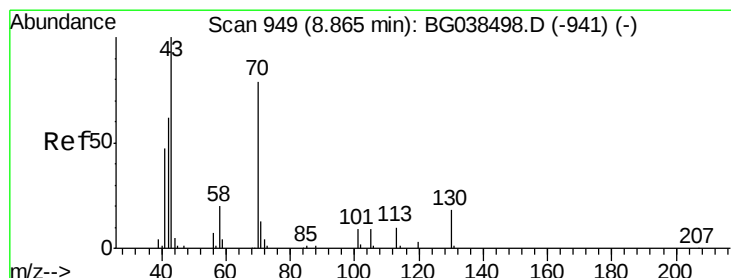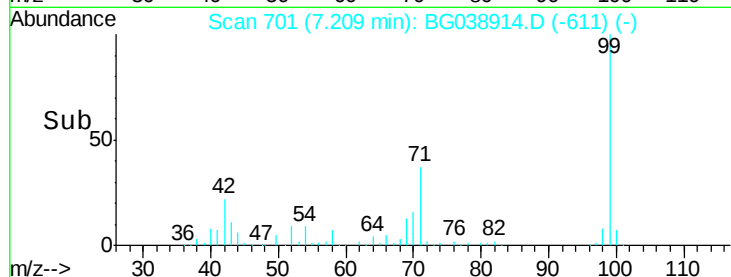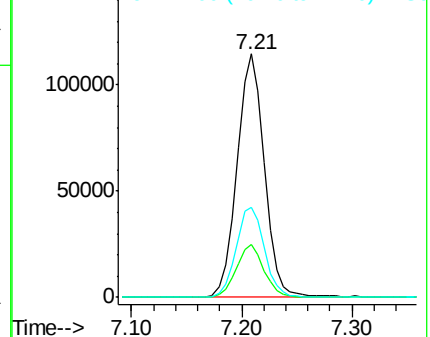

#19

n-Nitroso-di-n-propylamine

Concen: 15.516 ng

RT: 9.22 min Scan# 1044

Delta R.T. 0.36 min

Lab File: BG038914.D

Acq: 3 Jan 2019 21:59

Tgt Ion: 70 Resp: 22753


Ion Ratio Lower Upper

70 100



42 52.6 63.6 95.4#


101 0.0 9.2 13.8#

130 2.0 18.5 27.7#

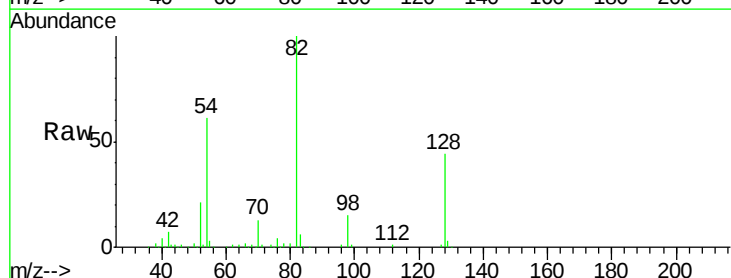

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

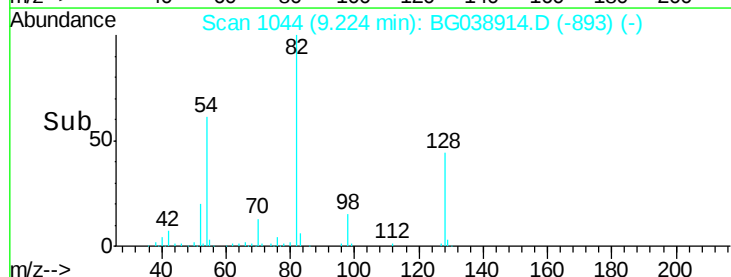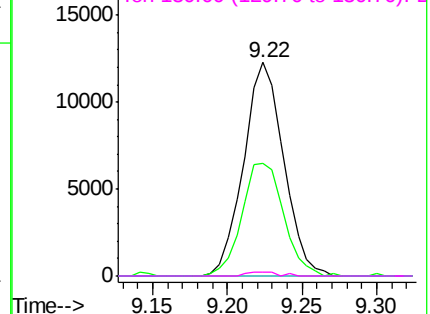


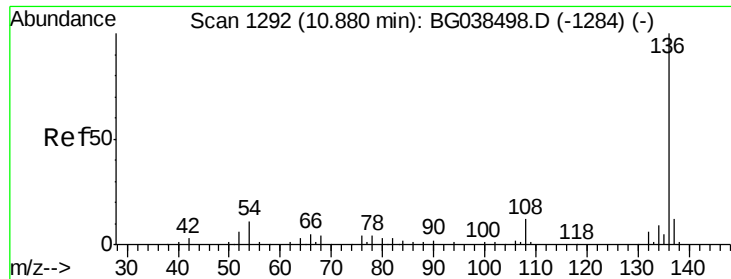




#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.86 min Scan# 1323
Delta R.T. -0.02 min
Lab File: BG038914.D
Acq: 3 Jan 2019 21:59

Instrument :
BNA_G
ClientSampleId :

Tot Ion:	136	Resp:	108158
Ion	Ratio	Lower	Upper
136	100		
137	11.5	9.3	13.9
54	10.1	8.5	12.7
68	4.2	3.5	5.3

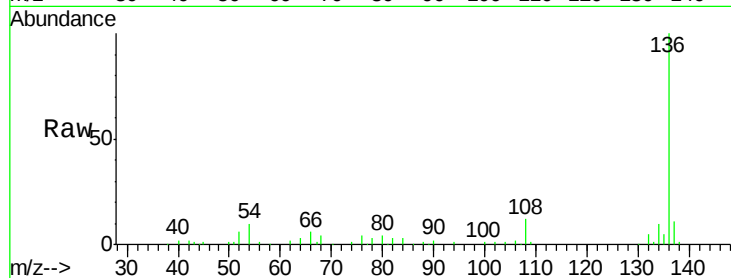


Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

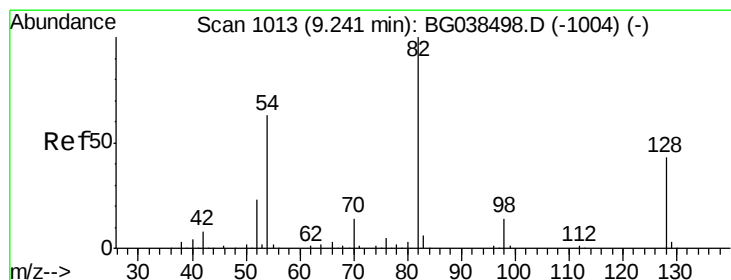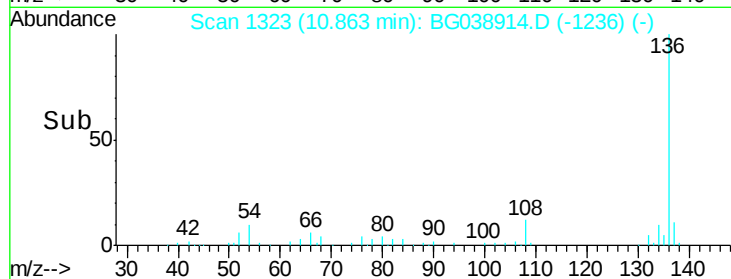
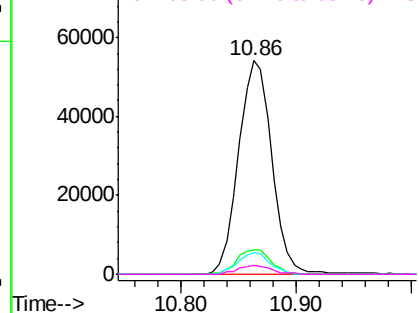



#23
Nitrobenzene-d5
Concen: 80.428 ng
RT: 9.22 min Scan# 1044
Delta R.T. -0.02 min
Lab File: BG038914.D
Acq: 3 Jan 2019 21:59

Tgt Ion:	82	Resp:	170276
Ion	Ratio	Lower	Upper
82	100		
128	44.5	34.6	52.0
54	61.4	50.6	76.0

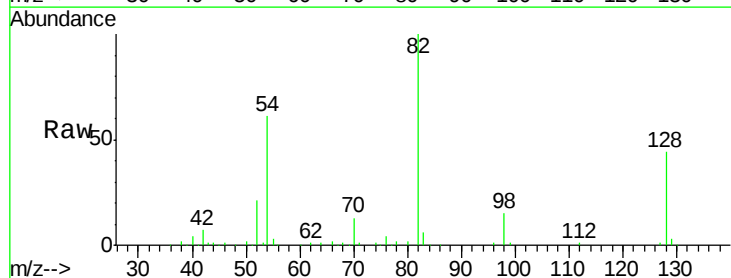

Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): BGC
Ion 54.00 (53.70 to 54.70): BGC

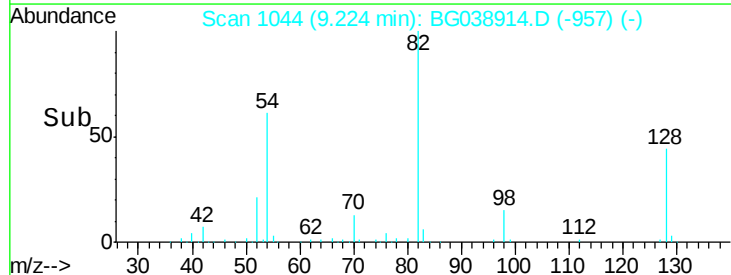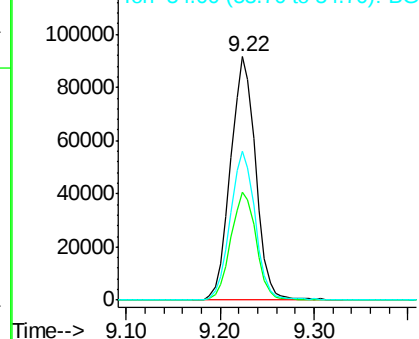

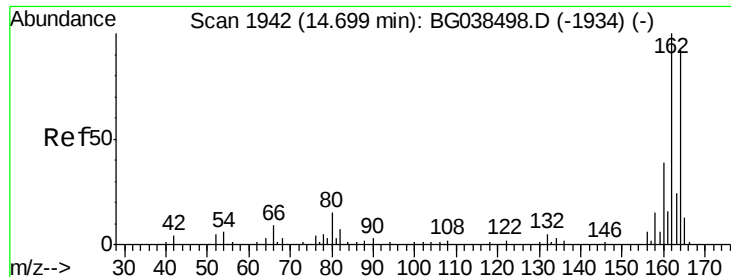

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 14.68 min Scan# 1973

Delta R.T. -0.02 min

Lab File: BG038914.D

Acq: 3 Jan 2019 21:59

Instrument :

BNA_G

ClientSampleId :


Tot Ion:164 Resp: 78549

Ion Ratio Lower Upper

164 100

162 102.1 86.6 130.0




160 43.2 34.2 51.2

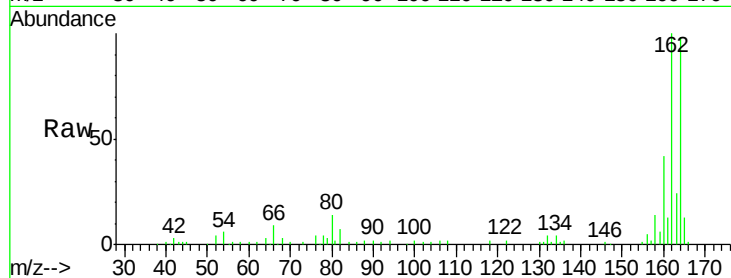

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

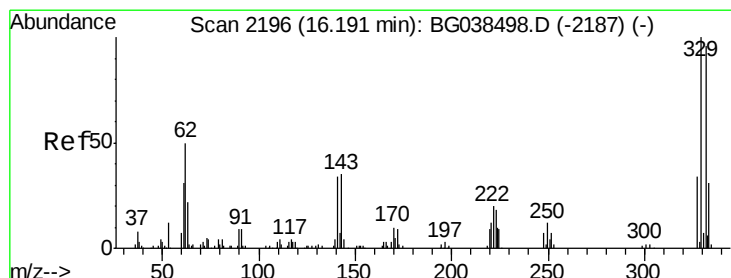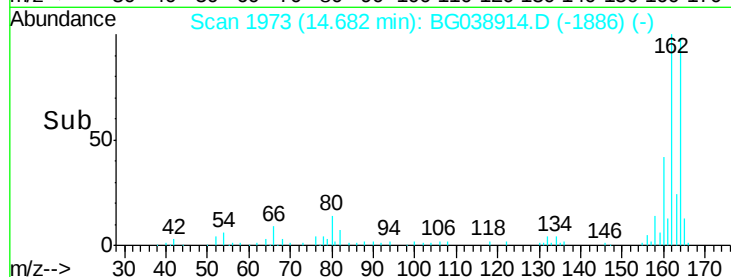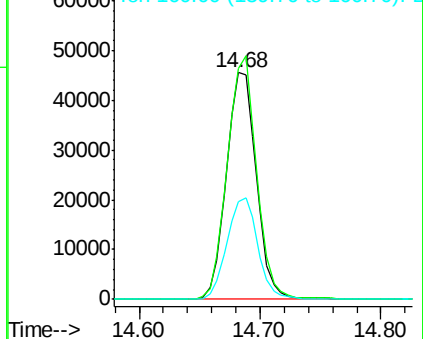

#42

2,4,6-Tribromophenol

Concen: 135.246 ng

RT: 16.17 min Scan# 2227

Delta R.T. -0.02 min

Lab File: BG038914.D

Acq: 3 Jan 2019 21:59


Tgt Ion:330 Resp: 146410

Ion Ratio Lower Upper

330 100

332 97.9 76.9 115.3



141 32.3 28.8 43.2

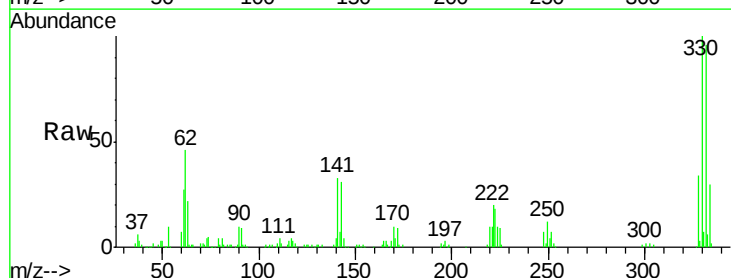


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

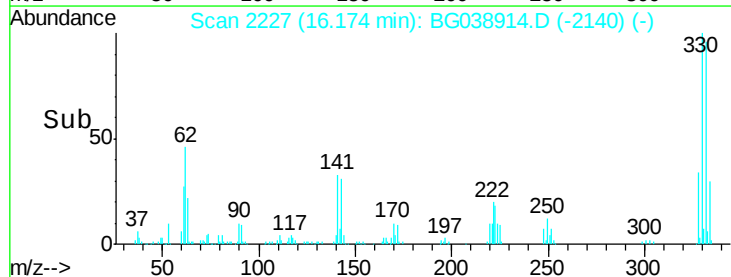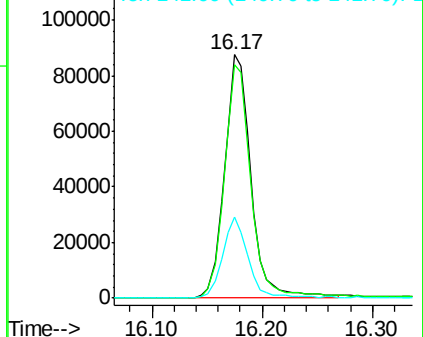


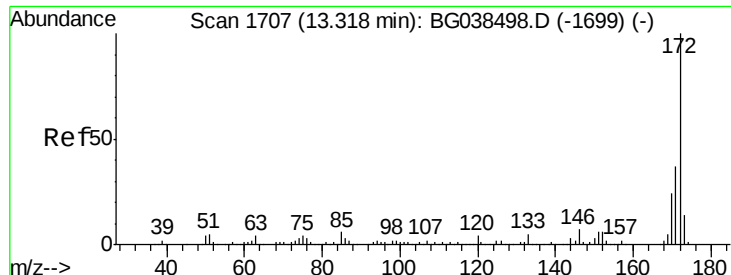




#45
 2-Fluorobiphenyl
 Concen: 79.677 ng
 RT: 13.30 min Scan# 1738
 Delta R.T. -0.02 min
 Lab File: BG038914.D
 Acq: 3 Jan 2019 21:59

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:172 Resp: 456212
 Ion Ratio Lower Upper
 172 100
 171 36.7 29.8 44.6
 170 23.6 19.5 29.3

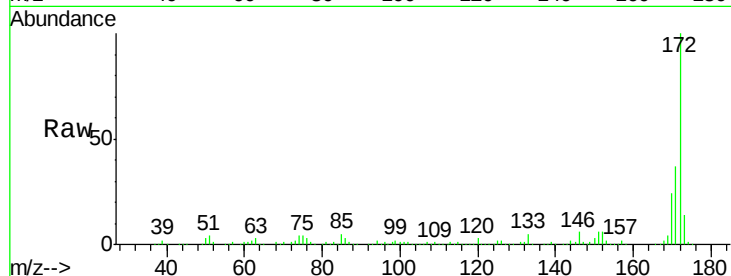


Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

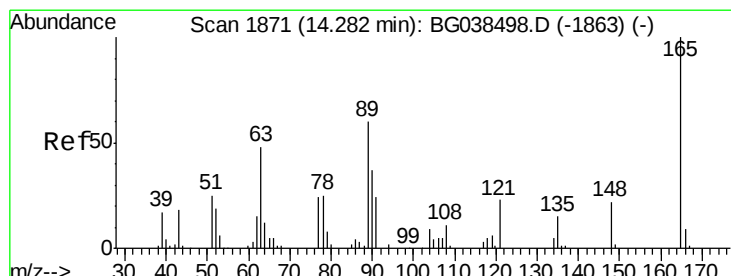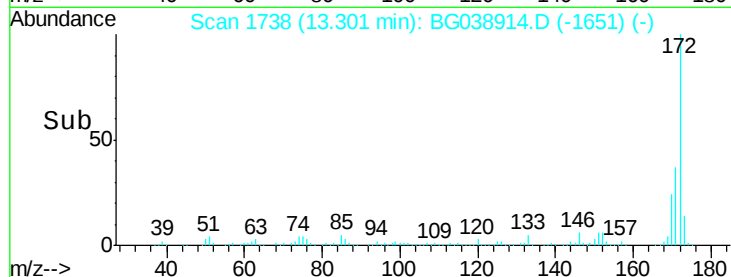
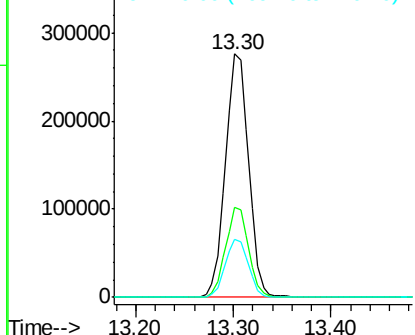



#51
 2,6-Dinitrotoluene
 Concen: 7.209 ng
 RT: 14.69 min Scan# 1974
 Delta R.T. 0.41 min
 Lab File: BG038914.D
 Acq: 3 Jan 2019 21:59

Tgt Ion:165 Resp: 10479
 Ion Ratio Lower Upper
 165 100
 63 0.0 51.8 77.6#
 89 3.1 47.9 71.9#

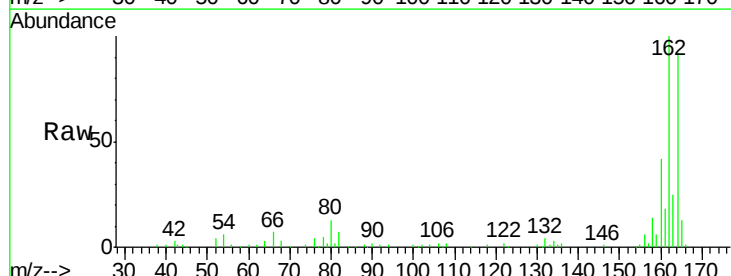

Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC

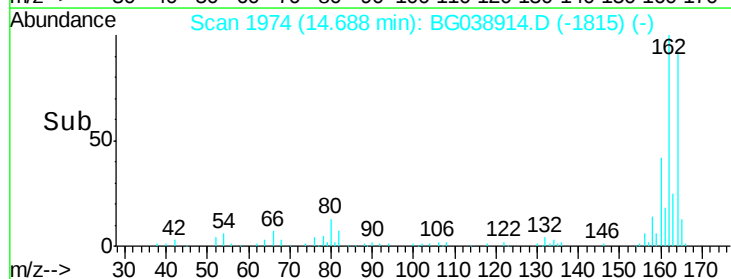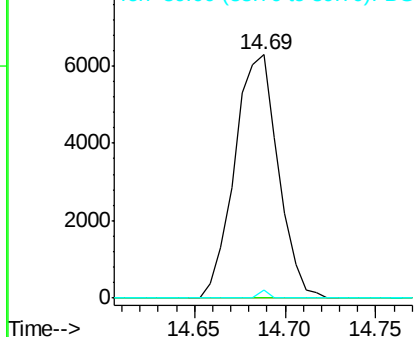


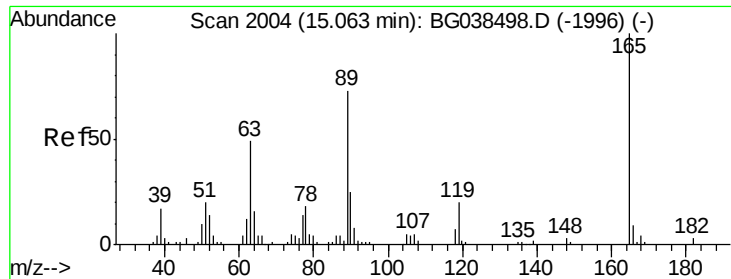




#57
 2,4-Dinitrotoluene
 Concen: 5.118 ng
 RT: 14.69 min Scan# 1974
 Delta R.T. -0.38 min
 Lab File: BG038914.D
 Acq: 3 Jan 2019 21:59

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:165 Resp: 10479
 Ion Ratio Lower Upper
 165 100
 63 0.0 39.0 58.4#
 89 3.1 58.0 87.0#
 182 0.0 2.3 3.5#

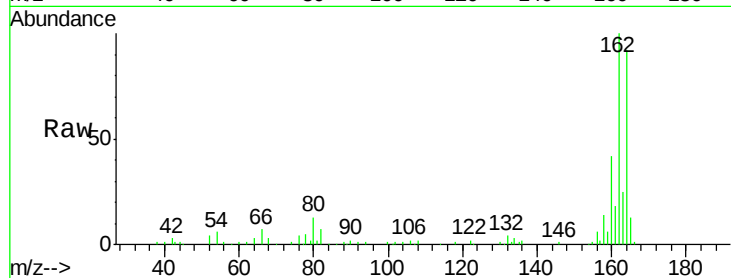


Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BGC
 Ion 89.00 (88.70 to 89.70): BGC
 Ion 182.00 (181.70 to 182.70): E

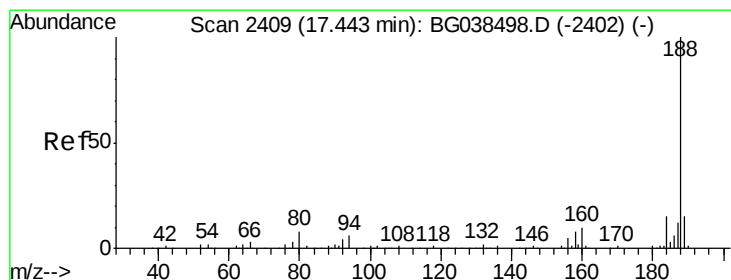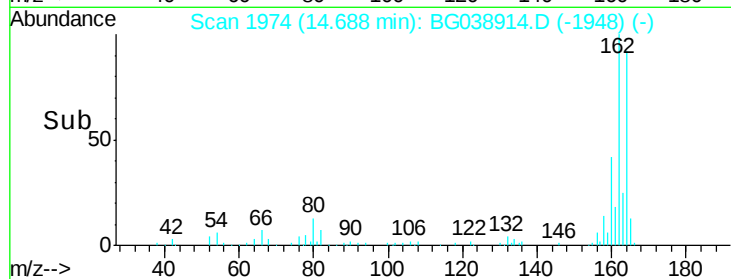
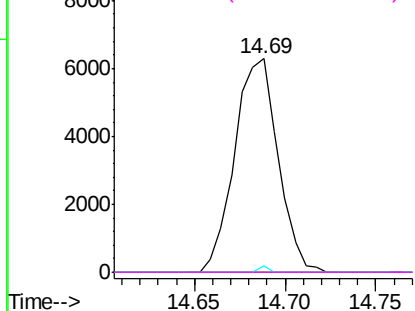



#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 17.43 min Scan# 2441
 Delta R.T. -0.01 min
 Lab File: BG038914.D
 Acq: 3 Jan 2019 21:59

Tgt Ion:188 Resp: 202179
 Ion Ratio Lower Upper
 188 100
 94 5.8 5.1 7.7
 80 7.1 6.1 9.1

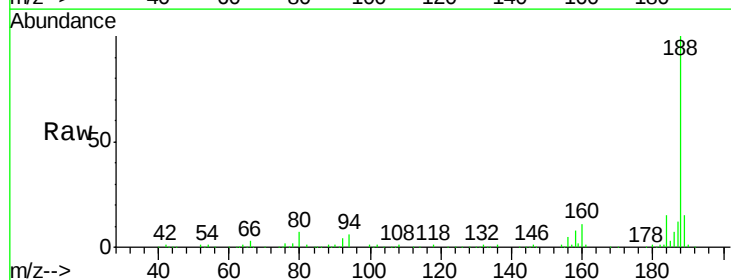

Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BGC
 Ion 80.00 (79.70 to 80.70): BGC

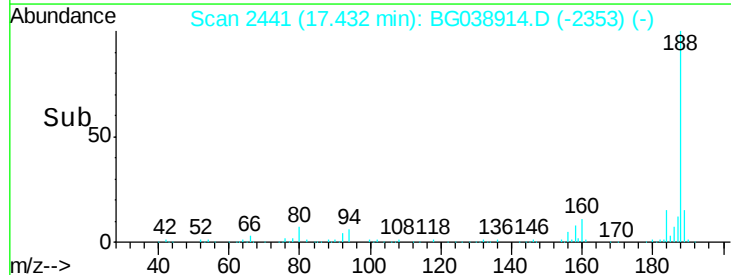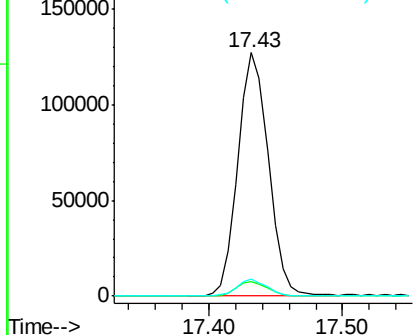


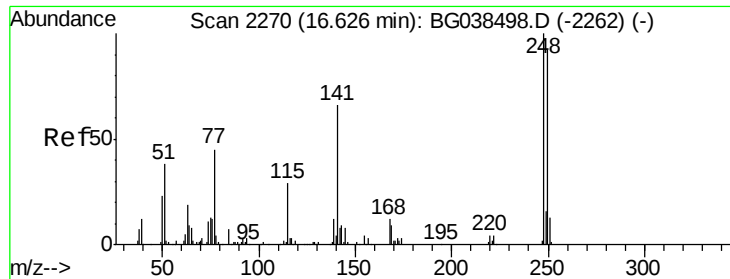




#67
4-Bromophenyl-phenylether
Concen: 3.786 ng
RT: 16.17 min Scan# 2227
Delta R.T. -0.45 min
Lab File: BG038914.D
Acq: 3 Jan 2019 21:59

Instrument :
BNA_G
ClientSampleId :

Tot Ion:248 Resp: 9349
Ion Ratio Lower Upper
248 100
250 253.2 73.4 110.2#
141 511.2 52.9 79.3#

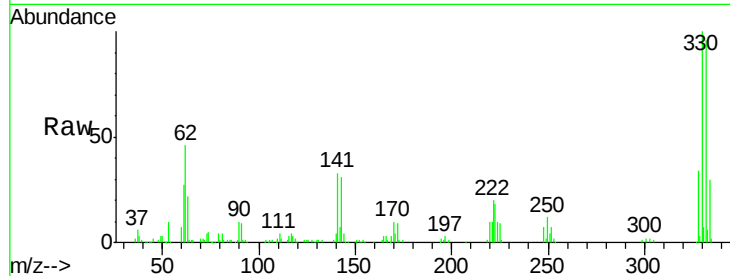


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

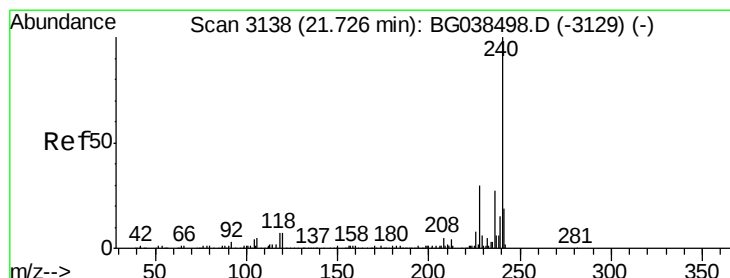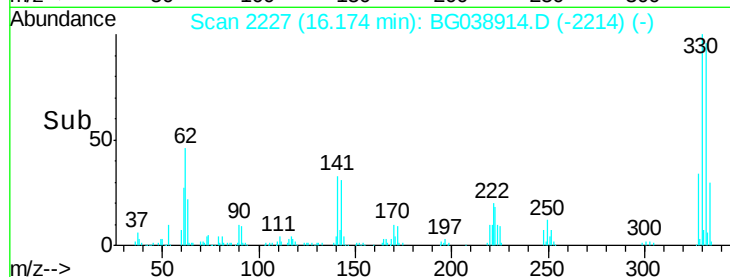
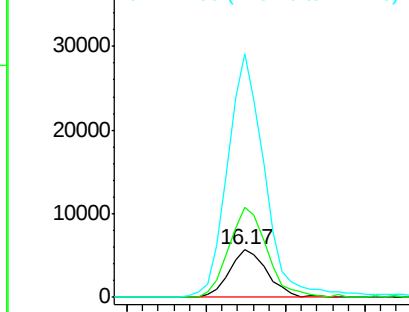



#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.71 min Scan# 3169
Delta R.T. -0.02 min
Lab File: BG038914.D
Acq: 3 Jan 2019 21:59

Tgt Ion:240 Resp: 204205
Ion Ratio Lower Upper
240 100
120 7.0 5.3 7.9
236 26.2 21.4 32.2

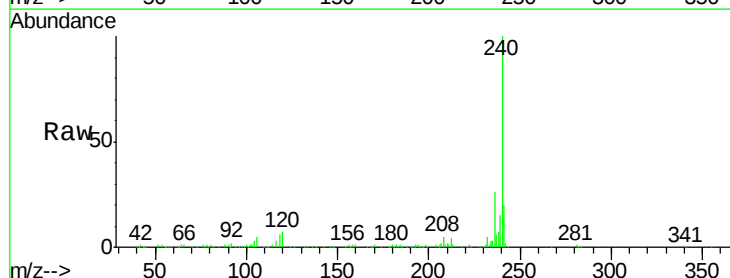

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

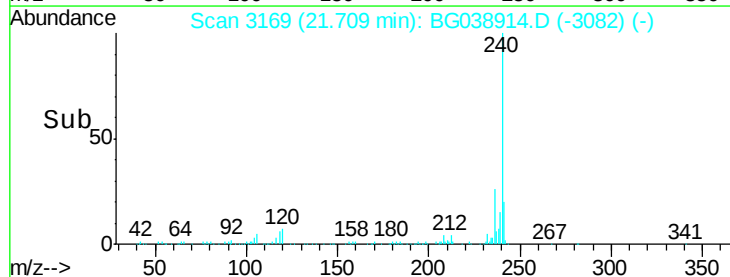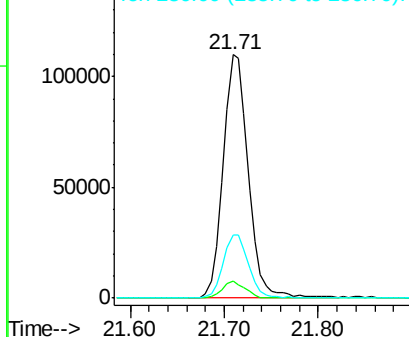

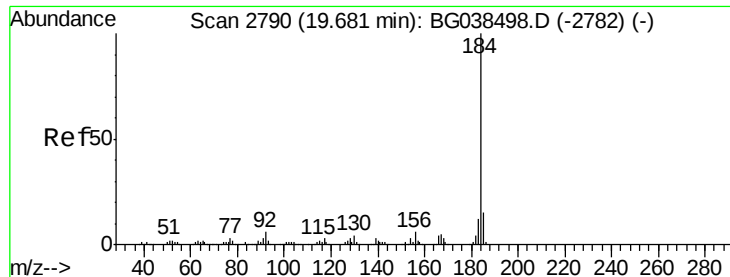

#77

Benzidine

Concen: 2.526 ng

RT: 20.03 min Scan# 2884

Delta R.T. 0.35 min

Lab File: BG038914.D

Acq: 3 Jan 2019 21:59

Instrument :

BNA_G

ClientSampleId :


Tot Ion:184 Resp: 15252

Ion Ratio Lower Upper

184 100

185 15.7 12.2 18.2




183 8.2 9.6 14.4#

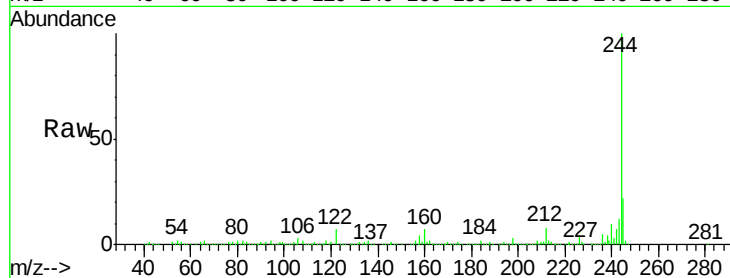

Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

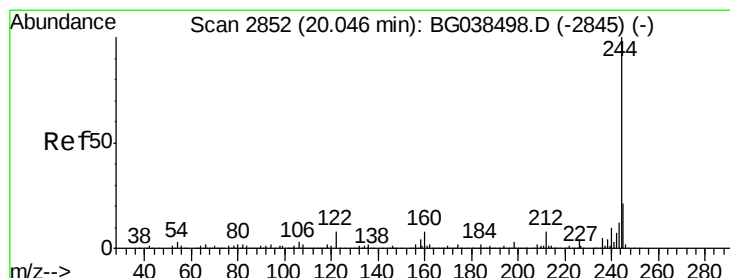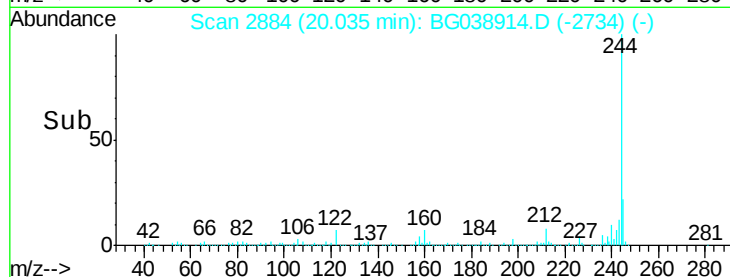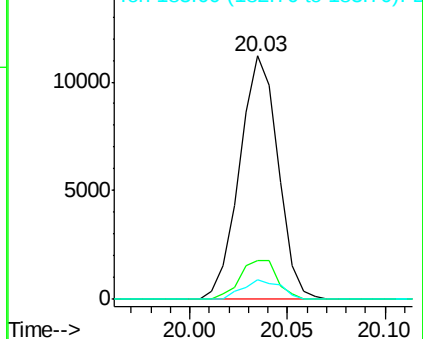

#79

Terphenyl-d14

Concen: 98.080 ng

RT: 20.03 min Scan# 2884

Delta R.T. -0.01 min

Lab File: BG038914.D

Acq: 3 Jan 2019 21:59


Tgt Ion:244 Resp: 920281

Ion Ratio Lower Upper

244 100

212 7.7 6.2 9.2



122 7.1 6.3 9.5

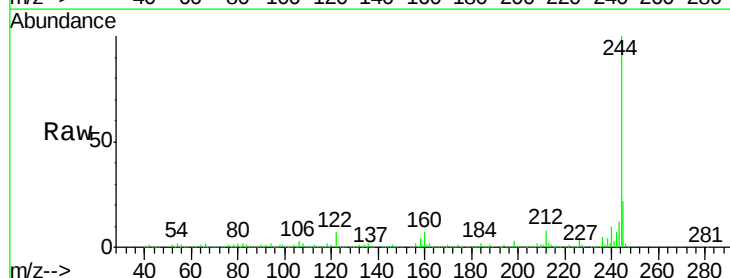


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

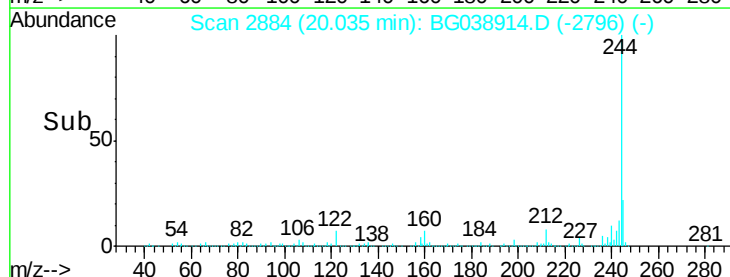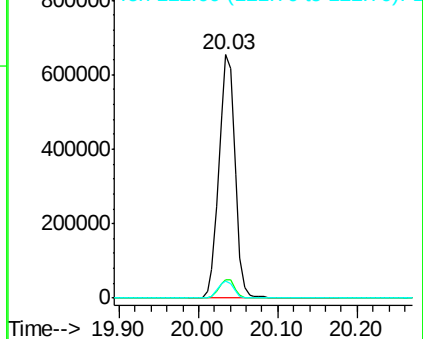

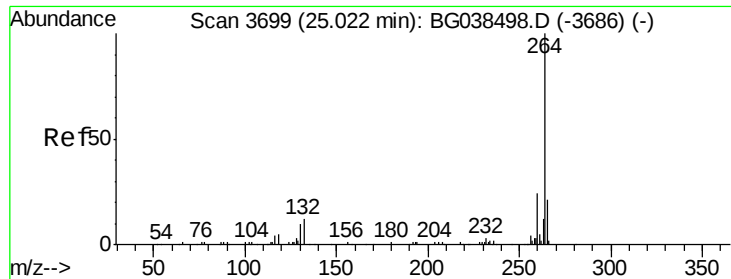

#87
Pervlene-d12
Concen: 20.000 ng
RT: 25.01 min Scan# 3730
Delta R.T. -0.02 min
Lab File: BG038914.D
Acq: 3 Jan 2019 21:59

Instrument :
BNA_G
ClientSampleId :

Tot Ion	Ratio	Lower	Upper
264	100		
260	21.3	18.9	28.3
265	21.0	17.0	25.4

