
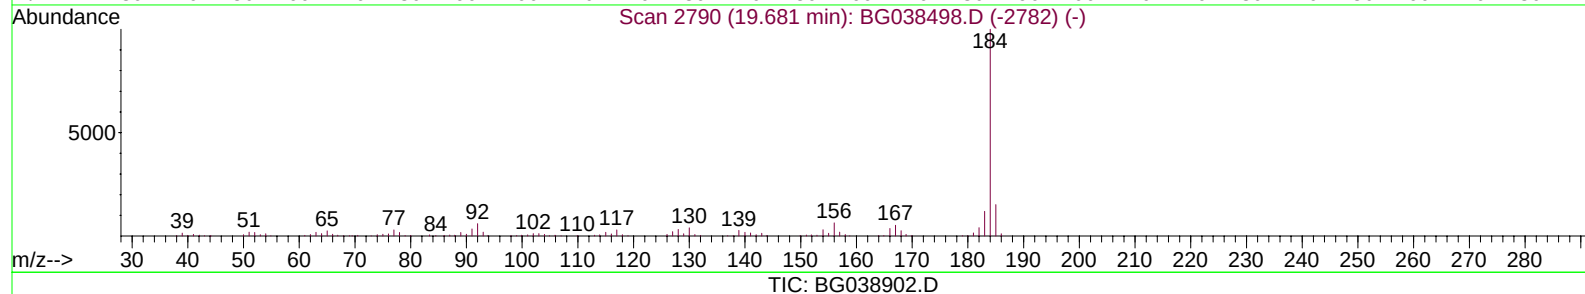
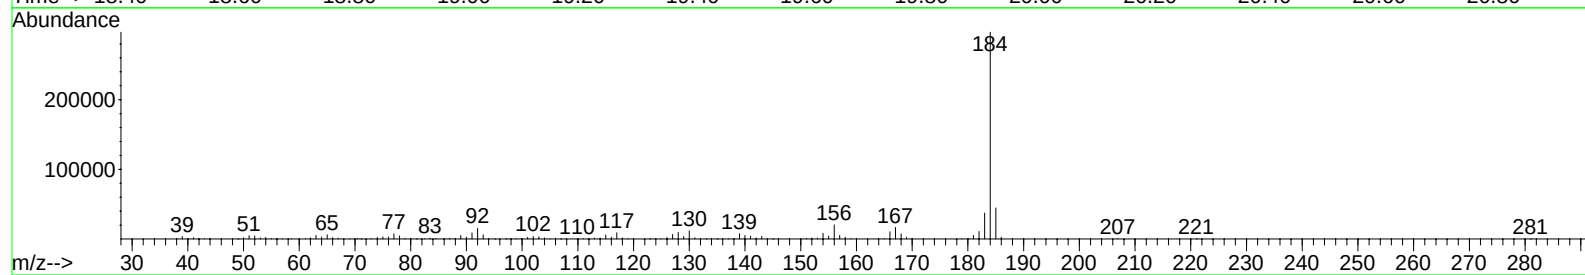


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010319\
 Data File : BG038902.D
 Acq On : 3 Jan 2019 9:50
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 11:02:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Dec 12 15:26:27 2018
 Response via : Initial Calibration

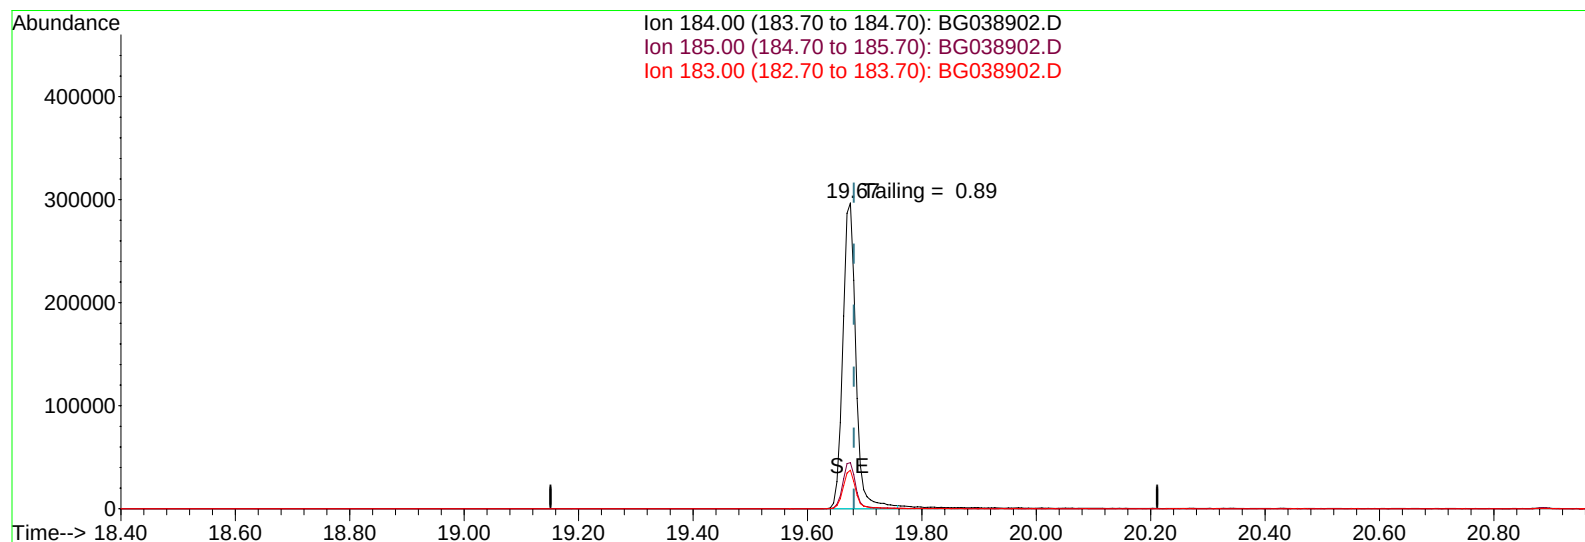

(77) Benzidine




19.675min (-0.006) 0.00ng

response 475881

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.06
183.00	12.00	12.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010319\
Data File : BG038902.D
Acq On : 3 Jan 2019 9:50
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 11:02:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG121218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 12 15:26:27 2018
Response via : Initial Calibration

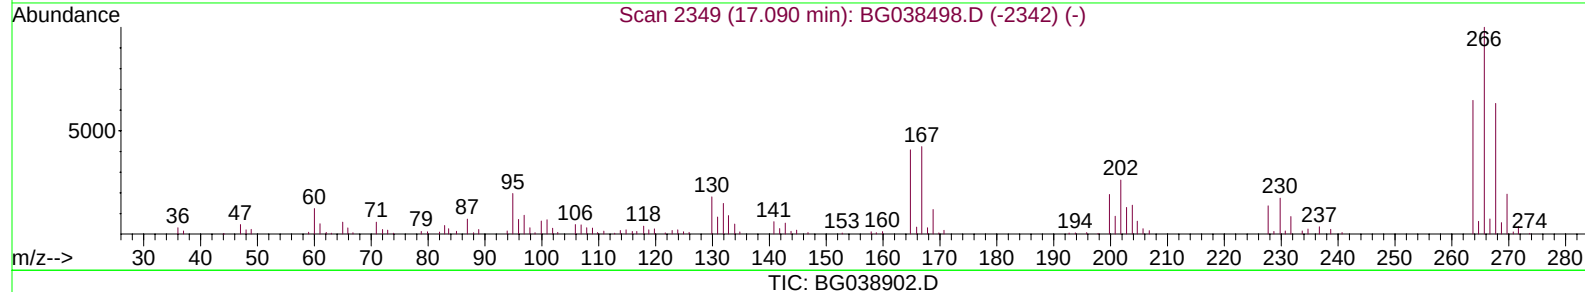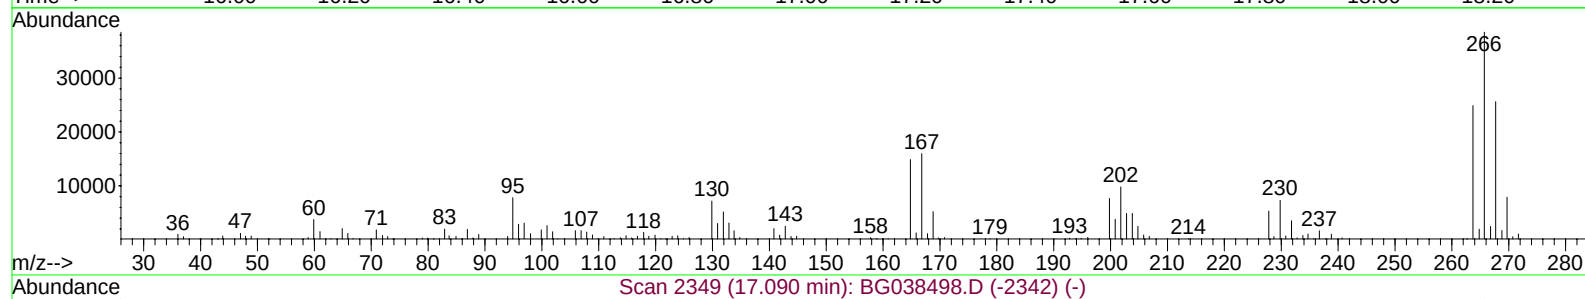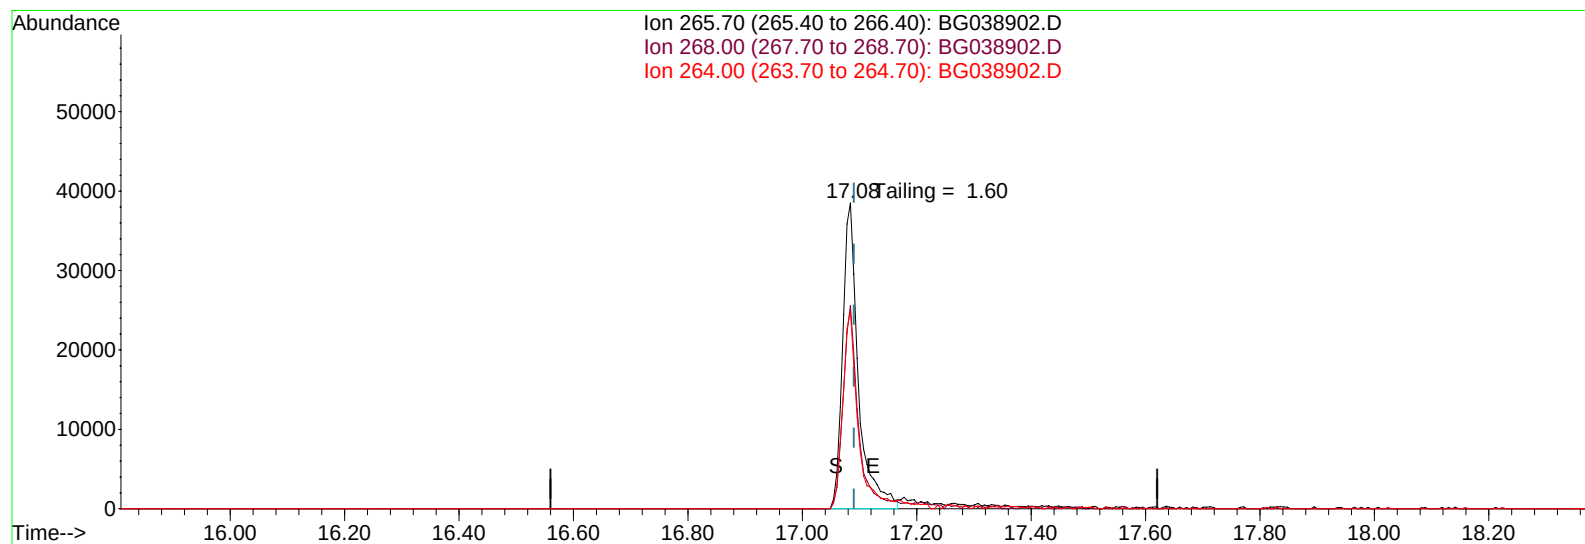

(70) Pentachlorophenol (C)

17.084min (-0.006) 19922.02ng

response 74292

Ion	Exp%	Act%
265.70	100	100
268.00	68.80	66.53
264.00	70.90	64.62
0.00	0.00	0.00