
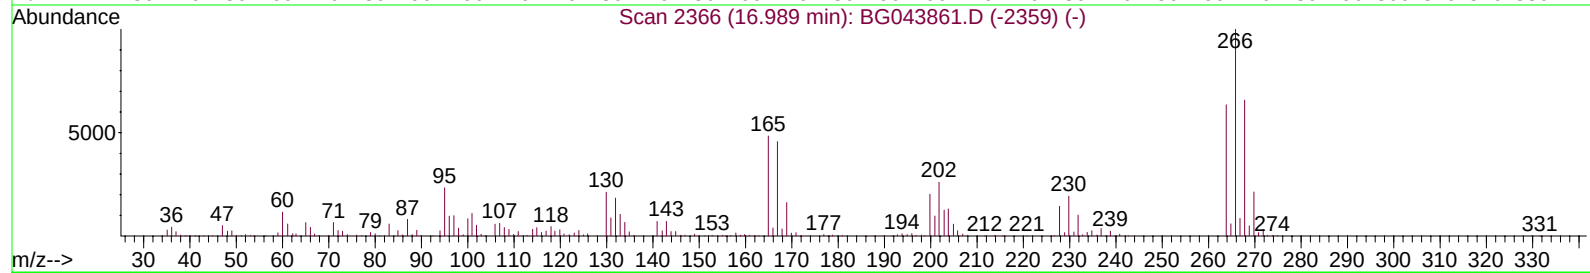
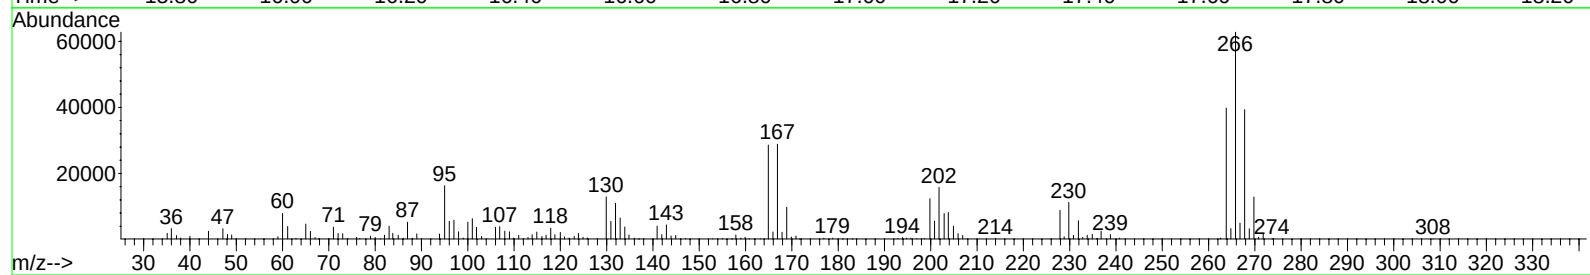


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010320\
Data File : BG043880.D
Acq On : 3 Jan 2020 9:36
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 17:17:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 31 13:32:23 2019
Response via : Initial Calibration

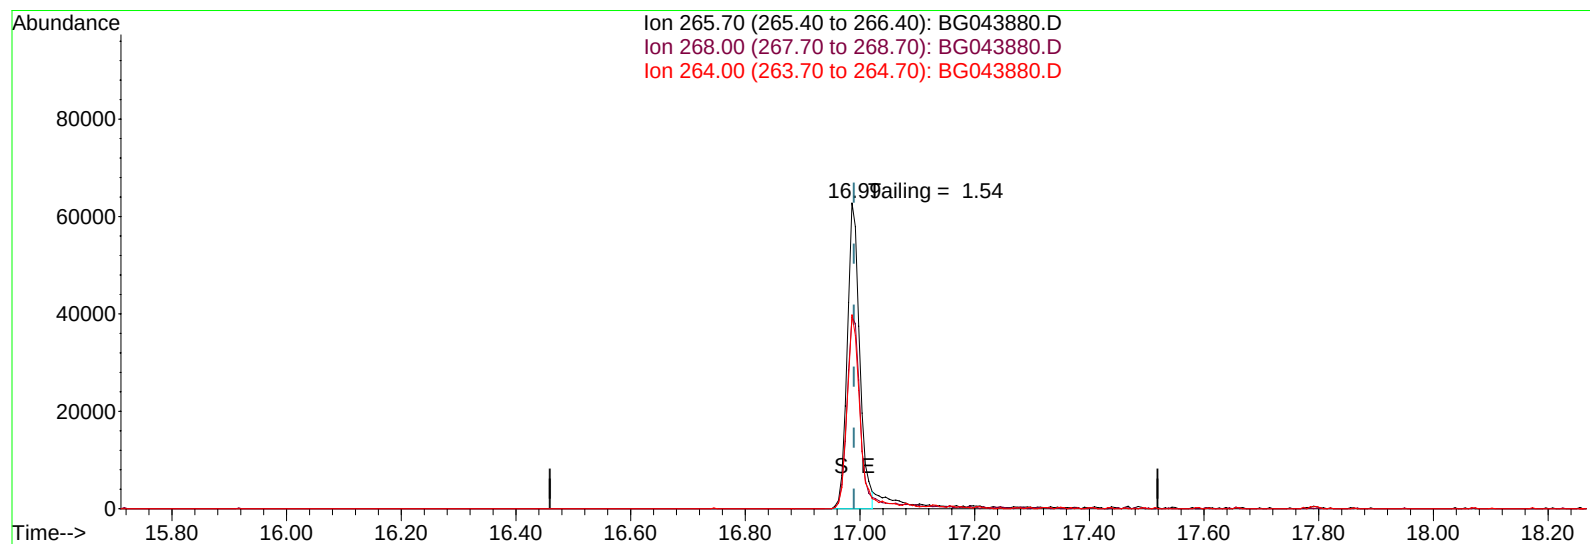

TIC: BG043880.D

(70) Pentachlorophenol (C)




16.986min (-0.003) 17535.55ng

response 102504

Ion	Exp%	Act%
265.70	100	100
268.00	65.80	62.66
264.00	63.50	63.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG010320\
 Data File : BG043880.D
 Acq On : 3 Jan 2020 9:36
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 17:17:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG123019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 31 13:32:23 2019
 Response via : Initial Calibration

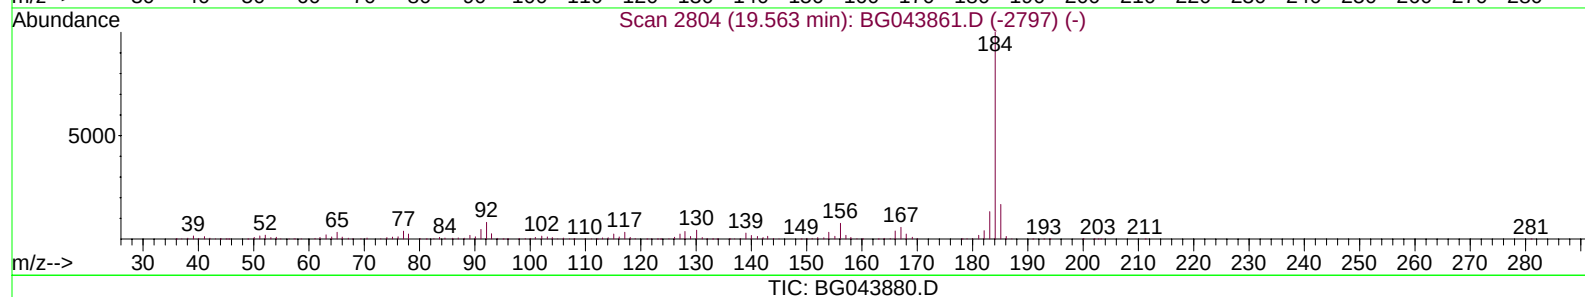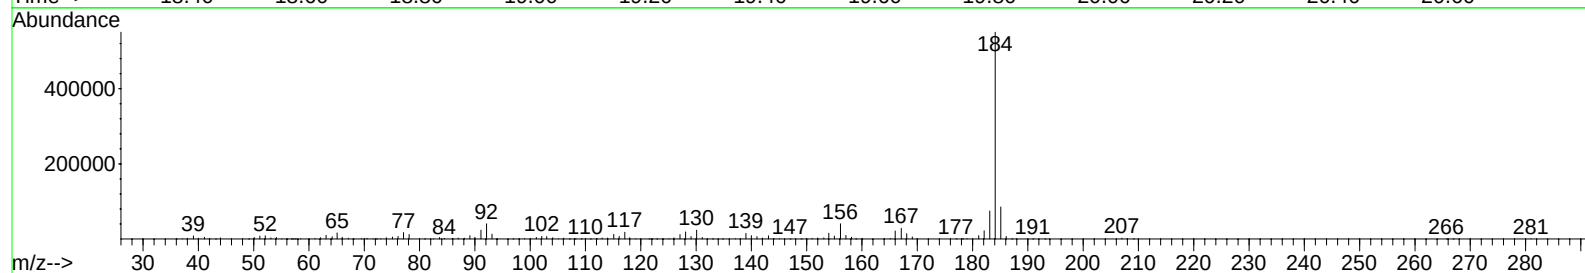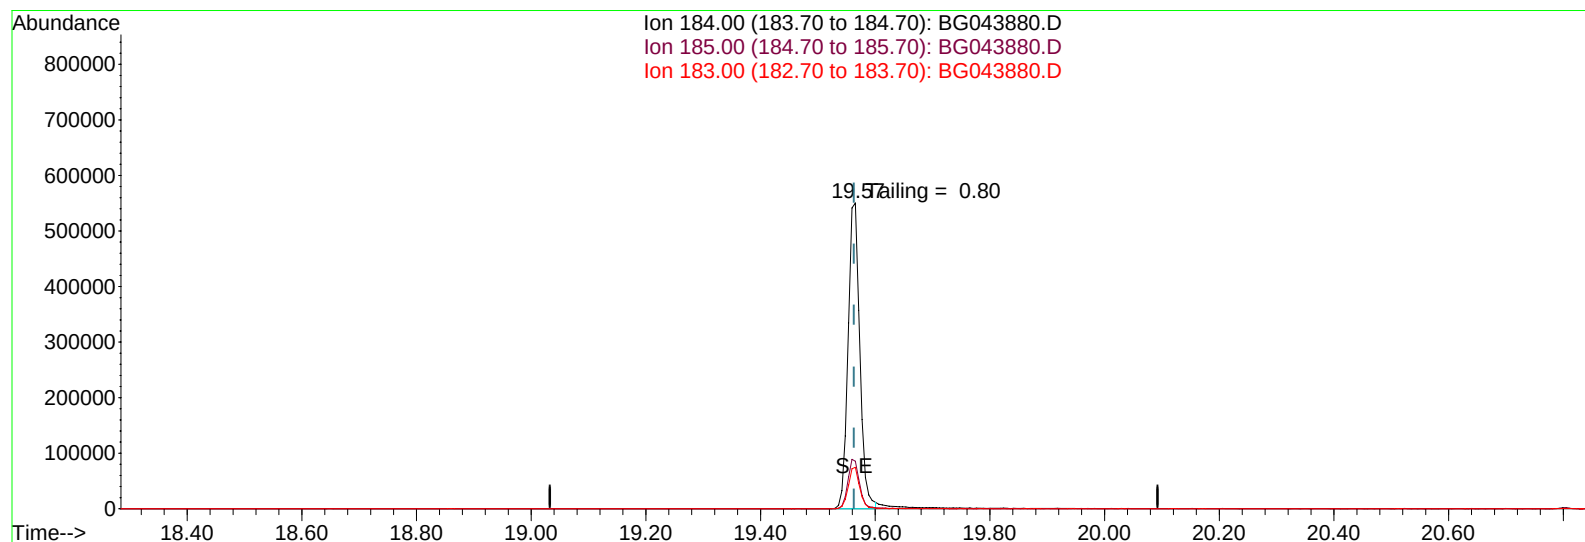

(77) Benzidine

19.565min (+0.003) 0.00ng

response 803551

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.53
183.00	13.20	13.57
0.00	0.00	0.00