


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG010320\
 Data File : BG043880.D
 Acq On : 3 Jan 2020 9:36
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

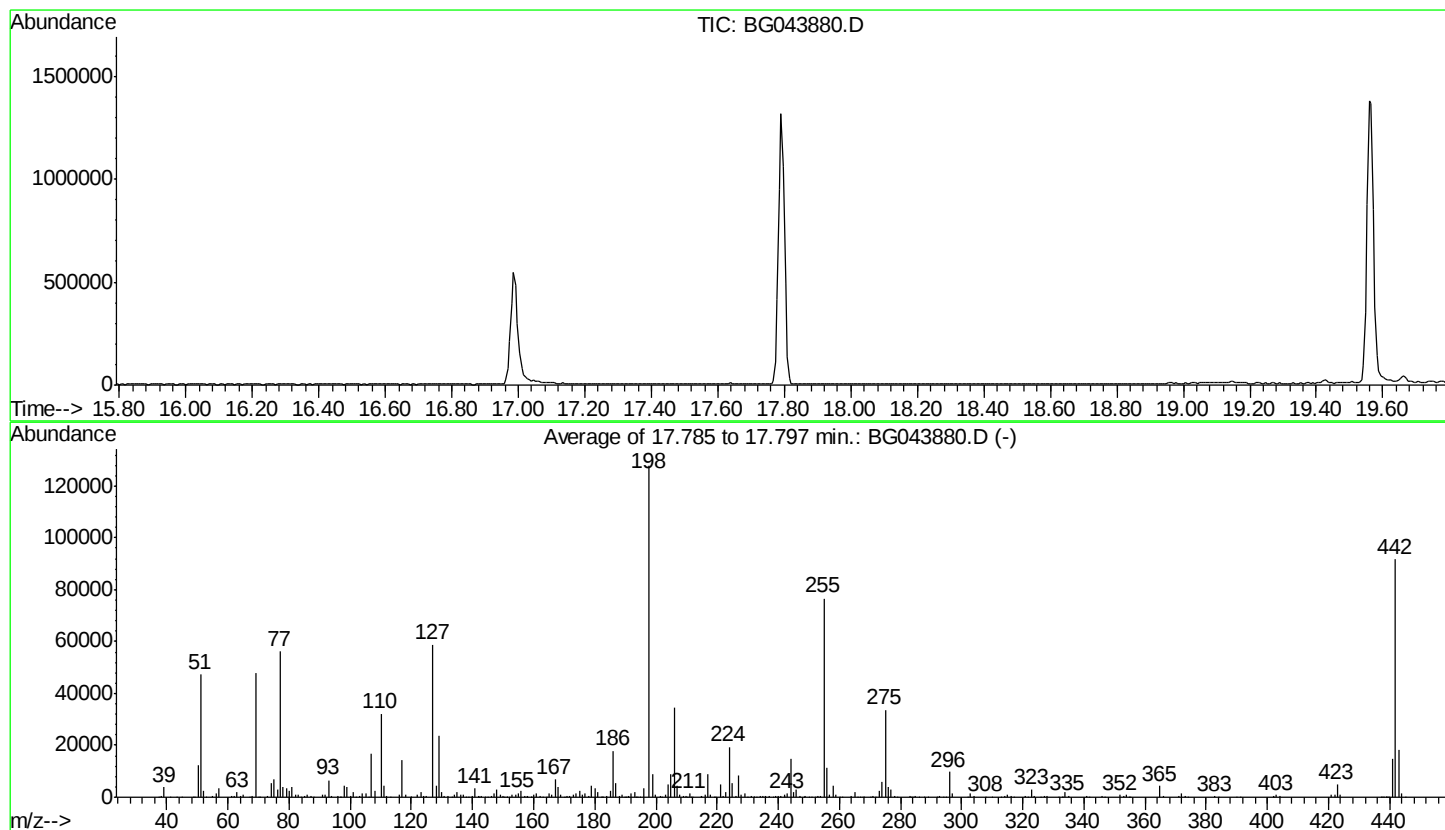

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.1	47362	PASS
68	69	0.00	2	1.5	718	PASS
69	198	0.00	100	37.4	47858	PASS
70	69	0.00	2	0.3	127	PASS
127	198	10	80	46.0	58848	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	127821	PASS
199	198	5	9	6.9	8876	PASS
275	198	10	60	26.3	33661	PASS
365	198	1	100	3.4	4304	PASS
441	198	0.01	100	11.5	14715	PASS
442	198	50	100	71.7	91698	PASS
443	442	15	24	20.0	18379	PASS