


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG010320\
 Data File : BG043887.D
 Acq On : 3 Jan 2020 14:40
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG123019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 31 13:32:23 2019

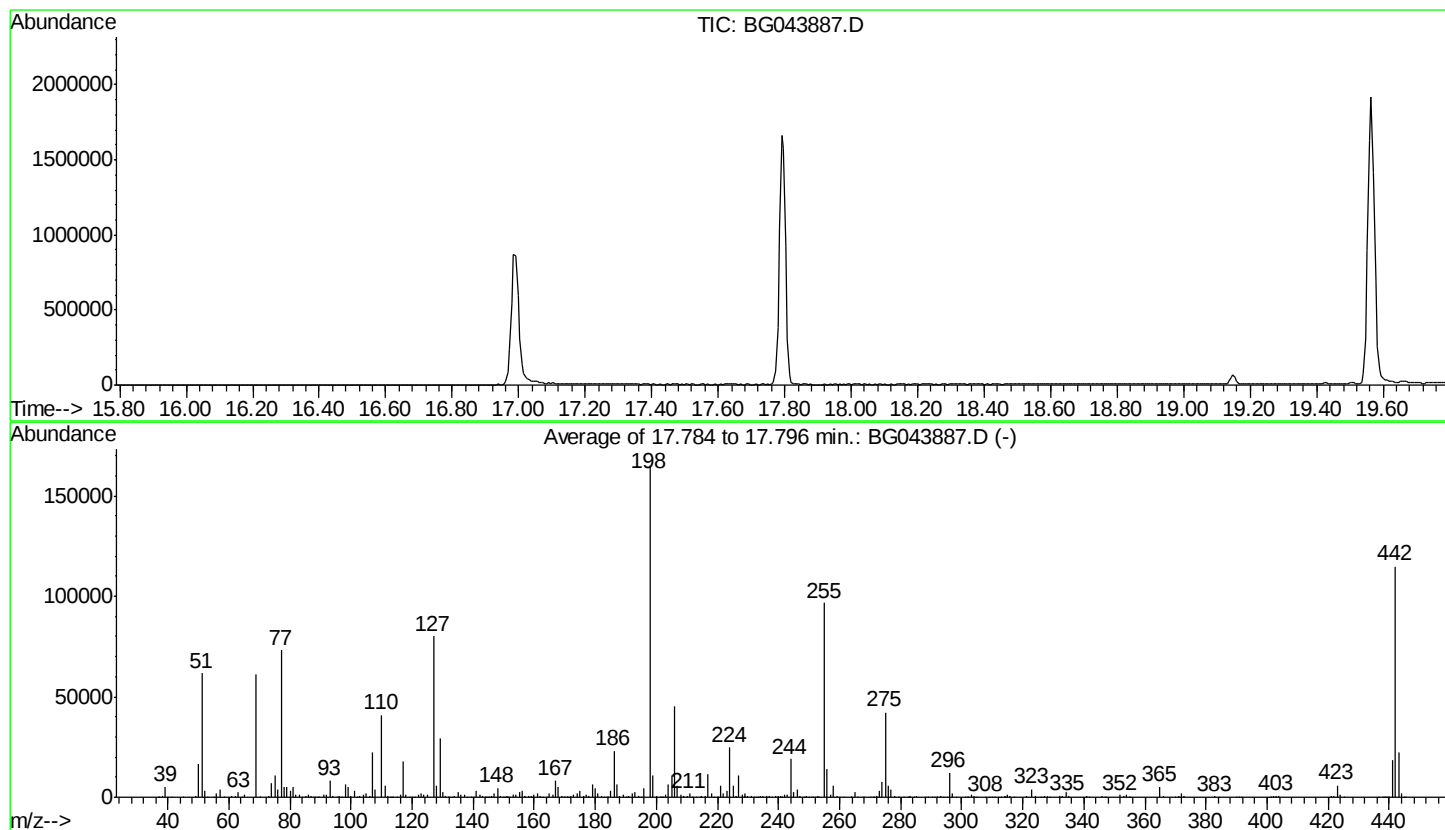

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	61608	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.2	61360	PASS
70	69	0.00	2	0.4	269	PASS
127	198	10	80	48.5	80098	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	165016	PASS
199	198	5	9	6.7	11072	PASS
275	198	10	60	25.6	42205	PASS
365	198	1	100	3.2	5285	PASS
441	198	0.01	100	11.3	18573	PASS
442	198	50	100	69.5	114749	PASS
443	442	15	24	19.2	22035	PASS