
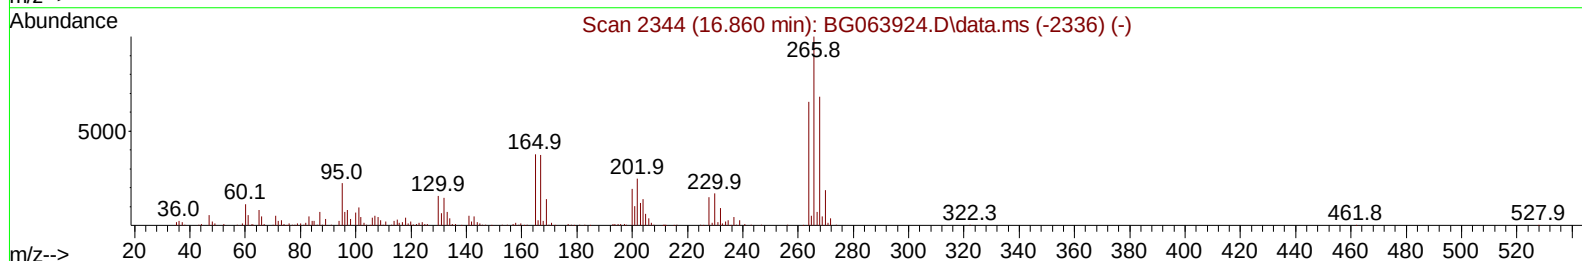
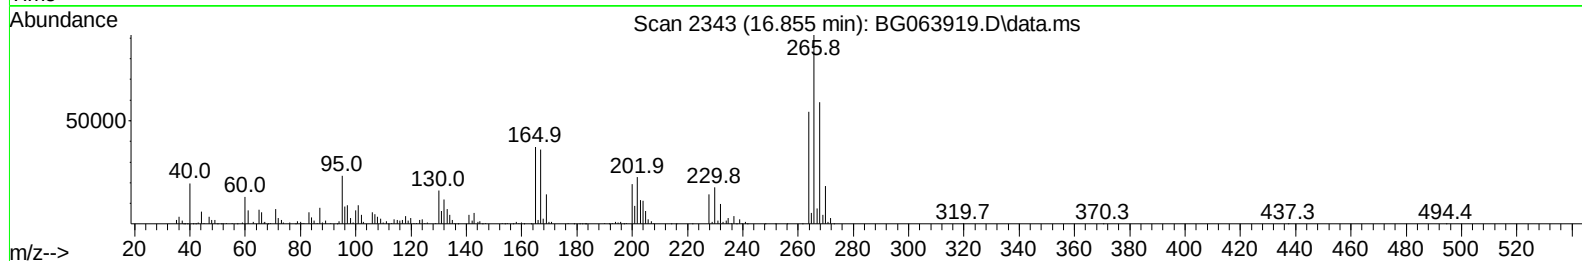


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010325\
Data File : BG063919.D
Acq On : 3 Jan 2025 10:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 23:23:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 23:17:54 2025
Response via : Initial Calibration

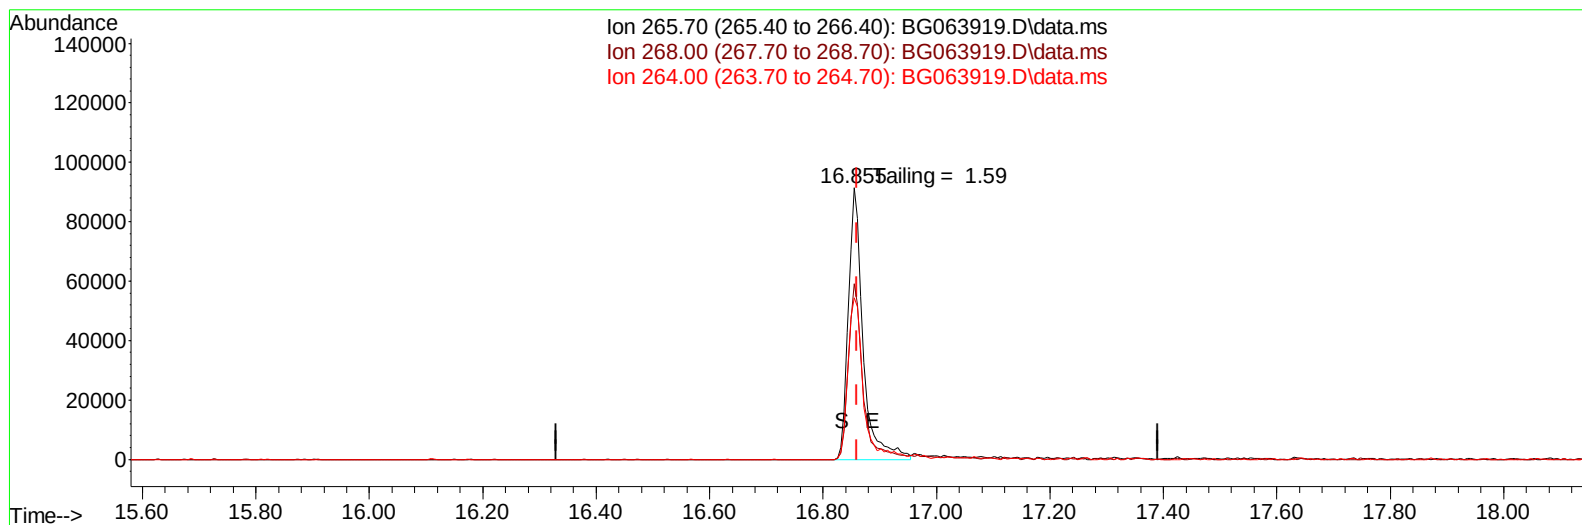

TIC: BG063919.D\data.ms

(70) Pentachlorophenol (C)




16.855min (-0.005) 545154.77 ng

response 165553

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.10	64.62
264.00	65.30	59.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010325\
Data File : BG063919.D
Acq On : 3 Jan 2025 10:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 03 23:23:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 23:17:54 2025
Response via : Initial Calibration

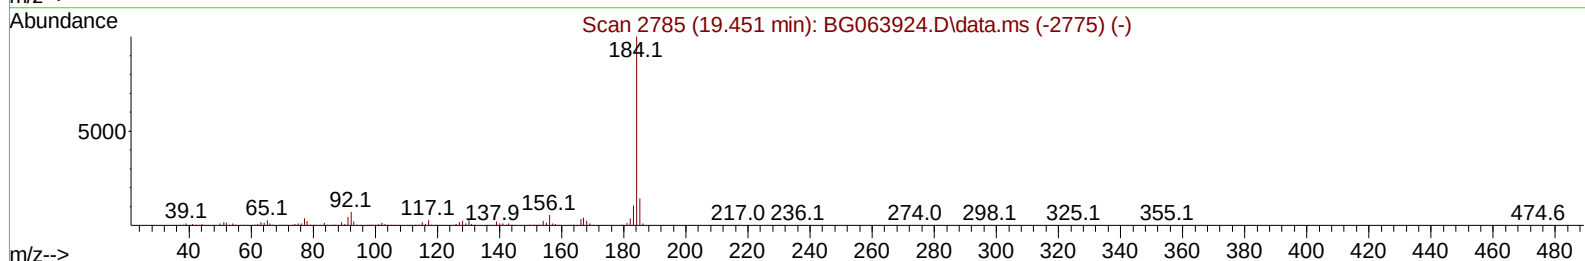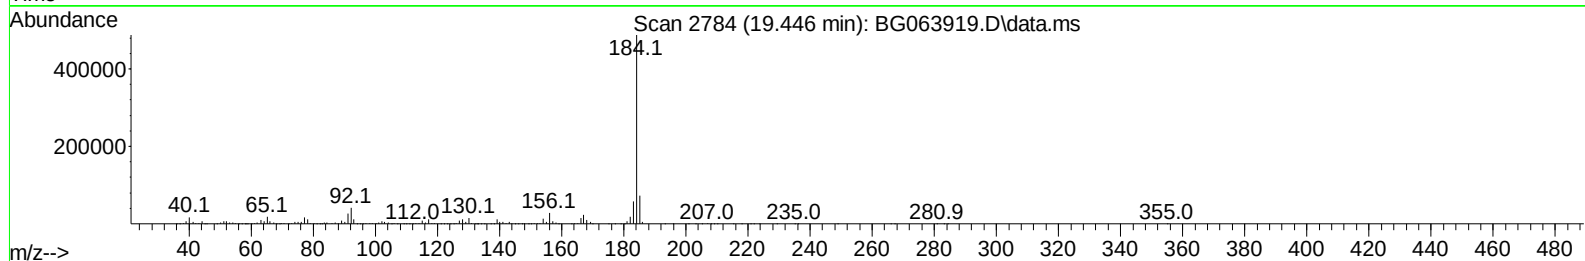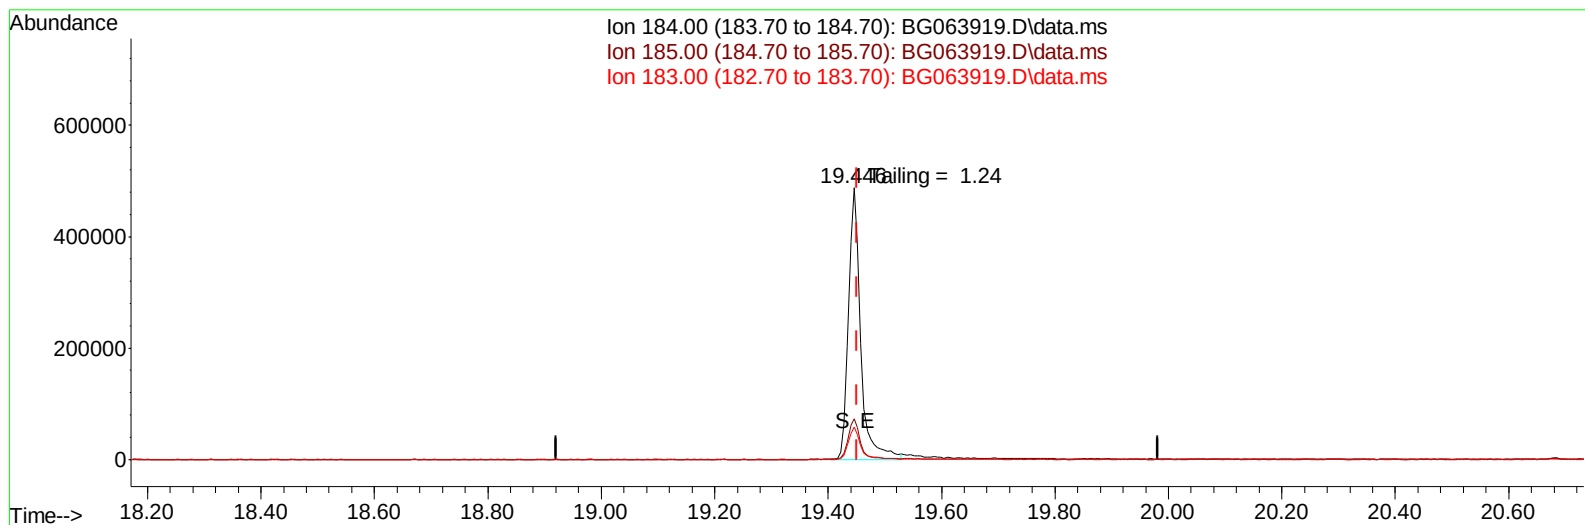

TIC: BG063919.D\data.ms

(77) Benzidine**19.446min (-0.005) 706717.18 ng****response 751524**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.90
183.00	10.50	12.04
0.00	0.00	0.00