

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010325\
Data File : BG063931.D
Acq On : 3 Jan 2025 18:40
Operator : RC/JU
Sample : PB165945BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB165945BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010325.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG063931.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.391	386	392	403	rBV	2240710	3464530	38.60%	10.072%
2	6.984	655	663	673	rBV	2163985	3596773	40.08%	10.456%
3	7.795	794	801	809	rVB	315579	537541	5.99%	1.563%
4	8.952	989	998	1005	rBV	1326324	2347625	26.16%	6.825%
5	10.585	1268	1276	1284	rBV	388703	736715	8.21%	2.142%
6	13.053	1689	1696	1706	rBV	3338100	5059930	56.38%	14.710%
7	14.440	1924	1932	1941	rBV	674158	1080426	12.04%	3.141%
8	15.938	2180	2187	2200	rBV	2479928	3812136	42.48%	11.082%
9	17.195	2394	2401	2413	rBV2	921184	1437113	16.01%	4.178%
10	19.827	2843	2849	2865	rBV	6713245	8974540	100.00%	26.089%
11	21.449	3119	3125	3134	rBV	989173	1634775	18.22%	4.752%
12	24.475	3629	3640	3659	rBV	599817	1716955	19.13%	4.991%




Sum of corrected areas: 34399059

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010325\
Data File : BG063931.D
Acq On : 3 Jan 2025 18:40
Operator : RC/JU
Sample : PB165945BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB165945BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

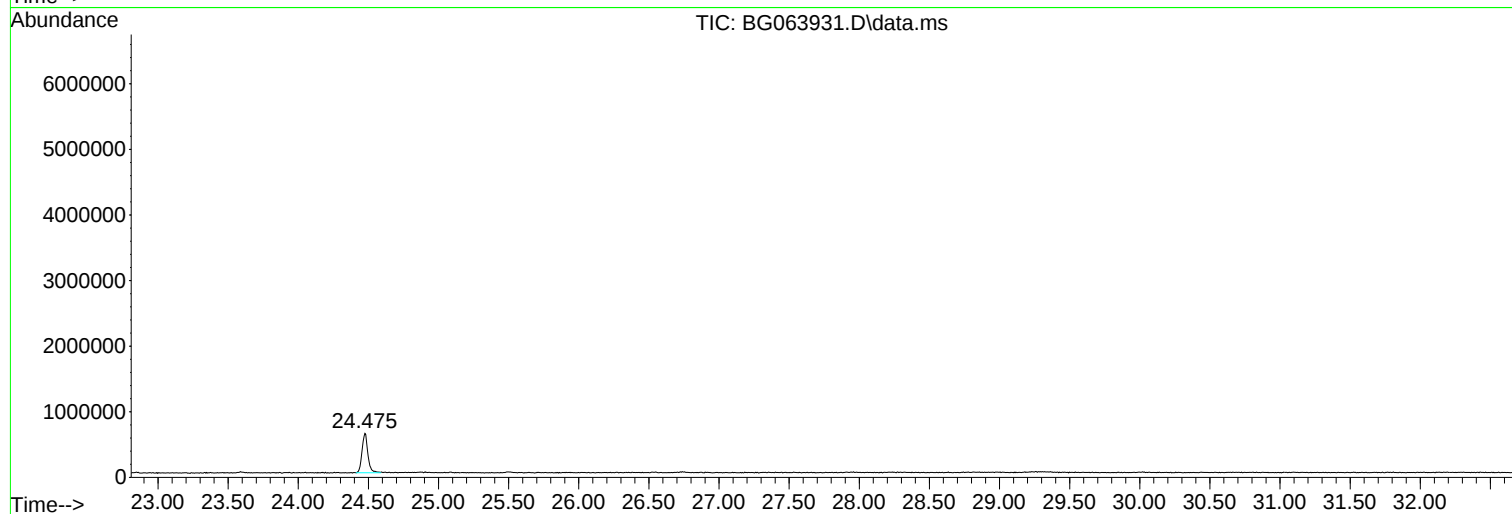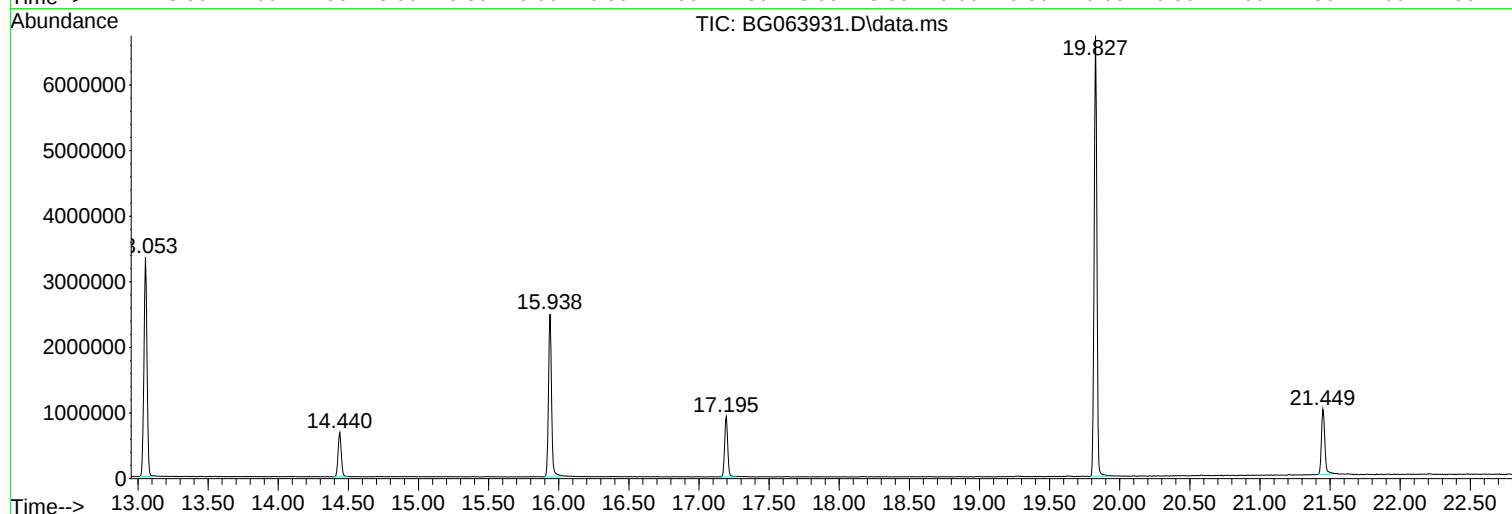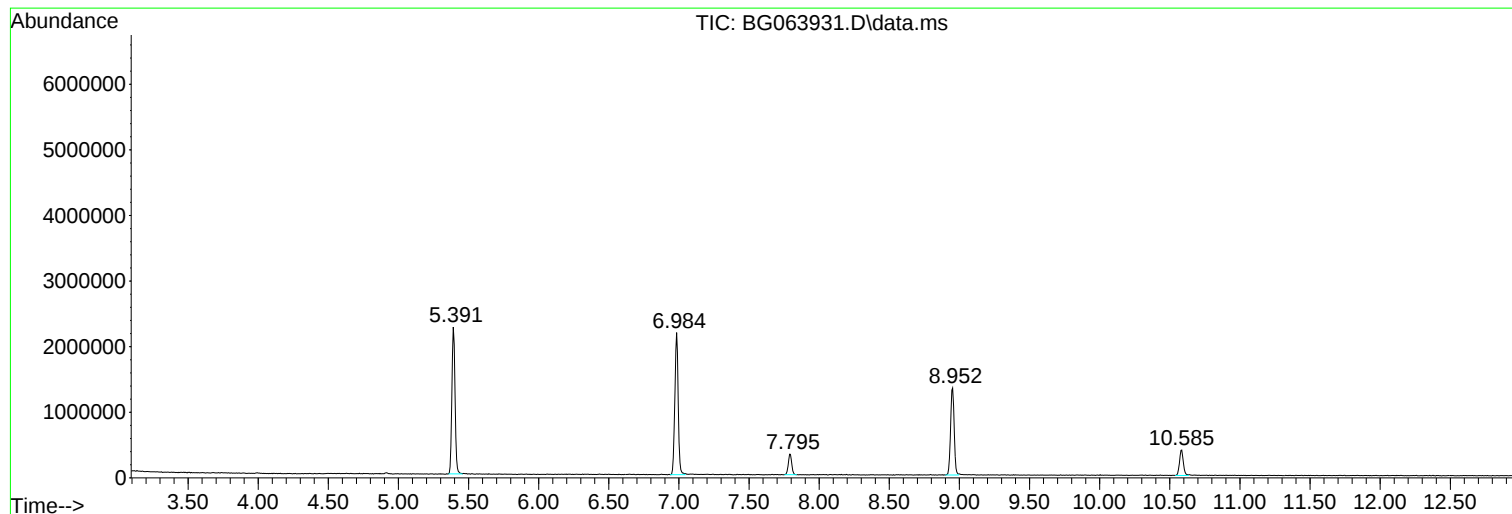

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010325\
Data File : BG063931.D
Acq On : 3 Jan 2025 18:40
Operator : RC/JU
Sample : PB165945BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB165945BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010325\
Data File : BG063931.D
Acq On : 3 Jan 2025 18:40
Operator : RC/JU
Sample : PB165945BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB165945BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------