
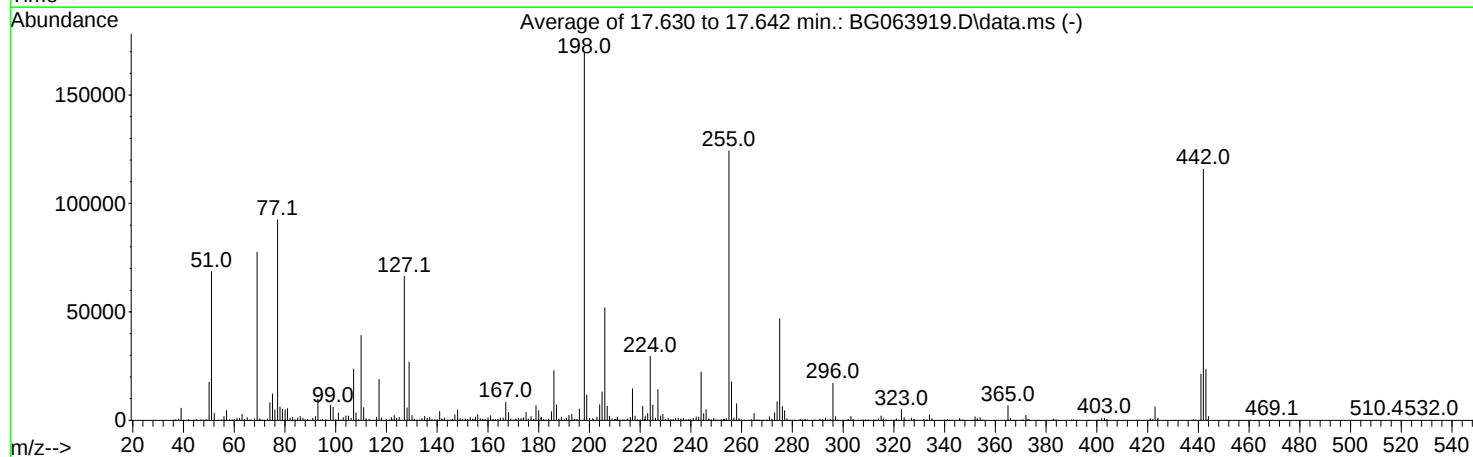


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010325\
Data File : BG063919.D
Acq On : 3 Jan 2025 10:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jan 03 23:17:54 2025

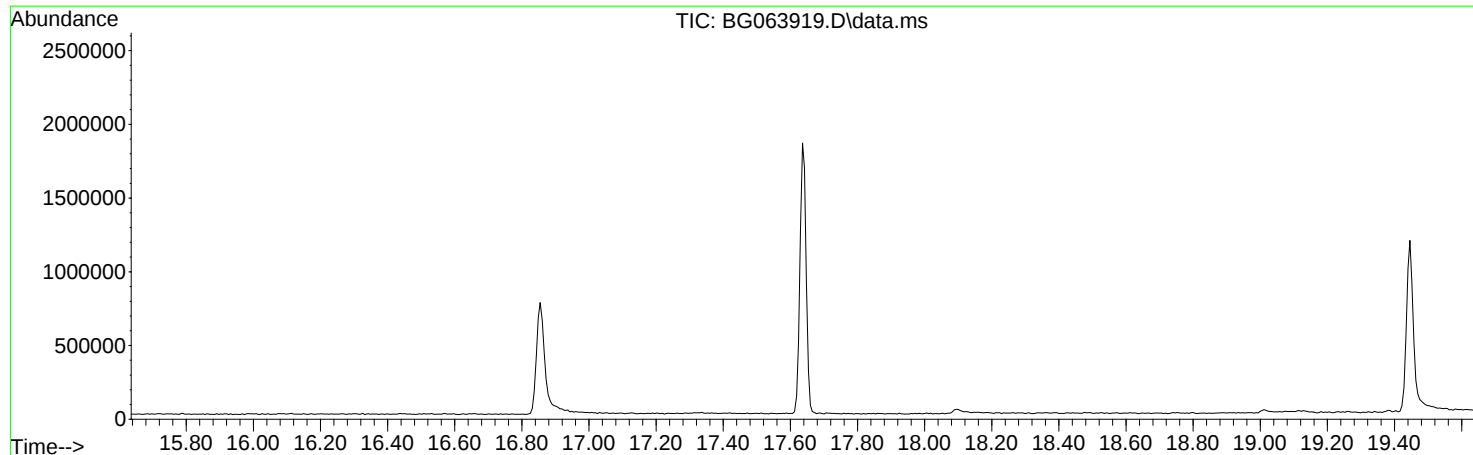

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	40.4	68593	PASS
68	69	0.00	2	1.0	762	PASS
69	198	0.00	100	45.7	77564	PASS
70	69	0.00	2	0.9	722	PASS
127	198	10	80	39.1	66373	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	169600	PASS
199	198	5	9	6.9	11744	PASS
275	198	10	60	27.6	46859	PASS
365	198	1	100	3.9	6682	PASS
441	198	0.01	100	12.5	21260	PASS
442	442	50	100	100.0	115773	PASS
443	442	15	24	20.2	23421	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/3/2025	BNA_G	<u>BG063919.D</u>
Compound Name	Response	Retention Time
DDT	581162	20.68
DDD	37577	20.245
DDE	640	19.734
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
38217	619379	6.17

Instrument :
BNA_G
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010325\
Data File : BG063919.D
Acq On : 3 Jan 2025 10:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 03 23:23:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 23:17:54 2025
Response via : Initial Calibration

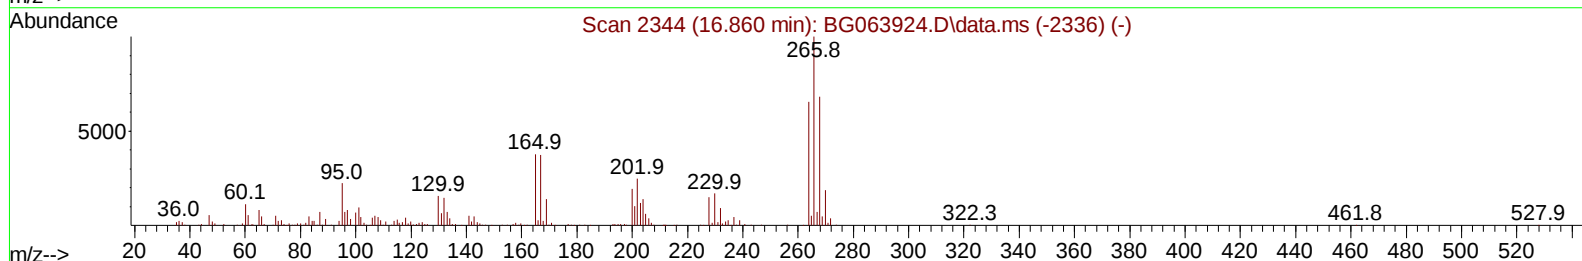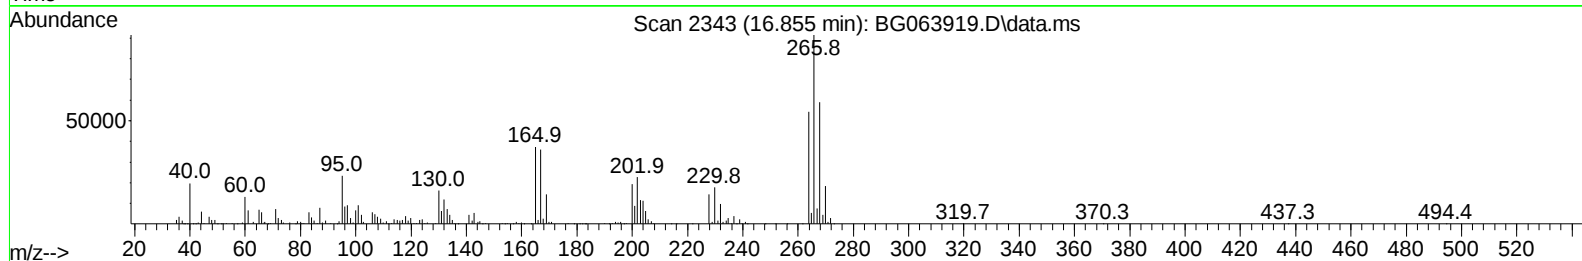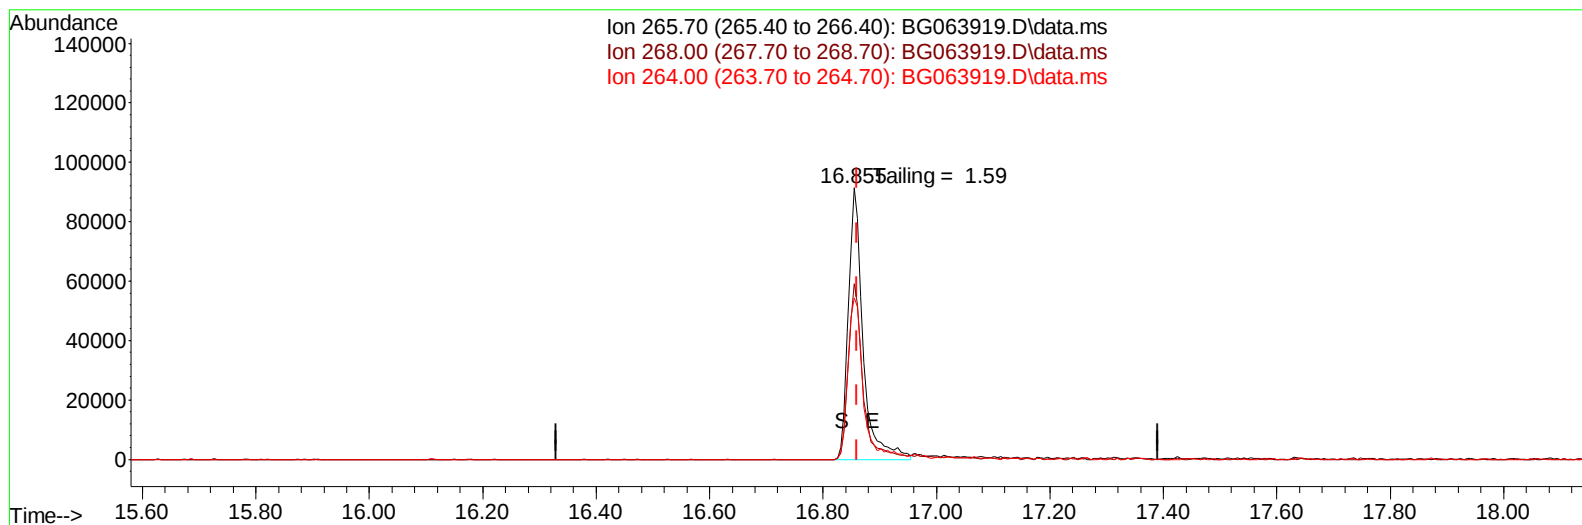

TIC: BG063919.D\data.ms

(70) Pentachlorophenol (C)

16.855min (-0.005) 545154.77 ng




response 165553

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.10	64.62
264.00	65.30	59.49
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010325\
Data File : BG063919.D
Acq On : 3 Jan 2025 10:22
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Jan 03 23:23:47 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG010325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 03 23:17:54 2025
Response via : Initial Calibration

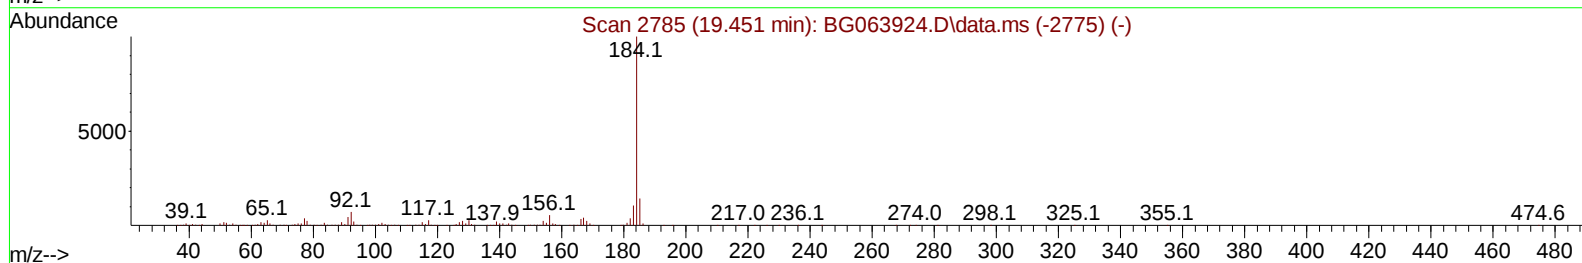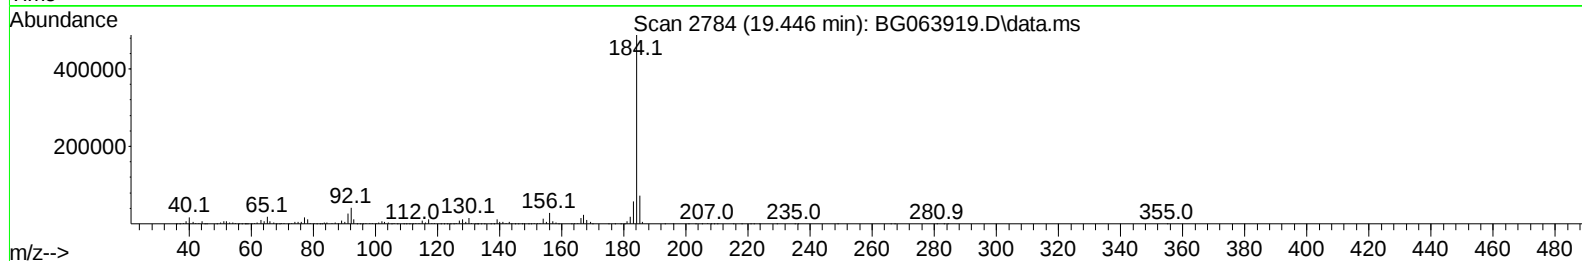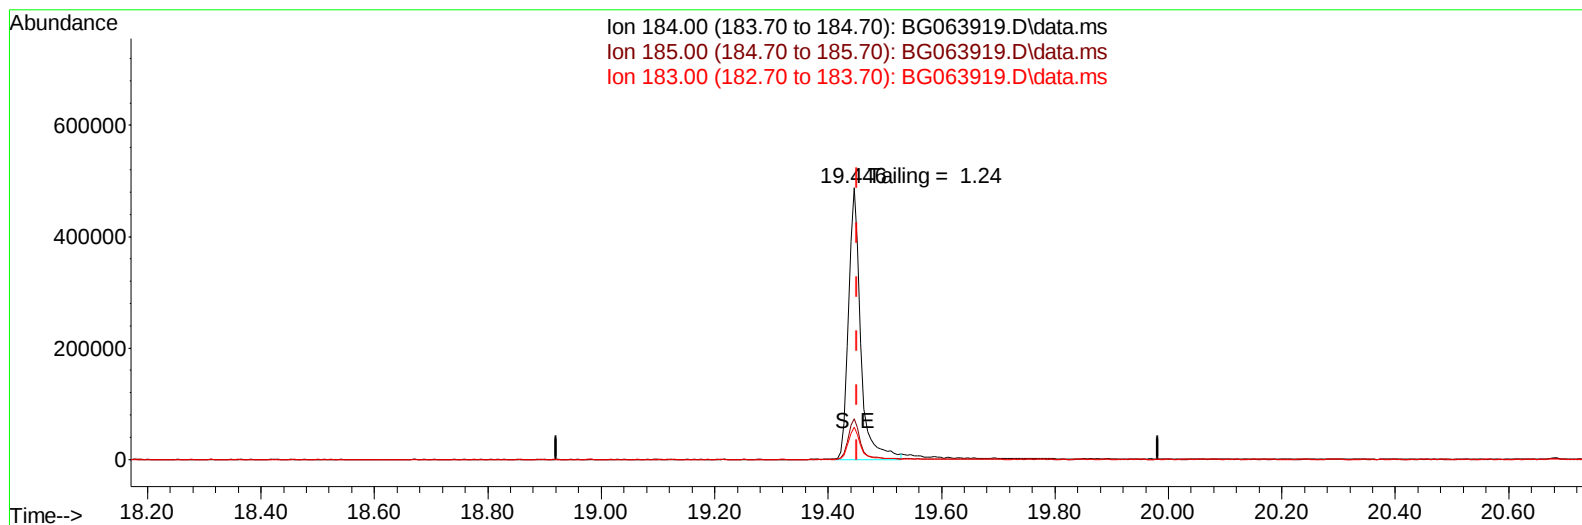

TIC: BG063919.D\data.ms

(77) Benzidine

19.446min (-0.005) 706717.18 ng

response 751524

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.90
183.00	10.50	12.04
0.00	0.00	0.00