

Data Path : U:\HPCHEM1\BNA G\DATA\BG010418\
 Data File : BG031928.D
 Acq On : 4 Jan 2018 23:06
 Operator : SJ/JU
 Sample : I7102-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BISP-SB-03

Quant Time: Jan 05 04:36:57 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 29 15:51:46 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.79	152	57238	20.00	ng	0.00
21) Naphthalene-d8	11.67	136	243534	20.00	ng	-0.01
38) Acenaphthene-d10	15.42	164	181287	20.00	ng	-0.01
63) Phenanthrene-d10	18.15	188	494327	20.00	ng	0.00
75) Chrysene-d12	22.50	240	575164	20.00	ng	-0.01
86) Perylene-d12	26.23	264	567865	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	6.21	112	325245	103.50	ng	0.00
7) Phenol-d6	7.89	99	420200	102.99	ng	0.00
23) Nitrobenzene-d5	9.98	82	228553	70.87	ng	0.00
41) 2,4,6-Tribromophenol	16.89	330	304409	110.05	ng	0.00
44) 2-Fluorobiphenyl	14.05	172	667330	46.20	ng	0.00
78) Terphenyl-d14	20.69	244	1314062	52.20	ng	0.00
Target Compounds						
10) Phenol	7.92	94	15965	3.876	ng	Qvalue 97
49) Dimethylphthalate	14.84	163	62467	3.911	ng	# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA G\DATA\BG010418\
Data File : BG031928.D
Acq On : 4 Jan 2018 23:06
Operator : SJ/JU
Sample : I7102-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BISP-SB-03

Quant Time: Jan 05 04:36:57 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG122117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 29 15:51:46 2017
Response via : Initial Calibration

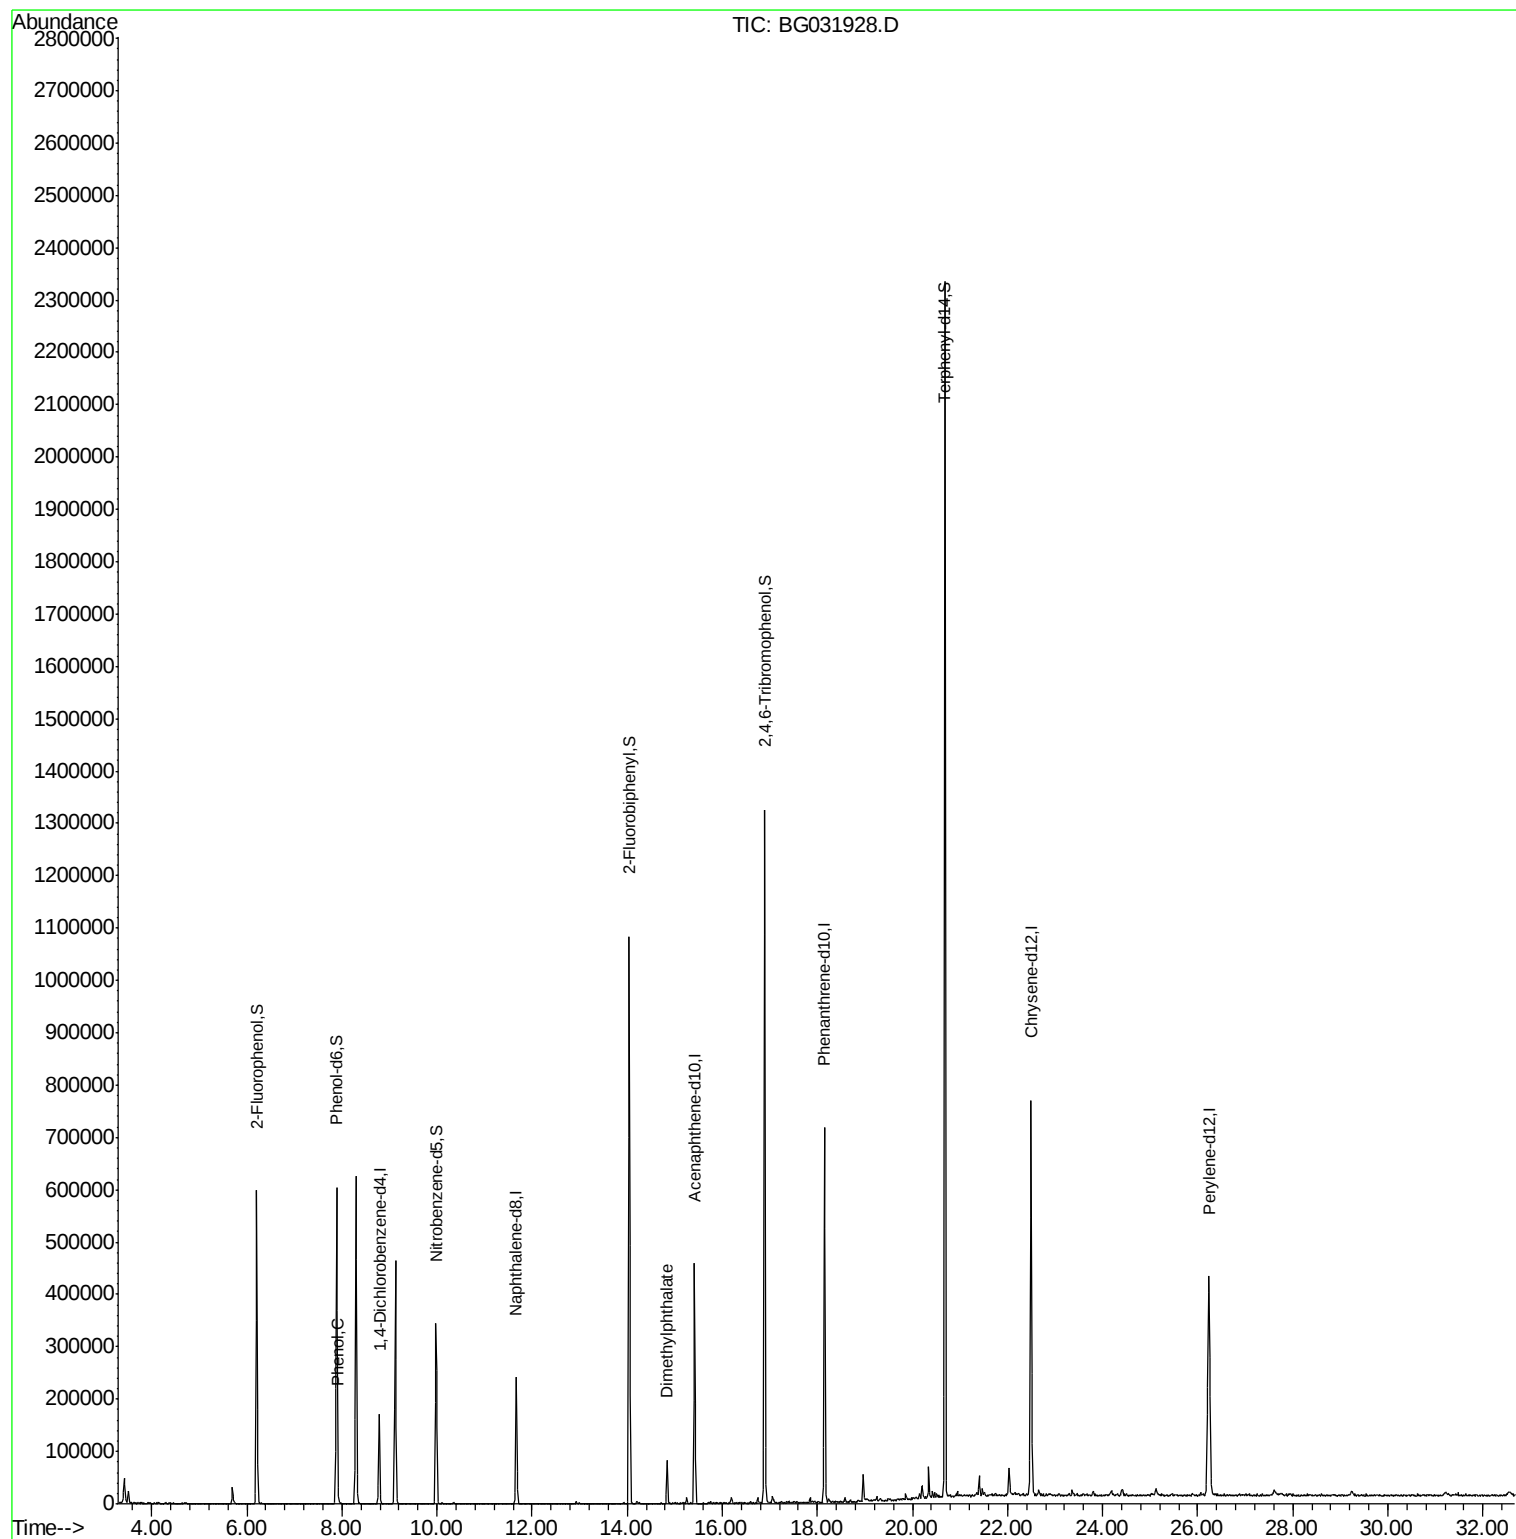

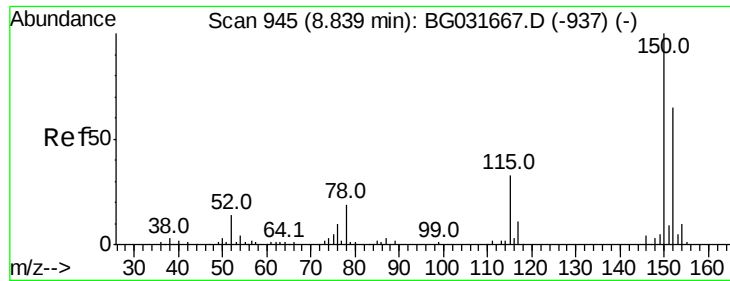


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.79 min Scan# 936
Delta R.T. -0.00 min
Lab File: BG031928.D
Acq: 4 Jan 2018 23:06

Instrument :
BNA_G
ClientSampleId :
BISP-SB-03

Tot Ion:152 Resp: 57238
Ion Ratio Lower Upper
152 100
150 159.9 126.6 189.8
115 55.0 53.0 79.4

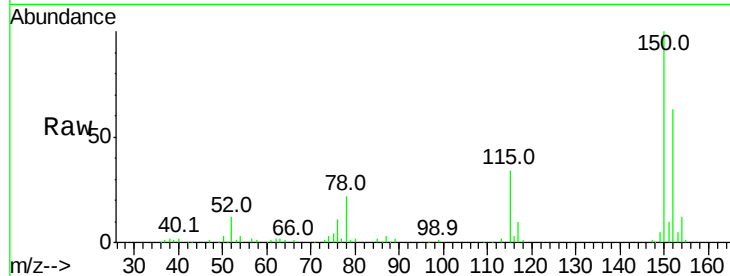


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

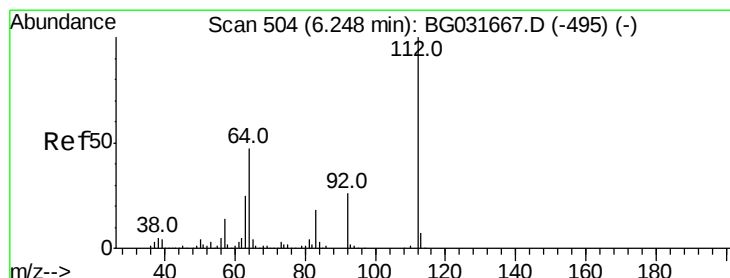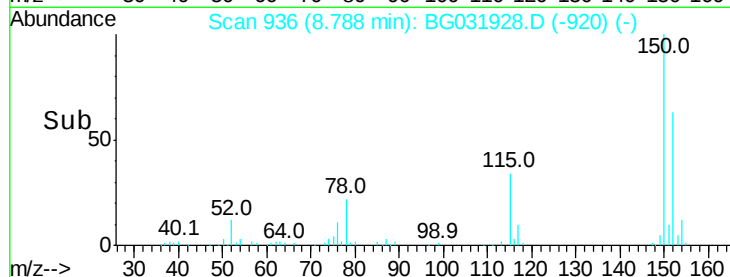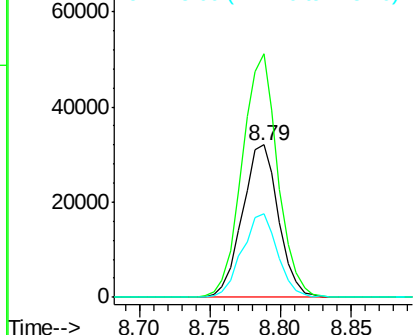



#5

2-Fluorophenol
Concen: 103.497 ng
RT: 6.21 min Scan# 497
Delta R.T. -0.00 min
Lab File: BG031928.D
Acq: 4 Jan 2018 23:06

Tgt Ion:112 Resp: 325245
Ion Ratio Lower Upper
112 100
64 49.2 56.3 84.5#
63 26.9 30.1 45.1#

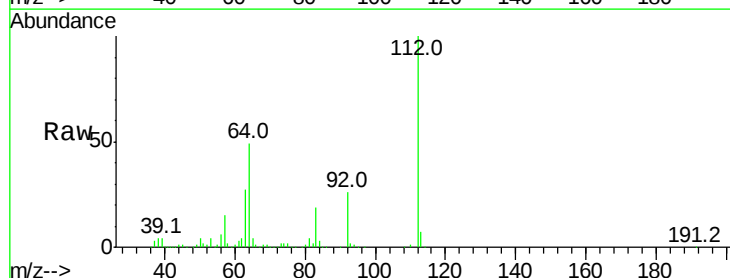

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

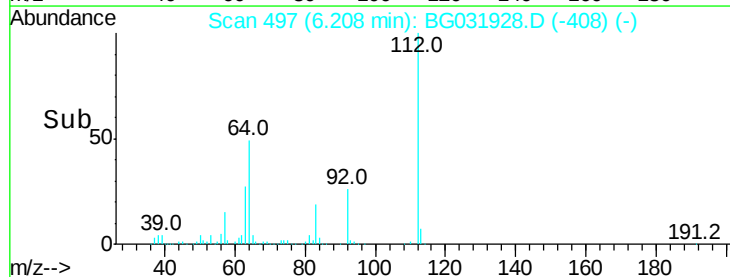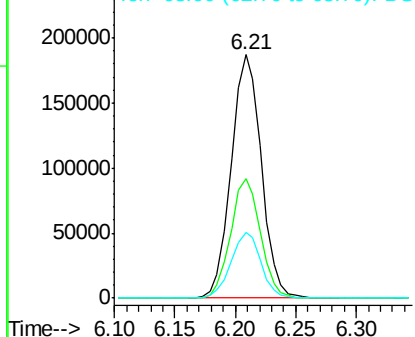



#7

Phenol-d6

Concen: 102.988 ng

RT: 7.89 min Scan# 783

Delta R.T. -0.00 min

Lab File: BG031928.D

Acq: 4 Jan 2018 23:06

Instrument :

BNA_G

ClientSampleId :

BISP-SB-03


Tot Ion: 99 Resp: 420200

Ion Ratio Lower Upper




99 100

42 14.2 14.1 21.1

71 33.8 26.1 39.1

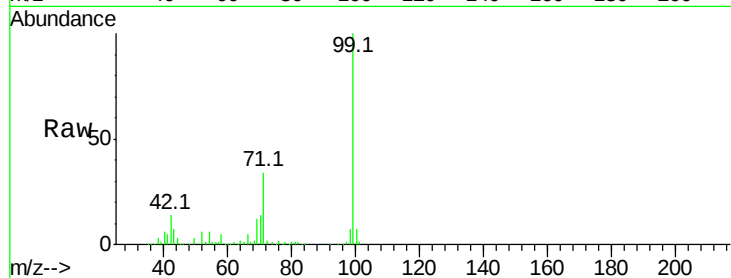

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

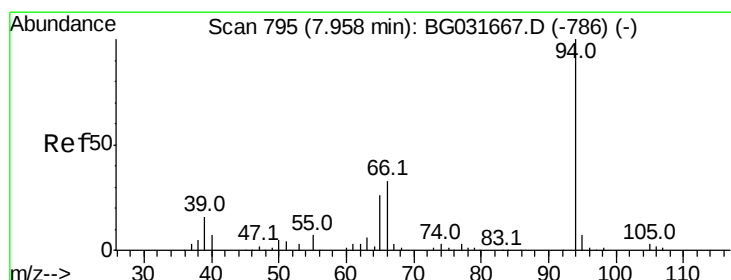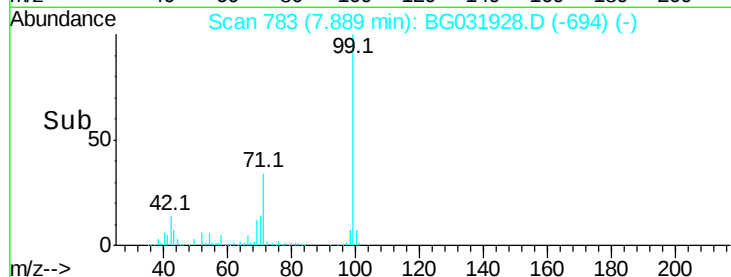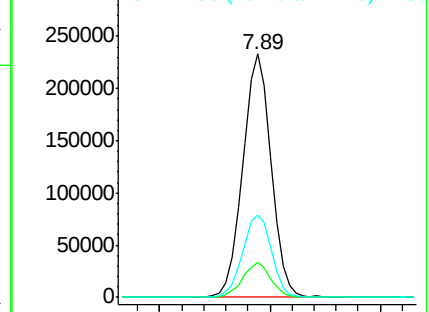

#10

Phenol

Concen: 3.876 ng

RT: 7.92 min Scan# 788

Delta R.T. -0.00 min

Lab File: BG031928.D

Acq: 4 Jan 2018 23:06


Tgt Ion: 94 Resp: 15965

Ion Ratio Lower Upper



94 100

65 31.1 11.9 51.9

66 44.9 22.2 62.2

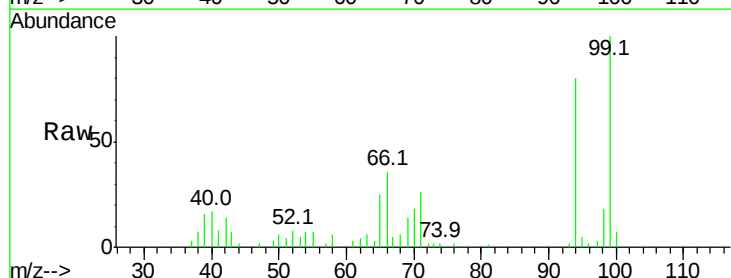

Abundance Ion 94.00 (93.70 to 94.70): BGC
Ion 65.00 (64.70 to 65.70): BGC
Ion 66.00 (65.70 to 66.70): BGC

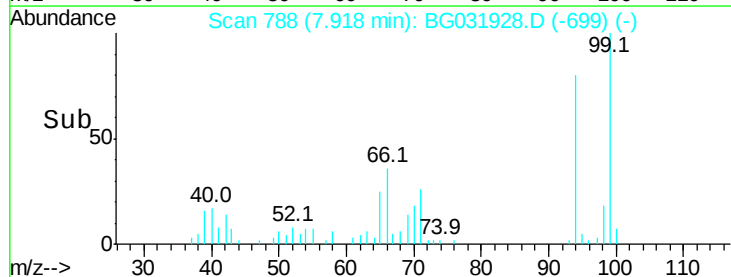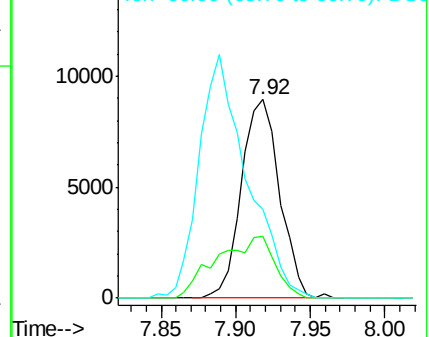



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 11.67 min Scan# 1426

Delta R.T. -0.01 min

Lab File: BG031928.D

Acq: 4 Jan 2018 23:06

Instrument :

BNA_G

ClientSampleId :

BISP-SB-03

Tot Ion:136 Resp: 243534



Ion Ratio Lower Upper

136 100

137 10.8 9.2 13.8

54 4.7 10.3 15.5#

68 4.3 4.5 6.7#

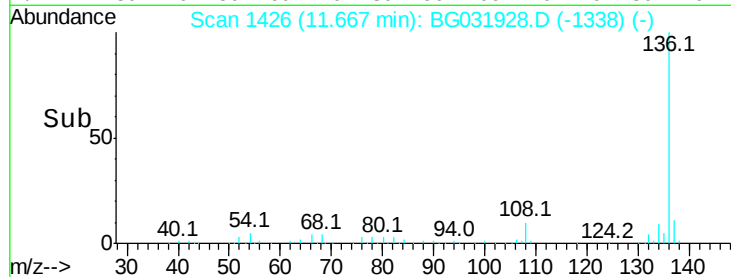
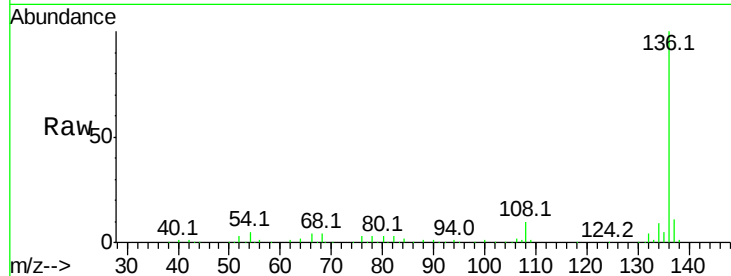


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BGC

Ion 68.00 (67.70 to 68.70): BGC

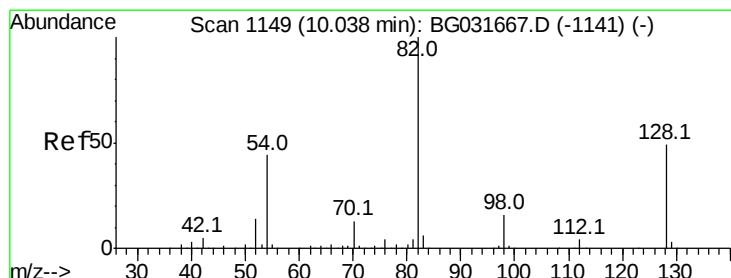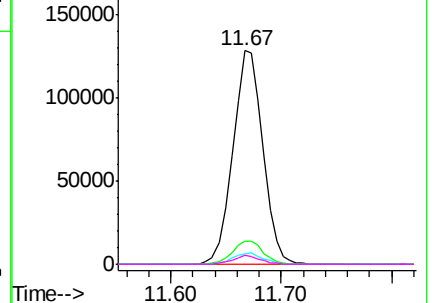

#23

Nitrobenzene-d5

Concen: 70.867 ng

RT: 9.98 min Scan# 1139

Delta R.T. -0.00 min

Lab File: BG031928.D

Acq: 4 Jan 2018 23:06



Tgt Ion: 82 Resp: 228553

Ion Ratio Lower Upper

82 100

128 50.5 29.7 44.5#


54 44.4 43.1 64.7

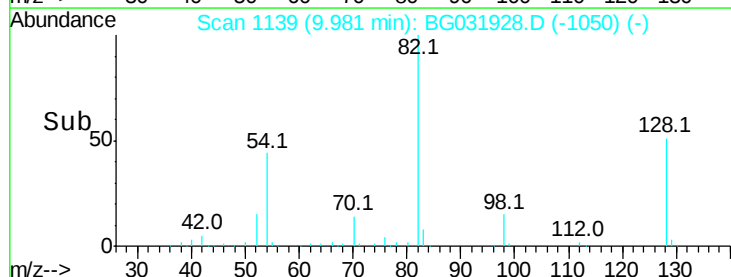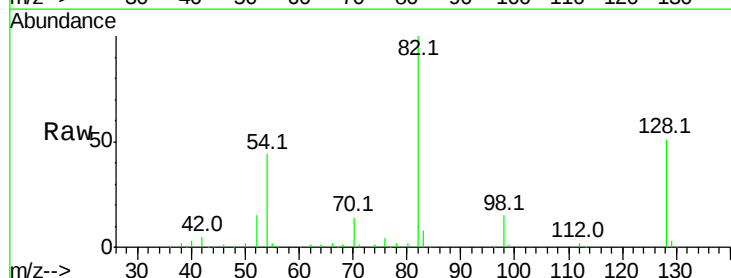


Abundance Ion 82.00 (81.70 to 82.70): BGC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BGC

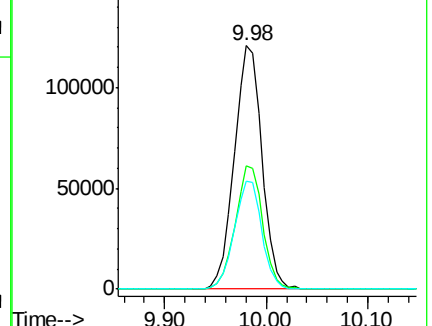

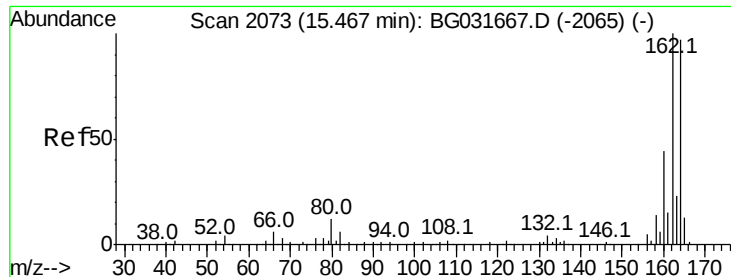

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 15.42 min Scan# 2064

Delta R.T. -0.01 min

Lab File: BG031928.D

Acq: 4 Jan 2018 23:06

Instrument :

BNA_G

ClientSampleId :

BISP-SB-03


Tot Ion:164 Resp: 181287

Ion Ratio Lower Upper

164 100

162 103.0 78.8 118.2




160 44.3 35.4 53.0

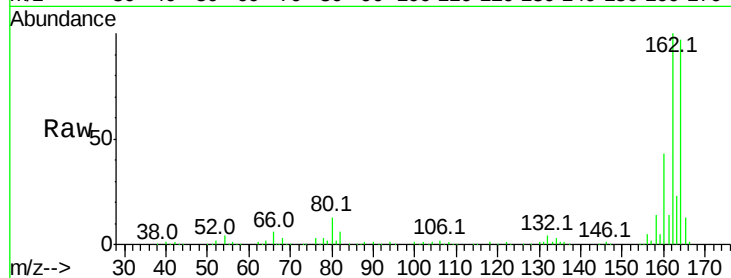

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

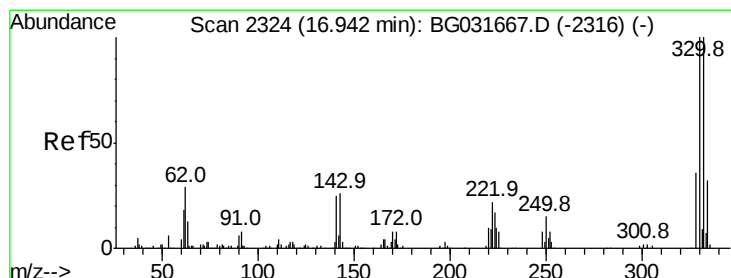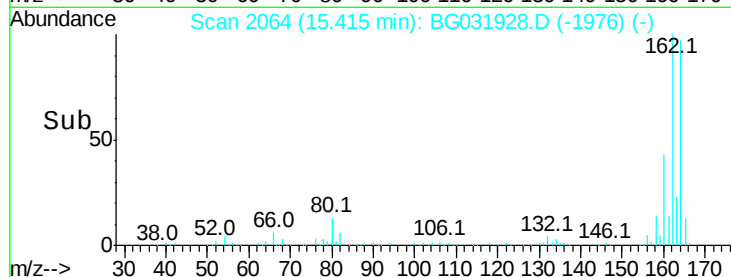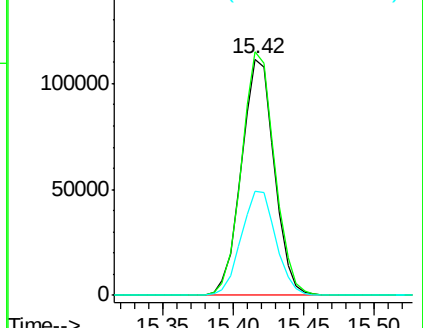

#41

2,4,6-Tribromophenol

Concen: 110.046 ng

RT: 16.89 min Scan# 2315

Delta R.T. -0.00 min

Lab File: BG031928.D

Acq: 4 Jan 2018 23:06


Tgt Ion:330 Resp: 304409

Ion Ratio Lower Upper

330 100

332 95.9 77.0 115.6



141 26.9 25.2 37.8

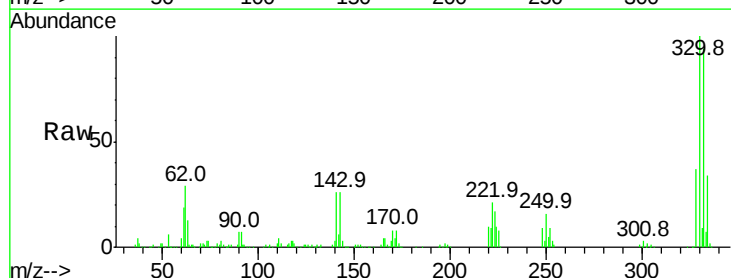

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E



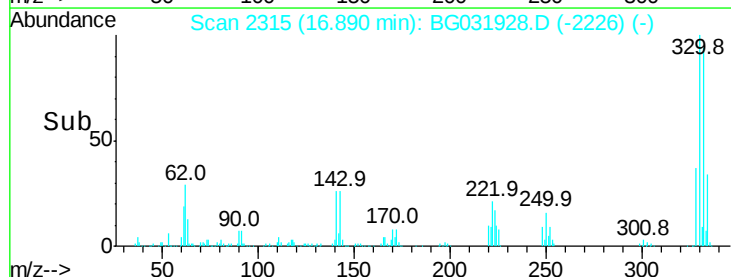
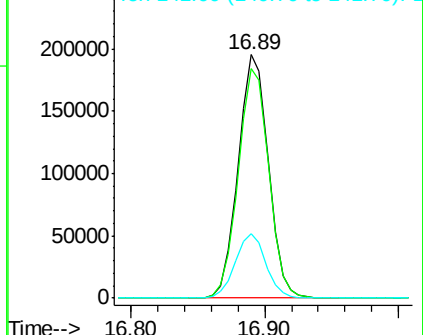




#44
2-Fluorobiphenyl
Concen: 46.202 ng
RT: 14.05 min Scan# 1831
Delta R.T. -0.00 min
Lab File: BG031928.D
Acq: 4 Jan 2018 23:06




Instrument :
BNA_G
ClientSampleId :
BISP-SB-03


Tot Ion:172 Resp: 667330
Ion Ratio Lower Upper
172 100
171 37.7 30.0 45.0
170 23.4 19.5 29.3

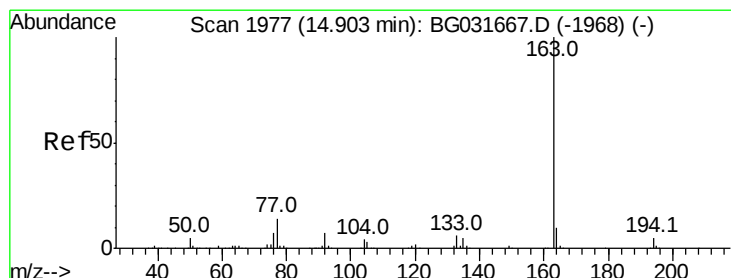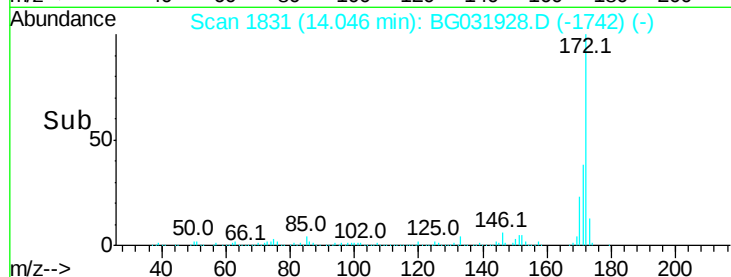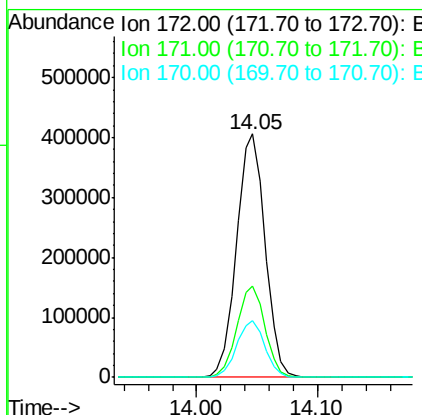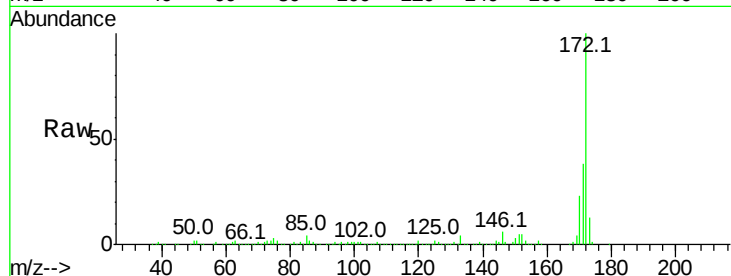

#49
Dimethylphthalate
Concen: 3.911 ng
RT: 14.84 min Scan# 1966
Delta R.T. -0.01 min
Lab File: BG031928.D
Acq: 4 Jan 2018 23:06

Tgt Ion:163 Resp: 62467
Ion Ratio Lower Upper
163 100
194 5.3 3.4 5.2#
164 12.0 8.2 12.4


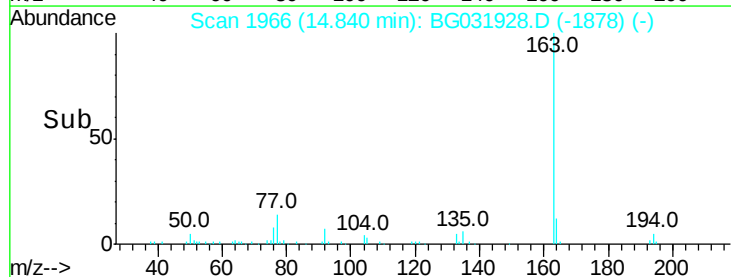
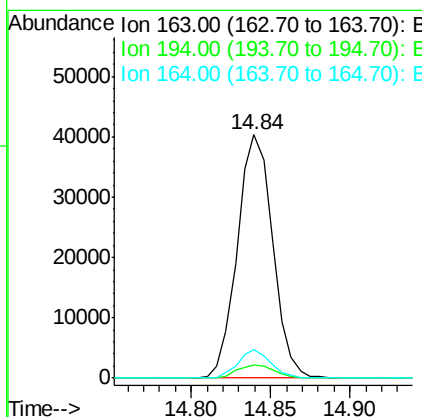
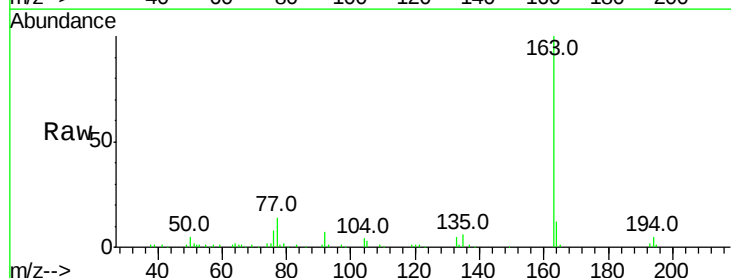


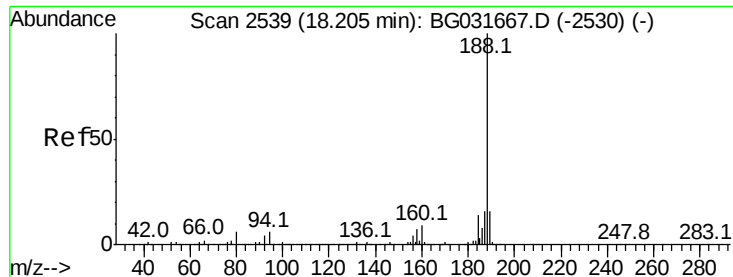

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 18.15 min Scan# 2530
Delta R.T. -0.00 min
Lab File: BG031928.D
Acq: 4 Jan 2018 23:06




Instrument :
BNA_G
ClientSampleId :
BISP-SB-03


Tot Ion:188 Resp: 494327
Ion Ratio Lower Upper
188 100
94 5.5 6.9 10.3#
80 6.0 7.7 11.5#

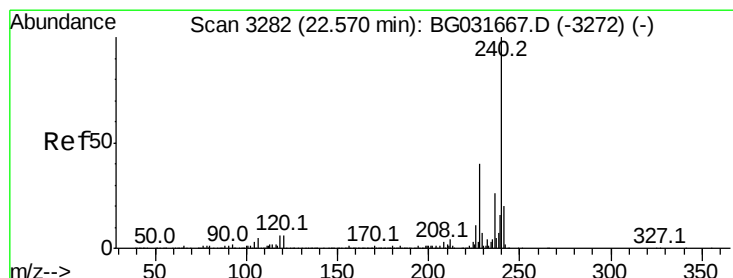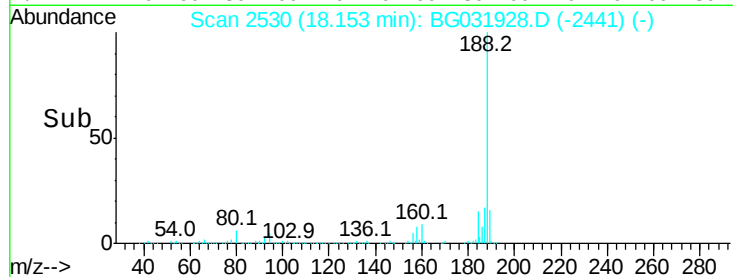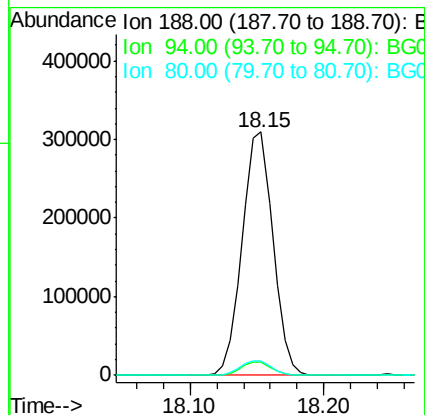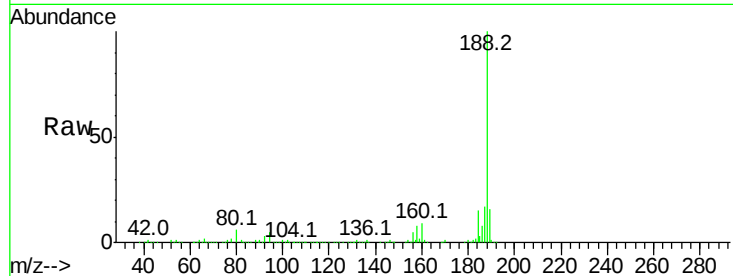

#75
Chrysene-d12
Concen: 20.000 ng
RT: 22.50 min Scan# 3269
Delta R.T. -0.01 min
Lab File: BG031928.D
Acq: 4 Jan 2018 23:06

Tgt Ion:240 Resp: 575164
Ion Ratio Lower Upper
240 100
120 5.7 6.8 10.2#
236 25.8 20.9 31.3

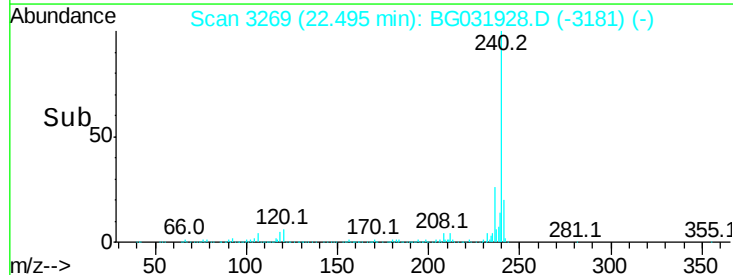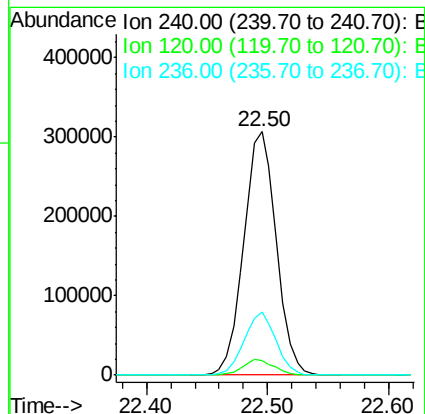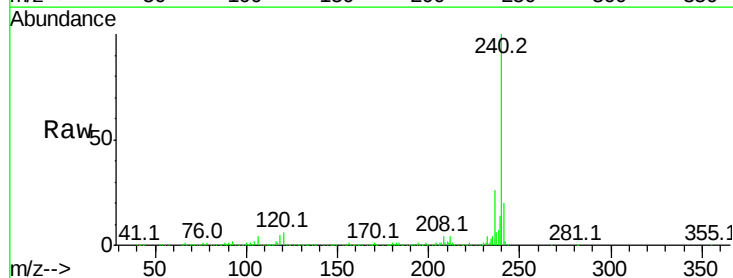

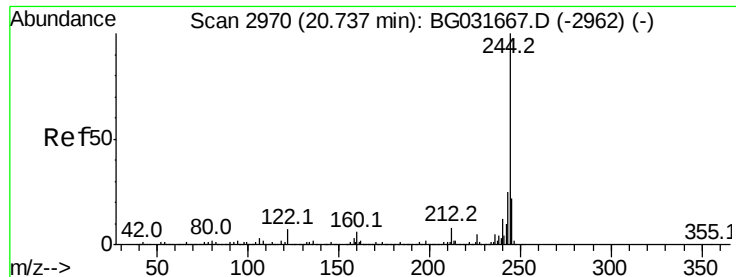

#78

Terphenyl-d14

Concen: 52.197 ng

RT: 20.69 min Scan# 2961

Delta R.T. -0.00 min

Lab File: BG031928.D

Acq: 4 Jan 2018 23:06

Instrument :

BNA_G

ClientSampleId :

BISP-SB-03


Tot Ion:244 Resp: 1314062

Ion Ratio Lower Upper

244 100

212 7.1 5.8 8.8




122 6.6 7.0 10.4#

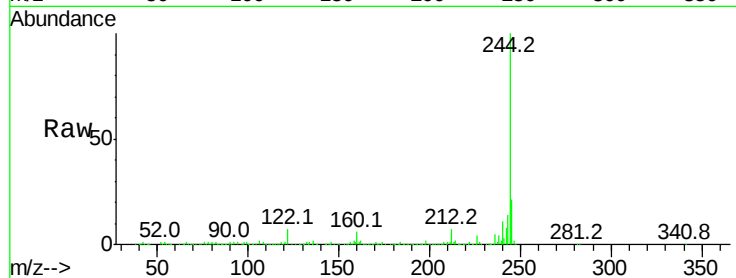

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

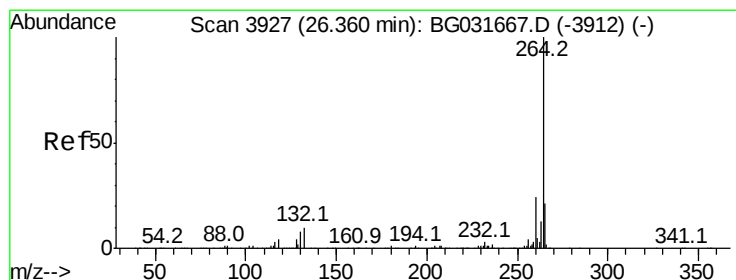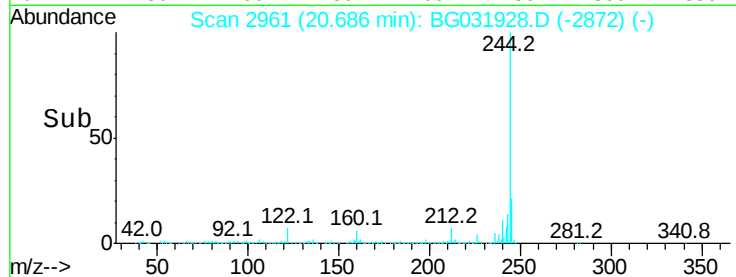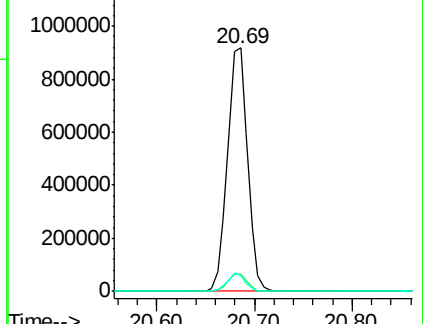

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.23 min Scan# 3905

Delta R.T. -0.02 min

Lab File: BG031928.D

Acq: 4 Jan 2018 23:06


Tgt Ion:264 Resp: 567865

Ion Ratio Lower Upper

264 100

260 24.3 17.4 26.0

265 20.9 17.7 26.5

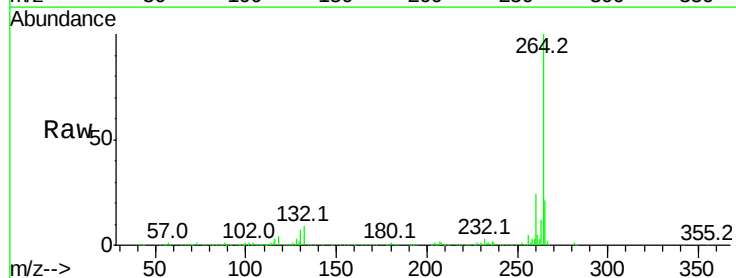

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

