

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010422\
 Data File : BG051866.D
 Acq On : 4 Jan 2022 12:03
 Operator : CG/JU
 Sample : PB141818BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK818

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

Signal : TIC: BG051866.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.585	13	16	22	rBV3	7848	11028	1.13%	0.120%
2	3.767	44	47	49	rVB3	1161	1094	0.11%	0.012%
3	3.967	80	81	85	rBV3	805	1079	0.11%	0.012%
4	4.014	85	89	103	rBV	98191	167890	17.24%	1.833%
5	4.225	124	125	127	rBV2	1400	988	0.10%	0.011%
6	4.372	145	150	151	rBV2	2521	2801	0.29%	0.031%
7	4.460	162	165	168	rBV	812	1046	0.11%	0.011%
8	4.566	180	183	186	rVB2	1036	1093	0.11%	0.012%
9	6.111	443	446	451	rVB	813	1306	0.13%	0.014%
10	6.164	451	455	456	rBV	704	1002	0.10%	0.011%
11	7.398	658	665	679	rBV	129528	218892	22.48%	2.390%
12	7.562	686	693	701	rVB	86586	148898	15.29%	1.626%
13	7.785	724	731	739	rVV2	117026	196741	20.21%	2.149%
14	8.261	805	812	821	rVV	97336	169715	17.43%	1.853%
15	8.960	924	931	938	rBV	143763	248347	25.51%	2.712%
16	9.430	1003	1011	1019	rVV	117697	212448	21.82%	2.320%
17	10.159	1128	1135	1143	rVB	98562	171953	17.66%	1.878%
18	10.705	1221	1228	1242	rVB	138101	250810	25.76%	2.739%
19	11.093	1287	1294	1302	rBV	131830	242100	24.87%	2.644%
20	11.222	1309	1316	1326	rBV	141058	260164	26.72%	2.841%
21	12.667	1558	1562	1567	rBV3	1407	2316	0.24%	0.025%
22	13.566	1709	1715	1717	rBV	641	1090	0.11%	0.012%
23	14.288	1831	1838	1845	rBV	290435	445375	45.74%	4.864%
24	14.588	1883	1889	1899	rBV	319948	500606	51.42%	5.467%
25	14.893	1934	1941	1949	rBV	231930	373292	38.34%	4.077%
26	15.070	1964	1971	1980	rBV	149196	253097	26.00%	2.764%
27	15.886	2102	2110	2119	rVB	412832	643649	66.11%	7.029%
28	15.986	2121	2127	2138	rVV2	135632	203843	20.94%	2.226%
29	16.127	2149	2151	2154	rVB2	1345	1150	0.12%	0.013%
30	16.562	2222	2225	2228	rBV2	963	1033	0.11%	0.011%
31	16.785	2260	2263	2265	rBV2	970	1285	0.13%	0.014%
32	16.855	2274	2275	2277	rBV	1042	986	0.10%	0.011%
33	17.108	2316	2318	2323	rVB	744	1156	0.12%	0.013%
34	17.419	2368	2371	2377	rBV2	1374	2615	0.27%	0.029%
35	17.643	2402	2409	2415	rBV	362544	545508	56.03%	5.957%
36	17.742	2419	2426	2436	rVV	513510	793704	81.52%	8.668%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010422\
 Data File : BG051866.D
 Acq On : 4 Jan 2022 12:03
 Operator : CG/JU
 Sample : PB141818BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK818

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
 Title : SVOA CALIBRATION

37	17.930	2454	2458	2461	rBV2	664	1078	0.11%	0.012%
38	18.248	2511	2512	2514	rBV2	1732	1014	0.10%	0.011%
39	18.301	2518	2521	2524	rBV2	1043	1297	0.13%	0.014%
40	18.430	2541	2543	2546	rVV4	1242	1250	0.13%	0.014%
41	18.512	2555	2557	2560	rVB2	1381	1380	0.14%	0.015%
42	18.547	2560	2563	2566	rBV3	1101	1497	0.15%	0.016%
43	18.659	2581	2582	2584	rBV2	1243	1047	0.11%	0.011%
44	18.706	2588	2590	2593	rBV2	906	1047	0.11%	0.011%
45	18.753	2595	2598	2599	rBV3	937	1058	0.11%	0.012%
46	18.870	2617	2618	2620	rVB2	2175	1059	0.11%	0.012%
47	18.900	2620	2623	2625	rBV3	1945	2338	0.24%	0.026%
48	18.953	2630	2632	2634	rBV	1038	1036	0.11%	0.011%
49	19.058	2648	2650	2653	rVB3	989	1004	0.10%	0.011%
50	19.293	2688	2690	2695	rBV4	1832	2510	0.26%	0.027%
51	19.329	2695	2696	2698	rVB2	1794	1071	0.11%	0.012%
52	19.346	2698	2699	2701	rBV2	1893	1282	0.13%	0.014%
53	19.464	2717	2719	2720	rVB2	2146	1010	0.10%	0.011%
54	19.475	2720	2721	2723	rBV2	1274	1077	0.11%	0.012%
55	19.581	2735	2739	2744	rVV5	9629	12920	1.33%	0.141%
56	19.652	2748	2751	2758	rVV6	6770	10984	1.13%	0.120%
57	19.775	2771	2772	2773	rBV	1982	1091	0.11%	0.012%
58	19.828	2779	2781	2782	rBV2	1531	1119	0.11%	0.012%
59	19.857	2784	2786	2787	rVB	2639	1467	0.15%	0.016%
60	19.875	2787	2789	2790	rBV	2667	1906	0.20%	0.021%
61	20.016	2807	2813	2819	rBV	706925	973613	100.00%	10.633%
62	20.192	2842	2843	2844	rBV	2528	1184	0.12%	0.013%
63	20.210	2844	2846	2848	rVV3	2276	1539	0.16%	0.017%
64	21.960	3137	3144	3151	rVB	331613	573606	58.92%	6.264%
65	24.433	3563	3565	3575	rVB7	15504	27011	2.77%	0.295%
66	25.203	3684	3696	3707	rBV2	271507	802412	82.42%	8.763%
67	25.438	3726	3736	3752	rVB2	169093	563975	57.93%	6.159%
68	26.237	3870	3872	3873	rBV	4971	3659	0.38%	0.040%
69	26.724	3951	3955	3967	rVB10	16302	46965	4.82%	0.513%
70	28.222	4205	4210	4211	rBV5	12619	19228	1.97%	0.210%
71	28.939	4330	4332	4333	rBV2	4824	2950	0.30%	0.032%
72	32.235	4891	4893	4894	rBV	6518	3165	0.33%	0.035%
73	32.517	4939	4941	4943	rBV3	5144	4885	0.50%	0.053%




Sum of corrected areas: 9156834

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010422\
Data File : BG051866.D
Acq On : 4 Jan 2022 12:03
Operator : CG/JU
Sample : PB141818BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

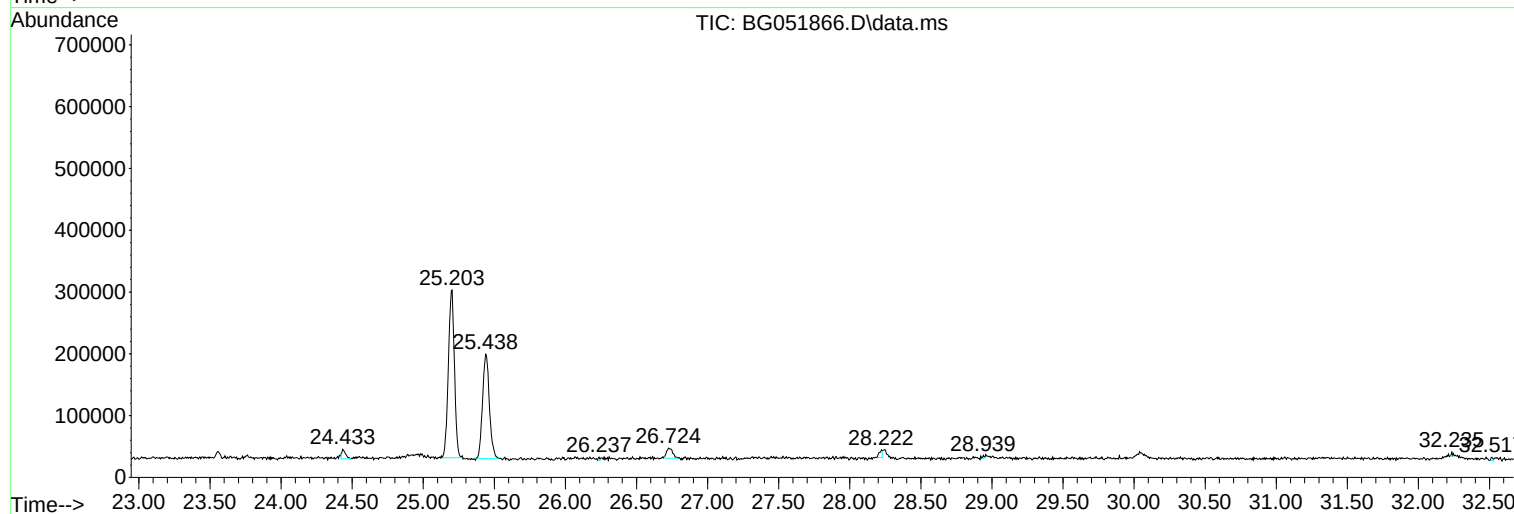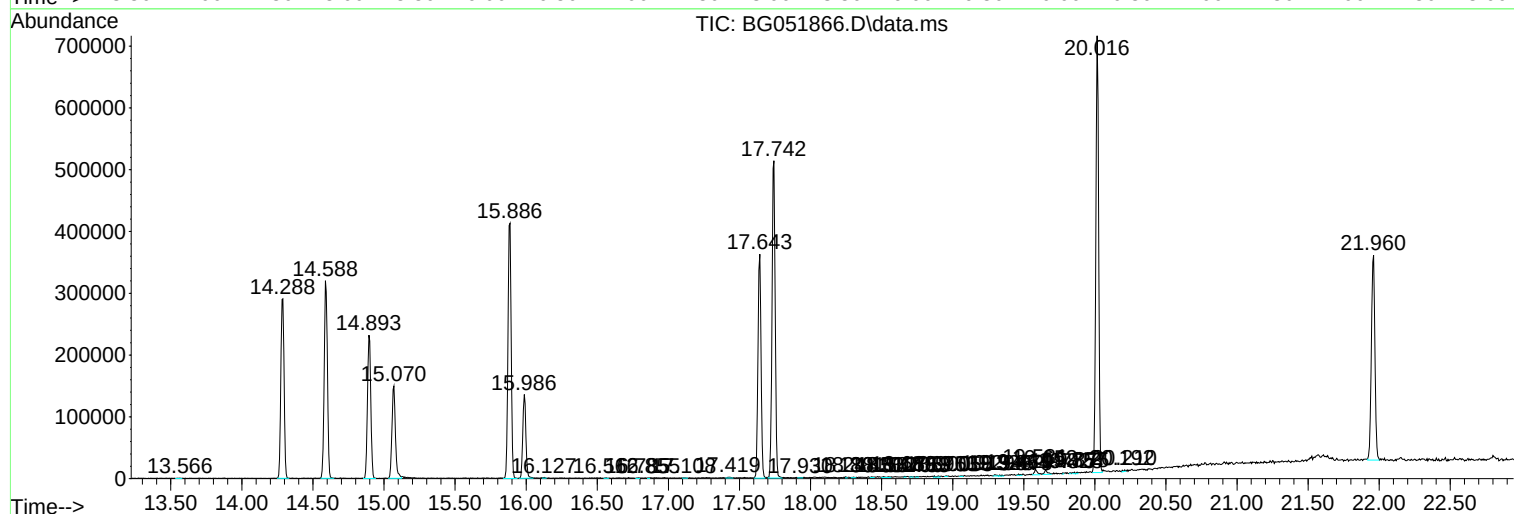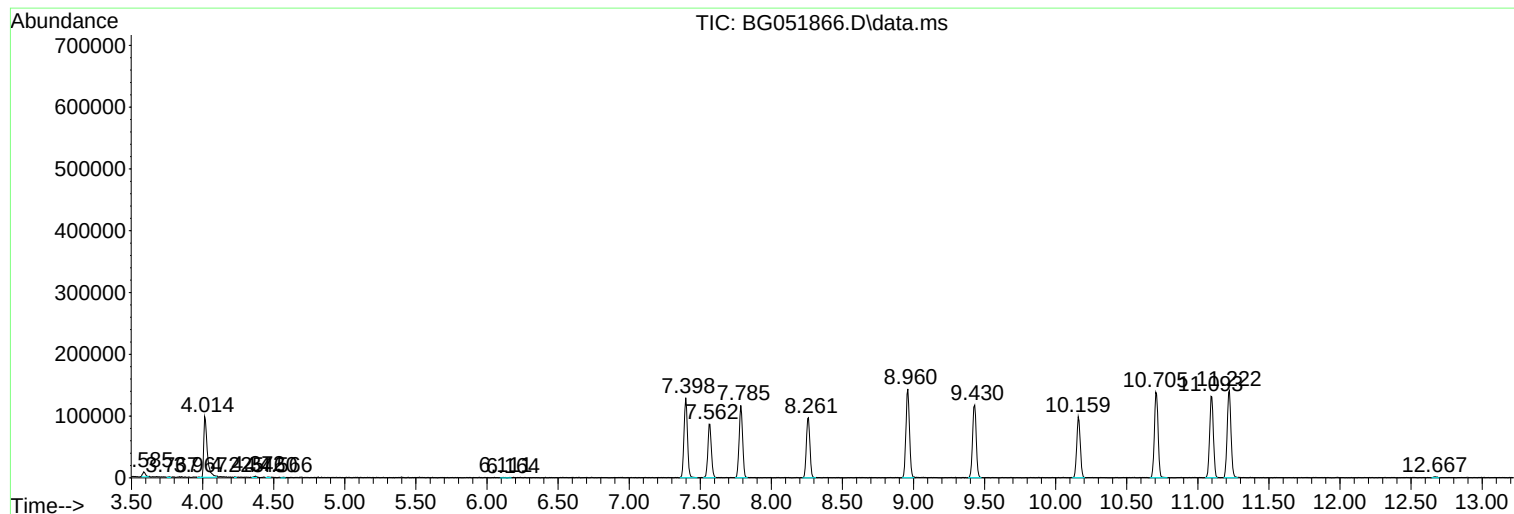

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010422\
Data File : BG051866.D
Acq On : 4 Jan 2022 12:03
Operator : CG/JU
Sample : PB141818BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG010422\
Data File : BG051866.D
Acq On : 4 Jan 2022 12:03
Operator : CG/JU
Sample : PB141818BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK818

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG121421.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc